

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081823\
 Data File : BP016656.D
 Acq On : 19 Aug 2023 00:21
 Operator : MA/JU
 Sample : PB154876BL
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK876

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016656.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	14	18	25	rVB	153045	205090	1.71%	0.163%
2	3.828	87	92	113	rBV	2073199	3166326	26.34%	2.509%
3	4.146	142	146	154	rVB	26297	39166	0.33%	0.031%
4	7.187	656	663	678	rBV	2433009	3862904	32.13%	3.061%
5	7.387	689	697	705	rBV	2026969	3077489	25.60%	2.439%
6	7.569	720	728	737	rBV	2355659	3695331	30.74%	2.929%
7	8.046	802	809	819	rBV	1417982	2279654	18.96%	1.807%
8	8.752	921	929	944	rBV	2962752	4803089	39.96%	3.807%
9	9.246	1003	1013	1027	rBV	2412074	3843323	31.97%	3.046%
10	9.963	1124	1135	1149	rBV	1947530	3164929	26.33%	2.508%
11	10.487	1215	1224	1240	rBV	2835315	4728151	39.33%	3.747%
12	10.881	1281	1291	1303	rBV	2130001	3535359	29.41%	2.802%
13	11.034	1308	1317	1337	rBV	2933963	5128462	42.66%	4.064%
14	12.457	1552	1559	1567	rBV	53132	85424	0.71%	0.068%
15	13.545	1739	1744	1749	rVV	23715	38819	0.32%	0.031%
16	13.663	1759	1764	1768	rVB6	9090	17458	0.15%	0.014%
17	14.110	1834	1840	1854	rBV	5147083	7256604	60.37%	5.751%
18	14.210	1854	1857	1869	rVB	7996	17913	0.15%	0.014%
19	14.404	1882	1890	1908	rBV	5817095	8766748	72.93%	6.948%
20	14.698	1934	1940	1956	rBV	3216515	4843830	40.29%	3.839%
21	14.904	1968	1975	1999	rBV	2428909	3824542	31.82%	3.031%
22	15.698	2103	2110	2120	rBV	7423837	10656448	88.65%	8.446%
23	15.816	2124	2130	2145	rVV	2084142	2859478	23.79%	2.266%
24	15.933	2145	2150	2155	rVB2	34070	56507	0.47%	0.045%
25	16.269	2203	2207	2213	rBV9	6770	13077	0.11%	0.010%
26	16.486	2240	2244	2250	rVB8	8145	14141	0.12%	0.011%
27	17.257	2370	2375	2377	rBV4	9326	17192	0.14%	0.014%
28	17.469	2404	2411	2421	rBV	4225713	5774412	48.04%	4.576%
29	17.569	2421	2428	2445	rVV2	8111829	11382535	94.69%	9.021%
30	18.310	2550	2554	2561	rBV3	64437	124762	1.04%	0.099%
31	19.374	2731	2735	2739	rBV	99409	125912	1.05%	0.100%
32	19.439	2742	2746	2752	rVV	91907	128789	1.07%	0.102%
33	19.545	2760	2764	2771	rBV6	38512	80649	0.67%	0.064%
34	19.804	2802	2808	2817	rBV	8914732	12021013	100.00%	9.527%
35	21.563	3102	3107	3113	rBV2	3343156	4582790	38.12%	3.632%
36	23.980	3510	3518	3528	rVB2	3709081	8175462	68.01%	6.479%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081823\
Data File : BP016656.D
Acq On : 19 Aug 2023 00:21
Operator : MA/JU
Sample : PB154876BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK876

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Title : SVOA CALIBRATION

37	24.151	3540	3547	3557	rVB	1788538	3784367	31.48%	2.999%
----	--------	------	------	------	-----	---------	---------	--------	--------




Sum of corrected areas: 126178145

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081823\
Data File : BP016656.D
Acq On : 19 Aug 2023 00:21
Operator : MA/JU
Sample : PB154876BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK876

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

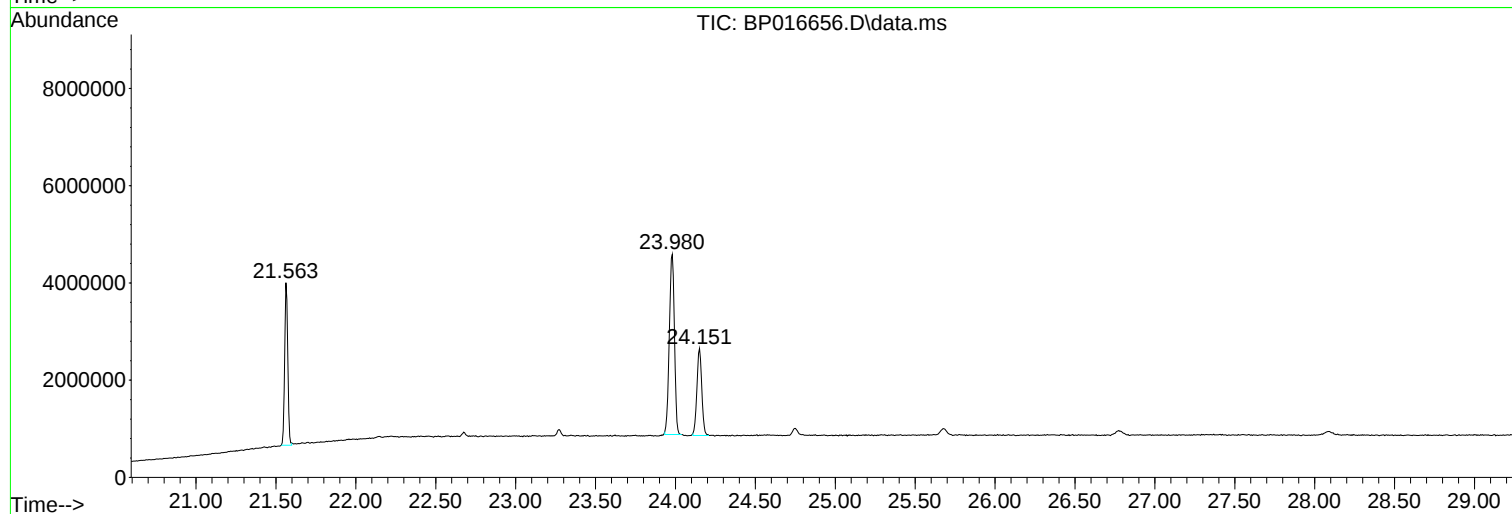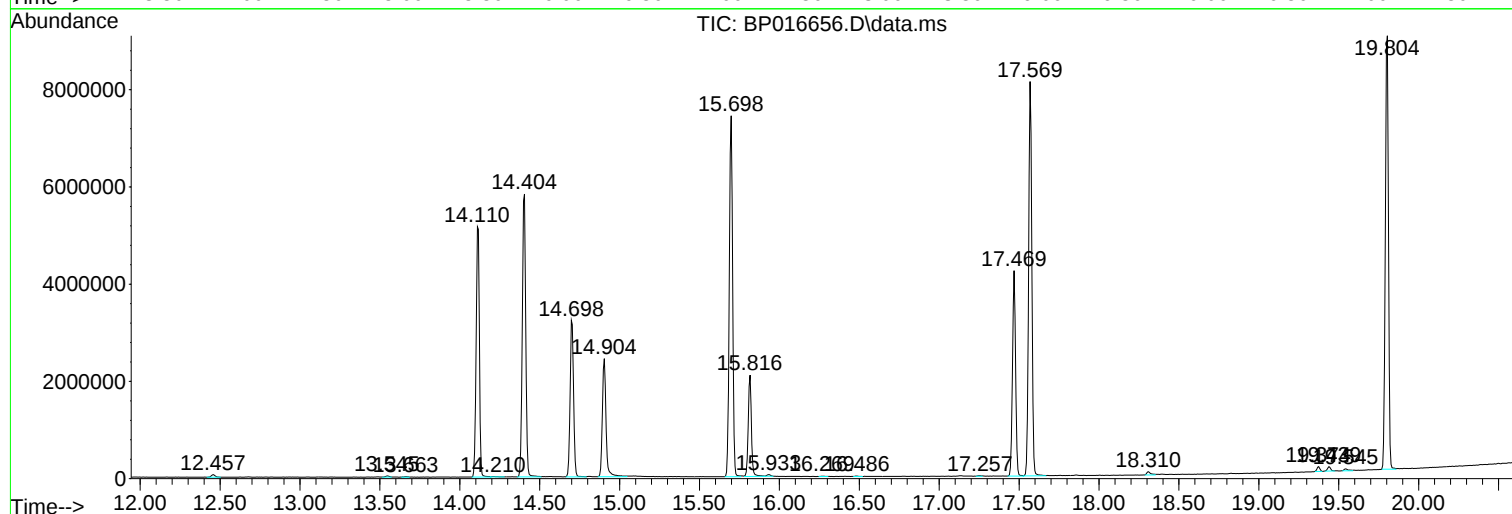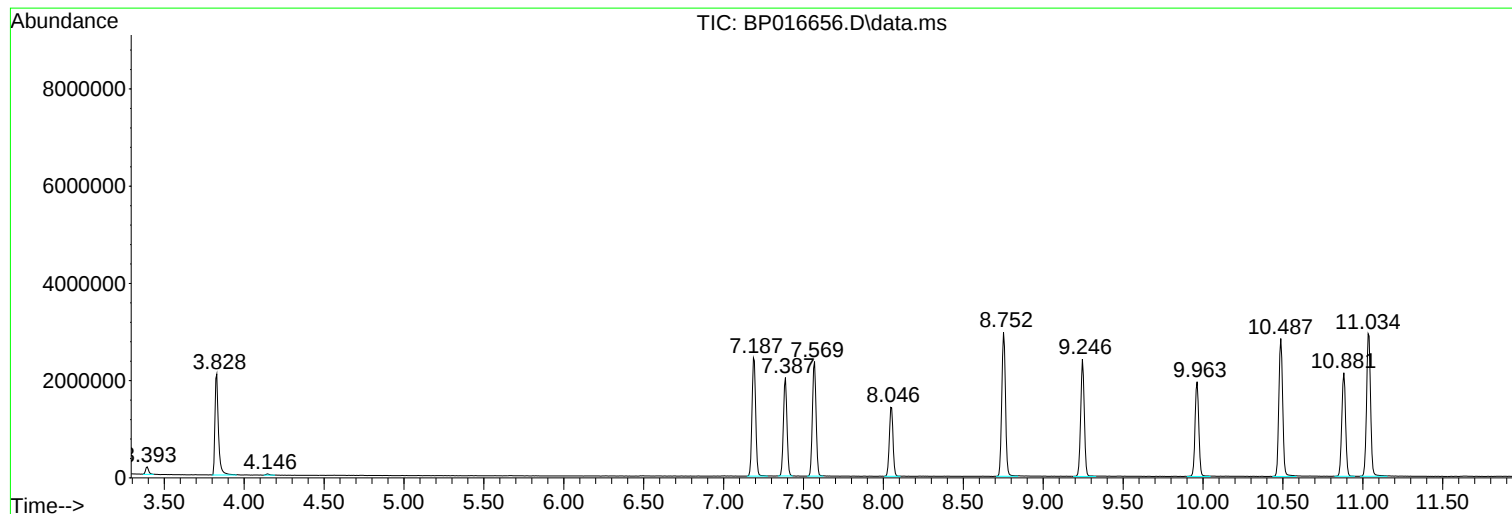

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081823\
Data File : BP016656.D
Acq On : 19 Aug 2023 00:21
Operator : MA/JU
Sample : PB154876BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK876

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081823\
Data File : BP016656.D
Acq On : 19 Aug 2023 00:21
Operator : MA/JU
Sample : PB154876BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK876

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------