

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081823\
 Data File : BP016661.D
 Acq On : 19 Aug 2023 03:45
 Operator : MA/JU
 Sample : 04049-03
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH944

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016661.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.346	5	10	16	rBV	432111	683876	6.12%	0.693%
2	3.393	16	18	21	rVV2	73778	91787	0.82%	0.093%
3	3.429	21	24	33	rVB	87838	127459	1.14%	0.129%
4	3.829	89	92	109	rBV	558498	879948	7.87%	0.891%
5	4.034	122	127	135	rVB	43737	73092	0.65%	0.074%
6	4.146	142	146	153	rVB	22803	35297	0.32%	0.036%
7	4.676	231	236	246	rVB	135968	200418	1.79%	0.203%
8	5.087	301	306	310	rBV2	10565	17523	0.16%	0.018%
9	5.287	336	340	343	rBV4	9963	14442	0.13%	0.015%
10	5.670	402	405	412	rVB6	6158	13221	0.12%	0.013%
11	6.299	508	512	519	rVB9	7616	14555	0.13%	0.015%
12	6.993	625	630	634	rBV8	9344	18871	0.17%	0.019%
13	7.187	657	663	671	rBV	404693	619491	5.54%	0.628%
14	7.387	687	697	704	rBV	1447424	2270117	20.31%	2.300%
15	7.569	720	728	737	rBV	1302819	2124194	19.00%	2.152%
16	7.640	737	740	750	rVB2	26928	52328	0.47%	0.053%
17	8.052	801	810	818	rBV	1258351	2048856	18.33%	2.076%
18	8.252	839	844	849	rBV4	9243	16212	0.15%	0.016%
19	8.752	921	929	939	rBV	1133240	1804670	16.15%	1.828%
20	8.834	939	943	950	rVB	27471	45743	0.41%	0.046%
21	9.246	1004	1013	1024	rBV	1711401	2841401	25.42%	2.879%
22	9.381	1030	1036	1040	rBV5	12557	26683	0.24%	0.027%
23	9.469	1047	1051	1056	rVB8	8053	12491	0.11%	0.013%
24	9.963	1127	1135	1150	rBV	1289860	2249919	20.13%	2.279%
25	10.134	1159	1164	1173	rVB	7986	18627	0.17%	0.019%
26	10.487	1215	1224	1238	rBV	1911978	3191930	28.56%	3.234%
27	10.881	1283	1291	1298	rBV	1843795	3078603	27.54%	3.119%
28	11.034	1309	1317	1329	rBV	1544018	2646900	23.68%	2.681%
29	11.622	1412	1417	1425	rBV9	11995	23118	0.21%	0.023%
30	11.693	1425	1429	1435	rVB9	7431	11748	0.11%	0.012%
31	11.969	1470	1476	1480	rBV4	8228	12659	0.11%	0.013%
32	12.146	1499	1506	1511	rVB7	7883	13027	0.12%	0.013%
33	12.322	1531	1536	1538	rBV4	7096	11445	0.10%	0.012%
34	12.452	1550	1558	1564	rBV2	35499	61386	0.55%	0.062%
35	13.281	1694	1699	1704	rBV2	53635	86771	0.78%	0.088%
36	13.546	1737	1744	1748	rBV	44741	75092	0.67%	0.076%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081823\
 Data File : BP016661.D
 Acq On : 19 Aug 2023 03:45
 Operator : MA/JU
 Sample : 04049-03
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH944

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Title : SVOA CALIBRATION

37	13.604	1748	1754	1761	rVV3	37730	64939	0.58%	0.066%
38	13.810	1779	1789	1793	rBV3	7341	21701	0.19%	0.022%
39	13.881	1797	1801	1806	rVB6	9408	15591	0.14%	0.016%
40	14.110	1833	1840	1850	rBV	4049087	5474108	48.98%	5.546%
41	14.240	1860	1862	1868	rVB7	7906	12826	0.11%	0.013%
42	14.316	1870	1875	1881	rBV10	10480	18083	0.16%	0.018%
43	14.399	1882	1889	1898	rBV	4483178	6329942	56.63%	6.413%
44	14.593	1917	1922	1933	rBV	249006	357876	3.20%	0.363%
45	14.699	1933	1940	1953	rVB	2797300	4064101	36.36%	4.117%
46	14.904	1968	1975	1991	rBV	290699	564894	5.05%	0.572%
47	15.075	2001	2004	2010	rBV8	10180	16984	0.15%	0.017%
48	15.434	2061	2065	2070	rVB5	10129	17178	0.15%	0.017%
49	15.693	2102	2109	2115	rBV	5631924	8121278	72.66%	8.227%
50	15.751	2115	2119	2124	rVV	413231	592857	5.30%	0.601%
51	15.810	2124	2129	2144	rVB	1770671	2452494	21.94%	2.485%
52	15.928	2145	2149	2151	rBV2	26216	33796	0.30%	0.034%
53	16.063	2169	2172	2178	rVB	18654	27917	0.25%	0.028%
54	16.410	2223	2231	2239	rVB	177711	293294	2.62%	0.297%
55	16.816	2298	2300	2303	rVB4	11900	12327	0.11%	0.012%
56	17.134	2351	2354	2360	rVB8	8401	13709	0.12%	0.014%
57	17.469	2404	2411	2421	rBV	3485814	4973636	44.50%	5.039%
58	17.569	2421	2428	2441	rBV	6944765	9645080	86.29%	9.771%
59	17.957	2491	2494	2499	rVB	13338	18379	0.16%	0.019%
60	18.087	2513	2516	2522	rVB4	26999	33360	0.30%	0.034%
61	18.304	2549	2553	2562	rBV	244614	393445	3.52%	0.399%
62	19.222	2706	2709	2714	rVB6	35596	41934	0.38%	0.042%
63	19.369	2731	2734	2738	rBV	82318	103256	0.92%	0.105%
64	19.439	2742	2746	2751	rVB	80339	114576	1.03%	0.116%
65	19.539	2759	2763	2771	rBV2	137188	229553	2.05%	0.233%
66	19.798	2801	2807	2817	rBV	8422466	11177182	100.00%	11.323%
67	21.563	3102	3107	3113	rBV	3684897	4887531	43.73%	4.951%
68	23.975	3509	3517	3528	rVB2	4058185	8955654	80.12%	9.073%
69	24.145	3540	3546	3556	rVB	1912640	4117029	36.83%	4.171%




Sum of corrected areas: 98710410

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081823\
Data File : BP016661.D
Acq On : 19 Aug 2023 03:45
Operator : MA/JU
Sample : 04049-03
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH944

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

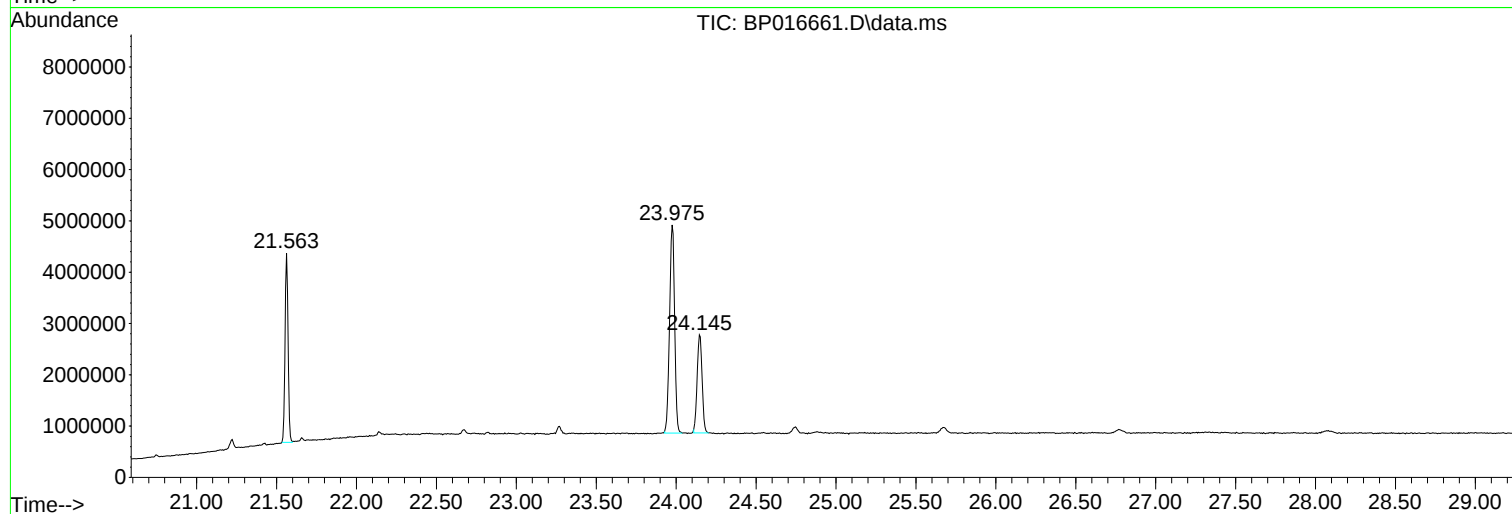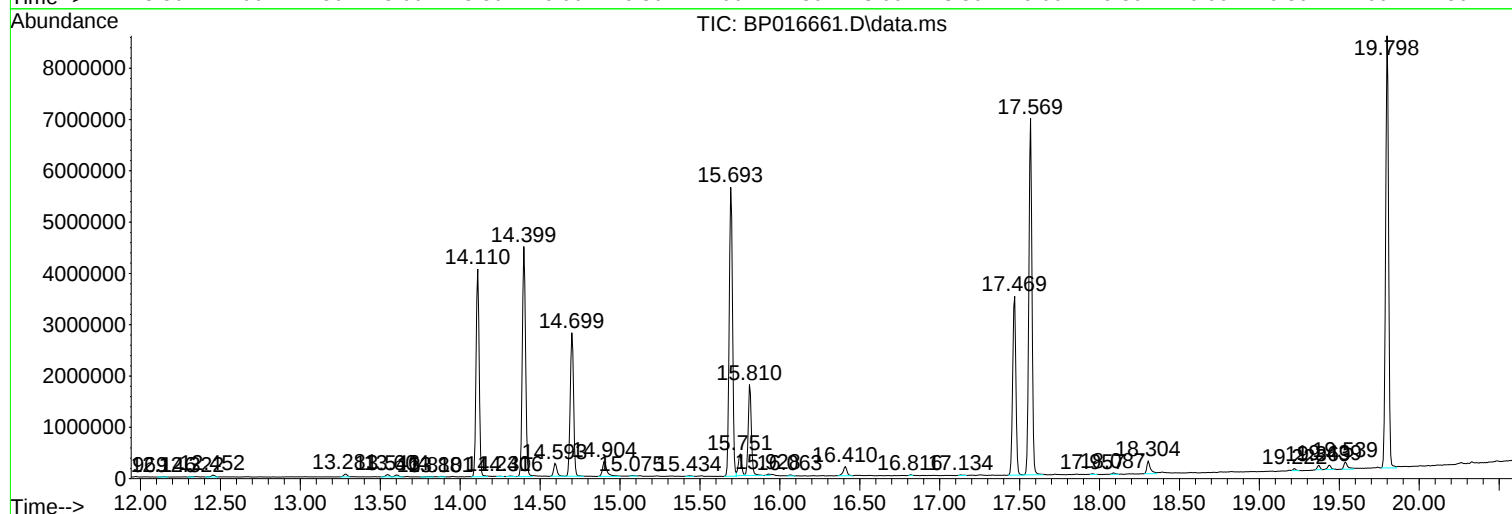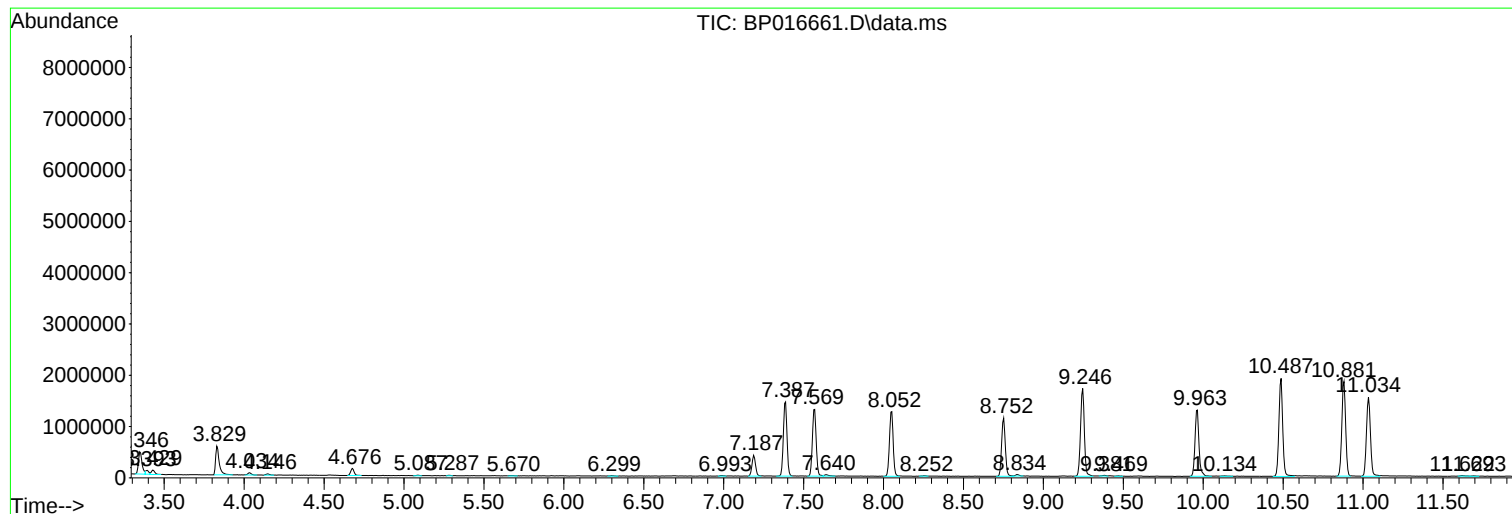

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081823\
Data File : BP016661.D
Acq On : 19 Aug 2023 03:45
Operator : MA/JU
Sample : 04049-03
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH944










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.751	2.92 ng/ul	592857	Acenaphthene-d10	14.698

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-4-fluoronitrobenzene	175	C6H3ClFNO2	000350-30-1	43
2			3-Chloro-4-fluoronitrobenzene	175	C6H3ClFNO2	000350-30-1	38
3			3-Chloro-4-fluoronitrobenzene	175	C6H3ClFNO2	000350-30-1	38
4			3-Chloro-4-fluoronitrobenzene	175	C6H3ClFNO2	000350-30-1	35
5			6-nitroquinoxaline	175	C8H5N3O2	1000468-31-8	35

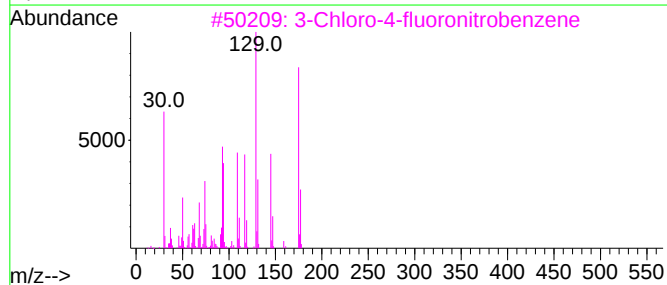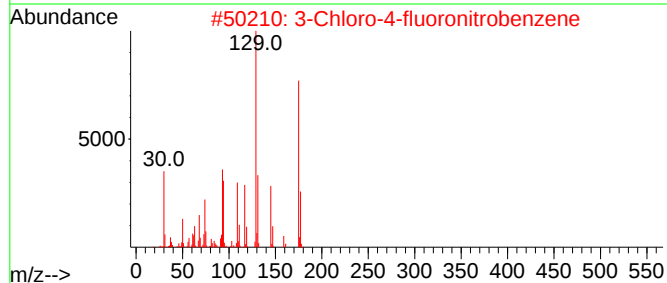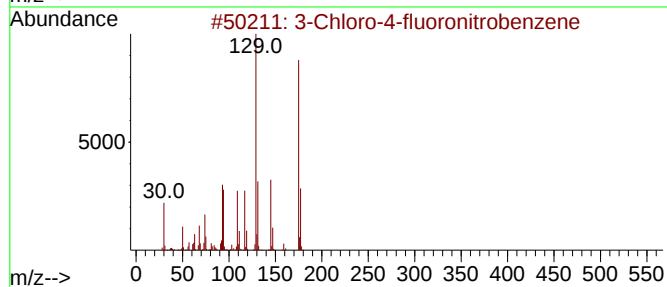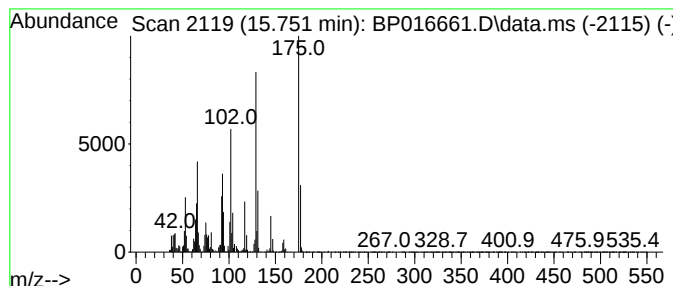

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081823\
Data File : BP016661.D
Acq On : 19 Aug 2023 03:45
Operator : MA/JU
Sample : 04049-03
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH944

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	15.751	2.9	ng/u1	592857	3	14.698	4064100	20.0