
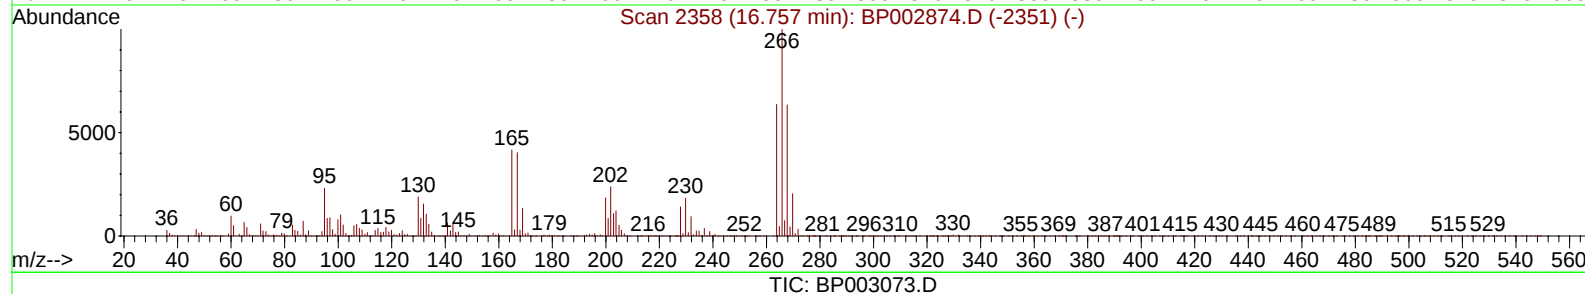
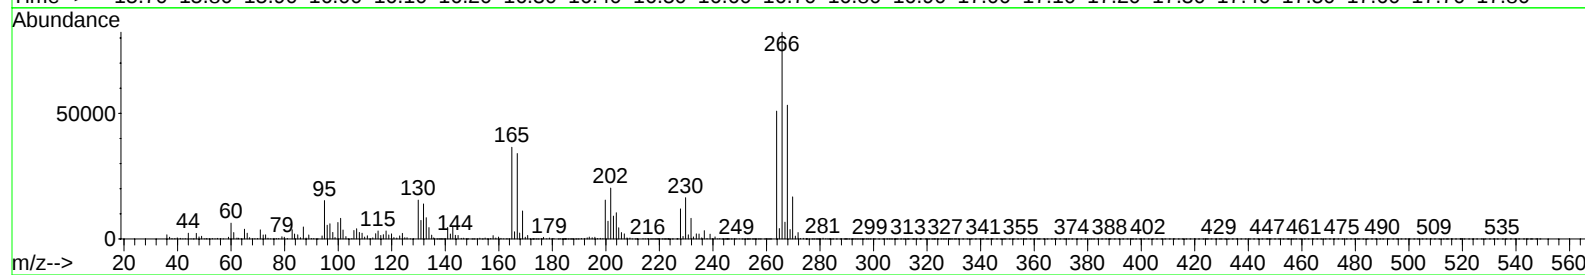


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP082120\
Data File : BP003073.D
Acq On : 21 Aug 2020 09:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 21 18:21:53 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 17 14:07:35 2020
Response via : Initial Calibration

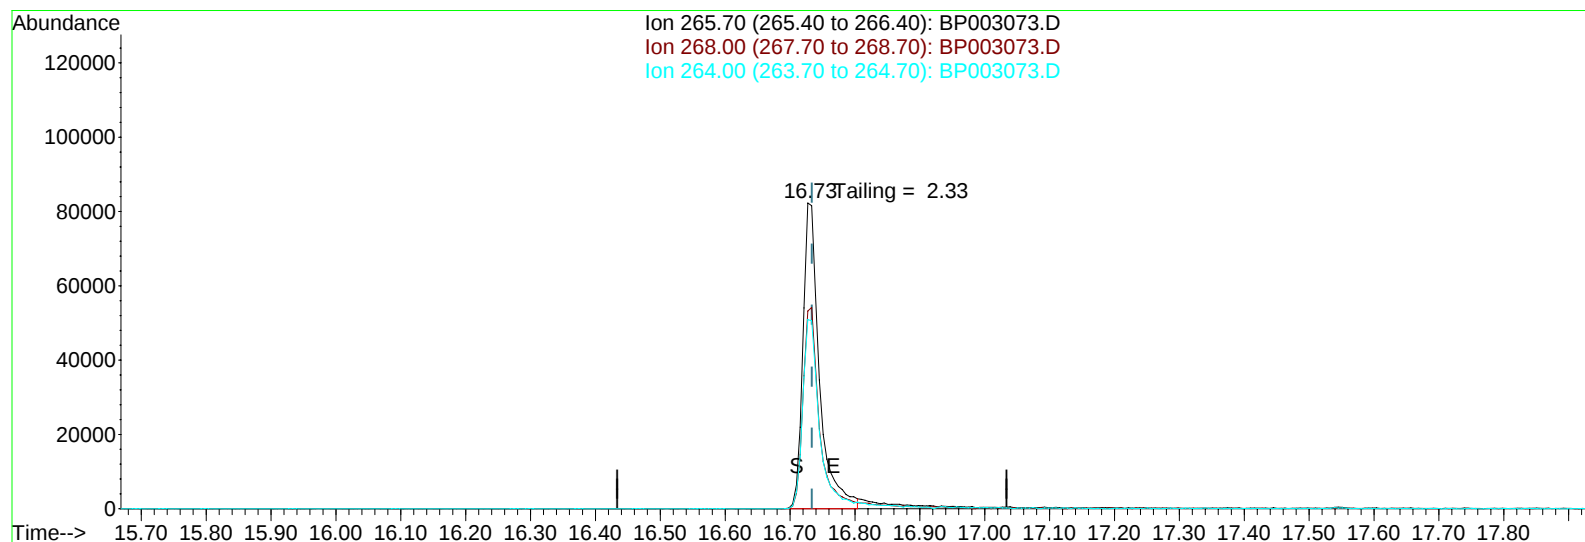

(70) Pentachlorophenol (C)




16.727min (-0.006) 734511.47ng

response 155434

Ion	Exp%	Act%
265.70	100	100
268.00	63.60	64.68
264.00	63.00	61.85
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP082120\
Data File : BP003073.D
Acq On : 21 Aug 2020 09:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 21 18:21:53 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 17 14:07:35 2020
Response via : Initial Calibration

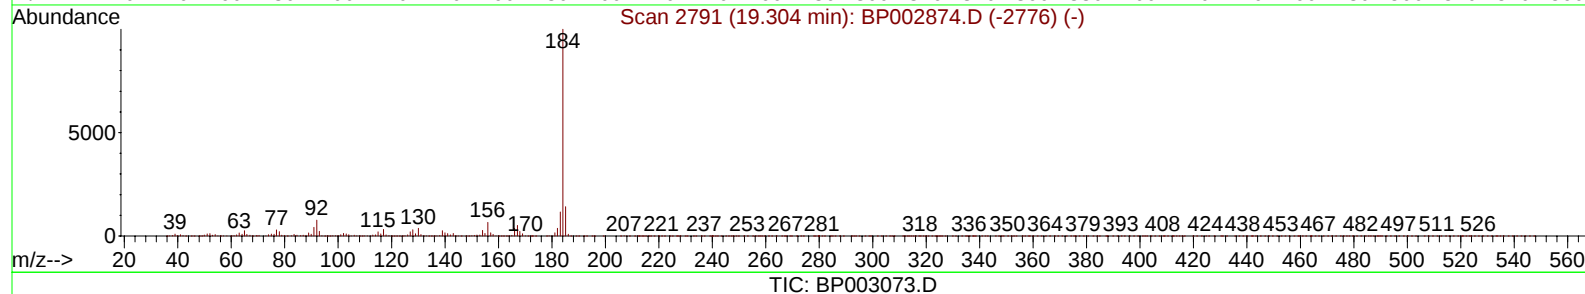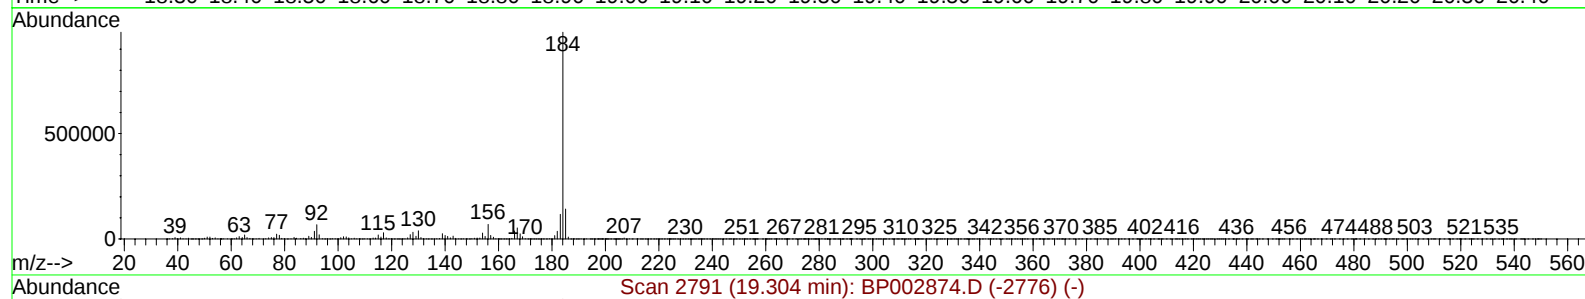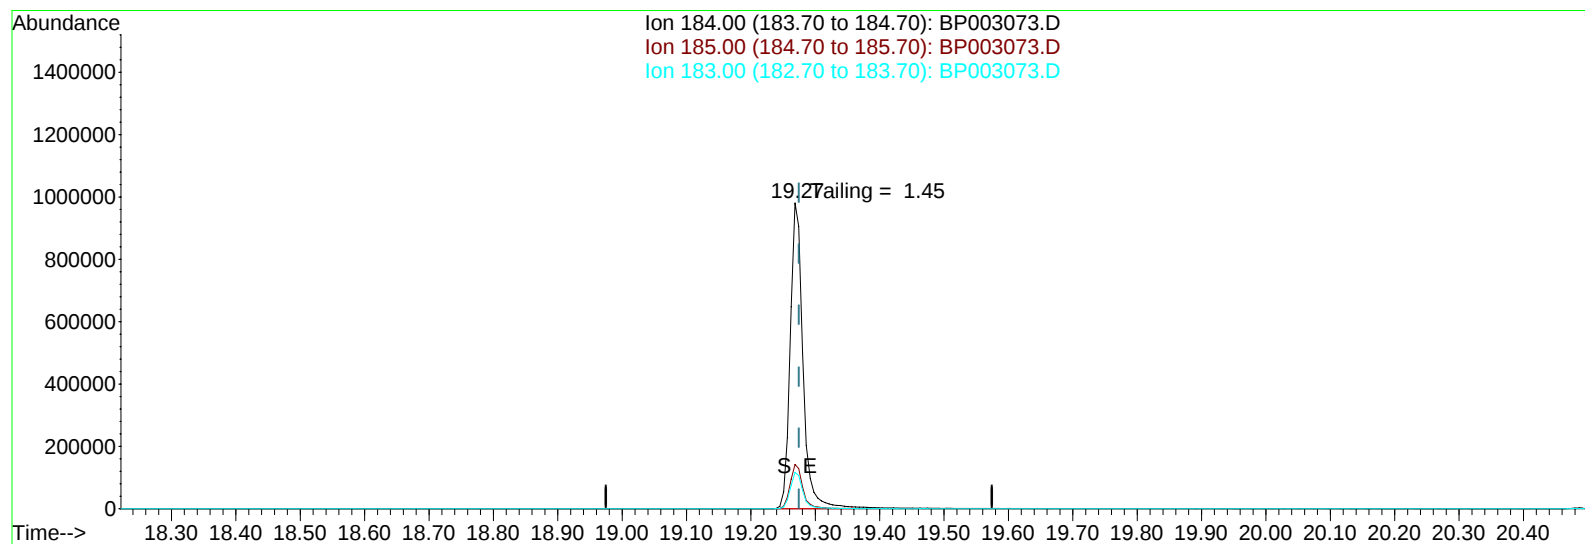

(77) Benzidine

19.268min (-0.006) 500451.85ng

response 1373449

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	14.49
183.00	11.70	11.90
0.00	0.00	0.00