


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP082120\
 Data File : BP003073.D
 Acq On : 21 Aug 2020 09:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP073020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 17 14:07:35 2020

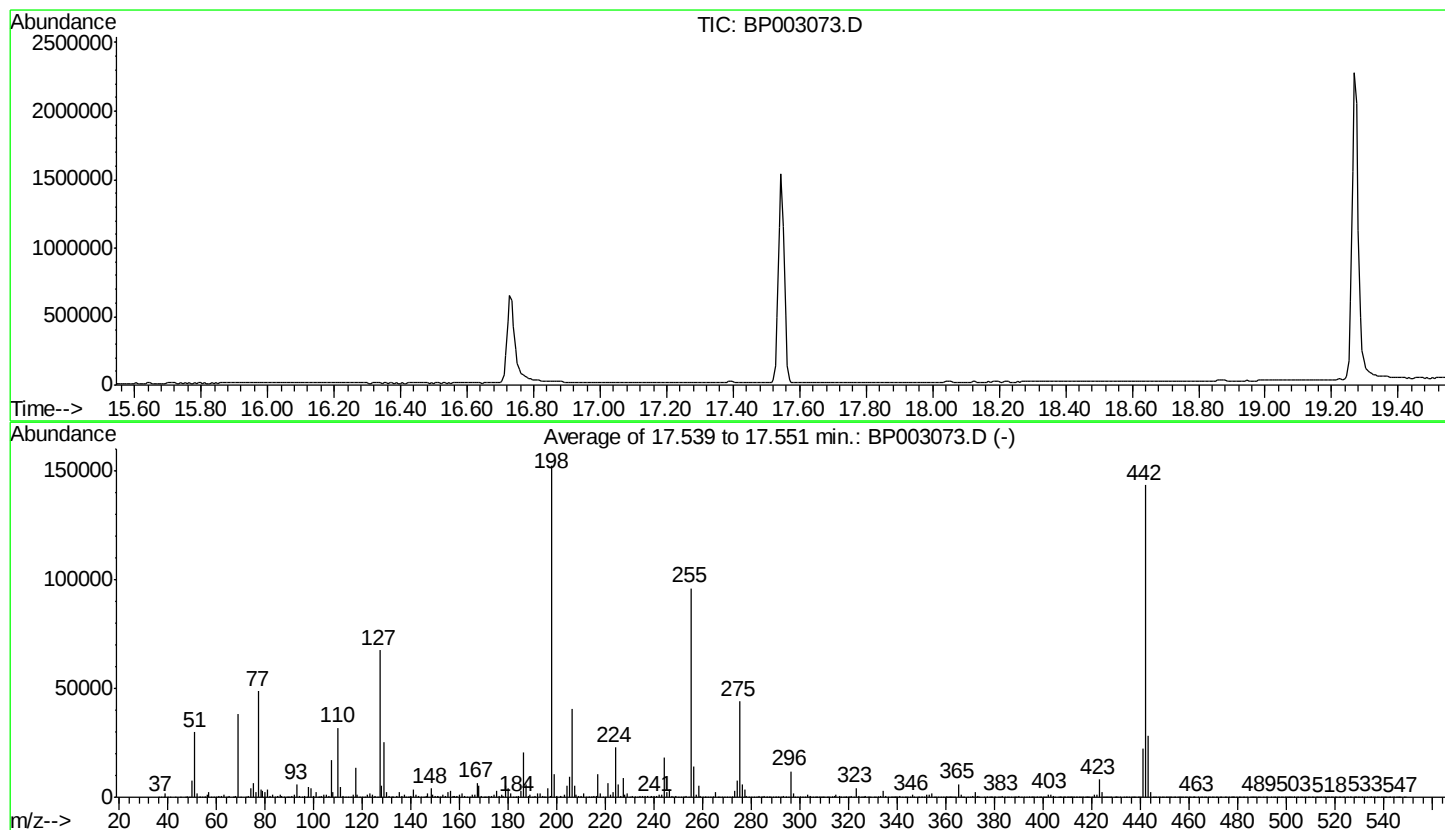

AutoFind: Scans 2491, 2492, 2493; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.7	30001	PASS
68	69	0.00	2	1.9	728	PASS
69	198	0.00	100	25.0	38129	PASS
70	69	0.00	2	0.4	145	PASS
127	198	10	80	44.4	67649	PASS
197	198	0.00	2	0.5	741	PASS
198	198	100	100	100.0	152469	PASS
199	198	5	9	7.0	10636	PASS
275	198	10	60	28.9	43997	PASS
365	198	1	100	3.9	5987	PASS
441	198	0.01	100	14.6	22205	PASS
442	198	50	100	94.1	143442	PASS
443	442	15	24	19.9	28557	PASS