

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082123\
 Data File : BP016675.D
 Acq On : 21 Aug 2023 15:04
 Operator : MA/JU
 Sample : 04049-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH8T5

Quant Time: Aug 21 18:01:53 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 17 01:38:34 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.046	152	226360	20.000	ng/u1	0.00
20) Naphthalene-d8	10.881	136	1054091	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.698	164	666019	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.463	188	1483729	20.000	ng/u1	0.00
79) Chrysene-d12	21.557	240	1174733	20.000	ng/u1	0.00
88) Perylene-d12	24.139	264	1064008	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	30243	5.077	ng/uL	0.00
4) Pyridine-d5	3.828	84	349810	19.301	ng/u1	0.00
7) Phenol-d5	7.187	99	242047	11.599	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.381	67	623570	45.367	ng/u1	0.00
11) 2-Chlorophenol-d4	7.563	132	557574	37.199	ng/u1	0.00
15) 4-Methylphenol-d8	8.751	113	427159	25.743	ng/u1	0.00
21) Nitrobenzene-d5	9.246	128	370667	49.976	ng/u1	0.00
24) 2-Nitrophenol-d4	9.963	143	366972	52.094	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.481	165	626148	45.166	ng/u1	-0.01
31) 4-Chloroaniline-d4	11.034	131	954754	40.139	ng/u1	0.00
46) Dimethylphthalate-d6	14.110	166	2371326	49.226	ng/u1	0.00
49) Acenaphthylene-d8	14.398	160	2633011	48.425	ng/u1	0.00
54) 4-Nitrophenol-d4	14.898	143	80800	8.234	ng/u1	0.00
60) Fluorene-d10	15.692	176	2053348	49.999	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.810	200	302579	42.867	ng/u1	0.00
73) Anthracene-d10	17.563	188	3486142	54.319	ng/u1	0.00
81) Pyrene-d10	19.798	212	3917861	63.650	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.968	264	2885765	56.593	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.428	88	26195	3.999	ng/uL	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082123\
Data File : BP016675.D
Acq On : 21 Aug 2023 15:04
Operator : MA/JU
Sample : 04049-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH8T5

Quant Time: Aug 21 18:01:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 17 01:38:34 2023
Response via : Initial Calibration

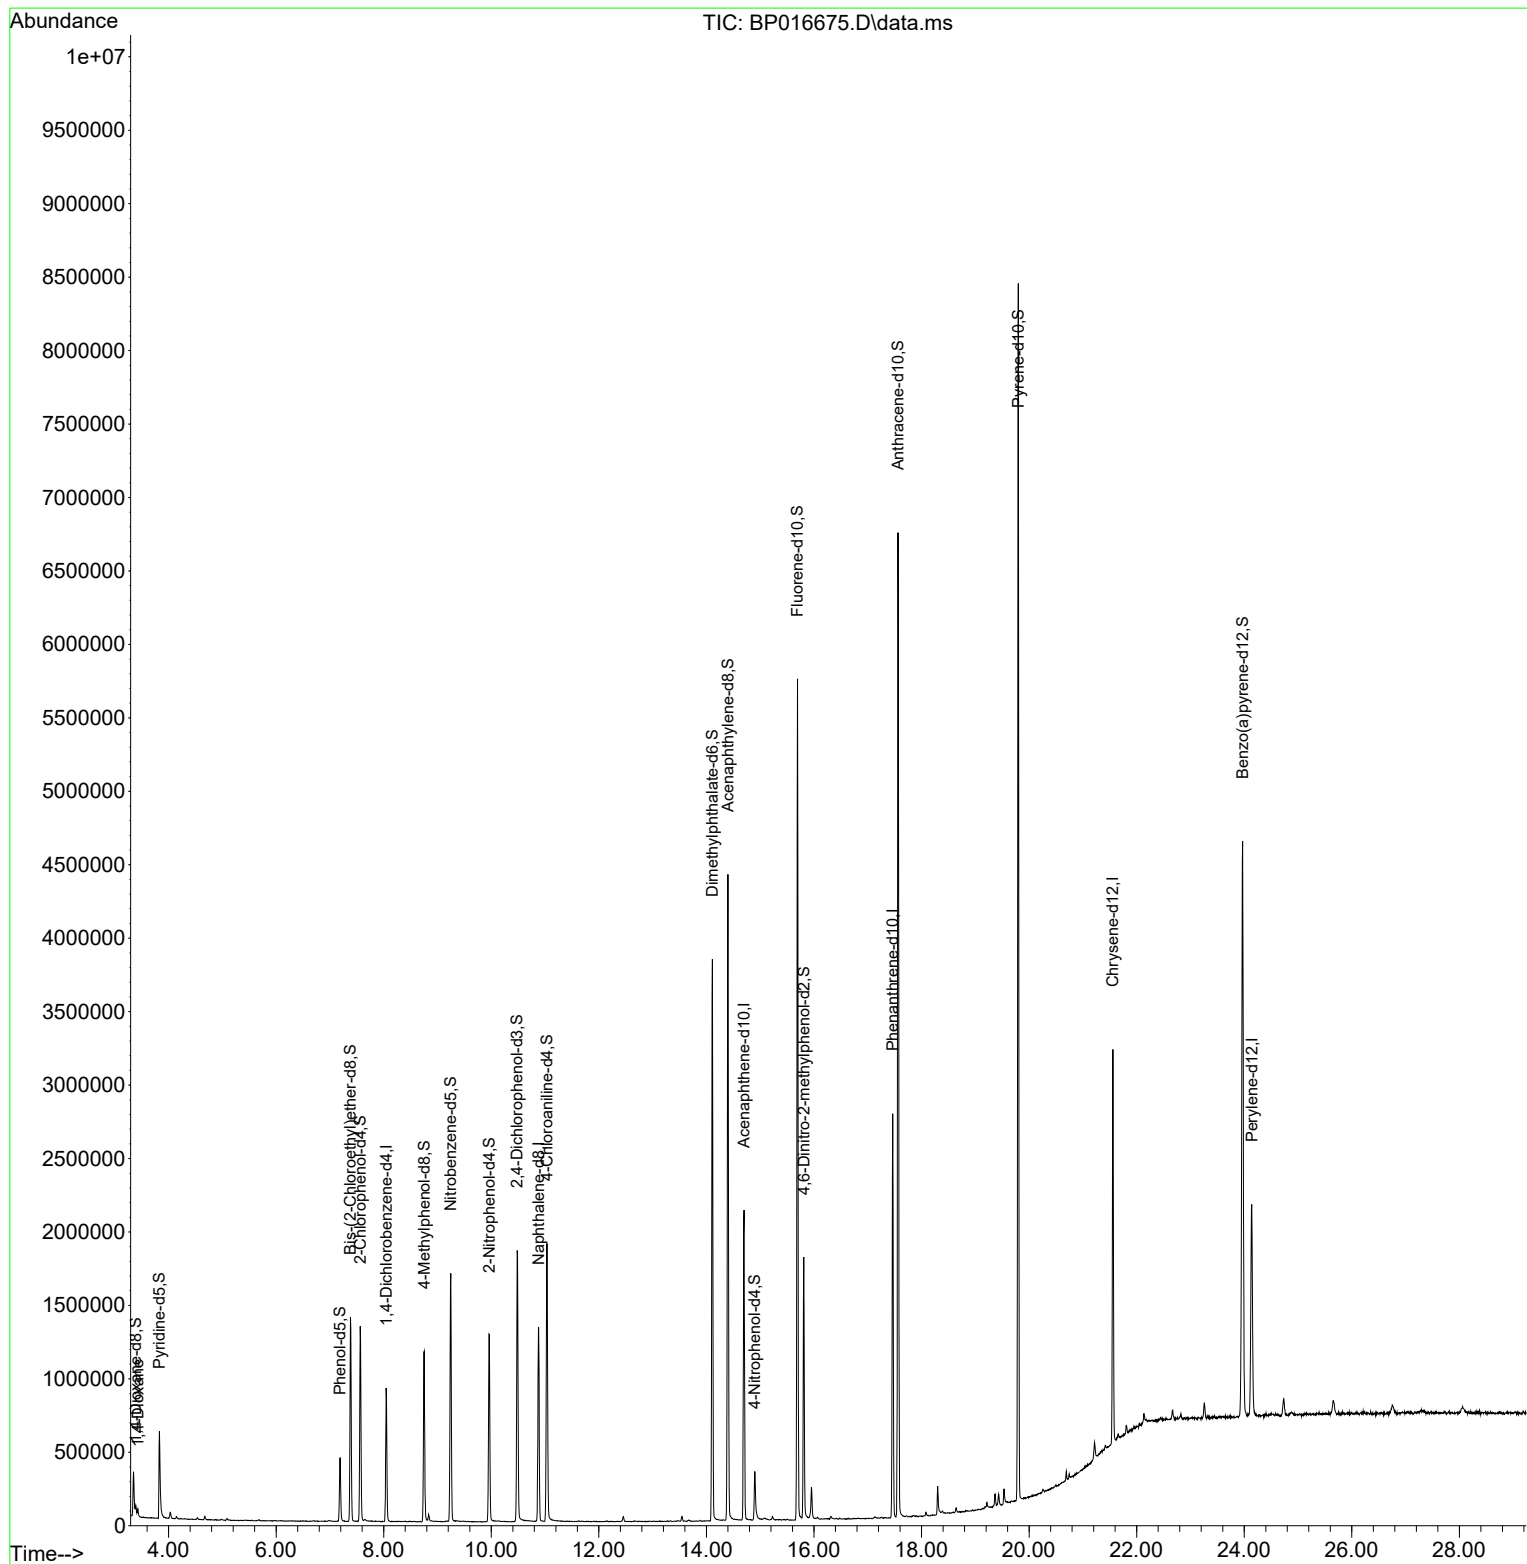

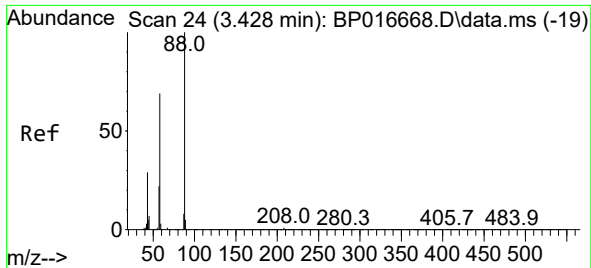

#2
 1,4-Dioxane
 Concen: 3.999 ng/uL
 RT: 3.428 min Scan# 24
 Delta R.T. -0.000 min
 Lab File: BP016675.D
 Acq: 21 Aug 2023 15:04

Instrument :
 BNA_P
 ClientSampleId :
 BH8T5

Tgt Ion: 88 Resp: 26195
 Ion Ratio Lower Upper
 88 100
 43 29.7 23.5 35.3
 58 66.3 57.1 85.7

