

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082123\
 Data File : BP016680.D
 Acq On : 21 Aug 2023 17:56
 Operator : MA/JU
 Sample : 04049-13
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH9K1

Quant Time: Aug 22 00:33:13 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 17 01:38:34 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.046	152	288047	20.000	ng/u1	0.00
20) Naphthalene-d8	10.875	136	1311588	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.698	164	821976	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.463	188	1831845	20.000	ng/u1	0.00
79) Chrysene-d12	21.557	240	1507544	20.000	ng/u1	0.00
88) Perylene-d12	24.139	264	1373843	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	22941	3.026	ng/uL	0.00
4) Pyridine-d5	3.828	84	328833	14.258	ng/u1	0.00
7) Phenol-d5	7.187	99	240039	9.039	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.381	67	728525	41.652	ng/u1	0.00
11) 2-Chlorophenol-d4	7.563	132	627212	32.884	ng/u1	0.00
15) 4-Methylphenol-d8	8.751	113	448736	21.251	ng/u1	0.00
21) Nitrobenzene-d5	9.246	128	431446	46.750	ng/u1	0.00
24) 2-Nitrophenol-d4	9.957	143	434197	49.536	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.481	165	720233	41.753	ng/u1	-0.01
31) 4-Chloroaniline-d4	11.034	131	1118804	37.802	ng/u1	0.00
46) Dimethylphthalate-d6	14.110	166	2630504	44.245	ng/u1	0.00
49) Acenaphthylene-d8	14.398	160	2996094	44.648	ng/u1	0.00
54) 4-Nitrophenol-d4	14.898	143	76958	6.354	ng/u1	0.00
60) Fluorene-d10	15.692	176	2297292	45.326	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.810	200	346218	39.728	ng/u1	0.00
73) Anthracene-d10	17.563	188	3812477	48.115	ng/u1	0.00
81) Pyrene-d10	19.798	212	4279525	54.177	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.968	264	3239332	49.200	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.428	88	82477	9.895	ng/uL	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082123\
Data File : BP016680.D
Acq On : 21 Aug 2023 17:56
Operator : MA/JU
Sample : 04049-13
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH9K1

Quant Time: Aug 22 00:33:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 17 01:38:34 2023
Response via : Initial Calibration

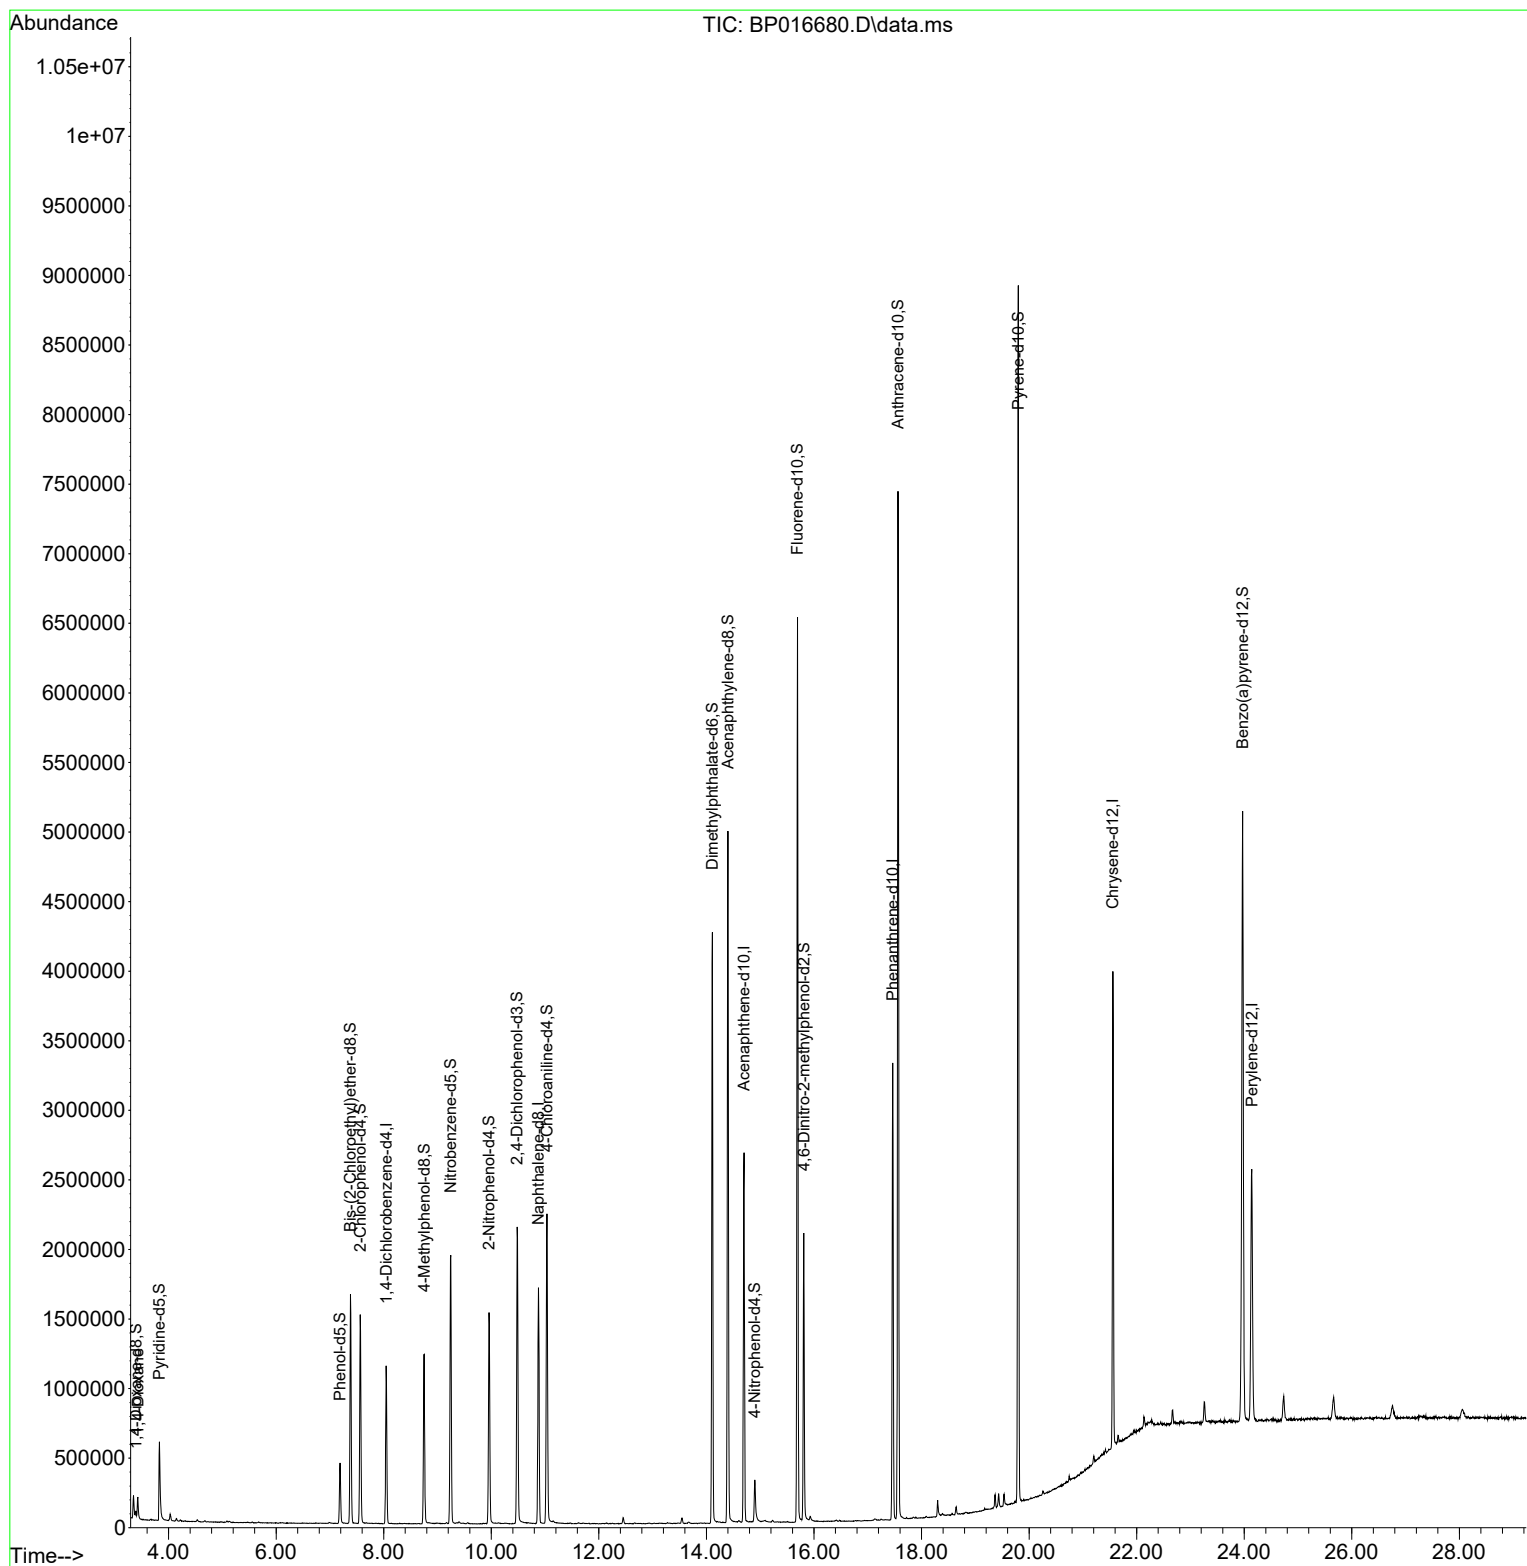

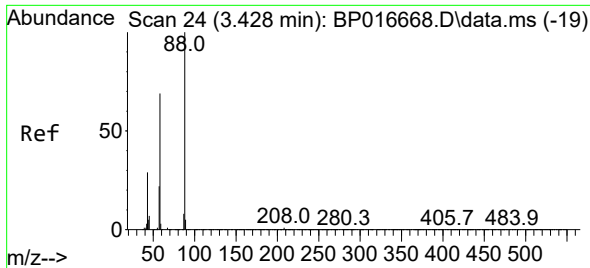

#2
 1,4-Dioxane
 Concen: 9.895 ng/uL
 RT: 3.428 min Scan# 24
 Delta R.T. -0.000 min
 Lab File: BP016680.D
 Acq: 21 Aug 2023 17:56

Instrument :
 BNA_P
 ClientSampleId :
 BH9K1

Tgt Ion: 88 Resp: 82477
 Ion Ratio Lower Upper
 88 100
 43 29.2 23.5 35.3
 58 67.1 57.1 85.7

