




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082123\
 Data File : BP016672.D
 Acq On : 21 Aug 2023 13:21
 Operator : MA/JU
 Sample : 04049-08
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHAL6

Manual IntegrationsAPPROVED

Quant Time: Aug 21 18:01:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 17 01:38:34 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/22/2023
 Supervised By :mohammad ahmed 08/22/2023

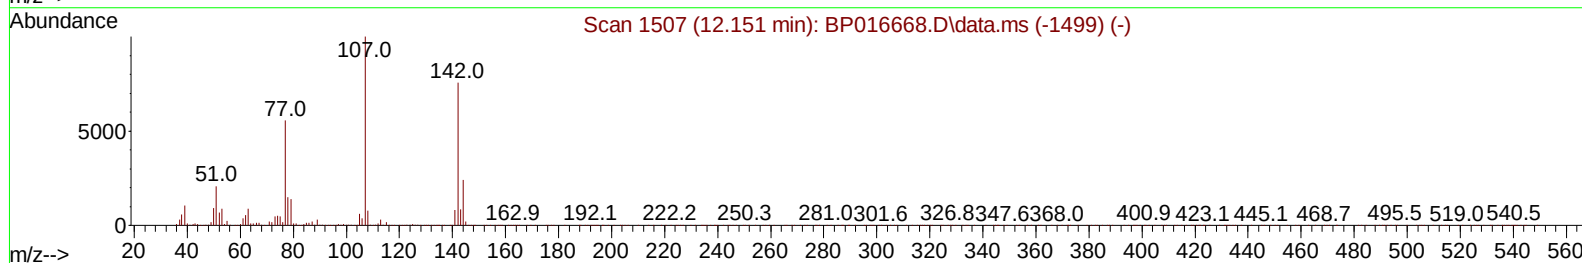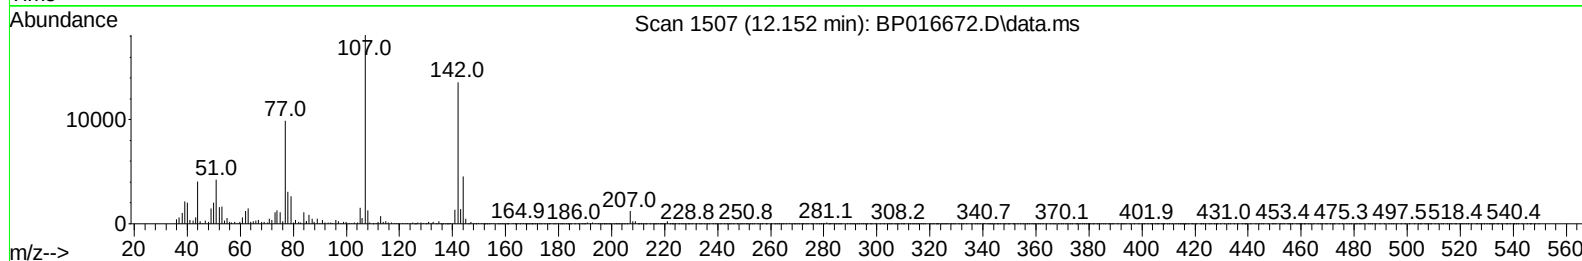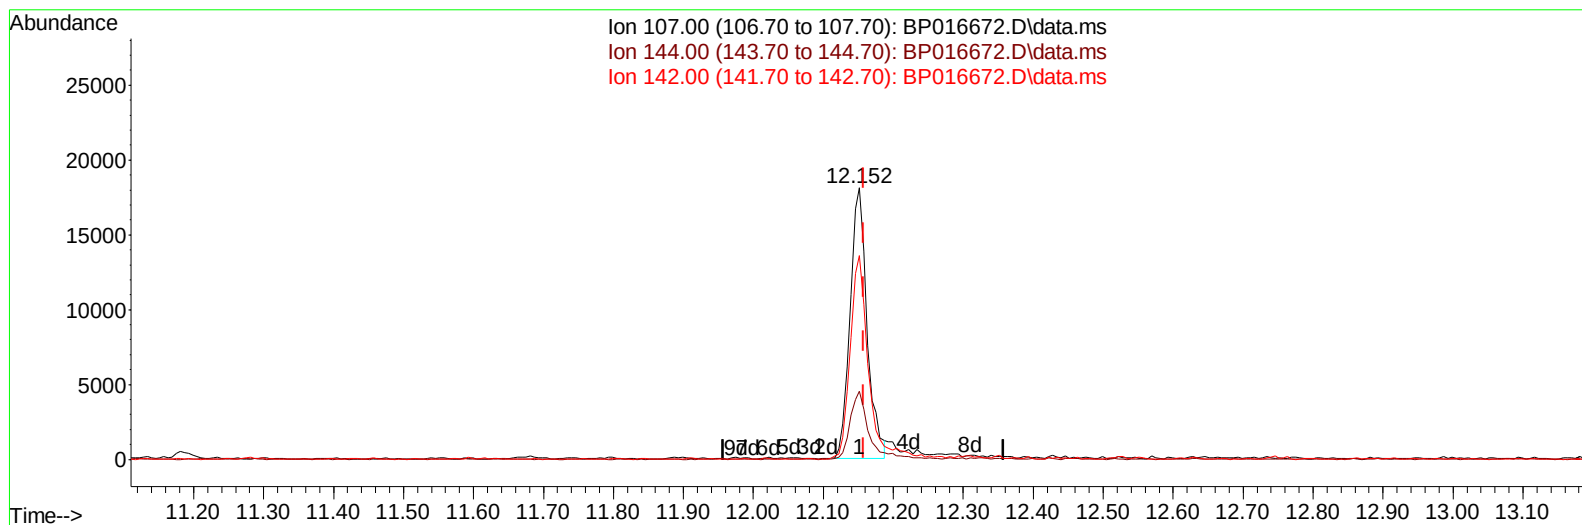

TIC: BP016672.D\data.ms

(35) 4-Chloro-3-methylphenol (C)

12.152min (-0.006) 1.49 ng/ul

response 30355

Ion	Exp%	Act%
107.00	100.00	100.00
144.00	23.80	25.03
142.00	75.30	75.04
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082123\
 Data File : BP016672.D
 Acq On : 21 Aug 2023 13:21
 Operator : MA/JU
 Sample : 04049-08
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHAL6

Manual IntegrationsAPPROVED

Quant Time: Aug 21 18:01:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 17 01:38:34 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/22/2023
 Supervised By :mohammad ahmed 08/22/2023

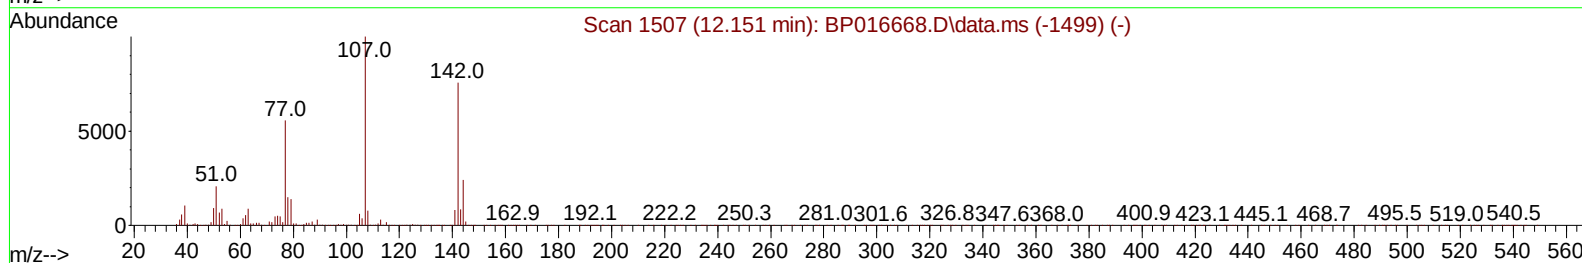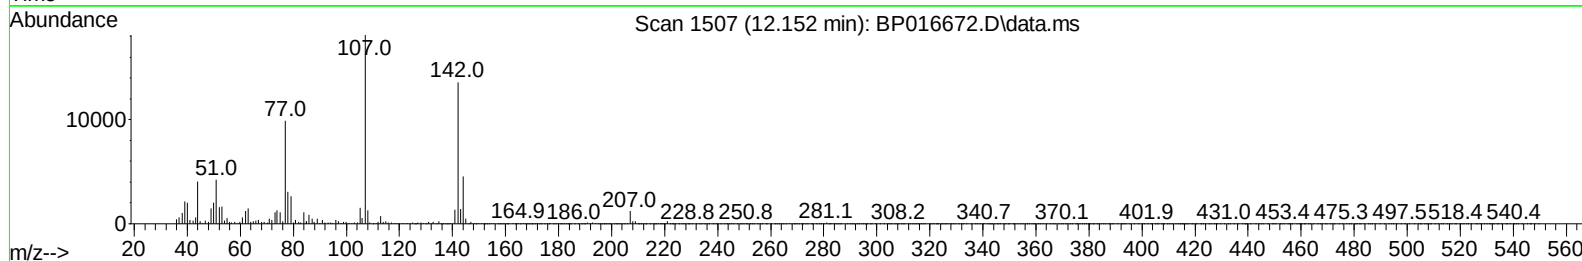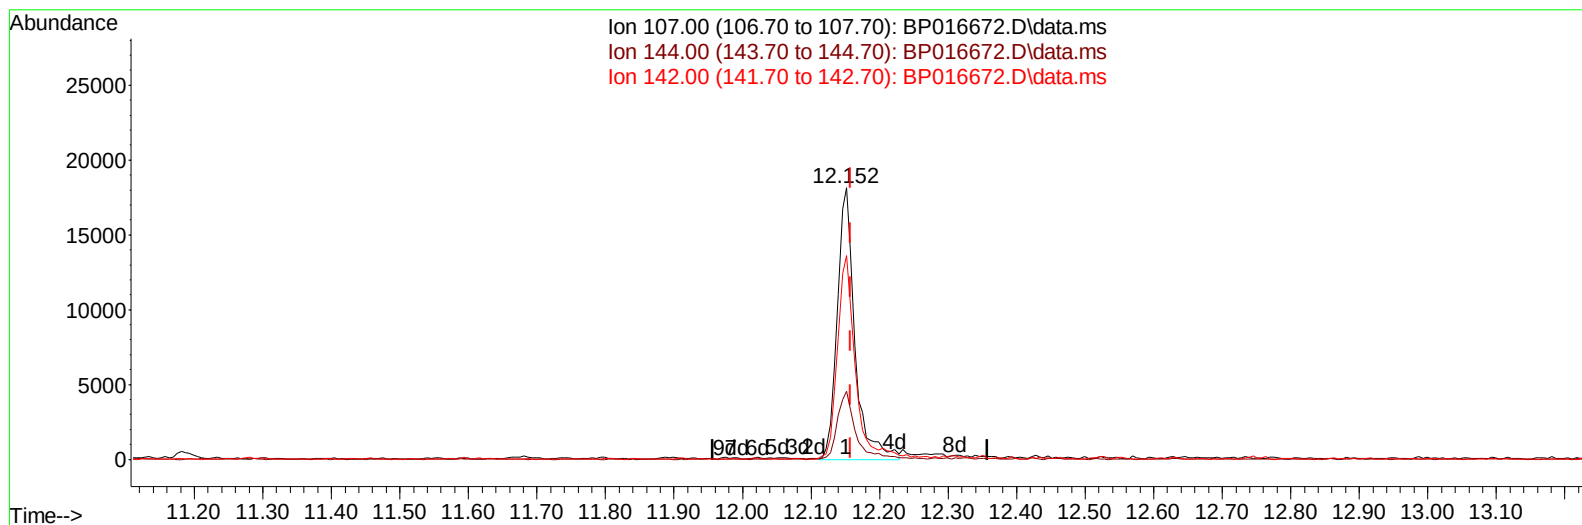

TIC: BP016672.D\data.ms

(35) 4-Chloro-3-methylphenol (C)

12.152min (-0.006) 1.59 ng/ul m

response 32380

Ion	Exp%	Act%
107.00	100.00	100.00
144.00	23.80	25.03
142.00	75.30	75.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082123\
 Data File : BP016672.D
 Acq On : 21 Aug 2023 13:21
 Operator : MA/JU
 Sample : 04049-08
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHAL6

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/22/2023
 Supervised By :mohammad ahmed 08/22/2023

Quant Time: Aug 21 18:21:36 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 17 01:38:34 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	8.046	152		273496	20.000	ng/ul	0.00
20) Naphthalene-d8	10.875	136		1228379	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.699	164		780989	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.463	188		1707555	20.000	ng/ul	0.00
79) Chrysene-d12	21.557	240		1272080	20.000	ng/ul	0.00
88) Perylene-d12	24.133	264		1158625	20.000	ng/ul	-0.01
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.393	96		20821	2.893	ng/uL	0.00
4) Pyridine-d5	3.829	84		200074	9.137	ng/ul	0.00
7) Phenol-d5	7.187	99		218053	8.648	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.381	67		608352	36.632	ng/ul	0.00
11) 2-Chlorophenol-d4	7.564	132		536632	29.631	ng/ul	0.00
15) 4-Methylphenol-d8	8.752	113		393656	19.635	ng/ul	0.00
21) Nitrobenzene-d5	9.246	128		349122	40.392	ng/ul	0.00
24) 2-Nitrophenol-d4	9.963	143		352736	42.968	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.487	165		588887	36.452	ng/ul	0.00
31) 4-Chloroaniline-d4	11.034	131		923885	33.330	ng/ul	0.00
46) Dimethylphthalate-d6	14.110	166		2308937	40.875	ng/ul	0.00
49) Acenaphthylene-d8	14.399	160		2551362	40.016	ng/ul	0.00
54) 4-Nitrophenol-d4	14.899	143		68663	5.967	ng/ul	0.00
60) Fluorene-d10	15.693	176		2054028	42.653	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.810	200		270069	33.246	ng/ul	0.00
73) Anthracene-d10	17.563	188		3434510	46.500	ng/ul	0.00
81) Pyrene-d10	19.792	212		3748052	56.231	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.969	264		2632784	47.416	ng/ul	0.00
Target Compounds							
35) 4-Chloro-3-methylphenol	12.152	107		32380m	1.594	ng/ul	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082123\
Data File : BP016672.D
Acq On : 21 Aug 2023 13:21
Operator : MA/JU
Sample : 04049-08
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAL6

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/22/2023
Supervised By :mohammad ahmed 08/22/2023

Quant Time: Aug 21 18:21:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 17 01:38:34 2023
Response via : Initial Calibration

