

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082123\
 Data File : BP016671.D
 Acq On : 21 Aug 2023 12:47
 Operator : MA/JU
 Sample : 04049-07
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH9T7

Quant Time: Aug 21 18:01:09 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 17 01:38:34 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.046	152	235282	20.000	ng/u1	0.00
20) Naphthalene-d8	10.875	136	1074887	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.698	164	661397	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.463	188	1451601	20.000	ng/u1	0.00
79) Chrysene-d12	21.557	240	1049926	20.000	ng/u1	0.00
88) Perylene-d12	24.139	264	958174	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	24618	3.976	ng/uL	0.00
4) Pyridine-d5	3.828	84	254900	13.531	ng/u1	0.00
7) Phenol-d5	7.187	99	199712	9.207	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.381	67	565273	39.566	ng/u1	0.00
11) 2-Chlorophenol-d4	7.564	132	500259	32.109	ng/u1	0.00
15) 4-Methylphenol-d8	8.746	113	377087	21.863	ng/u1	-0.01
21) Nitrobenzene-d5	9.246	128	325459	43.032	ng/u1	0.00
24) 2-Nitrophenol-d4	9.958	143	329521	45.872	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.487	165	576140	40.755	ng/u1	0.00
31) 4-Chloroaniline-d4	11.034	131	722608	29.792	ng/u1	0.00
46) Dimethylphthalate-d6	14.110	166	2227460	46.562	ng/u1	0.00
49) Acenaphthylene-d8	14.398	160	2427488	44.957	ng/u1	0.00
54) 4-Nitrophenol-d4	14.898	143	59824	6.139	ng/u1	0.00
60) Fluorene-d10	15.693	176	1907612	46.775	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.810	200	273016	39.535	ng/u1	0.00
73) Anthracene-d10	17.563	188	3114818	49.608	ng/u1	0.00
81) Pyrene-d10	19.798	212	3402305	61.845	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.969	264	2360890	51.414	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.428	88	57540	8.452	ng/uL	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082123\
Data File : BP016671.D
Acq On : 21 Aug 2023 12:47
Operator : MA/JU
Sample : 04049-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH9T7

Quant Time: Aug 21 18:01:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 17 01:38:34 2023
Response via : Initial Calibration

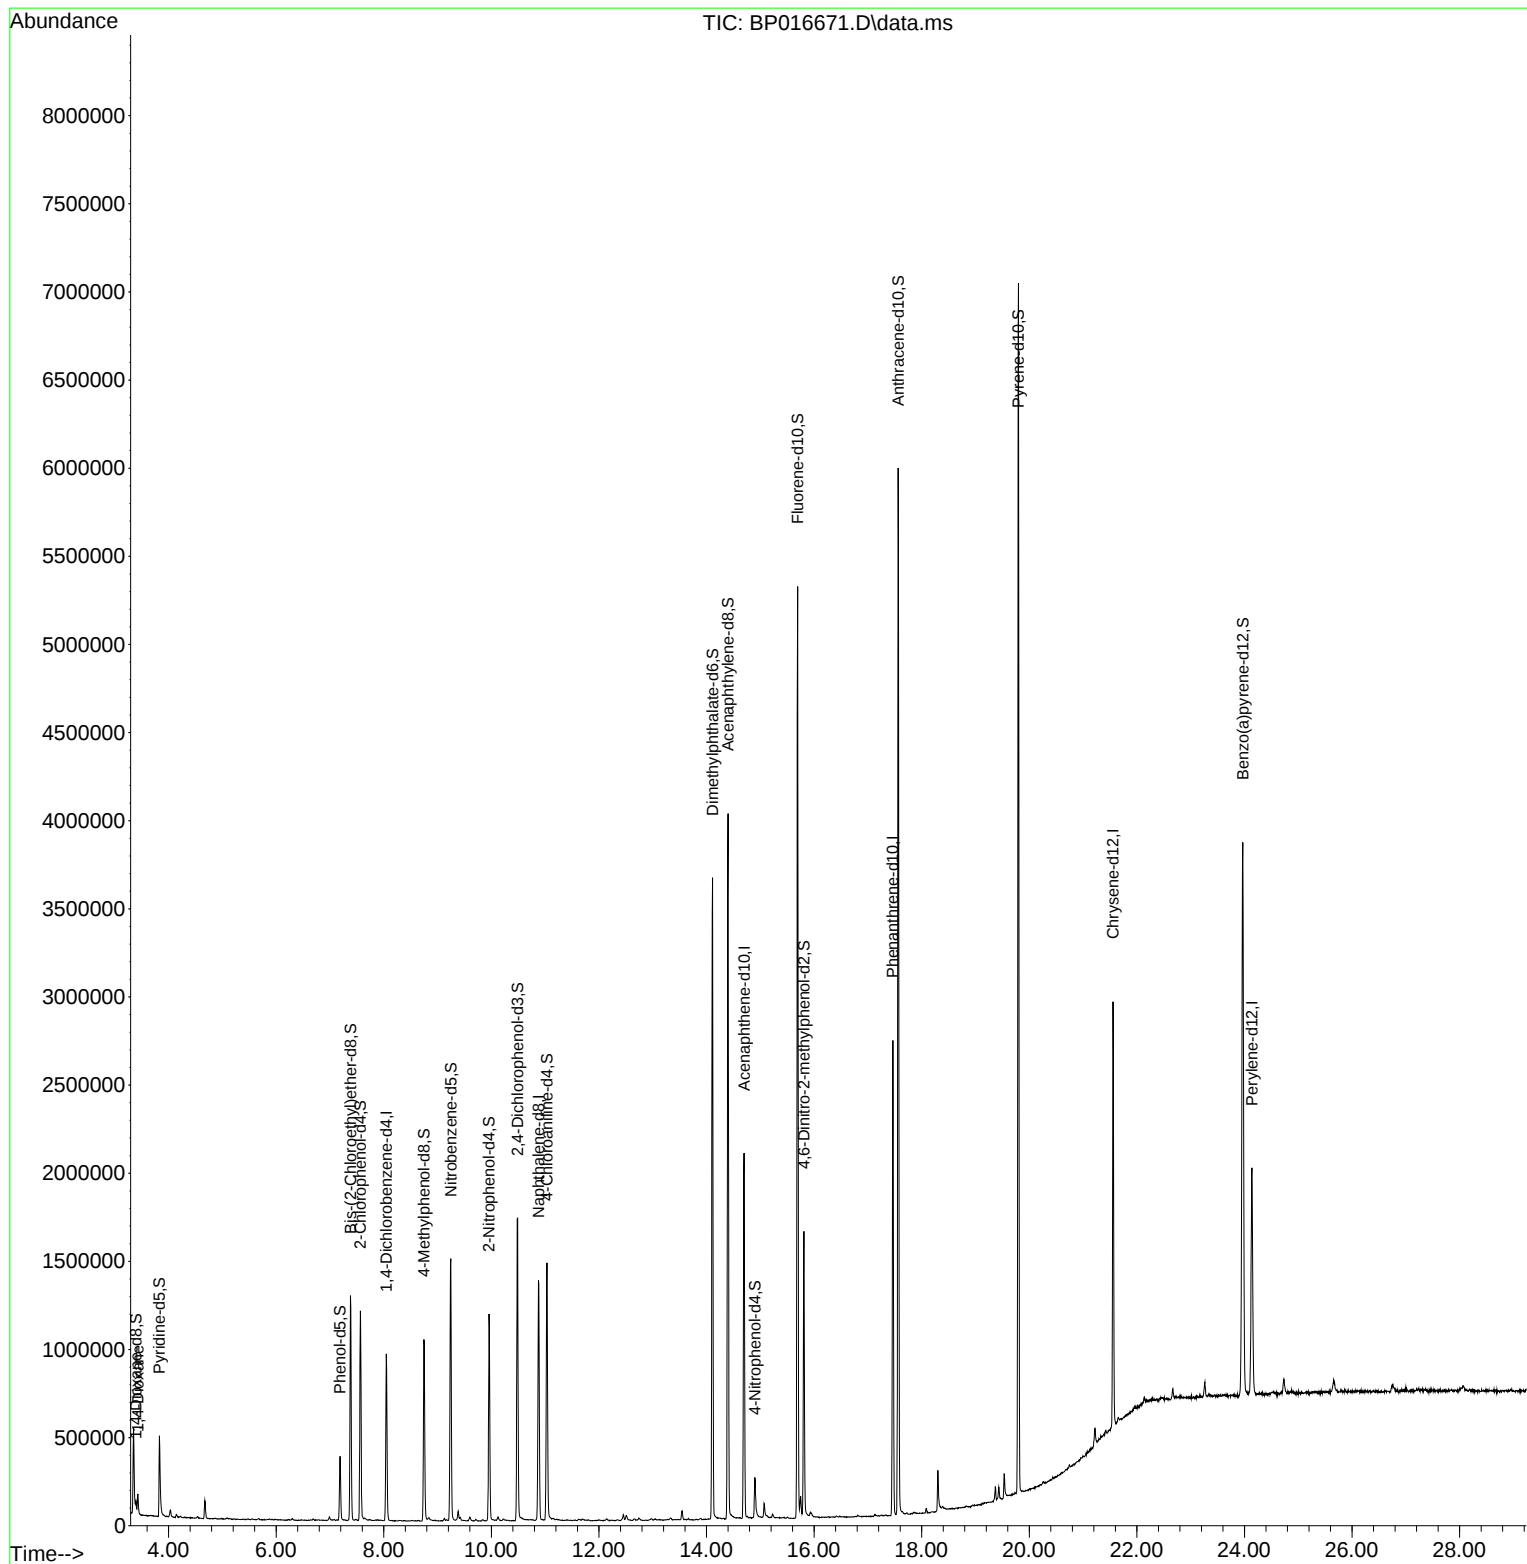

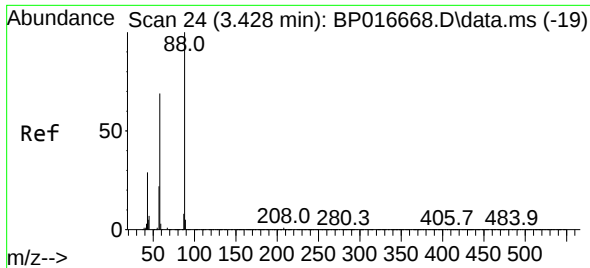

#2
 1,4-Dioxane
 Concen: 8.452 ng/uL
 RT: 3.428 min Scan# 24
 Delta R.T. 0.000 min
 Lab File: BP016671.D
 Acq: 21 Aug 2023 12:47

Instrument :
 BNA_P
 ClientSampleId :
 BH9T7

Tgt Ion: 88 Resp: 57540
 Ion Ratio Lower Upper
 88 100
 43 30.6 23.5 35.3
 58 71.7 57.1 85.7

