

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082123\
 Data File : BP016679.D
 Acq On : 21 Aug 2023 17:22
 Operator : MA/JU
 Sample : 04049-12
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH9J8

Quant Time: Aug 21 19:24:54 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 17 01:38:34 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.046	152	315824	20.000	ng/u1	0.00
20) Naphthalene-d8	10.881	136	1444997	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.698	164	903982	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.463	188	1955648	20.000	ng/u1	0.00
79) Chrysene-d12	21.563	240	1587133	20.000	ng/u1	0.00
88) Perylene-d12	24.139	264	1448882	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	23044	2.773	ng/uL	0.00
4) Pyridine-d5	3.828	84	326417	12.908	ng/u1	0.00
7) Phenol-d5	7.187	99	215113	7.388	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.381	67	633490	33.033	ng/u1	0.00
11) 2-Chlorophenol-d4	7.564	132	540814	25.860	ng/u1	0.00
15) 4-Methylphenol-d8	8.746	113	397401	17.165	ng/u1	-0.01
21) Nitrobenzene-d5	9.246	128	369514	36.343	ng/u1	0.00
24) 2-Nitrophenol-d4	9.958	143	367201	38.025	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.481	165	622196	32.740	ng/u1	-0.01
31) 4-Chloroaniline-d4	11.034	131	967669	29.677	ng/u1	0.00
46) Dimethylphthalate-d6	14.110	166	2416418	36.957	ng/u1	0.00
49) Acenaphthylene-d8	14.398	160	2660397	36.049	ng/u1	0.00
54) 4-Nitrophenol-d4	14.898	143	69773	5.238	ng/u1	0.00
60) Fluorene-d10	15.693	176	2078002	37.280	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.810	200	302211	32.483	ng/u1	0.00
73) Anthracene-d10	17.563	188	3432429	40.576	ng/u1	0.00
81) Pyrene-d10	19.798	212	3854804	46.353	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.969	264	2860679	41.199	ng/u1	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.428	88	9199	1.007	ng/uL 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082123\
Data File : BP016679.D
Acq On : 21 Aug 2023 17:22
Operator : MA/JU
Sample : 04049-12
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH9J8

Quant Time: Aug 21 19:24:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 17 01:38:34 2023
Response via : Initial Calibration

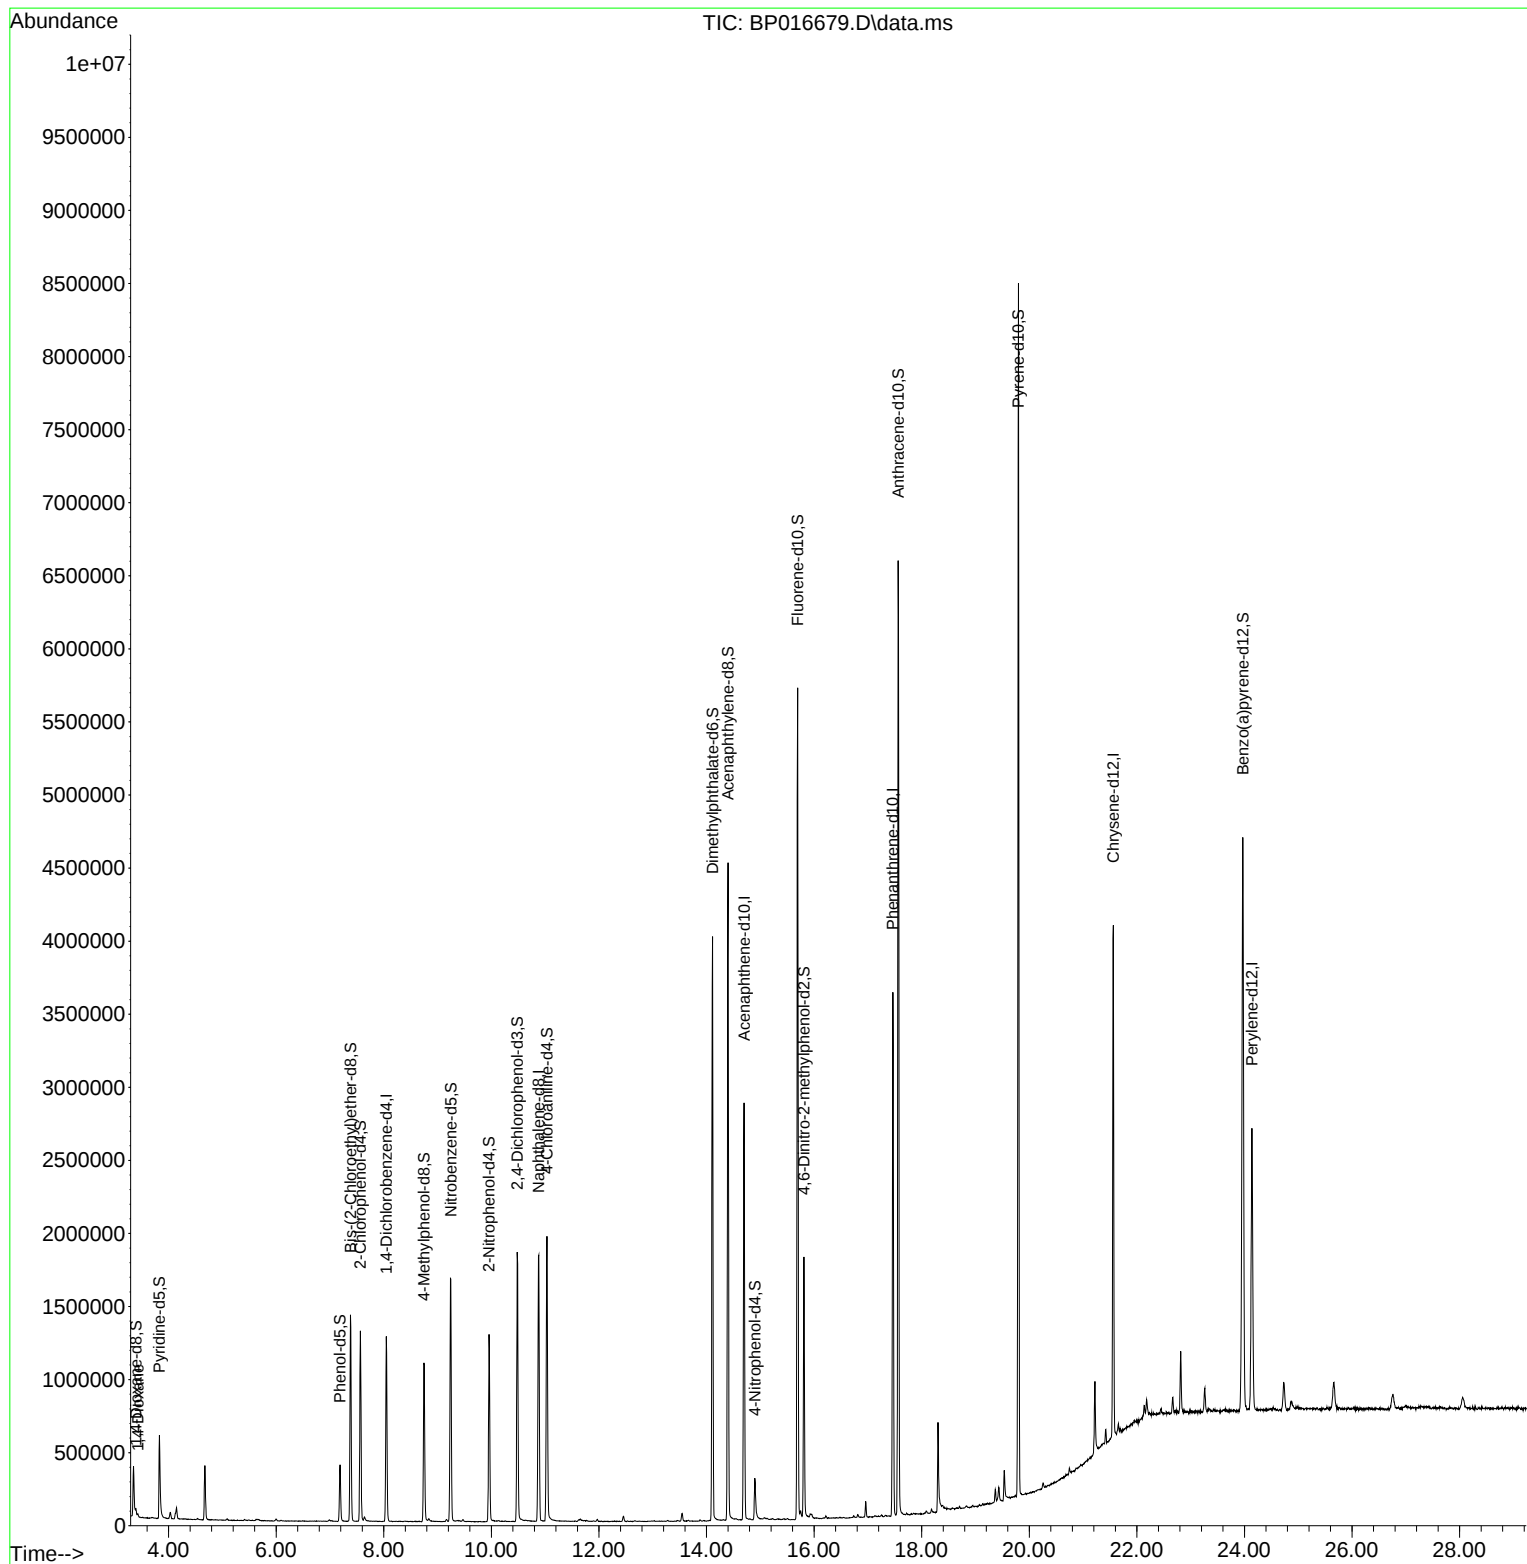

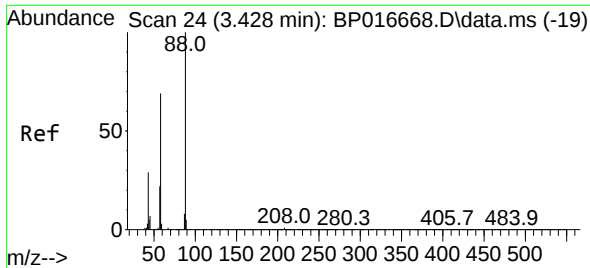

#2
 1,4-Dioxane
 Concen: 1.007 ng/uL
 RT: 3.428 min Scan# 24
 Delta R.T. 0.000 min
 Lab File: BP016679.D
 Acq: 21 Aug 2023 17:22

Instrument :
 BNA_P
 ClientSampleId :
 BH9J8

Tgt Ion:	88	Resp:	9199
Ion	Ratio	Lower	Upper
88	100		
43	34.3	23.5	35.3
58	63.6	57.1	85.7

