

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082123\
 Data File : BP016672.D
 Acq On : 21 Aug 2023 13:21
 Operator : MA/JU
 Sample : 04049-08
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHAL6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016672.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	14	18	28	rVB	47848	80773	0.78%	0.090%
2	3.829	89	92	106	rBV	336007	553002	5.36%	0.613%
3	4.034	122	127	133	rVB	40379	63924	0.62%	0.071%
4	4.146	143	146	151	rVB	21042	27732	0.27%	0.031%
5	4.534	207	212	217	rBV	39384	52863	0.51%	0.059%
6	5.928	444	449	454	rBV	35243	50111	0.49%	0.056%
7	6.099	474	478	485	rVB3	11796	20879	0.20%	0.023%
8	6.987	625	629	635	rBV4	14678	23458	0.23%	0.026%
9	7.187	656	663	674	rBV	401086	646295	6.27%	0.716%
10	7.381	689	696	705	rBV	1348945	2110882	20.47%	2.339%
11	7.564	718	727	738	rBV	1248340	2022397	19.61%	2.241%
12	7.722	750	754	760	rVB9	8059	12537	0.12%	0.014%
13	8.046	801	809	820	rBV	1088760	1774438	17.21%	1.966%
14	8.128	820	823	831	rVB8	13952	26167	0.25%	0.029%
15	8.640	907	910	915	rBV7	8491	14139	0.14%	0.016%
16	8.752	922	929	946	rBV	1059203	1754969	17.02%	1.945%
17	8.899	950	954	959	rVB4	11473	19707	0.19%	0.022%
18	9.158	990	998	1002	rBV3	15442	26719	0.26%	0.030%
19	9.246	1004	1013	1026	rVV	1587088	2640920	25.61%	2.927%
20	9.364	1028	1033	1038	rVB7	17222	31475	0.31%	0.035%
21	9.958	1126	1134	1150	rBV	1246858	2047647	19.86%	2.269%
22	10.134	1160	1164	1175	rBV9	7893	19795	0.19%	0.022%
23	10.481	1215	1223	1232	rBV	1725668	2933135	28.44%	3.250%
24	10.793	1268	1276	1281	rVB6	7705	19712	0.19%	0.022%
25	10.875	1282	1290	1304	rVB	1564922	2661232	25.81%	2.949%
26	11.034	1308	1317	1335	rBV	1856440	3144406	30.49%	3.485%
27	11.558	1400	1406	1409	rBV7	8325	14751	0.14%	0.016%
28	11.622	1412	1417	1424	rVV5	13773	26006	0.25%	0.029%
29	12.152	1495	1507	1514	rBV	83787	157127	1.52%	0.174%
30	12.457	1553	1559	1564	rVB	35304	58471	0.57%	0.065%
31	12.952	1638	1643	1650	rVB	83744	118966	1.15%	0.132%
32	13.275	1692	1698	1704	rVB9	9165	15567	0.15%	0.017%
33	13.540	1737	1743	1751	rBV3	38762	75167	0.73%	0.083%
34	13.634	1754	1759	1767	rBV4	22934	48753	0.47%	0.054%
35	14.110	1833	1840	1852	rBV	3804135	5229214	50.71%	5.795%
36	14.310	1869	1874	1879	rVB9	7627	14396	0.14%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082123\
 Data File : BP016672.D
 Acq On : 21 Aug 2023 13:21
 Operator : MA/JU
 Sample : 04049-08
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHAL6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Title : SVOA CALIBRATION

37	14.399	1882	1889	1904	rBV2	4103919	6109194	59.24%	6.770%
38	14.663	1928	1934	1935	rBV	148677	189042	1.83%	0.209%
39	14.699	1935	1940	1946	rVV	2441518	3607477	34.98%	3.998%
40	14.757	1946	1950	1955	rVB	58195	82600	0.80%	0.092%
41	14.899	1967	1974	1990	rBV	264916	529678	5.14%	0.587%
42	15.093	2001	2007	2008	rBV6	5523	10750	0.10%	0.012%
43	15.122	2008	2012	2021	rVB9	21875	38782	0.38%	0.043%
44	15.357	2047	2052	2058	rBV	38802	59625	0.58%	0.066%
45	15.504	2074	2077	2081	rVB4	7743	11822	0.11%	0.013%
46	15.693	2102	2109	2119	rBV	5709694	8084744	78.40%	8.959%
47	15.810	2123	2129	2145	rVV	1612697	2193188	21.27%	2.430%
48	15.928	2145	2149	2153	rVB3	25346	36617	0.36%	0.041%
49	16.063	2168	2172	2178	rVB2	19551	29781	0.29%	0.033%
50	17.022	2332	2335	2341	rVB4	13148	19282	0.19%	0.021%
51	17.128	2350	2353	2359	rVB8	8970	13964	0.14%	0.015%
52	17.245	2369	2373	2379	rVB5	8617	15560	0.15%	0.017%
53	17.381	2393	2396	2399	rBV3	10192	12322	0.12%	0.014%
54	17.463	2403	2410	2420	rBV	3087274	4403766	42.70%	4.880%
55	17.563	2420	2427	2437	rVV2	6636457	9343616	90.61%	10.354%
56	17.640	2438	2440	2445	rVB6	25817	33526	0.33%	0.037%
57	18.092	2511	2517	2522	rBV	1158101	1342704	13.02%	1.488%
58	18.298	2548	2552	2560	rBV3	85595	138054	1.34%	0.153%
59	18.387	2564	2567	2570	rBV	18100	22200	0.22%	0.025%
60	19.369	2730	2734	2738	rBV2	80761	104684	1.02%	0.116%
61	19.434	2741	2745	2749	rVB	72478	97783	0.95%	0.108%
62	19.534	2758	2762	2766	rBV5	58612	87513	0.85%	0.097%
63	19.792	2801	2806	2816	rBV	7594150	10312417	100.00%	11.428%
64	21.557	3101	3106	3116	rBV	2911298	3815522	37.00%	4.228%
65	23.963	3508	3515	3526	rVB2	3541917	7550558	73.22%	8.367%
66	24.133	3538	3544	3562	rVB	1537350	3403852	33.01%	3.772%




Sum of corrected areas: 90238355

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082123\
Data File : BP016672.D
Acq On : 21 Aug 2023 13:21
Operator : MA/JU
Sample : 04049-08
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAL6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

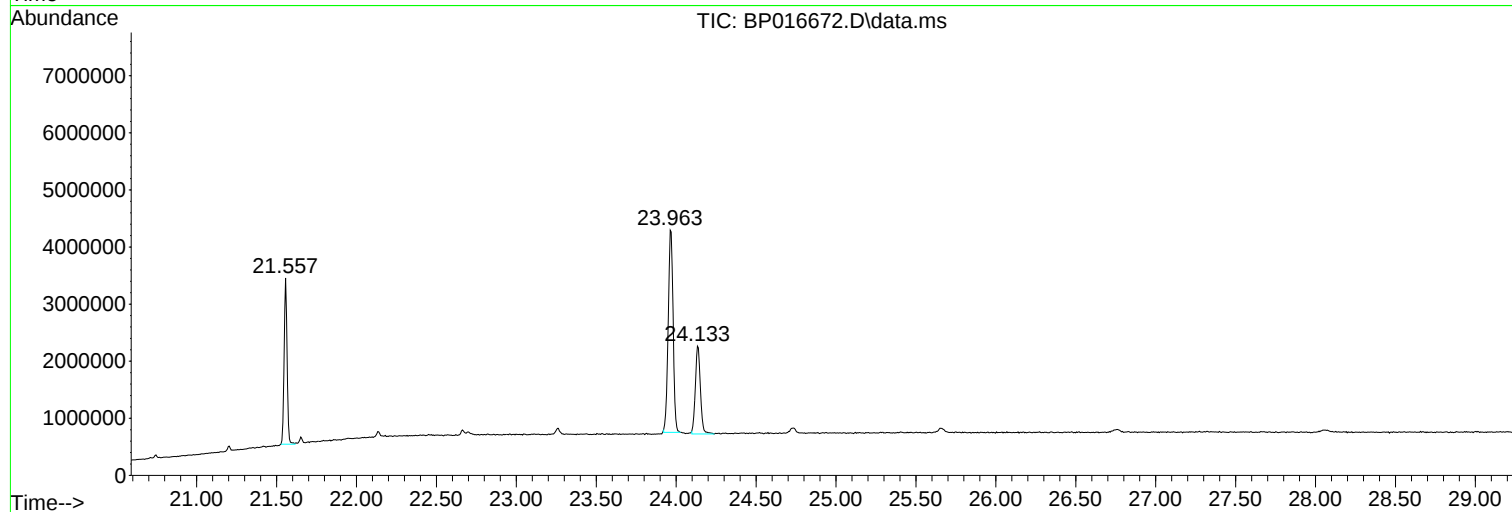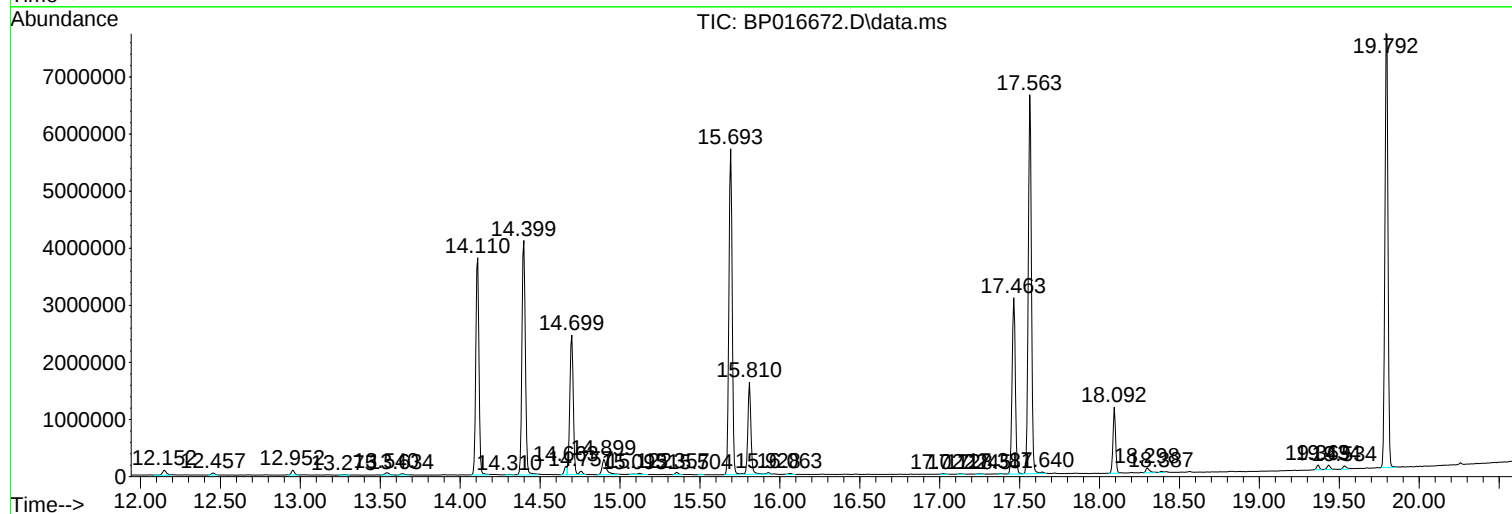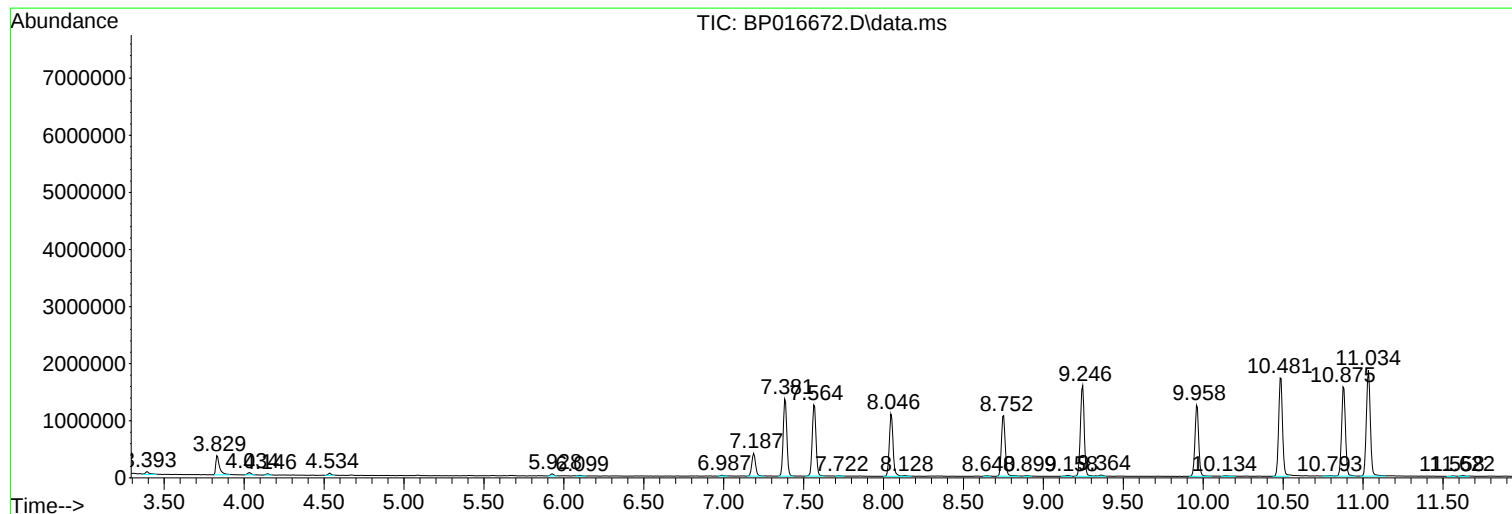

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082123\
Data File : BP016672.D
Acq On : 21 Aug 2023 13:21
Operator : MA/JU
Sample : 04049-08
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAL6










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 7,9-Di-tert-butyl-1-oxaspiro... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
18.093	6.10 ng/ul	1342700	Phenanthrene-d10	17.463

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	7,9-Di-tert-butyl-1-oxaspiro(4,5...	276	C17H24O3	082304-66-3	98		
2	2,5-Cyclohexadien-1-one, 2,6-bis...	232	C16H24O	006738-27-8	83		
3	7,9-Di-tert-butyl-1-oxaspiro(4,5...	276	C17H24O3	082304-66-3	70		
4	1-(3-Amino-4,6-dimethylthieno[2,...	220	C11H12N2OS	052505-42-7	50		
5	Ethanone, 1-(5,6,7,8-tetrahydro-...	220	C14H20O2	071596-88-8	50		

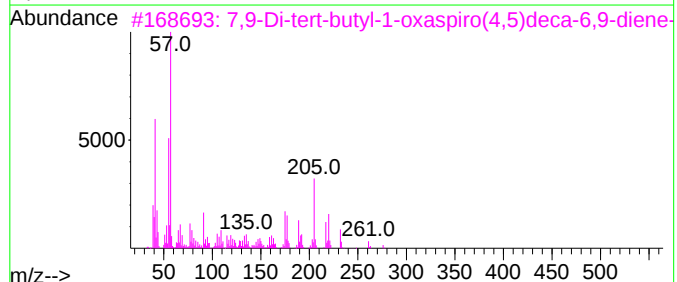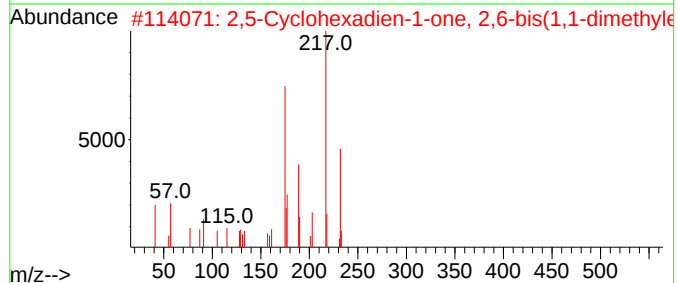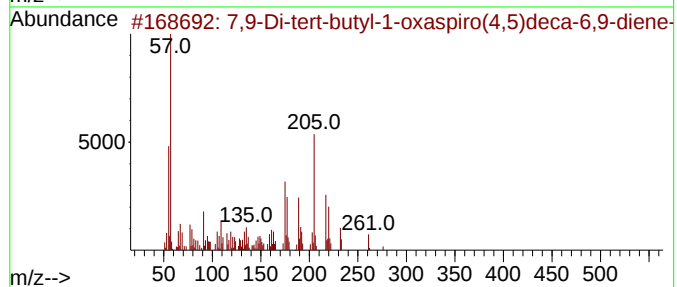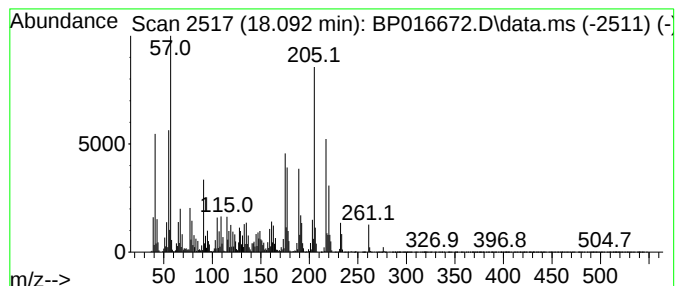

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082123\
Data File : BP016672.D
Acq On : 21 Aug 2023 13:21
Operator : MA/JU
Sample : 04049-08
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAL6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
7,9-Di-tert-but...	18.093	6.1	ng/ul	1342700	4	17.463	4403770	20.0