

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082123\
 Data File : BP016673.D
 Acq On : 21 Aug 2023 13:56
 Operator : MA/JU
 Sample : 04049-09
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH9M3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016673.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.346	5	10	21	rBV	1037752	1696154	16.51%	1.842%
2	3.428	21	24	34	rVB	128688	188948	1.84%	0.205%
3	3.828	89	92	112	rVV	416737	676273	6.58%	0.734%
4	4.034	122	127	133	rVB	36201	56150	0.55%	0.061%
5	4.146	143	146	154	rVB2	18130	28738	0.28%	0.031%
6	4.675	230	236	252	rVB	1578281	2470805	24.05%	2.683%
7	5.669	400	405	410	rBV6	7932	14940	0.15%	0.016%
8	6.734	581	586	591	rBV	19190	30163	0.29%	0.033%
9	7.187	657	663	675	rBV	320995	490416	4.77%	0.532%
10	7.381	688	696	707	rBV	1236646	1962676	19.10%	2.131%
11	7.563	720	727	739	rBV	1128576	1802080	17.54%	1.957%
12	7.652	739	742	749	rVB4	7141	15293	0.15%	0.017%
13	8.046	802	809	819	rBV	1110028	1763181	17.16%	1.914%
14	8.746	920	928	938	rBV	913773	1503229	14.63%	1.632%
15	8.834	938	943	953	rVB	100796	160950	1.57%	0.175%
16	9.246	1005	1013	1023	rBV	1475569	2440897	23.76%	2.650%
17	9.469	1047	1051	1061	rVB8	7206	15369	0.15%	0.017%
18	9.957	1125	1134	1148	rBV	1139953	1876499	18.26%	2.037%
19	10.481	1216	1223	1240	rBV	1642268	2791713	27.17%	3.031%
20	10.875	1282	1290	1303	rBV	1609962	2727221	26.54%	2.961%
21	11.034	1309	1317	1332	rBV	1667382	2859120	27.83%	3.104%
22	11.969	1470	1476	1482	rBV	29694	45915	0.45%	0.050%
23	12.457	1553	1559	1566	rBV2	31787	55849	0.54%	0.061%
24	13.545	1736	1744	1750	rBV2	25582	44853	0.44%	0.049%
25	13.675	1760	1766	1772	rBV9	6073	14759	0.14%	0.016%
26	13.951	1809	1813	1818	rBV2	18537	27233	0.27%	0.030%
27	14.110	1833	1840	1855	rBV	3538204	5022359	48.88%	5.453%
28	14.398	1881	1889	1904	rBV	3888209	5643181	54.92%	6.127%
29	14.698	1933	1940	1949	rBV	2511461	3679729	35.81%	3.995%
30	14.898	1967	1974	1990	rBV	221551	435330	4.24%	0.473%
31	15.069	2001	2003	2009	rVV7	5050	11165	0.11%	0.012%
32	15.122	2010	2012	2020	rVB9	12430	16632	0.16%	0.018%
33	15.228	2025	2030	2038	rBV	30540	52858	0.51%	0.057%
34	15.504	2073	2077	2083	rVB5	10490	18855	0.18%	0.020%
35	15.692	2101	2109	2116	rBV	5340040	7488330	72.88%	8.130%
36	15.745	2116	2118	2123	rVV4	53665	85628	0.83%	0.093%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082123\
 Data File : BP016673.D
 Acq On : 21 Aug 2023 13:56
 Operator : MA/JU
 Sample : 04049-09
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH9M3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Title : SVOA CALIBRATION

37	15.810	2123	2129	2144	rVV	1704252	2338183	22.76%	2.539%
38	15.951	2145	2153	2164	rVB2	64808	158592	1.54%	0.172%
39	16.810	2296	2299	2306	rVB8	8406	14358	0.14%	0.016%
40	17.463	2403	2410	2420	rBV	3238372	4551378	44.30%	4.942%
41	17.563	2421	2427	2444	rVV2	6366705	8895500	86.58%	9.658%
42	18.186	2529	2533	2536	rBV5	12874	19724	0.19%	0.021%
43	18.298	2547	2552	2562	rBV	261663	436605	4.25%	0.474%
44	19.363	2730	2733	2737	rVB2	74867	92107	0.90%	0.100%
45	19.433	2741	2745	2751	rVB	80542	120530	1.17%	0.131%
46	19.533	2758	2762	2768	rBV2	137646	206944	2.01%	0.225%
47	19.792	2801	2806	2815	rBV	7765313	10274476	100.00%	11.156%
48	21.557	3101	3106	3113	rBV	3368024	4440432	43.22%	4.821%
49	23.968	3508	3516	3530	rVB2	3944994	8433702	82.08%	9.157%
50	24.139	3538	3545	3554	rVB	1833070	3906288	38.02%	4.241%




Sum of corrected areas: 92102310

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082123\
Data File : BP016673.D
Acq On : 21 Aug 2023 13:56
Operator : MA/JU
Sample : 04049-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH9M3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

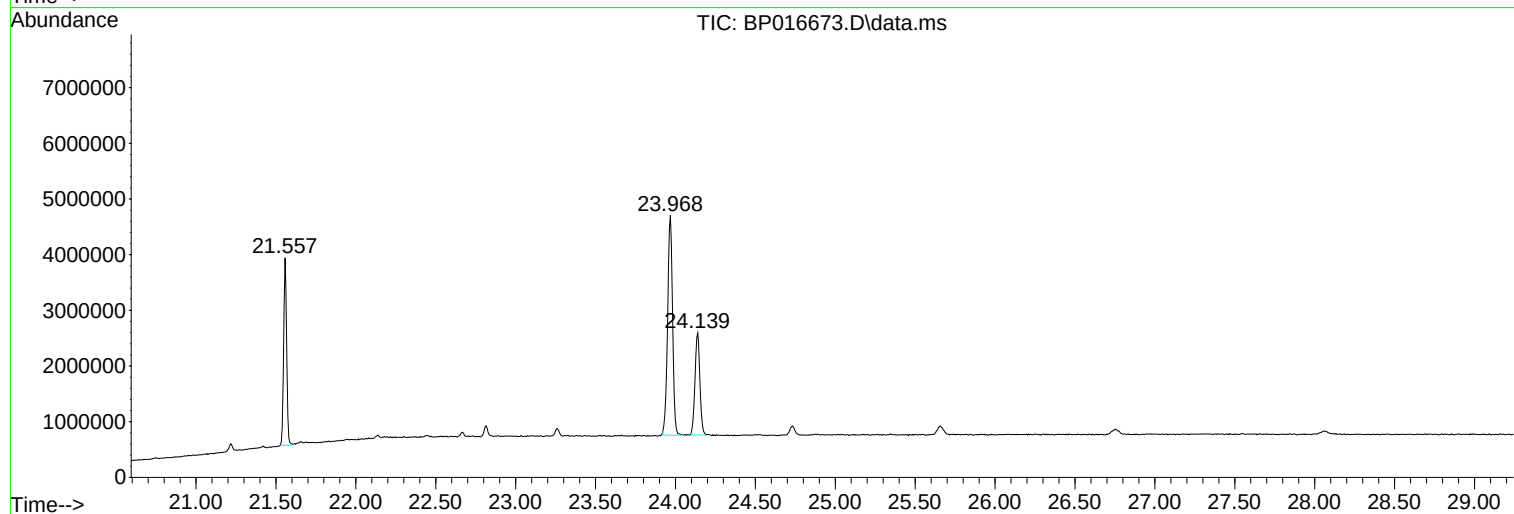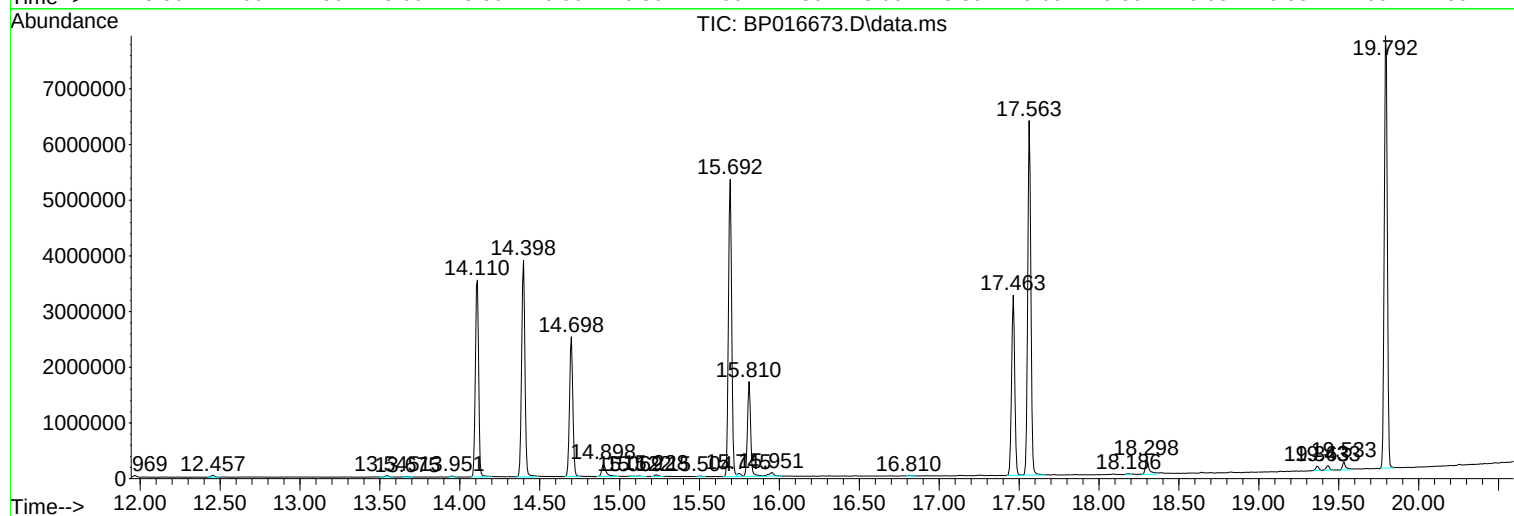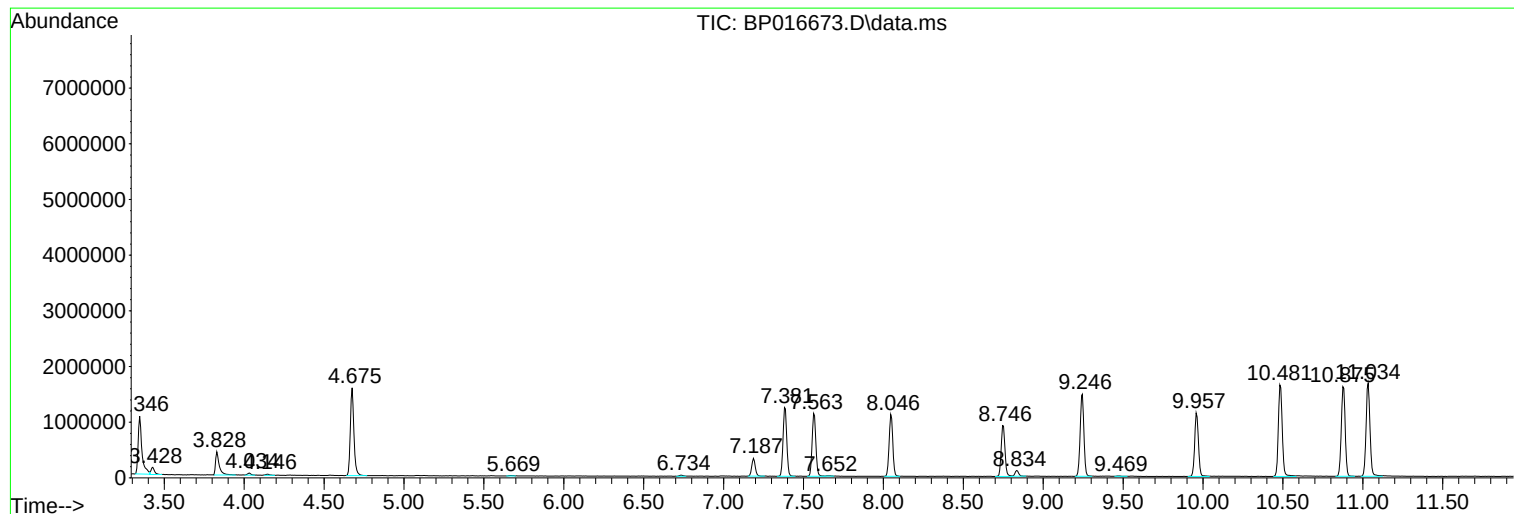

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082123\
Data File : BP016673.D
Acq On : 21 Aug 2023 13:56
Operator : MA/JU
Sample : 04049-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH9M3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.675	28.03 ng/ul	2470810	1,4-Dichlorobenzene-d4	8.046

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	96
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	16

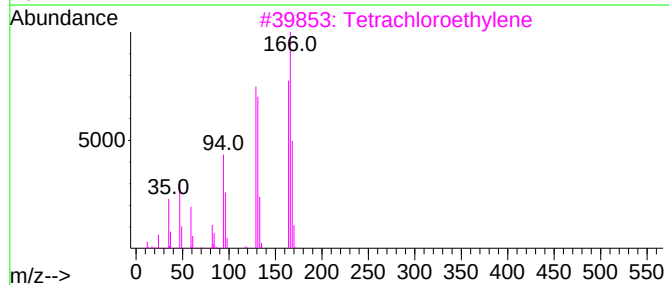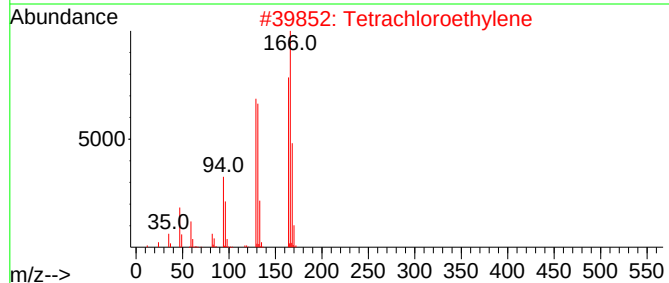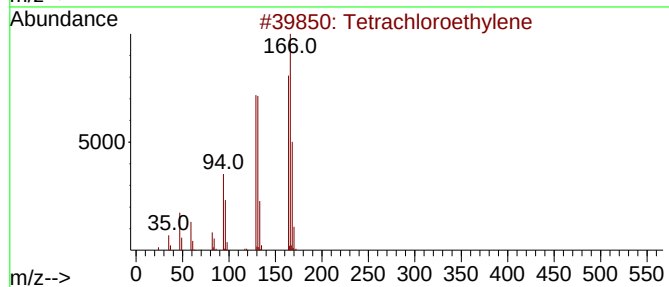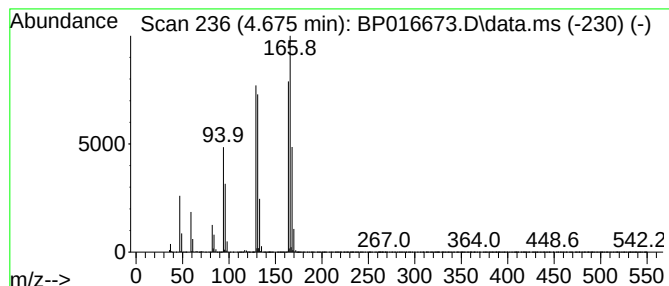

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082123\
Data File : BP016673.D
Acq On : 21 Aug 2023 13:56
Operator : MA/JU
Sample : 04049-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH9M3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.675	28.0	ng/ul	2470810	1	8.046	1763180	20.0