

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082123\
 Data File : BP016680.D
 Acq On : 21 Aug 2023 17:56
 Operator : MA/JU
 Sample : 04049-13
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH9K1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016680.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.346	6	10	15	rBV	160805	234358	2.00%	0.230%
2	3.387	15	17	20	rVV2	52292	69978	0.60%	0.069%
3	3.428	20	24	34	rVB	160402	233835	1.99%	0.230%
4	3.828	88	92	109	rBV	563444	895412	7.64%	0.879%
5	4.028	122	126	134	rVB	47282	69374	0.59%	0.068%
6	4.146	142	146	152	rVB	19171	27721	0.24%	0.027%
7	4.216	156	158	162	rVB2	9839	13290	0.11%	0.013%
8	4.534	207	212	217	rVB6	14246	22908	0.20%	0.022%
9	4.675	232	236	241	rVB7	9715	15175	0.13%	0.015%
10	5.122	310	312	321	rVB5	10051	18141	0.15%	0.018%
11	5.552	382	385	391	rVB7	7560	13033	0.11%	0.013%
12	5.669	399	405	410	rBV6	7453	13485	0.12%	0.013%
13	6.981	624	628	635	rBV6	7557	16822	0.14%	0.017%
14	7.187	655	663	674	rBV	434987	686828	5.86%	0.674%
15	7.381	689	696	704	rBV	1644733	2524139	21.53%	2.478%
16	7.563	719	727	739	rBV	1501170	2362626	20.15%	2.320%
17	8.046	802	809	820	rBV	1134757	1796677	15.32%	1.764%
18	8.751	919	929	941	rBV	1218334	2016209	17.19%	1.980%
19	9.163	994	999	1004	rBV7	7717	13209	0.11%	0.013%
20	9.246	1005	1013	1025	rVV	1928692	3203108	27.32%	3.145%
21	9.399	1035	1039	1045	rVB6	10954	19254	0.16%	0.019%
22	9.563	1060	1067	1072	rBV10	7151	14292	0.12%	0.014%
23	9.957	1126	1134	1149	rBV	1518038	2519338	21.49%	2.474%
24	10.481	1212	1223	1240	rBV	2133278	3616612	30.84%	3.551%
25	10.875	1282	1290	1298	rBV	1695889	2817527	24.03%	2.766%
26	11.034	1309	1317	1333	rBV	2224258	3799851	32.41%	3.731%
27	11.145	1335	1336	1341	rVB5	10954	16304	0.14%	0.016%
28	11.622	1410	1417	1419	rBV8	7358	12399	0.11%	0.012%
29	12.451	1552	1558	1564	rBV	43885	67875	0.58%	0.067%
30	12.669	1590	1595	1600	rBV8	6054	12896	0.11%	0.013%
31	13.545	1738	1744	1751	rVB	39906	69322	0.59%	0.068%
32	13.675	1761	1766	1775	rVB9	10436	26684	0.23%	0.026%
33	14.110	1833	1840	1853	rBV	4245917	5937365	50.64%	5.830%
34	14.398	1882	1889	1905	rBV2	4970164	7224311	61.61%	7.093%
35	14.604	1919	1924	1928	rBV2	10969	19587	0.17%	0.019%
36	14.698	1933	1940	1948	rBV	2652814	3805886	32.46%	3.737%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082123\
 Data File : BP016680.D
 Acq On : 21 Aug 2023 17:56
 Operator : MA/JU
 Sample : 04049-13
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH9K1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Title : SVOA CALIBRATION

37	14.898	1968	1974	1993	rBV	301634	576233	4.91%	0.566%
38	15.228	2025	2030	2037	rVB3	13158	23405	0.20%	0.023%
39	15.692	2102	2109	2119	rBV	6504048	9036130	77.06%	8.872%
40	15.810	2123	2129	2138	rVV	2061344	2721905	23.21%	2.673%
41	15.928	2145	2149	2159	rVB3	31780	61911	0.53%	0.061%
42	17.463	2403	2410	2420	rBV	3283465	4709188	40.16%	4.624%
43	17.563	2420	2427	2447	rVV2	7386252	10354296	88.31%	10.166%
44	18.298	2548	2552	2561	rBV	116570	182019	1.55%	0.179%
45	18.645	2607	2611	2617	rBV3	53678	71534	0.61%	0.070%
46	19.369	2730	2734	2738	rVB2	93161	119230	1.02%	0.117%
47	19.433	2742	2745	2752	rVB	95446	123720	1.06%	0.121%
48	19.533	2758	2762	2769	rBV2	87586	142996	1.22%	0.140%
49	19.798	2801	2807	2816	rBV	8741176	11725599	100.00%	11.513%
50	21.557	3101	3106	3114	rBV2	3418291	4504882	38.42%	4.423%
51	23.968	3508	3516	3527	rVB2	4366383	9414487	80.29%	9.244%
52	24.139	3538	3545	3554	rVB	1794274	3853972	32.87%	3.784%




Sum of corrected areas: 101847338

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082123\
Data File : BP016680.D
Acq On : 21 Aug 2023 17:56
Operator : MA/JU
Sample : 04049-13
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH9K1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

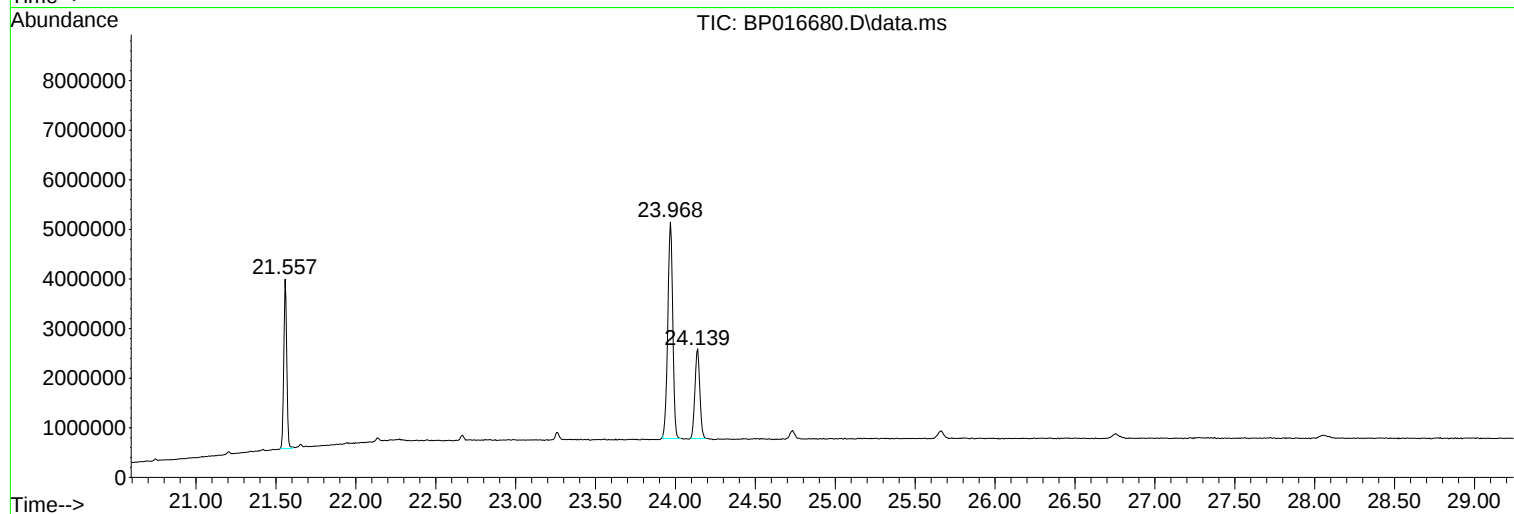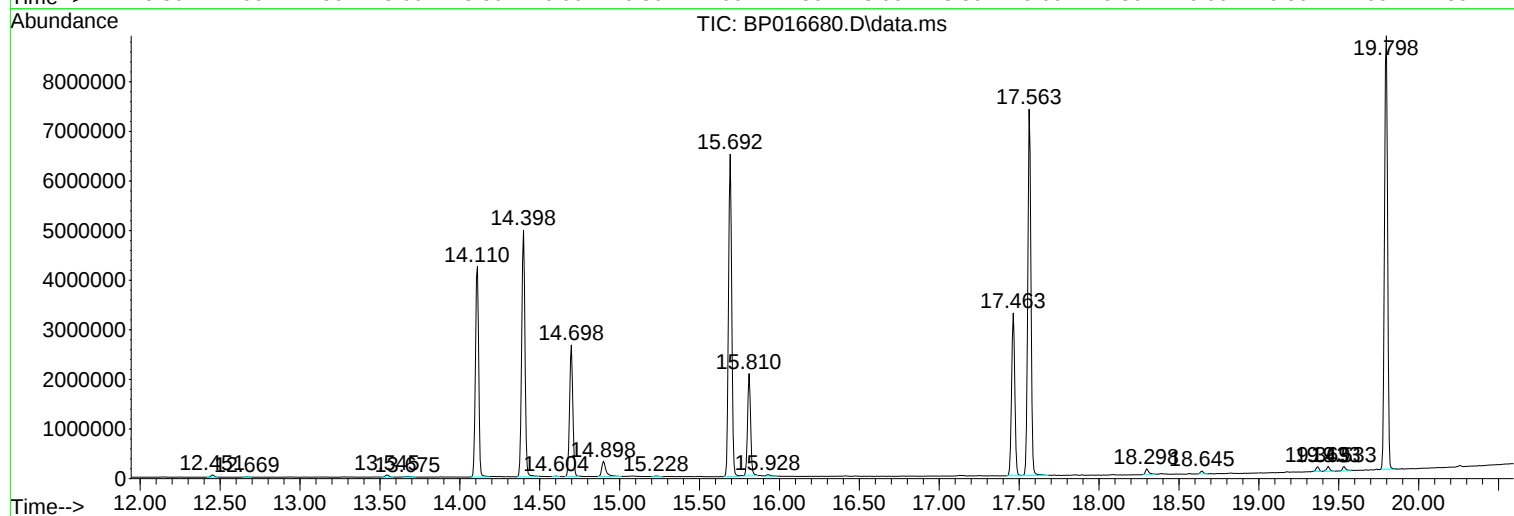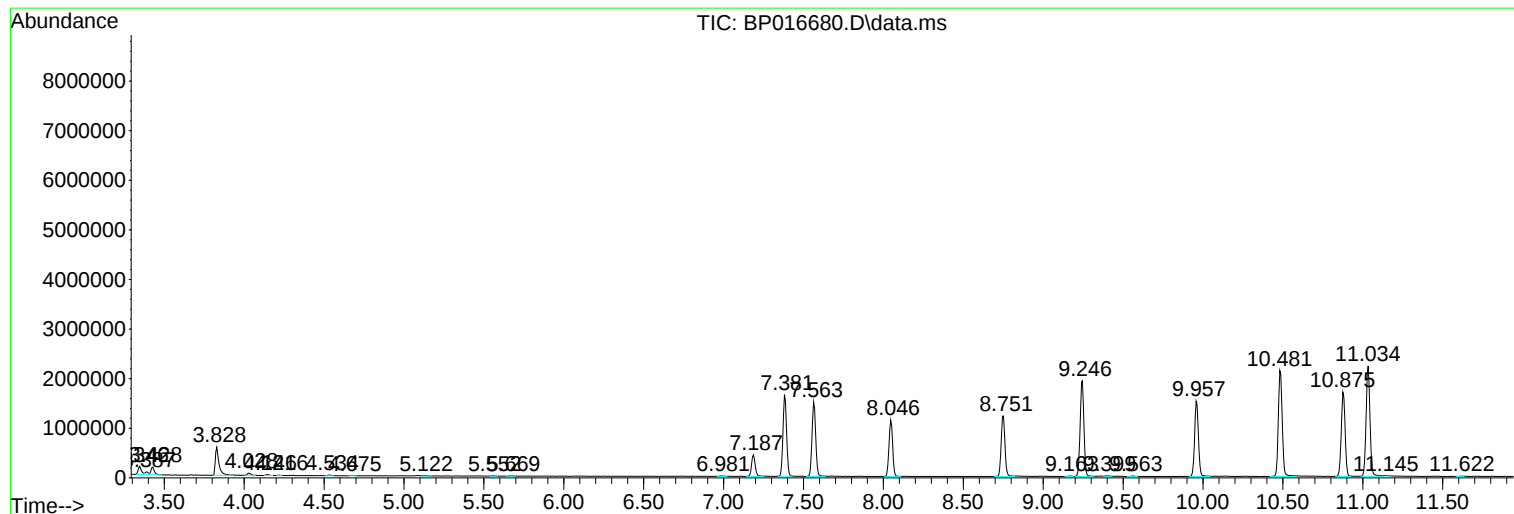

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082123\
Data File : BP016680.D
Acq On : 21 Aug 2023 17:56
Operator : MA/JU
Sample : 04049-13
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH9K1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082123\
Data File : BP016680.D
Acq On : 21 Aug 2023 17:56
Operator : MA/JU
Sample : 04049-13
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH9K1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc