

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082123\
 Data File : BP016682.D
 Acq On : 21 Aug 2023 19:39
 Operator : MA/JU
 Sample : PB154953BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK953

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016682.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.387	13	17	29	rVB	111555	172690	1.65%	0.166%
2	3.822	87	91	114	rBV	1498328	2434733	23.24%	2.345%
3	4.146	141	146	152	rBV2	19907	34072	0.33%	0.033%
4	7.187	654	663	679	rBV	1884459	2957949	28.23%	2.849%
5	7.381	688	696	706	rBV	1519871	2315311	22.10%	2.230%
6	7.563	719	727	738	rBV	1761371	2771755	26.45%	2.670%
7	8.046	802	809	820	rBV	1231950	1911919	18.25%	1.842%
8	8.752	919	929	942	rBV	2209481	3667928	35.00%	3.533%
9	9.240	1004	1012	1025	rBV	1768053	2892310	27.60%	2.786%
10	9.957	1125	1134	1152	rBV	1444586	2371041	22.63%	2.284%
11	10.481	1213	1223	1238	rBV	2140805	3620156	34.55%	3.487%
12	10.875	1282	1290	1298	rBV	1806322	2988879	28.52%	2.879%
13	11.034	1309	1317	1336	rBV	2289636	3962990	37.82%	3.817%
14	12.451	1552	1558	1568	rBV2	39399	66948	0.64%	0.064%
15	13.545	1737	1744	1748	rBV2	20153	34545	0.33%	0.033%
16	13.663	1757	1764	1765	rBV6	9175	12962	0.12%	0.012%
17	14.104	1833	1839	1853	rBV	3881749	5526109	52.74%	5.323%
18	14.398	1879	1889	1906	rBV	4518707	6668486	63.64%	6.423%
19	14.698	1933	1940	1951	rBV	2763595	4129268	39.41%	3.978%
20	14.898	1967	1974	1997	rBV	1780897	2979071	28.43%	2.870%
21	15.692	2099	2109	2123	rBV	5718579	8285094	79.07%	7.981%
22	15.810	2123	2129	2142	rVV	1591582	2183228	20.83%	2.103%
23	15.928	2145	2149	2153	rVB2	27764	44522	0.42%	0.043%
24	16.392	2225	2228	2236	rBV10	4011	12441	0.12%	0.012%
25	17.122	2350	2352	2356	rBV4	8842	10873	0.10%	0.010%
26	17.463	2403	2410	2420	rBV	3583581	5020465	47.91%	4.836%
27	17.563	2420	2427	2438	rBV2	6755533	9367449	89.40%	9.023%
28	18.298	2549	2552	2562	rBV8	33545	65831	0.63%	0.063%
29	19.369	2730	2734	2739	rBV2	78312	105050	1.00%	0.101%
30	19.433	2741	2745	2752	rVB2	71407	97559	0.93%	0.094%
31	19.533	2760	2762	2768	rBV5	22811	28057	0.27%	0.027%
32	19.798	2801	2807	2819	rBV	7591461	10478688	100.00%	10.094%
33	21.557	3101	3106	3115	rBV2	3479675	4651634	44.39%	4.481%
34	23.968	3508	3516	3529	rVB2	3863121	8021066	76.55%	7.726%
35	24.139	3538	3545	3556	rVB	1827048	3923745	37.45%	3.780%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082123\
Data File : BP016682.D
Acq On : 21 Aug 2023 19:39
Operator : MA/JU
Sample : PB154953BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK953

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 103814824

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082123\
Data File : BP016682.D
Acq On : 21 Aug 2023 19:39
Operator : MA/JU
Sample : PB154953BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK953

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

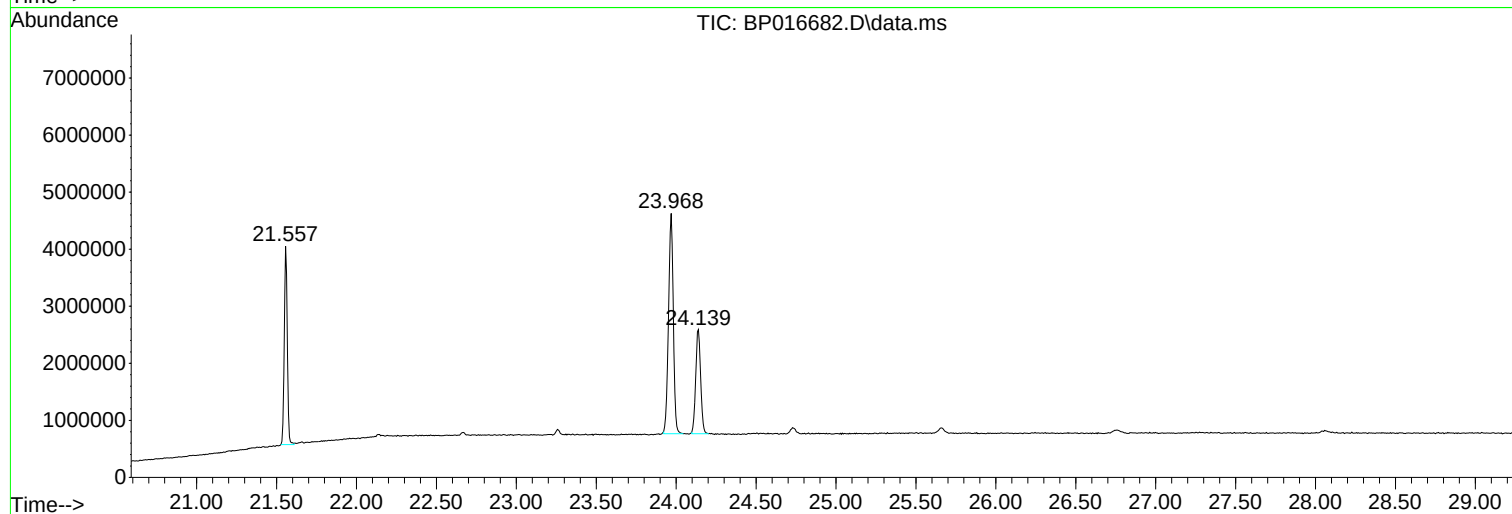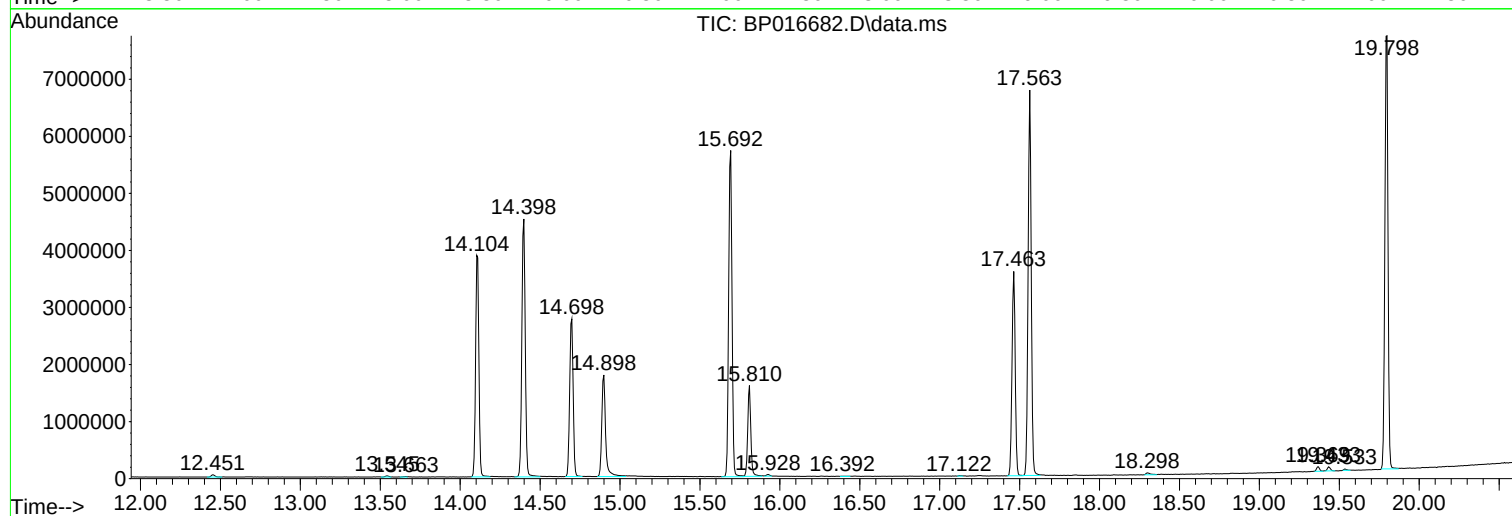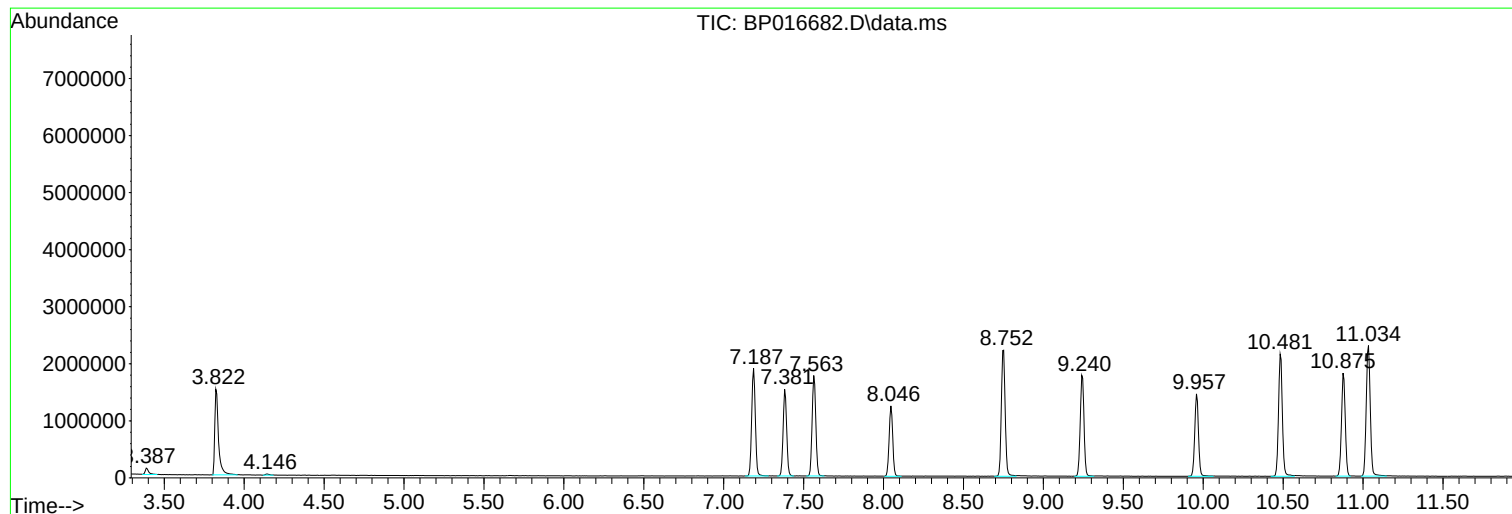

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082123\
Data File : BP016682.D
Acq On : 21 Aug 2023 19:39
Operator : MA/JU
Sample : PB154953BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK953

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082123\
Data File : BP016682.D
Acq On : 21 Aug 2023 19:39
Operator : MA/JU
Sample : PB154953BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK953

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------