

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082123\
 Data File : BP016684.D
 Acq On : 21 Aug 2023 20:48
 Operator : MA/JU
 Sample : 04049-16
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH8T9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016684.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.346	5	10	15	rBV	284547	429737	3.22%	0.355%
2	3.393	15	18	21	rVB	53859	63751	0.48%	0.053%
3	3.828	88	92	104	rBV	615948	929949	6.96%	0.768%
4	4.034	122	127	134	rVB	51245	86457	0.65%	0.071%
5	4.146	142	146	150	rBV	20569	29265	0.22%	0.024%
6	4.675	229	236	254	rBV	4448021	7013385	52.52%	5.791%
7	5.087	302	306	309	rBV2	11771	13829	0.10%	0.011%
8	5.675	400	406	410	rBV6	9105	16894	0.13%	0.014%
9	6.093	473	477	483	rVB5	14482	26318	0.20%	0.022%
10	6.981	623	628	633	rBV4	11580	20802	0.16%	0.017%
11	7.187	655	663	675	rBV	510181	810551	6.07%	0.669%
12	7.381	687	696	708	rBV	1697822	2618569	19.61%	2.162%
13	7.563	719	727	738	rBV	1650056	2553299	19.12%	2.108%
14	7.640	738	740	750	rVV5	10811	23070	0.17%	0.019%
15	7.740	750	757	764	rVV3	24826	59366	0.44%	0.049%
16	7.975	791	797	801	rBV	37993	59290	0.44%	0.049%
17	8.046	801	809	821	rVB	1381679	2157276	16.16%	1.781%
18	8.746	921	928	940	rBV	1435650	2287787	17.13%	1.889%
19	8.840	940	944	950	rVB9	8483	16460	0.12%	0.014%
20	8.963	960	965	969	rVB5	11230	18053	0.14%	0.015%
21	9.240	1003	1012	1024	rBV	2028116	3354815	25.12%	2.770%
22	9.469	1047	1051	1057	rVB2	10107	15448	0.12%	0.013%
23	9.957	1126	1134	1149	rBV	1622750	2610248	19.55%	2.155%
24	10.481	1215	1223	1238	rBV	2317979	3841911	28.77%	3.172%
25	10.875	1282	1290	1306	rBV	2021217	3375578	25.28%	2.787%
26	11.034	1309	1317	1331	rBV	2259247	3921231	29.37%	3.238%
27	11.622	1412	1417	1423	rVB9	8549	15550	0.12%	0.013%
28	11.969	1470	1476	1479	rBV3	9605	16086	0.12%	0.013%
29	12.010	1479	1483	1489	rVB7	9214	15962	0.12%	0.013%
30	12.451	1551	1558	1564	rBV2	44534	69548	0.52%	0.057%
31	13.545	1737	1744	1748	rBV	34292	56547	0.42%	0.047%
32	13.951	1806	1813	1816	rBV4	9907	14682	0.11%	0.012%
33	14.110	1833	1840	1854	rBV	4648099	6629714	49.65%	5.474%
34	14.398	1881	1889	1910	rBV	5124810	7630595	57.14%	6.301%
35	14.563	1914	1917	1924	rVB8	11435	20473	0.15%	0.017%
36	14.698	1933	1940	1950	rBV	3196946	4540406	34.00%	3.749%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082123\
 Data File : BP016684.D
 Acq On : 21 Aug 2023 20:48
 Operator : MA/JU
 Sample : 04049-16
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH8T9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Title : SVOA CALIBRATION

37	14.898	1967	1974	1995	rBV	428954	814706	6.10%	0.673%
38	15.069	1998	2003	2005	rVV6	12050	19774	0.15%	0.016%
39	15.122	2009	2012	2015	rVB5	14348	17635	0.13%	0.015%
40	15.334	2043	2048	2052	rBV6	14124	23251	0.17%	0.019%
41	15.504	2074	2077	2082	rVB5	8948	13852	0.10%	0.011%
42	15.692	2101	2109	2123	rBV	6650502	9974104	74.69%	8.236%
43	15.810	2123	2129	2145	rVV	2219748	3139996	23.51%	2.593%
44	15.928	2145	2149	2161	rVB3	35987	75767	0.57%	0.063%
45	16.475	2237	2242	2245	rBV7	9150	15414	0.12%	0.013%
46	16.757	2285	2290	2295	rBV3	20656	32267	0.24%	0.027%
47	16.810	2296	2299	2305	rBV7	12920	19734	0.15%	0.016%
48	17.463	2403	2410	2420	rBV	3896647	5623112	42.11%	4.643%
49	17.563	2420	2427	2444	rVV2	8173800	11720207	87.77%	9.678%
50	18.181	2528	2532	2536	rBV6	14193	22873	0.17%	0.019%
51	18.298	2547	2552	2562	rBV	271607	445544	3.34%	0.368%
52	19.363	2730	2733	2737	rBV2	100637	129417	0.97%	0.107%
53	19.433	2741	2745	2749	rVB	107546	147079	1.10%	0.121%
54	19.528	2758	2761	2769	rBV	168510	276211	2.07%	0.228%
55	19.792	2800	2806	2817	rBV	9912693	13353223	100.00%	11.026%
56	21.557	3101	3106	3113	rBV	3881397	5110975	38.28%	4.220%
57	23.963	3507	3515	3530	rVB2	4617987	10304298	77.17%	8.509%
58	24.133	3538	3544	3560	rVB	2052356	4463431	33.43%	3.686%




Sum of corrected areas: 121105772

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082123\
Data File : BP016684.D
Acq On : 21 Aug 2023 20:48
Operator : MA/JU
Sample : 04049-16
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH8T9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

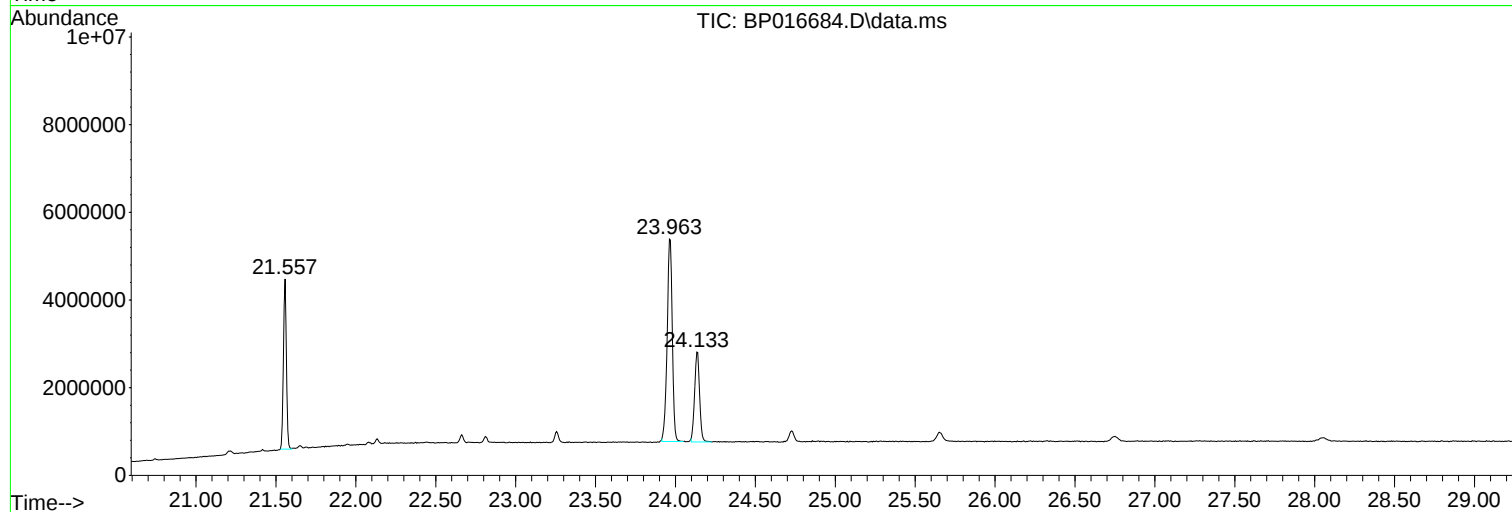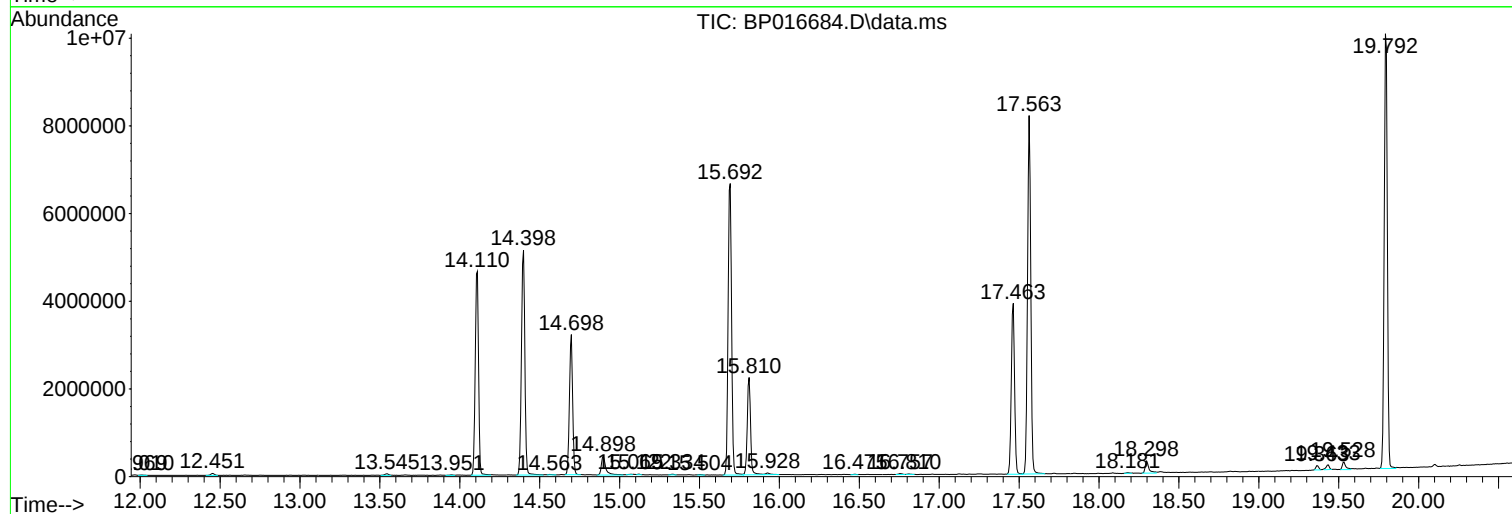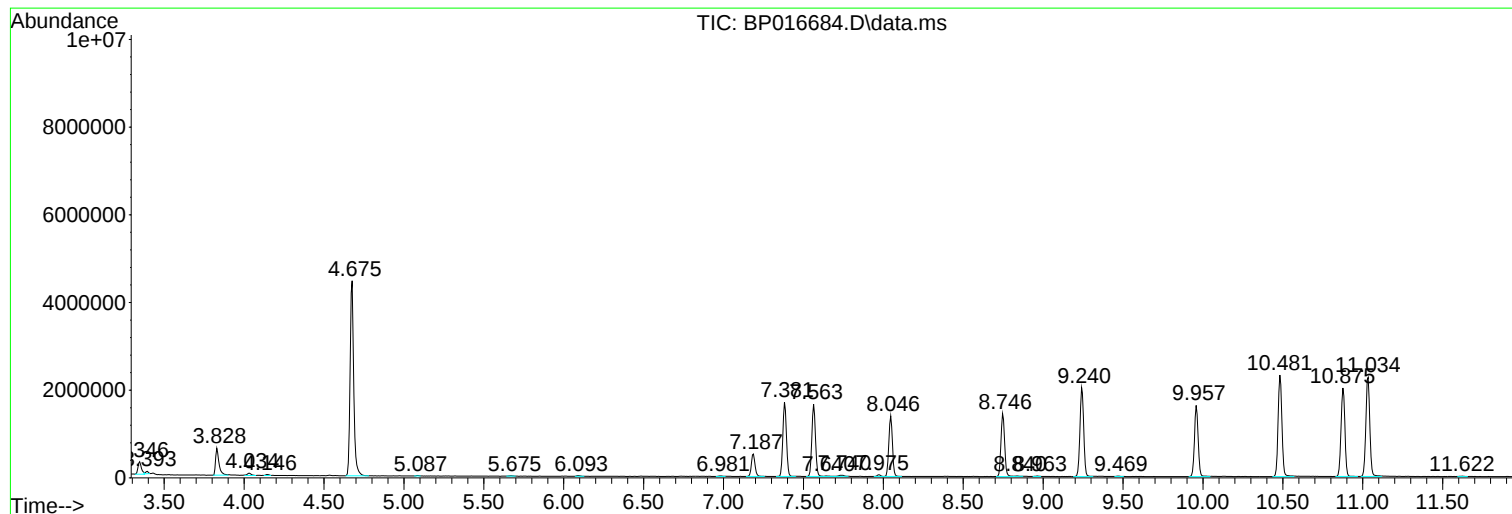

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082123\
Data File : BP016684.D
Acq On : 21 Aug 2023 20:48
Operator : MA/JU
Sample : 04049-16
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH8T9










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.675	65.02 ng/ul	7013390	1,4-Dichlorobenzene-d4	8.046

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	96
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	38

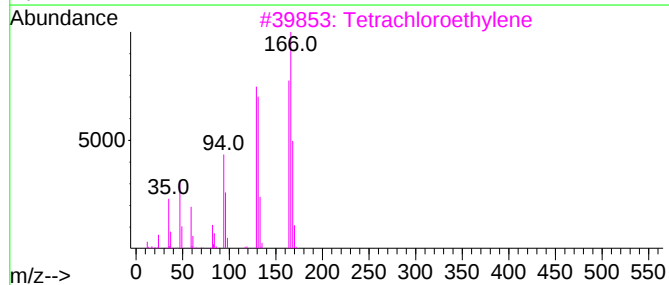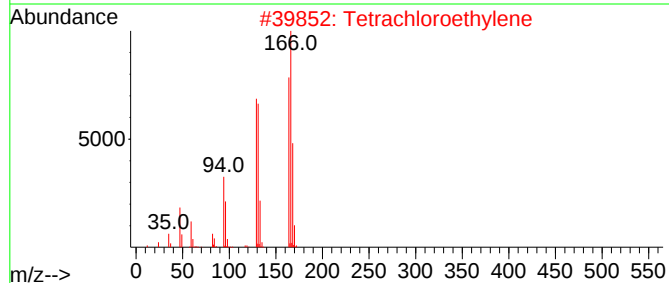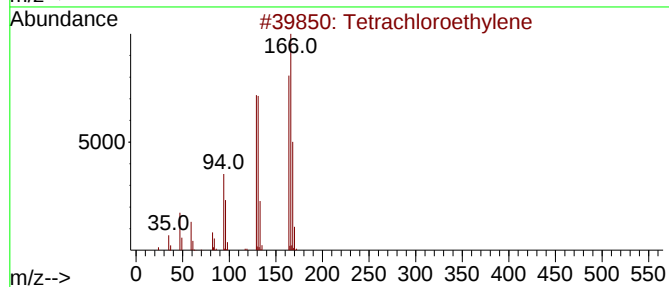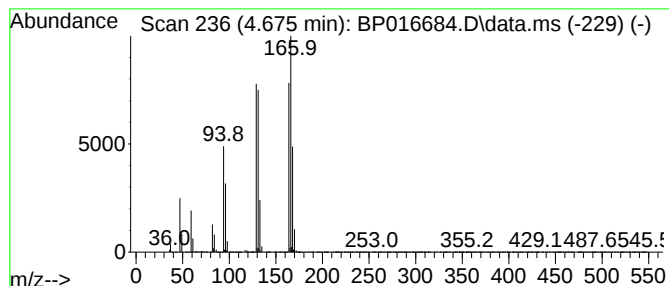

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082123\
Data File : BP016684.D
Acq On : 21 Aug 2023 20:48
Operator : MA/JU
Sample : 04049-16
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH8T9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.675	65.0	ng/ul	7013390	1	8.046	2157280	20.0