

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082223\
 Data File : BP016694.D
 Acq On : 22 Aug 2023 09:11
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020697

Quant Time: Aug 23 00:42:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 17 01:38:34 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.040	152	377559	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.875	136	1718566	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.698	164	1057460	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.463	188	2310552	20.000	ng/u1	0.00
79) Chrysene-d12	21.563	240	1999710	20.000	ng/u1	0.00
88) Perylene-d12	24.145	264	2031688	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	79634	8.015	ng/uL	0.00
4) Pyridine-d5	3.822	84	574959	19.019	ng/u1	0.00
7) Phenol-d5	7.181	99	659377	18.943	ng/u1	-0.01
9) Bis-(2-Chloroethyl)eth...	7.375	67	450621	19.655	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.558	132	493385	19.735	ng/u1	-0.01
15) 4-Methylphenol-d8	8.746	113	538450	19.455	ng/u1	-0.01
21) Nitrobenzene-d5	9.240	128	255010	21.089	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.957	143	256053	22.294	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.481	165	476055	21.062	ng/u1	-0.01
31) 4-Chloroaniline-d4	11.028	131	758753	19.565	ng/u1	-0.01
46) Dimethylphthalate-d6	14.104	166	1536104	20.084	ng/u1	0.00
49) Acenaphthylene-d8	14.393	160	1779687	20.615	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.898	143	296167	19.008	ng/u1	0.00
60) Fluorene-d10	15.692	176	1284936	19.706	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.810	200	213652	19.437	ng/u1	0.00
73) Anthracene-d10	17.563	188	1988246	19.894	ng/u1	0.00
81) Pyrene-d10	19.798	212	2288124	21.837	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.974	264	1943888	19.965	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.423	88	85598	7.835	ng/uL	98
5) Pyridine	3.840	79	605468	19.304	ng/u1	99
6) Benzaldehyde	7.193	77	440880	22.977	ng/u1	99
8) Phenol	7.211	94	696923	18.733	ng/u1	97
10) Bis(2-Chloroethyl)ether	7.469	93	580241	19.308	ng/u1	95
12) 2-Chlorophenol	7.593	128	514403	19.555	ng/u1	99
13) 2-Methylphenol	8.475	108	521132	19.284	ng/u1	99
14) 2,2'-oxybis(1-Chloropr...	8.552	45	481853	11.504	ng/u1	99
16) Acetophenone	8.887	105	884772	19.796	ng/u1	98
17) N-Nitroso-di-n-propyla...	8.863	70	496910	20.730	ng/u1	99
18) 4-Methylphenol	8.810	108	574344	19.338	ng/u1	97
19) Hexachloroethane	9.116	117	211001	19.199	ng/u1	99
22) Nitrobenzene	9.281	77	703767	20.790	ng/u1	99
23) Isophorone	9.799	82	1355327	21.198	ng/u1	100
25) 2-Nitrophenol	9.987	139	291357	22.190	ng/u1	99
26) 2,4-Dimethylphenol	10.022	107	627838	20.283	ng/u1	99
27) Bis(2-Chloroethoxy)met...	10.281	93	827524	20.191	ng/u1	99
29) 2,4-Dichlorophenol	10.505	162	484498	20.834	ng/u1	99
30) Naphthalene	10.928	128	1749207	19.481	ng/u1	100
32) 4-Chloroaniline	11.052	127	746645	19.439	ng/u1	99
33) Hexachlorobutadiene	11.157	225	280628	20.019	ng/u1	99
34) Caprolactam	11.869	113	179267	19.815	ng/u1	95
35) 4-Chloro-3-methylphenol	12.146	107	588723	20.711	ng/u1	99
36) 2-Methylnaphthalene	12.522	142	1192456	19.826	ng/u1	99

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082223\
 Data File : BP016694.D
 Acq On : 22 Aug 2023 09:11
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020697

Quant Time: Aug 23 00:42:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 17 01:38:34 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.746	142	1204179	19.884	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.875	216	568275	20.092	ng/ul	99
40) Hexachlorocyclopentadiene	12.822	237	355764	20.673	ng/ul	99
41) 2,4,6-Trichlorophenol	13.122	196	382766	21.745	ng/ul	97
42) 2,4,5-Trichlorophenol	13.193	196	413228	21.657	ng/ul	100
43) 1,1'-Biphenyl	13.528	154	1550136	19.721	ng/ul	99
44) 2-Chloronaphthalene	13.575	162	1211713	19.813	ng/ul	99
45) 2-Nitroaniline	13.804	65	409887	22.166	ng/ul	99
47) Dimethylphthalate	14.151	163	1546452	19.775	ng/ul	99
48) 2,6-Dinitrotoluene	14.293	165	297025	21.928	ng/ul	96
50) Acenaphthylene	14.428	152	2035436	20.020	ng/ul	99
51) 3-Nitroaniline	14.634	138	322062	21.206	ng/ul	94
52) Acenaphthene	14.763	153	1324542	19.462	ng/ul	98
53) 2,4-Dinitrophenol	14.828	184	197319	26.168	ng/ul	97
55) 4-Nitrophenol	14.916	109	242325	19.131	ng/ul	98
56) Dibenzofuran	15.098	168	1804334	19.432	ng/ul	100
57) 2,4-Dinitrotoluene	15.075	165	443228	21.851	ng/ul	95
58) 2,3,4,6-Tetrachlorophenol	15.310	232	341210	21.343	ng/ul	96
59) Diethylphthalate	15.510	149	1574321	19.690	ng/ul	99
61) Fluorene	15.745	166	1490857	19.581	ng/ul	100
62) 4-Chlorophenyl-phenyle...	15.740	204	700812	19.608	ng/ul	97
63) 4-Nitroaniline	15.804	138	311882	21.458	ng/ul	95
66) 4,6-Dinitro-2-methylph...	15.828	198	239573	19.657	ng/ul	96
67) N-Nitrosodiphenylamine	15.963	169	1257138	20.072	ng/ul	100
68) 4-Bromophenyl-phenylether	16.639	248	415751	20.153	ng/ul	97
69) Hexachlorobenzene	16.722	284	471827	19.574	ng/ul	96
70) Atrazine	16.916	200	455320	20.207	ng/ul	99
71) Pentachlorophenol	17.087	266	294302	19.830	ng/ul	98
72) Phenanthrene	17.504	178	2359278	19.381	ng/ul	99
74) Anthracene	17.598	178	2388069	19.531	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.481	216	602346	20.513	ng/ul	97
76) Pentachlorobenzene	14.987	250	531043	20.156	ng/ul	99
77) Carbazole	17.881	167	2214288	19.651	ng/ul	99
78) Di-n-butylphthalate	18.392	149	2742363	21.024	ng/ul	100
80) Fluoranthene	19.469	202	2730918	21.837	ng/ul	100
82) Pyrene	19.828	202	2826031	21.400	ng/ul	98
83) Butylbenzylphthalate	20.680	149	1256300	23.616	ng/ul	98
84) 3,3'-Dichlorobenzidine	21.480	252	820077	18.833	ng/ul	98
85) Benzo(a)anthracene	21.545	228	2687558	19.998	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.422	149	1837172	23.796	ng/ul	99
87) Chrysene	21.604	228	2466661	19.614	ng/ul	99
89) Di-n-octyl phthalate	22.404	149	3028896	23.892	ng/ul	100
90) Benzo(b)fluoranthene	23.339	252	2401840	19.854	ng/ul	99
91) Benzo(k)fluoranthene	23.392	252	2456014	20.465	ng/ul	99
93) Benzo(a)pyrene	24.027	252	2222382	19.475	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.886	276	2343072	17.397	ng/ul	100
95) Dibenzo(a,h)anthracene	26.915	278	1952431	17.419	ng/ul	99
96) Benzo(g,h,i)perylene	27.745	276	1814305	16.926	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082223\
Data File : BP016694.D
Acq On : 22 Aug 2023 09:11
Operator : MA/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SSTD020697

Quant Time: Aug 23 00:42:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 17 01:38:34 2023
Response via : Initial Calibration




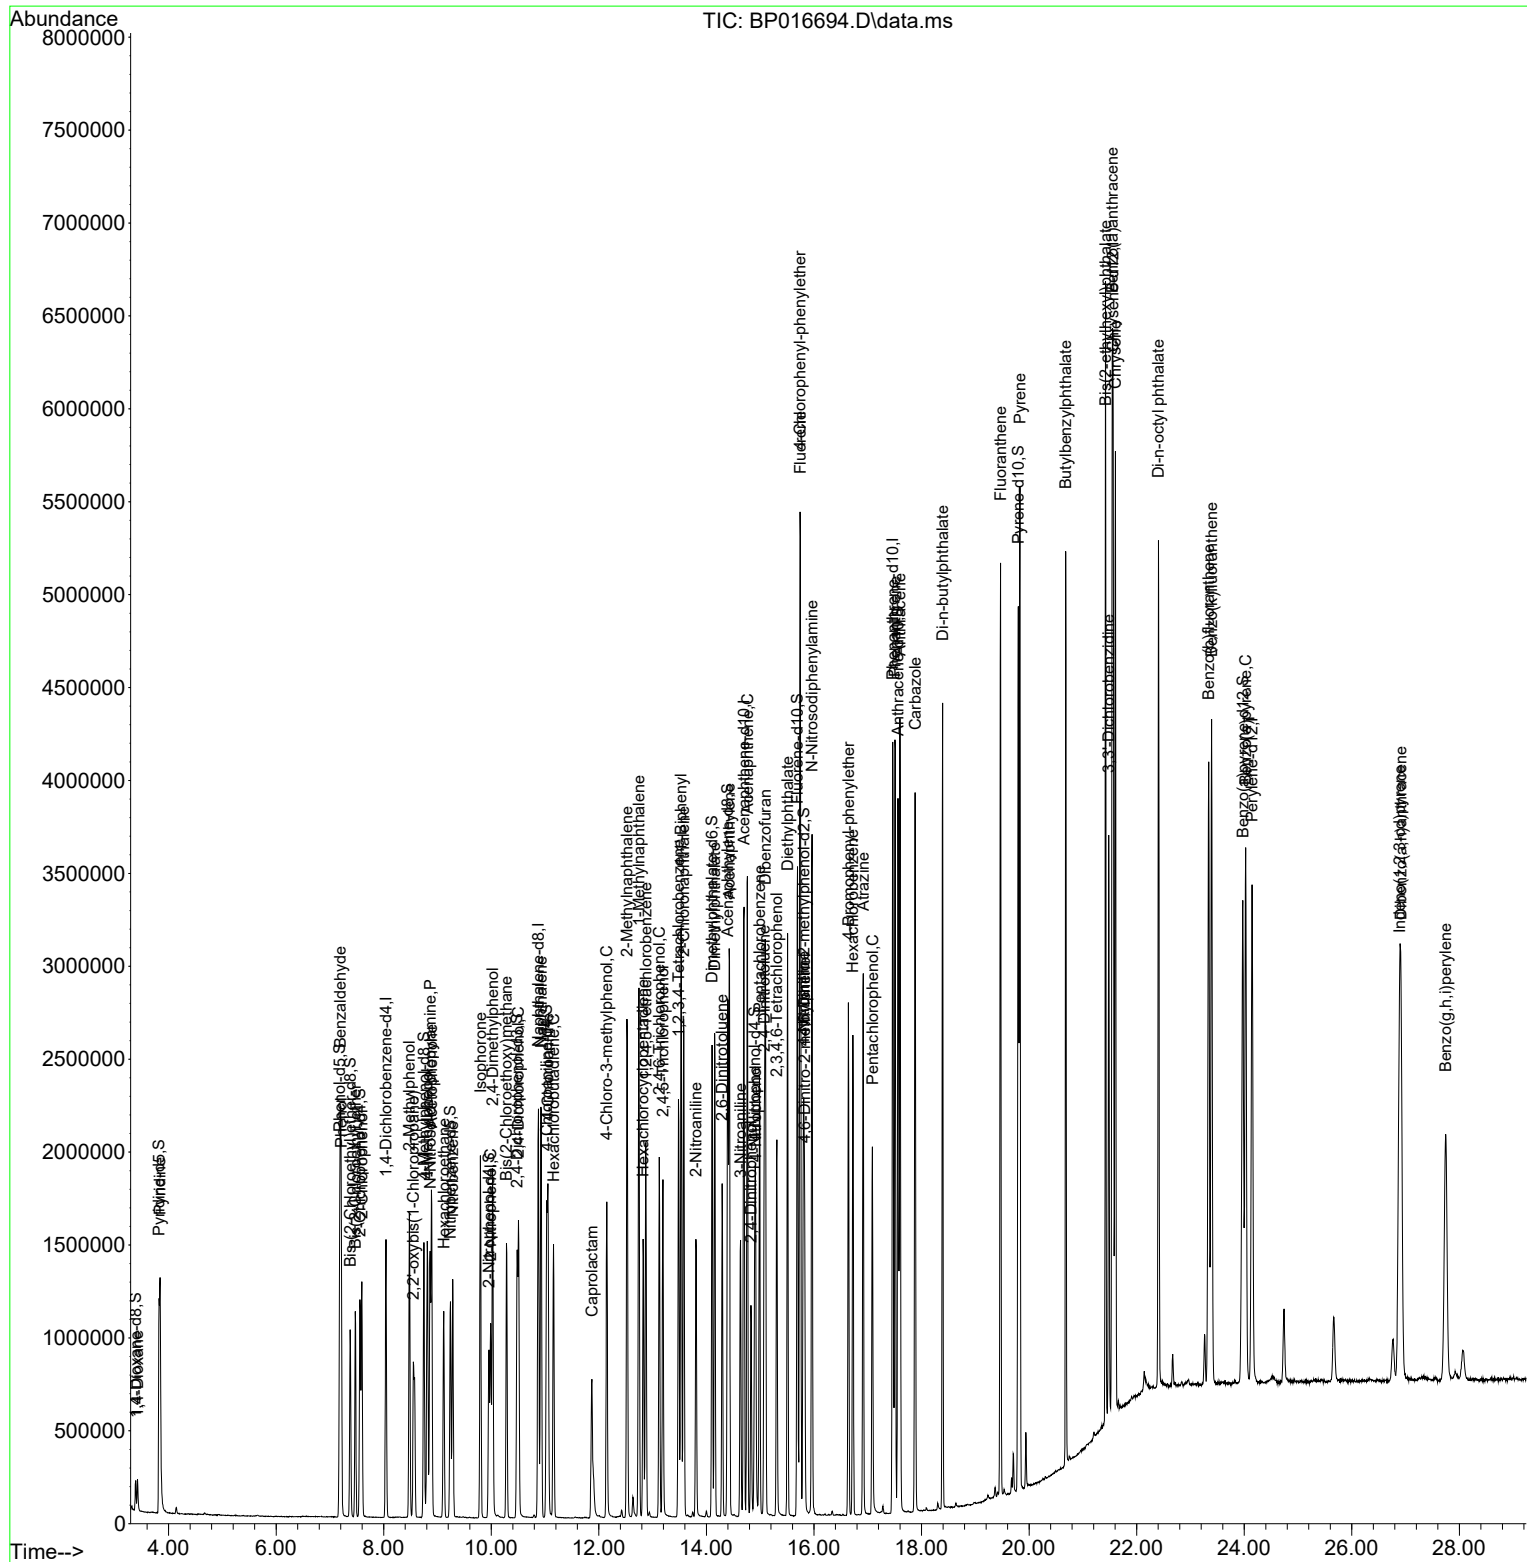


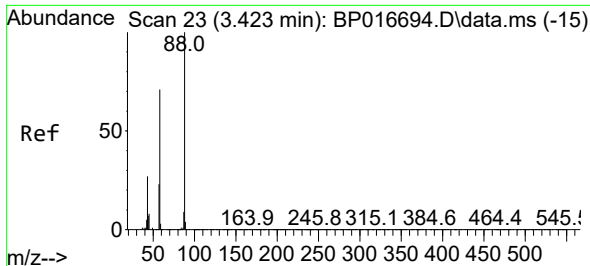

#2
1,4-Dioxane
Concen: 7.835 ng/uL
RT: 3.423 min Scan# 21
Delta R.T. -0.006 min
Lab File: BP016694.D
Acq: 22 Aug 2023 09:11




Instrument :
BNA_P
ClientSampleId :
SSTD020697


Tgt Ion: 88 Resp: 85598
Ion Ratio Lower Upper
88 100
43 27.7 23.5 35.3
58 69.9 57.1 85.7

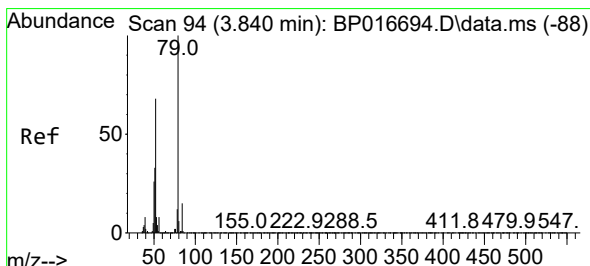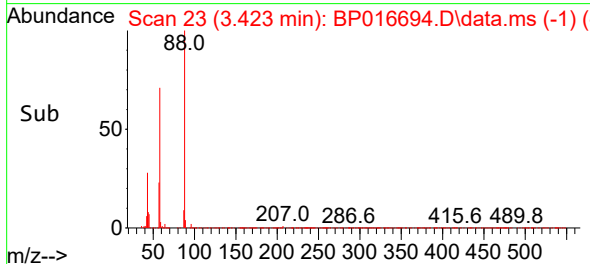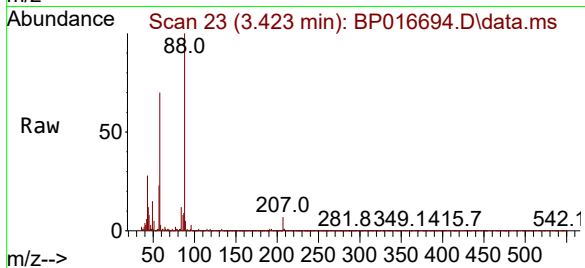

#5
Pyridine
Concen: 19.304 ng/uL
RT: 3.840 min Scan# 94
Delta R.T. -0.012 min
Lab File: BP016694.D
Acq: 22 Aug 2023 09:11

Tgt Ion: 79 Resp: 605468
Ion Ratio Lower Upper
79 100
52 70.3 56.6 84.8
51 33.3 26.9 40.3


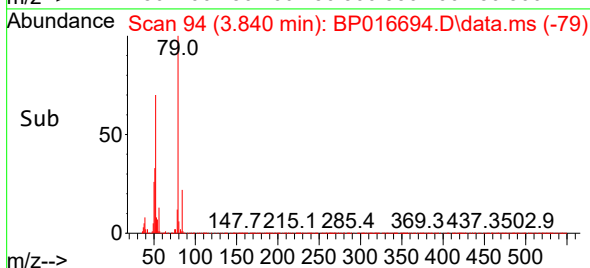

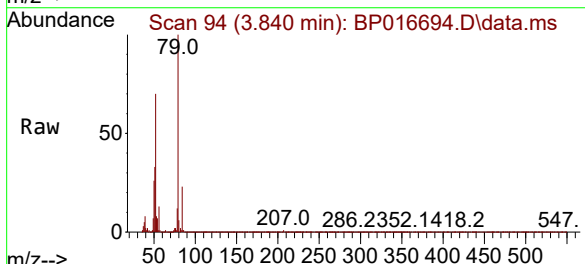




#6
Benzaldehyde
Concen: 22.977 ng/ul
RT: 7.193 min Scan# 664
Delta R.T. -0.012 min
Lab File: BP016694.D
Acq: 22 Aug 2023 09:11




Instrument :
BNA_P
ClientSampleId :
SSTD020697


Tgt Ion: 77 Resp: 440880
Ion Ratio Lower Upper
77 100
105 90.9 71.8 107.6
106 87.5 70.2 105.2



#8
Phenol
Concen: 18.733 ng/ul
RT: 7.211 min Scan# 667
Delta R.T. -0.012 min
Lab File: BP016694.D
Acq: 22 Aug 2023 09:11

Tgt Ion: 94 Resp: 696923
Ion Ratio Lower Upper
94 100
65 28.9 22.3 33.5
66 37.8 28.7 43.1



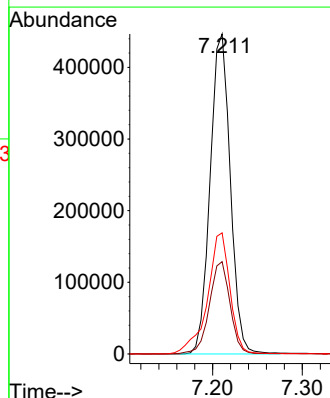





#10
 Bis(2-Chloroethyl)ether
 Concen: 19.308 ng/ul
 RT: 7.469 min Scan# 711
 Delta R.T. -0.012 min
 Lab File: BP016694.D
 Acq: 22 Aug 2023 09:11




Instrument :
 BNA_P
 ClientSampleId :
 SSTD020697


Tgt Ion: 93 Resp: 580241
 Ion Ratio Lower Upper
 93 100
 63 80.0 60.1 90.1
 95 33.1 25.4 38.2



#12
 2-Chlorophenol
 Concen: 19.555 ng/ul
 RT: 7.593 min Scan# 732
 Delta R.T. -0.012 min
 Lab File: BP016694.D
 Acq: 22 Aug 2023 09:11

Tgt Ion:128 Resp: 514403
 Ion Ratio Lower Upper
 128 100
 64 50.6 41.4 62.0
 130 32.5 26.0 39.0





#13

2-Methylphenol

Concen: 19.284 ng/ul

RT: 8.475 min Scan# 882

Delta R.T. -0.012 min

Lab File: BP016694.D

Acq: 22 Aug 2023 09:11

Instrument :

BNA_P

ClientSampleId :





SSTD020697

Tgt Ion:108 Resp: 521132

Ion Ratio Lower Upper

108 100

107 89.3 70.5 105.7



#14

2,2'-oxybis(1-Chloropropane)

Concen: 11.504 ng/ul

RT: 8.552 min Scan# 895

Delta R.T. -0.018 min

Lab File: BP016694.D

Acq: 22 Aug 2023 09:11




Tgt Ion: 45 Resp: 481853


Ion Ratio Lower Upper

45 100

77 15.0 12.1 18.1

79 10.9 8.2 12.4









#16
Acetophenone
Concen: 19.796 ng/ul
RT: 8.887 min Scan# 912
Delta R.T. -0.012 min
Lab File: BP016694.D
Acq: 22 Aug 2023 09:11




Instrument :
BNA_P
ClientSampleId :
SSTD020697


Tgt Ion:105 Resp: 884772
Ion Ratio Lower Upper
105 100
77 82.8 64.4 96.6
51 27.0 21.2 31.8



#17
N-Nitroso-di-n-propylamine
Concen: 20.730 ng/ul
RT: 8.863 min Scan# 948
Delta R.T. -0.006 min
Lab File: BP016694.D
Acq: 22 Aug 2023 09:11

Tgt Ion: 70 Resp: 496910
Ion Ratio Lower Upper
70 100
42 54.2 43.0 64.4
101 9.0 6.8 10.2
130 18.4 14.2 21.4



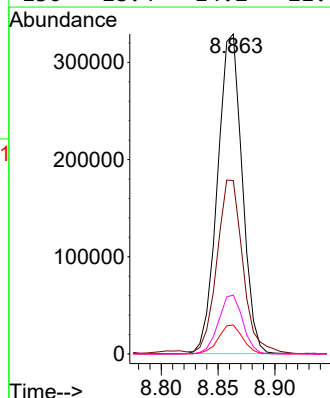





#18
4-Methylphenol
Concen: 19.338 ng/ul
RT: 8.810 min Scan# 911
Delta R.T. -0.012 min
Lab File: BP016694.D
Acq: 22 Aug 2023 09:11




Instrument :
BNA_P
ClientSampleId :
SSTD020697


Tgt Ion:108 Resp: 574344
Ion Ratio Lower Upper
108 100
107 112.5 87.3 130.9



#19
Hexachloroethane
Concen: 19.199 ng/ul
RT: 9.116 min Scan# 991
Delta R.T. -0.012 min
Lab File: BP016694.D
Acq: 22 Aug 2023 09:11

Tgt Ion:117 Resp: 211001
Ion Ratio Lower Upper
117 100
201 91.0 71.8 107.6
199 55.9 45.2 67.8









#22
Nitrobenzene
Concen: 20.790 ng/ul
RT: 9.281 min Scan# 1019
Delta R.T. -0.012 min
Lab File: BP016694.D
Acq: 22 Aug 2023 09:11




Instrument :
BNA_P
ClientSampleId :
SSTD020697


Tgt Ion: 77 Resp: 703767
Ion Ratio Lower Upper
77 100
123 40.0 32.5 48.7
65 13.2 10.3 15.5



#23
Isophorone
Concen: 21.198 ng/ul
RT: 9.799 min Scan# 1107
Delta R.T. -0.006 min
Lab File: BP016694.D
Acq: 22 Aug 2023 09:11

Tgt Ion: 82 Resp: 1355327
Ion Ratio Lower Upper
82 100
95 6.7 5.3 7.9
138 15.7 12.7 19.1


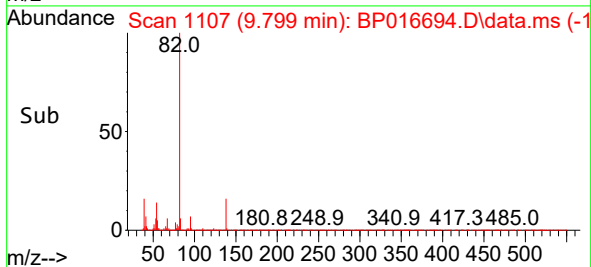

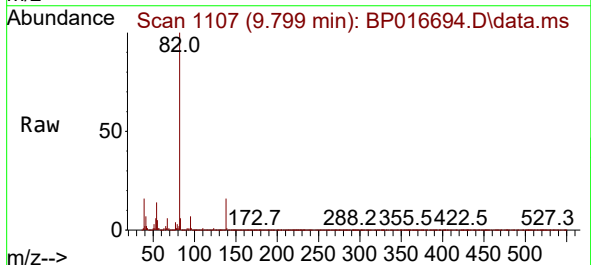




#25
2-Nitrophenol
Concen: 22.190 ng/ul
RT: 9.987 min Scan# 1139
Delta R.T. -0.012 min
Lab File: BP016694.D
Acq: 22 Aug 2023 09:11




Instrument :
BNA_P
ClientSampleId :
SSTD020697


Tgt Ion:139 Resp: 291357
Ion Ratio Lower Upper
139 100
65 58.9 46.4 69.6
109 32.2 25.3 37.9



#26
2,4-Dimethylphenol
Concen: 20.283 ng/ul
RT: 10.022 min Scan# 1145
Delta R.T. -0.012 min
Lab File: BP016694.D
Acq: 22 Aug 2023 09:11

Tgt Ion:107 Resp: 627838
Ion Ratio Lower Upper
107 100
121 49.3 39.1 58.7
122 84.3 66.9 100.3









#27
 Bis(2-Chloroethoxy)methane
 Concen: 20.191 ng/ul
 RT: 10.281 min Scan# 1189
 Delta R.T. -0.012 min
 Lab File: BP016694.D
 Acq: 22 Aug 2023 09:11




Instrument :
 BNA_P
 ClientSampleId :
 SSTD020697


Tgt Ion: 93 Resp: 827524
 Ion Ratio Lower Upper
 93 100
 95 31.8 25.8 38.8
 123 10.2 8.7 13.1



#29
 2,4-Dichlorophenol
 Concen: 20.834 ng/ul
 RT: 10.505 min Scan# 1227
 Delta R.T. -0.012 min
 Lab File: BP016694.D
 Acq: 22 Aug 2023 09:11

Tgt Ion: 162 Resp: 484498
 Ion Ratio Lower Upper
 162 100
 164 64.6 52.9 79.3
 98 41.0 32.7 49.1









#30
Naphthalene
Concen: 19.481 ng/ul
RT: 10.928 min Scan# 1299
Delta R.T. -0.006 min
Lab File: BP016694.D
Acq: 22 Aug 2023 09:11




Instrument :
BNA_P
ClientSampleId :
SSTD020697


Tgt Ion:128 Resp: 1749207
Ion Ratio Lower Upper
128 100
129 10.8 8.6 13.0
127 13.2 10.3 15.5



#32
4-Chloroaniline
Concen: 19.439 ng/ul
RT: 11.052 min Scan# 1320
Delta R.T. -0.012 min
Lab File: BP016694.D
Acq: 22 Aug 2023 09:11

Tgt Ion:127 Resp: 746645
Ion Ratio Lower Upper
127 100
129 32.8 25.6 38.4





#33

Hexachlorobutadiene

Concen: 20.019 ng/ul

RT: 11.157 min Scan# 11

Delta R.T. -0.012 min

Lab File: BP016694.D

Acq: 22 Aug 2023 09:11

Instrument :

BNA_P

ClientSampleId :

SSTD020697





Tgt Ion:225 Resp: 280628

Ion Ratio Lower Upper

225 100

223 63.0 50.2 75.2

227 64.7 50.8 76.2

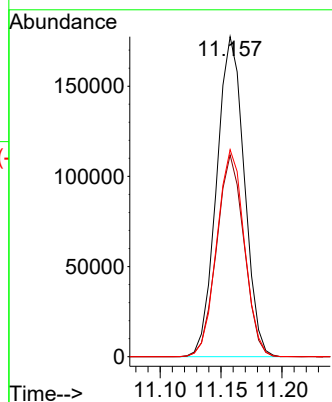

#34

Caprolactam

Concen: 19.815 ng/ul

RT: 11.869 min Scan# 1459

Delta R.T. -0.000 min

Lab File: BP016694.D

Acq: 22 Aug 2023 09:11




Tgt Ion:113 Resp: 179267


Ion Ratio Lower Upper

113 100

55 178.5 134.8 202.2

56 130.1 101.5 152.3









#35
4-Chloro-3-methylphenol
Concen: 20.711 ng/ul
RT: 12.146 min Scan# 1506
Delta R.T. -0.012 min
Lab File: BP016694.D
Acq: 22 Aug 2023 09:11




Instrument :
BNA_P
ClientSampleId :
SSTD020697


Tgt Ion:107 Resp: 588723
Ion Ratio Lower Upper
107 100
144 24.9 19.0 28.6
142 74.8 60.2 90.4

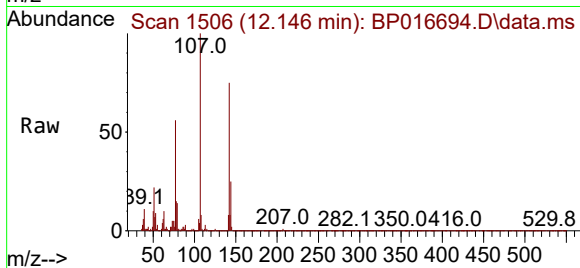

#36
2-Methylnaphthalene
Concen: 19.826 ng/ul
RT: 12.522 min Scan# 1570
Delta R.T. -0.012 min
Lab File: BP016694.D
Acq: 22 Aug 2023 09:11

Tgt Ion:142 Resp: 1192456
Ion Ratio Lower Upper
142 100
141 88.4 71.4 107.0

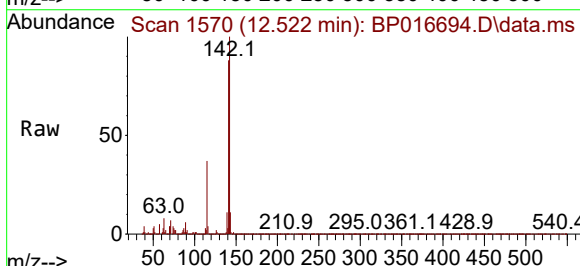



#37

1-Methylnaphthalene

Concen: 19.884 ng/ul

RT: 12.746 min Scan# 1608

Delta R.T. -0.006 min

Lab File: BP016694.D

Acq: 22 Aug 2023 09:11

Instrument :

BNA_P

ClientSampleId :

SSTD020697





Tgt Ion:142 Resp: 1204179

Ion Ratio Lower Upper

142 100

141 93.8 74.5 111.7

116 3.9 3.0 4.4



#39

1,2,4,5-Tetrachlorobenzene

Concen: 20.092 ng/ul

RT: 12.875 min Scan# 1630

Delta R.T. -0.006 min

Lab File: BP016694.D

Acq: 22 Aug 2023 09:11

Tgt Ion:216 Resp: 568275




Ion Ratio Lower Upper


216 100

214 78.7 63.8 95.6

179 22.5 17.9 26.9

108 20.7 16.3 24.5


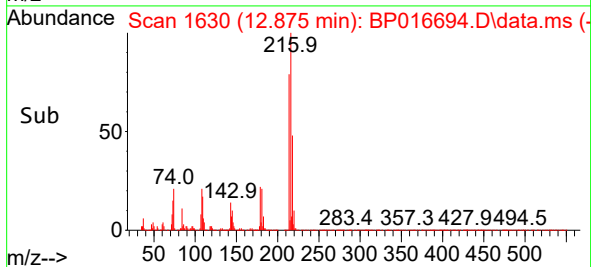
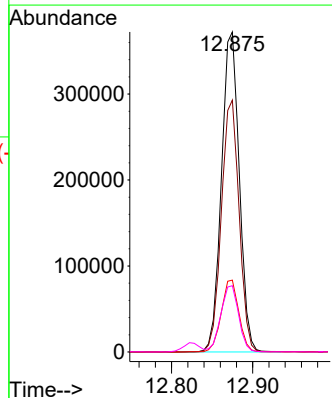
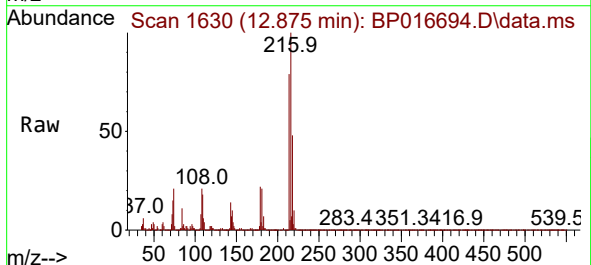




#40
Hexachlorocyclopentadiene
Concen: 20.673 ng/ul
RT: 12.822 min Scan# 1621
Delta R.T. -0.012 min
Lab File: BP016694.D
Acq: 22 Aug 2023 09:11




Instrument :
BNA_P
ClientSampleId :
SSTD020697


Tgt Ion:237 Resp: 355764
Ion Ratio Lower Upper
237 100
235 63.2 49.7 74.5
272 11.8 9.8 14.8



#41
2,4,6-Trichlorophenol
Concen: 21.745 ng/ul
RT: 13.122 min Scan# 1672
Delta R.T. -0.012 min
Lab File: BP016694.D
Acq: 22 Aug 2023 09:11

Tgt Ion:196 Resp: 382766
Ion Ratio Lower Upper
196 100
198 92.7 77.0 115.4
200 31.0 24.9 37.3









#42
2,4,5-Trichlorophenol
Concen: 21.657 ng/ul
RT: 13.193 min Scan# 1
Delta R.T. -0.006 min
Lab File: BP016694.D
Acq: 22 Aug 2023 09:11




Instrument :
BNA_P
ClientSampleId :
SSTD020697


Tgt Ion:196 Resp: 413228
Ion Ratio Lower Upper
196 100
198 95.5 76.7 115.1
200 30.1 24.2 36.2



#43
1,1'-Biphenyl
Concen: 19.721 ng/ul
RT: 13.528 min Scan# 1741
Delta R.T. -0.012 min
Lab File: BP016694.D
Acq: 22 Aug 2023 09:11

Tgt Ion:154 Resp: 1550136
Ion Ratio Lower Upper
154 100
153 39.9 31.4 47.2
76 16.6 13.0 19.4









#44
2-Chloronaphthalene
Concen: 19.813 ng/ul
RT: 13.575 min Scan# 1749
Delta R.T. -0.012 min
Lab File: BP016694.D
Acq: 22 Aug 2023 09:11




Instrument :
BNA_P
ClientSampleId :
SSTD020697


Tgt Ion:162 Resp: 1211713
Ion Ratio Lower Upper
162 100
164 31.9 25.8 38.6
127 40.7 32.9 49.3

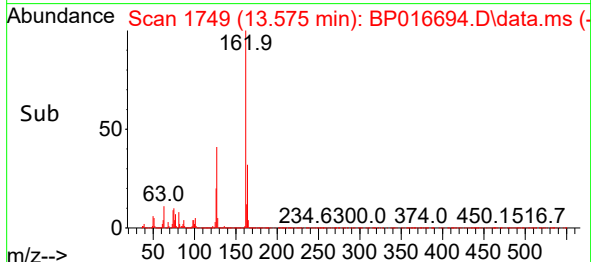

#45
2-Nitroaniline
Concen: 22.166 ng/ul
RT: 13.804 min Scan# 1788
Delta R.T. -0.006 min
Lab File: BP016694.D
Acq: 22 Aug 2023 09:11

Tgt Ion: 65 Resp: 409887
Ion Ratio Lower Upper
65 100
92 66.3 54.5 81.7
138 90.9 72.1 108.1









#47
Dimethylphthalate
Concen: 19.775 ng/ul
RT: 14.151 min Scan# 1847
Delta R.T. -0.006 min
Lab File: BP016694.D
Acq: 22 Aug 2023 09:11




Instrument :
BNA_P
ClientSampleId :
SSTD020697


Tgt Ion:163 Resp: 1546452
Ion Ratio Lower Upper
163 100
194 3.8 3.0 4.6
164 10.1 7.8 11.8



#48
2,6-Dinitrotoluene
Concen: 21.928 ng/ul
RT: 14.293 min Scan# 1871
Delta R.T. -0.006 min
Lab File: BP016694.D
Acq: 22 Aug 2023 09:11

Tgt Ion:165 Resp: 297025
Ion Ratio Lower Upper
165 100
89 70.0 53.2 79.8
121 23.0 18.8 28.2



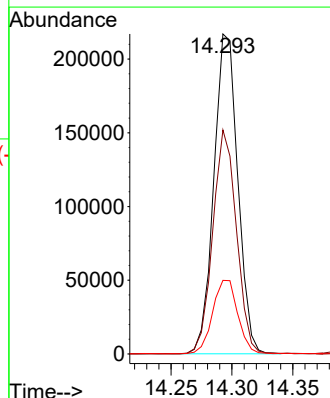



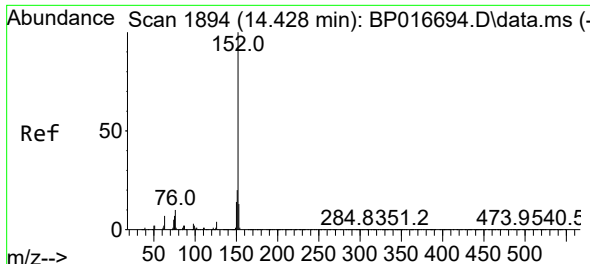

#50
Acenaphthylene
Concen: 20.020 ng/ul
RT: 14.428 min Scan# 1894
Delta R.T. -0.006 min
Lab File: BP016694.D
Acq: 22 Aug 2023 09:11




Instrument :
BNA_P
ClientSampleId :
SSTD020697


Tgt Ion:152 Resp: 2035436
Ion Ratio Lower Upper
152 100
151 20.1 15.7 23.5
153 12.9 10.6 15.8

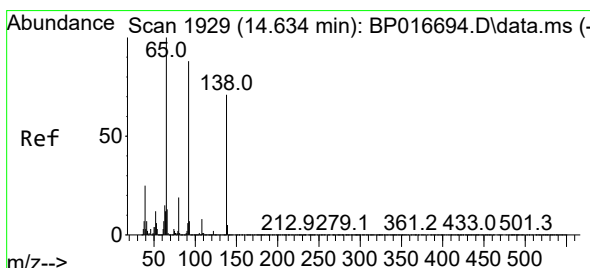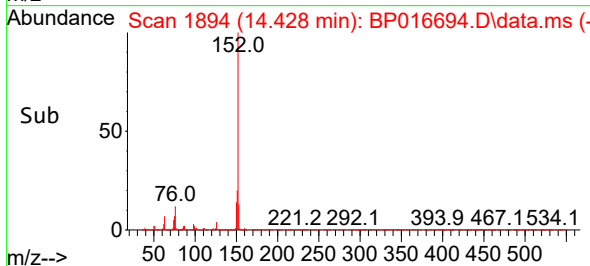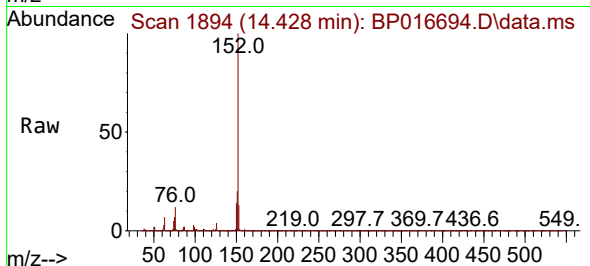

#51
3-Nitroaniline
Concen: 21.206 ng/ul
RT: 14.634 min Scan# 1929
Delta R.T. -0.000 min
Lab File: BP016694.D
Acq: 22 Aug 2023 09:11

Tgt Ion:138 Resp: 322062
Ion Ratio Lower Upper
138 100
108 11.6 10.9 16.3
92 124.2 105.0 157.6


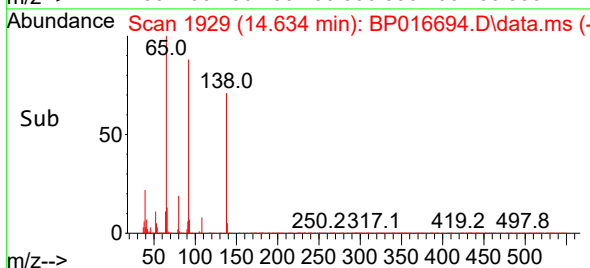
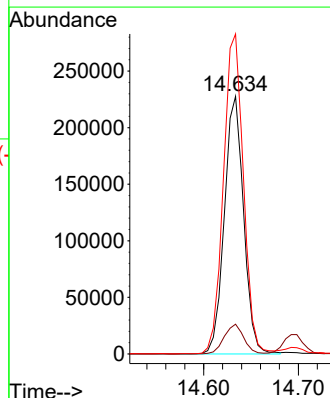
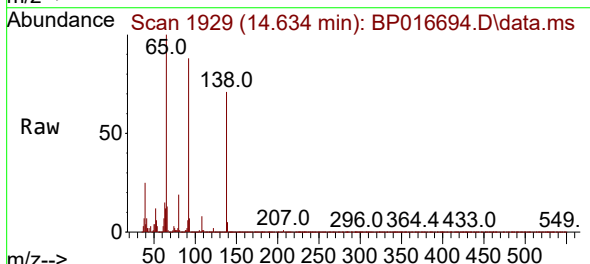




#52
Acenaphthene
Concen: 19.462 ng/ul
RT: 14.763 min Scan# 1951
Delta R.T. -0.006 min
Lab File: BP016694.D
Acq: 22 Aug 2023 09:11




Instrument :
BNA_P
ClientSampleId :
SSTD020697


Tgt Ion:153 Resp: 1324542
Ion Ratio Lower Upper
153 100
152 48.2 38.7 58.1
154 87.7 72.0 108.0

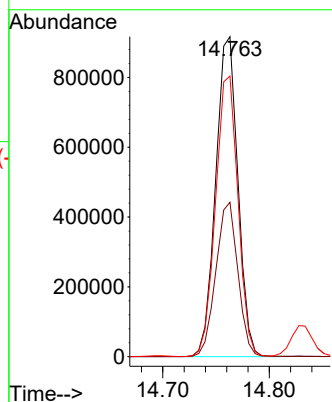

#53
2,4-Dinitrophenol
Concen: 26.168 ng/ul
RT: 14.828 min Scan# 1962
Delta R.T. -0.006 min
Lab File: BP016694.D
Acq: 22 Aug 2023 09:11

Tgt Ion:184 Resp: 197319
Ion Ratio Lower Upper
184 100
63 82.1 65.0 97.6
154 65.6 56.2 84.2


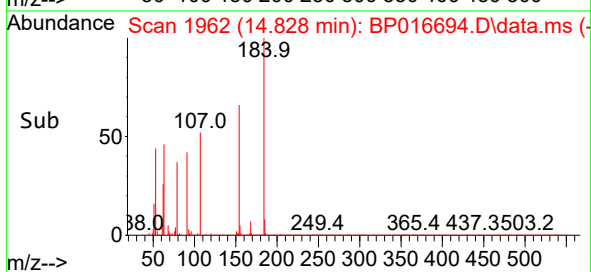
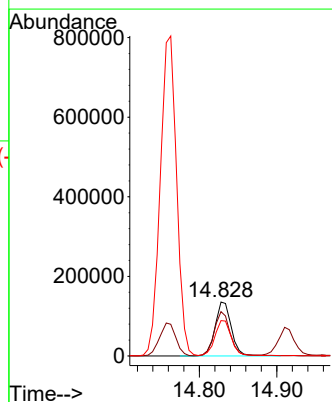





#55
4-Nitrophenol
Concen: 19.131 ng/ul
RT: 14.916 min Scan# 1977
Delta R.T. -0.000 min
Lab File: BP016694.D
Acq: 22 Aug 2023 09:11




Instrument :
BNA_P
ClientSampleId :
SSTD020697


Tgt Ion:109 Resp: 242325
Ion Ratio Lower Upper
109 100
139 128.6 101.1 151.7
65 138.6 108.9 163.3



#56
Dibenzofuran
Concen: 19.432 ng/ul
RT: 15.098 min Scan# 2008
Delta R.T. -0.006 min
Lab File: BP016694.D
Acq: 22 Aug 2023 09:11

Tgt Ion:168 Resp: 1804334
Ion Ratio Lower Upper
168 100
139 39.0 31.4 47.0









#57
2,4-Dinitrotoluene
Concen: 21.851 ng/ul
RT: 15.075 min Scan# 2004
Delta R.T. -0.006 min
Lab File: BP016694.D
Acq: 22 Aug 2023 09:11




Instrument :
BNA_P
ClientSampleId :
SSTD020697


Tgt Ion:165 Resp: 443228
Ion Ratio Lower Upper
165 100
63 54.2 40.4 60.6
182 2.5 1.9 2.9

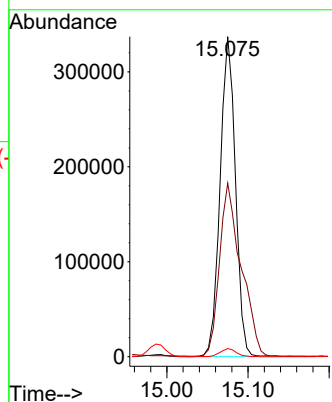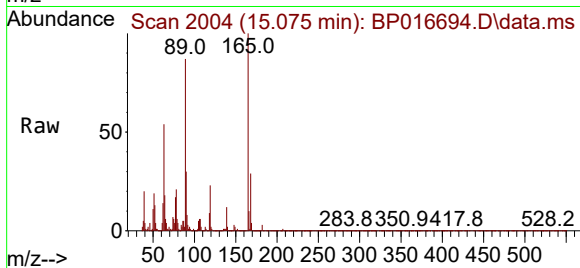

#58
2,3,4,6-Tetrachlorophenol
Concen: 21.343 ng/ul
RT: 15.310 min Scan# 2044
Delta R.T. -0.006 min
Lab File: BP016694.D
Acq: 22 Aug 2023 09:11

Tgt Ion:232 Resp: 341210
Ion Ratio Lower Upper
232 100
131 49.3 42.9 64.3
130 2.7 2.2 3.4
166 33.0 26.7 40.1


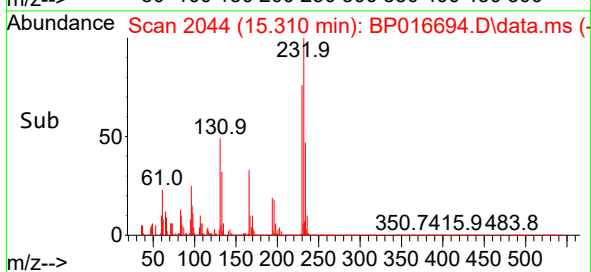






#59
Diethylphthalate
Concen: 19.690 ng/ul
RT: 15.510 min Scan# 2078
Delta R.T. -0.006 min
Lab File: BP016694.D
Acq: 22 Aug 2023 09:11




Instrument :
BNA_P
ClientSampleId :
SSTD020697


Tgt Ion:149 Resp: 1574321
Ion Ratio Lower Upper
149 100
177 21.0 16.5 24.7
150 12.6 10.0 15.0



#61
Fluorene
Concen: 19.581 ng/ul
RT: 15.745 min Scan# 2118
Delta R.T. -0.006 min
Lab File: BP016694.D
Acq: 22 Aug 2023 09:11

Tgt Ion:166 Resp: 1490857
Ion Ratio Lower Upper
166 100
165 97.7 78.3 117.5
167 13.5 10.8 16.2









#62
4-Chlorophenyl-phenylether
Concen: 19.608 ng/ul
RT: 15.740 min Scan# 2117
Delta R.T. -0.006 min
Lab File: BP016694.D
Acq: 22 Aug 2023 09:11




Instrument :
BNA_P
ClientSampleId :
SSTD020697


Tgt Ion:204 Resp: 700812
Ion Ratio Lower Upper
204 100
206 33.1 25.5 38.3
141 62.2 52.2 78.2

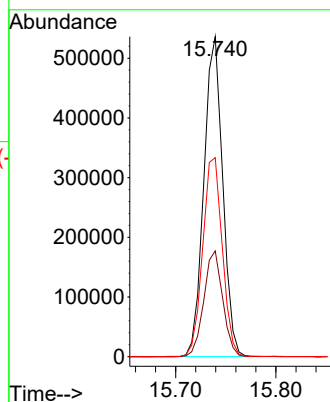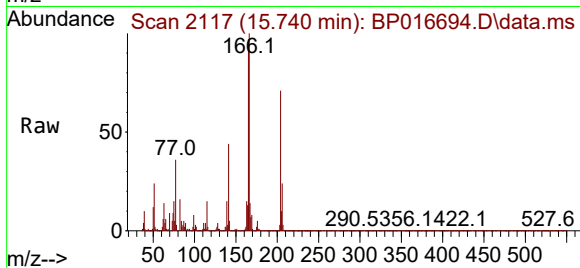

#63
4-Nitroaniline
Concen: 21.458 ng/ul
RT: 15.804 min Scan# 2128
Delta R.T. -0.000 min
Lab File: BP016694.D
Acq: 22 Aug 2023 09:11

Tgt Ion:138 Resp: 311882
Ion Ratio Lower Upper
138 100
92 55.7 46.7 70.1
108 97.1 73.7 110.5




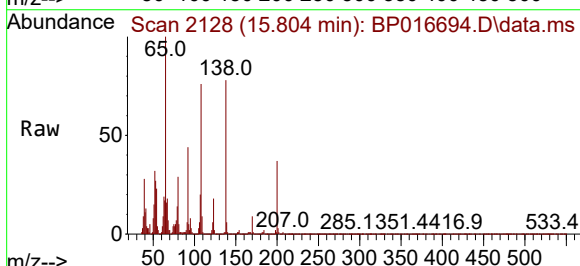




#66
4,6-Dinitro-2-methylphenol
Concen: 19.657 ng/ul
RT: 15.828 min Scan# 2132
Delta R.T. -0.000 min
Lab File: BP016694.D
Acq: 22 Aug 2023 09:11




Instrument :
BNA_P
ClientSampleId :
SSTD020697


Tgt Ion:198 Resp: 239573
Ion Ratio Lower Upper
198 100
182 4.3 3.9 5.9
77 30.0 25.8 38.6



#67
N-Nitrosodiphenylamine
Concen: 20.072 ng/ul
RT: 15.963 min Scan# 2155
Delta R.T. -0.000 min
Lab File: BP016694.D
Acq: 22 Aug 2023 09:11

Tgt Ion:169 Resp: 1257138
Ion Ratio Lower Upper
169 100
168 66.9 53.9 80.9
167 36.2 29.0 43.6









#68
4-Bromophenyl-phenylether
Concen: 20.153 ng/ul
RT: 16.639 min Scan# 21
Delta R.T. -0.006 min
Lab File: BP016694.D
Acq: 22 Aug 2023 09:11




Instrument :
BNA_P
ClientSampleId :
SSTD020697


Tgt Ion:248 Resp: 415751
Ion Ratio Lower Upper
248 100
250 99.7 76.9 115.3
141 86.3 67.6 101.4



#69
Hexachlorobenzene
Concen: 19.574 ng/ul
RT: 16.722 min Scan# 2284
Delta R.T. -0.006 min
Lab File: BP016694.D
Acq: 22 Aug 2023 09:11

Tgt Ion:284 Resp: 471827
Ion Ratio Lower Upper
284 100
142 41.9 31.9 47.9
249 33.4 24.7 37.1

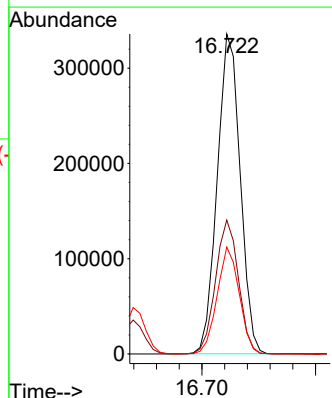



#70

Atrazine

Concen: 20.207 ng/ul

RT: 16.916 min Scan# 2317

Delta R.T. -0.000 min

Lab File: BP016694.D

Acq: 22 Aug 2023 09:11

Instrument :

BNA_P

ClientSampleId :

SSTD020697





Tgt Ion:200 Resp: 455320

Ion Ratio Lower Upper

200 100

173 27.0 22.2 33.2

215 47.7 38.4 57.6

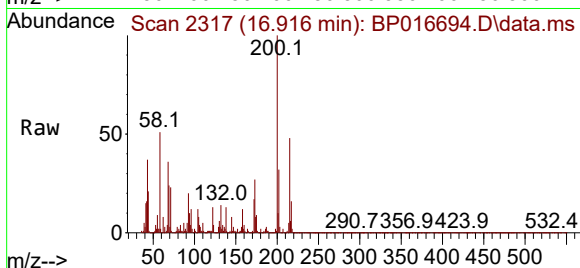

#71

Pentachlorophenol

Concen: 19.830 ng/ul

RT: 17.087 min Scan# 2346

Delta R.T. -0.006 min

Lab File: BP016694.D

Acq: 22 Aug 2023 09:11




Tgt Ion:266 Resp: 294302


Ion Ratio Lower Upper

266 100

264 63.3 50.7 76.1

268 63.9 53.0 79.6

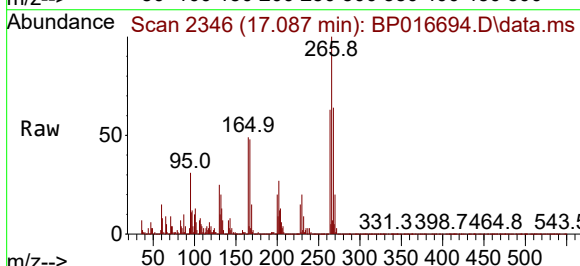

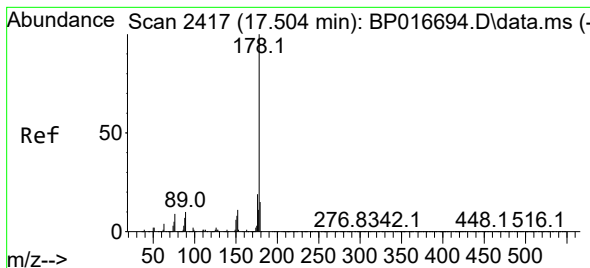

#72

Phenanthrene

Concen: 19.381 ng/ul

RT: 17.504 min Scan# 2417

Delta R.T. -0.006 min

Lab File: BP016694.D

Acq: 22 Aug 2023 09:11

Instrument :

BNA_P

ClientSampleId :

SSTD020697





Tgt Ion:178 Resp: 2359278

Ion Ratio Lower Upper

178 100

179 15.4 12.4 18.6

176 18.9 15.5 23.3

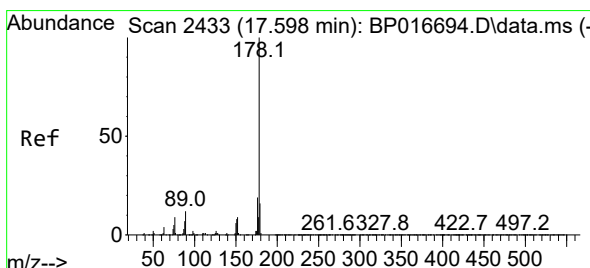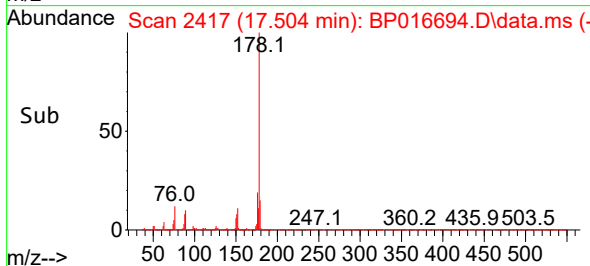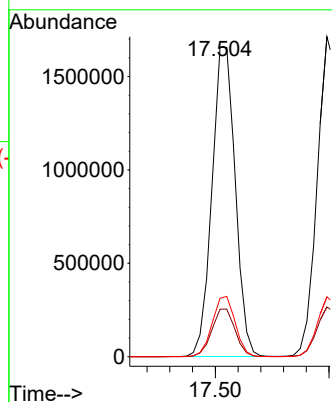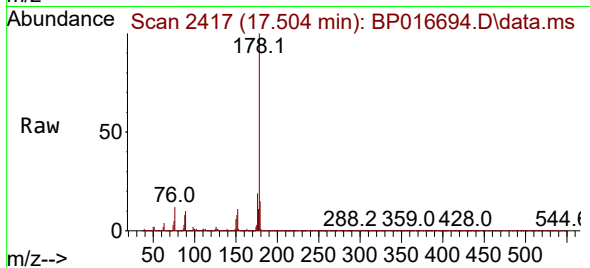

#74

Anthracene

Concen: 19.531 ng/ul

RT: 17.598 min Scan# 2433

Delta R.T. -0.006 min

Lab File: BP016694.D

Acq: 22 Aug 2023 09:11




Tgt Ion:178 Resp: 2388069


Ion Ratio Lower Upper

178 100

179 15.6 12.5 18.7

176 18.7 14.9 22.3

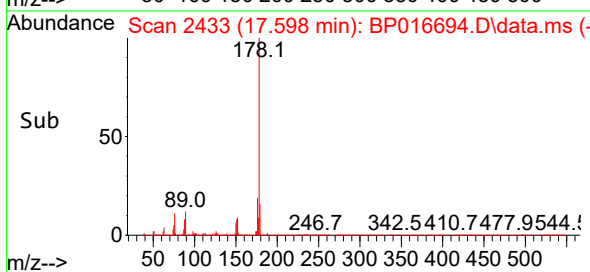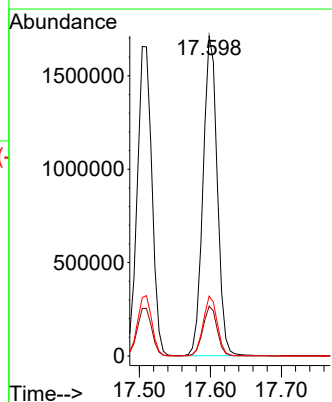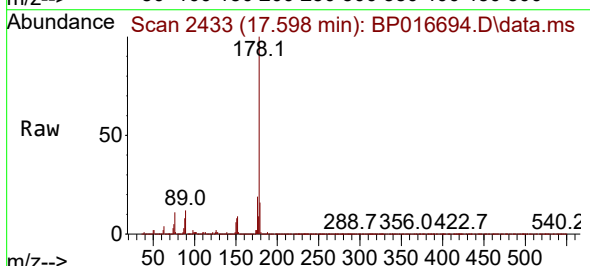



#75

1,2,3,4-Tetrachlorobenzene

Concen: 20.513 ng/uL

RT: 13.481 min Scan# 1733

Delta R.T. -0.012 min

Lab File: BP016694.D

Acq: 22 Aug 2023 09:11

Instrument :

BNA_P

ClientSampleId :

SSTD020697





Tgt Ion:216 Resp: 602346

Ion Ratio Lower Upper

216 100

214 77.9 65.4 98.2

218 47.9 39.3 58.9

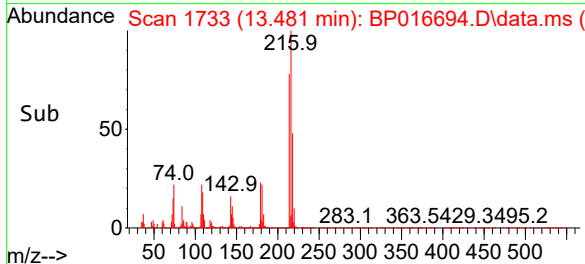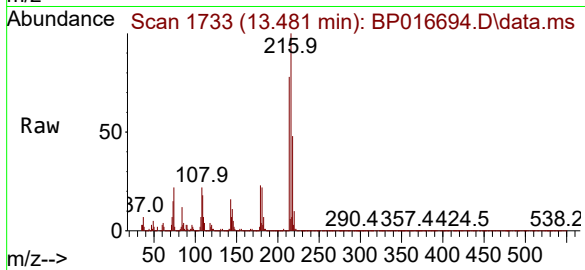

#76

Pentachlorobenzene

Concen: 20.156 ng/uL

RT: 14.987 min Scan# 1989

Delta R.T. -0.006 min

Lab File: BP016694.D

Acq: 22 Aug 2023 09:11




Tgt Ion:250 Resp: 531043


Ion Ratio Lower Upper

250 100

248 63.4 50.2 75.2

252 62.9 51.0 76.4

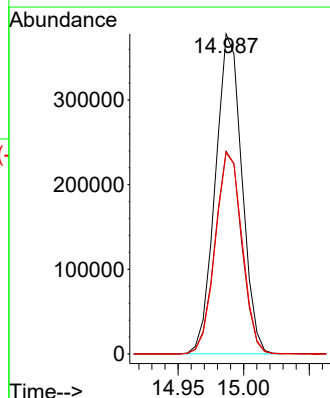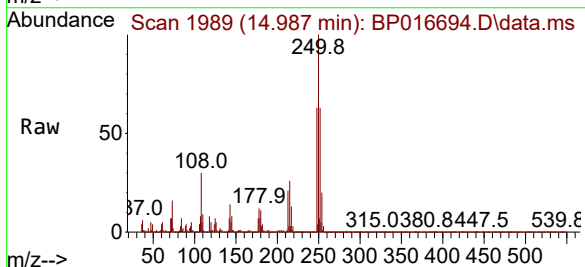



#77

Carbazole

Concen: 19.651 ng/ul

RT: 17.881 min Scan# 2481

Delta R.T. -0.000 min

Lab File: BP016694.D

Acq: 22 Aug 2023 09:11

Instrument :

BNA_P

ClientSampleId :

SSTD020697





Tgt Ion:167 Resp: 2214288

Ion Ratio Lower Upper

167 100

166 21.7 16.8 25.2

139 13.4 10.6 16.0



#78

Di-n-butylphthalate

Concen: 21.024 ng/ul

RT: 18.392 min Scan# 2568

Delta R.T. -0.000 min

Lab File: BP016694.D

Acq: 22 Aug 2023 09:11




Tgt Ion:149 Resp: 2742363


Ion Ratio Lower Upper

149 100

150 9.3 7.3 10.9

104 5.7 4.6 6.8

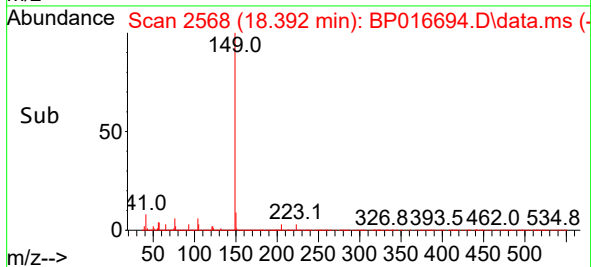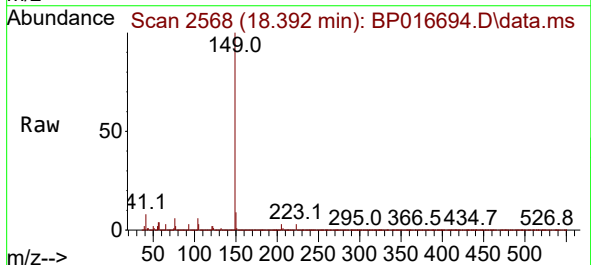



#80

Fluoranthene

Concen: 21.837 ng/ul

RT: 19.469 min Scan# 21

Delta R.T. -0.000 min

Lab File: BP016694.D

Acq: 22 Aug 2023 09:11

Instrument :

BNA_P

ClientSampleId :

SSTD020697





Tgt Ion:202 Resp: 2730918

Ion Ratio Lower Upper

202 100

101 13.4 10.6 16.0

100 10.2 8.1 12.1



#82

Pyrene

Concen: 21.400 ng/ul

RT: 19.828 min Scan# 2812

Delta R.T. -0.000 min

Lab File: BP016694.D

Acq: 22 Aug 2023 09:11




Tgt Ion:202 Resp: 2826031


Ion Ratio Lower Upper

202 100

101 15.8 13.4 20.2

100 12.9 11.0 16.4





#83

Butylbenzylphthalate

Concen: 23.616 ng/ul

RT: 20.680 min Scan# 2957

Delta R.T. -0.006 min

Lab File: BP016694.D

Acq: 22 Aug 2023 09:11

Instrument :

BNA_P

ClientSampleId :

SSTD020697





Tgt Ion:149 Resp: 1256300

Ion Ratio Lower Upper

149 100

91 82.5 67.8 101.6

206 18.3 14.4 21.6



#84

3,3'-Dichlorobenzidine

Concen: 18.833 ng/ul

RT: 21.480 min Scan# 3093

Delta R.T. -0.000 min

Lab File: BP016694.D

Acq: 22 Aug 2023 09:11




Tgt Ion:252 Resp: 820077


Ion Ratio Lower Upper

252 100

254 62.6 51.3 76.9

126 13.1 10.2 15.4





#85

Benzo(a)anthracene

Concen: 19.998 ng/ul

RT: 21.545 min Scan# 3104

Delta R.T. -0.000 min

Lab File: BP016694.D

Acq: 22 Aug 2023 09:11

Instrument :

BNA_P

ClientSampleId :

SSTD020697





Tgt Ion:228 Resp: 2687558

Ion Ratio Lower Upper

228 100

229 19.8 15.8 23.6

226 27.0 21.8 32.6

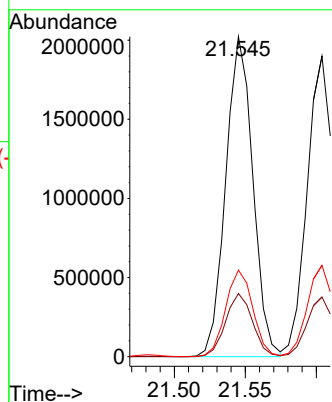

#86

Bis(2-ethylhexyl)phthalate

Concen: 23.796 ng/ul

RT: 21.422 min Scan# 3083

Delta R.T. -0.000 min

Lab File: BP016694.D

Acq: 22 Aug 2023 09:11




Tgt Ion:149 Resp: 1837172


Ion Ratio Lower Upper

149 100

167 26.4 20.9 31.3

279 3.6 2.6 4.0





#87

Chrysene

Concen: 19.614 ng/ul

RT: 21.604 min Scan# 3114

Delta R.T. -0.000 min

Lab File: BP016694.D

Acq: 22 Aug 2023 09:11

Instrument :

BNA_P

ClientSampleId :

SSTD020697





Tgt Ion:228 Resp: 2466661

Ion Ratio Lower Upper

228 100

226 30.4 24.6 36.8

229 19.9 16.4 24.6

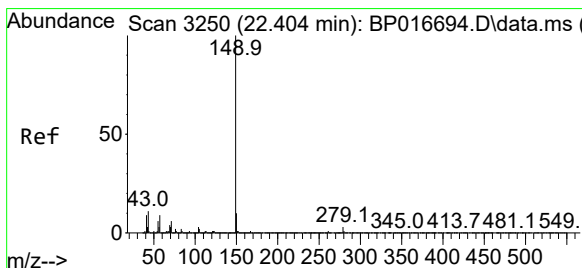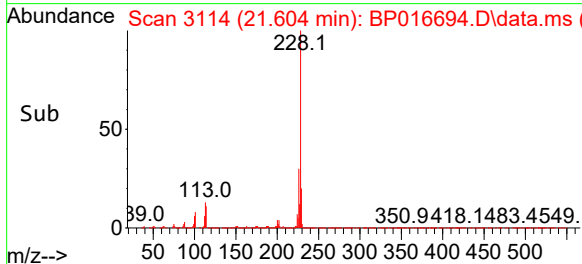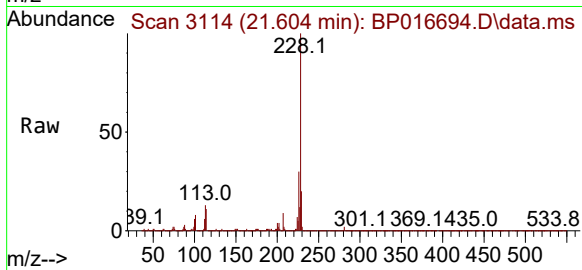

#89

Di-n-octyl phthalate

Concen: 23.892 ng/ul




RT: 22.404 min Scan# 3250


Delta R.T. -0.006 min

Lab File: BP016694.D

Acq: 22 Aug 2023 09:11

Tgt Ion:149 Resp: 3028896

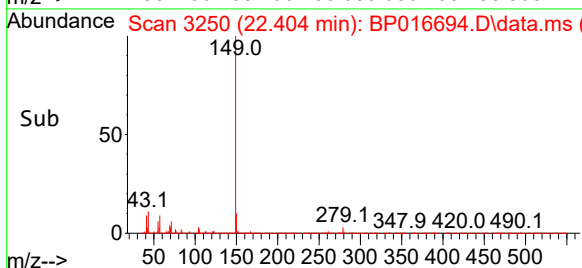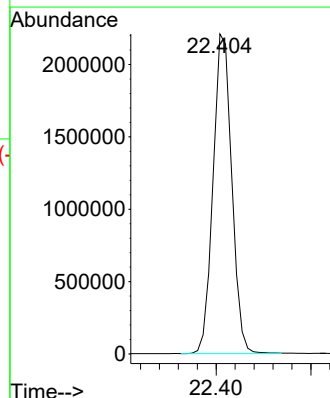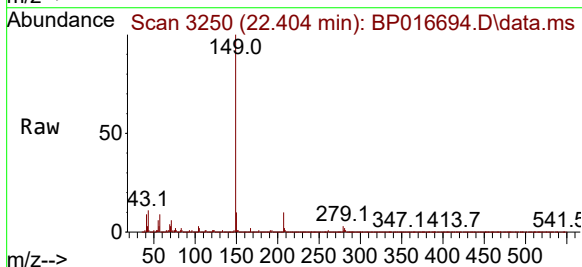



#90

Benzo(b)fluoranthene

Concen: 19.854 ng/ul

RT: 23.339 min Scan# 3409

Delta R.T. -0.000 min

Lab File: BP016694.D

Acq: 22 Aug 2023 09:11

Instrument :

BNA_P

ClientSampleId :

SSTD020697





Tgt Ion:252 Resp: 2401840

Ion Ratio Lower Upper

252 100

253 22.4 17.4 26.2

125 12.0 10.0 15.0

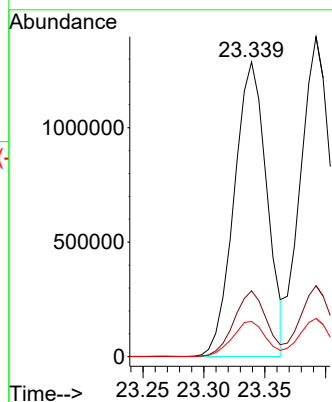

#91

Benzo(k)fluoranthene

Concen: 20.465 ng/ul

RT: 23.392 min Scan# 3418

Delta R.T. -0.000 min

Lab File: BP016694.D

Acq: 22 Aug 2023 09:11




Tgt Ion:252 Resp: 2456014


Ion Ratio Lower Upper

252 100

253 22.2 18.0 27.0

125 11.9 9.8 14.8





#93

Benzo(a)pyrene

Concen: 19.475 ng/ul

RT: 24.027 min Scan# 3526

Delta R.T. -0.000 min

Lab File: BP016694.D

Acq: 22 Aug 2023 09:11

Instrument :

BNA_P

ClientSampleId :

SSTD020697





Tgt Ion:252 Resp: 2222382

Ion Ratio Lower Upper

252 100

253 21.5 17.7 26.5

125 13.2 10.6 15.8

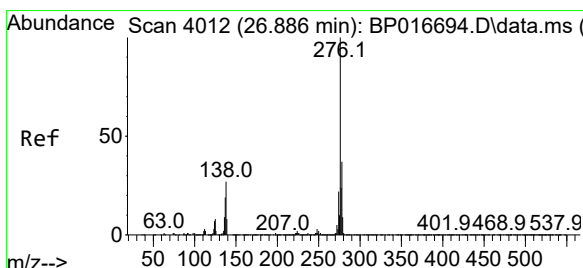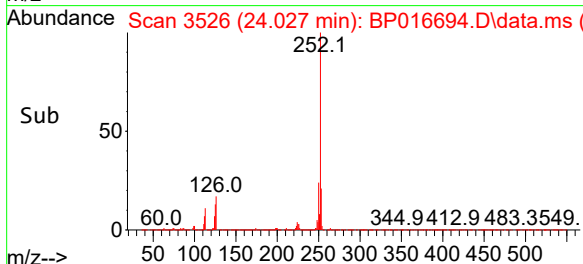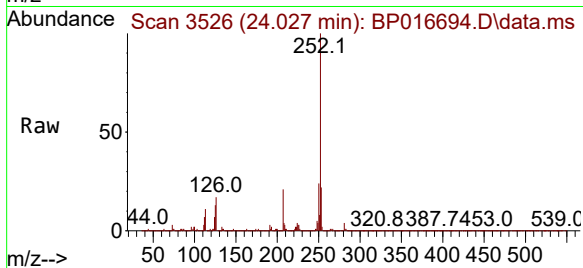

#94

Indeno(1,2,3-cd)pyrene

Concen: 17.397 ng/ul

RT: 26.886 min Scan# 4012

Delta R.T. -0.000 min

Lab File: BP016694.D

Acq: 22 Aug 2023 09:11




Tgt Ion:276 Resp: 2343072


Ion Ratio Lower Upper

276 100

138 26.8 21.7 32.5

277 24.4 19.5 29.3

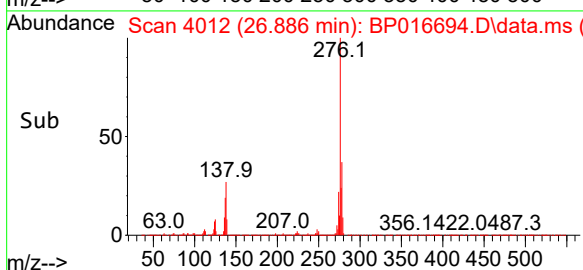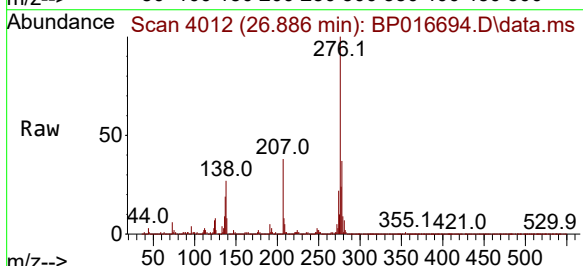



#95

Dibenzo(a,h)anthracene

Concen: 17.419 ng/ul

RT: 26.915 min Scan# 4017

Delta R.T. -0.000 min

Lab File: BP016694.D

Acq: 22 Aug 2023 09:11

Instrument :

BNA_P

ClientSampleId :

SSTD020697





Tgt Ion:278 Resp: 1952431

Ion Ratio Lower Upper

278 100

139 19.3 15.5 23.3

279 24.9 19.1 28.7

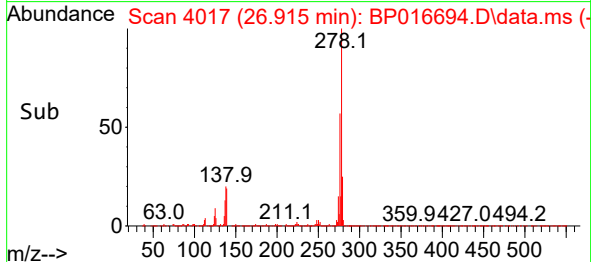

#96

Benzo(g,h,i)perylene

Concen: 16.926 ng/ul

RT: 27.745 min Scan# 4158

Delta R.T. -0.000 min

Lab File: BP016694.D

Acq: 22 Aug 2023 09:11

Tgt Ion:276 Resp: 1814305

Ion Ratio Lower Upper

276 100

138 25.8 21.5 32.3

277 23.6 19.3 28.9

