
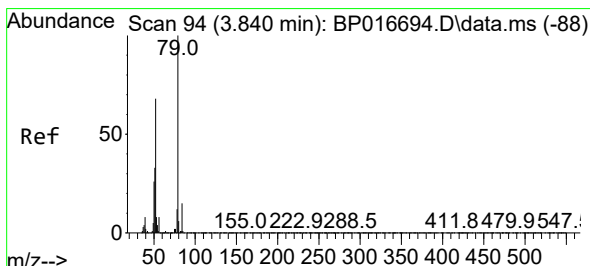
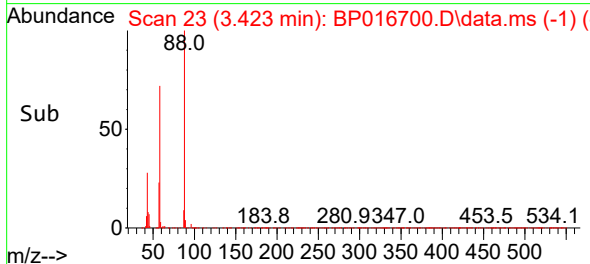
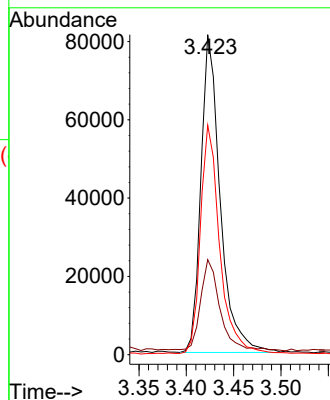


#2
 1,4-Dioxane
 Concen: 14.993 ng/uL
 RT: 3.423 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BP016700.D
 Acq: 22 Aug 2023 12:52




Instrument :
 BNA_P
 ClientSampleId :
 SLCS972


Tgt Ion: 88 Resp: 115008
 Ion Ratio Lower Upper
 88 100
 43 29.7 23.5 35.3
 58 71.7 57.1 85.7

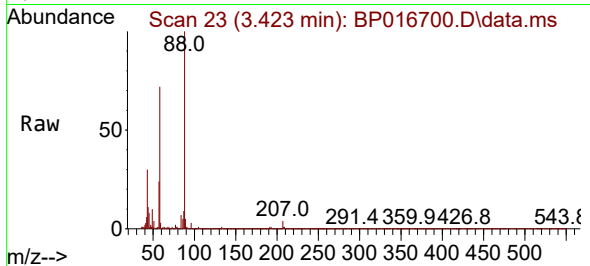

#5
 Pyridine
 Concen: 33.954 ng/uL
 RT: 3.846 min Scan# 95
 Delta R.T. -0.006 min
 Lab File: BP016700.D
 Acq: 22 Aug 2023 12:52

Tgt Ion: 79 Resp: 747731
 Ion Ratio Lower Upper
 79 100
 52 68.0 56.6 84.8
 51 33.0 26.9 40.3


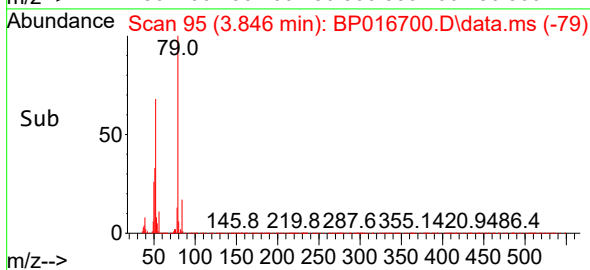
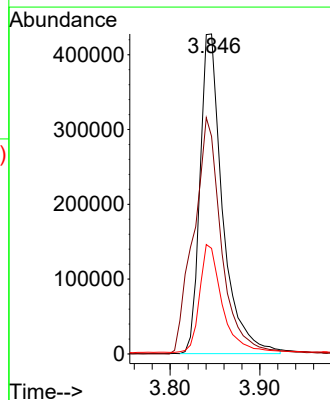
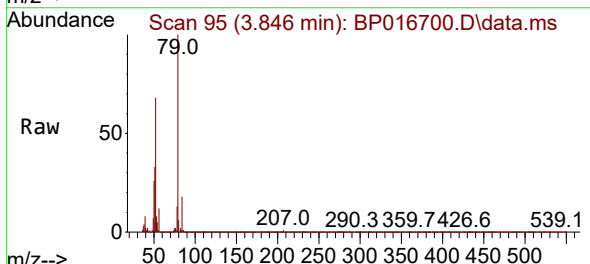




#6
Benzaldehyde
Concen: 42.804 ng/ul
RT: 7.199 min Scan# 60
Delta R.T. -0.006 min
Lab File: BP016700.D
Acq: 22 Aug 2023 12:52




Instrument :
BNA_P
ClientSampleId :
SLCS972


Tgt Ion: 77 Resp: 576662
Ion Ratio Lower Upper
77 100
105 90.6 71.8 107.6
106 88.4 70.2 105.2

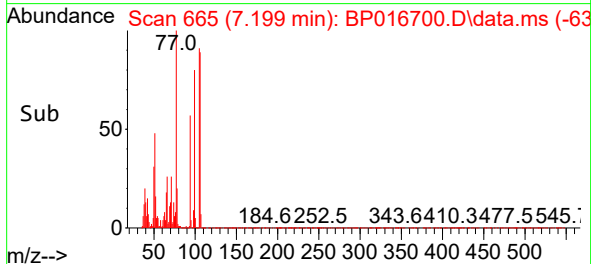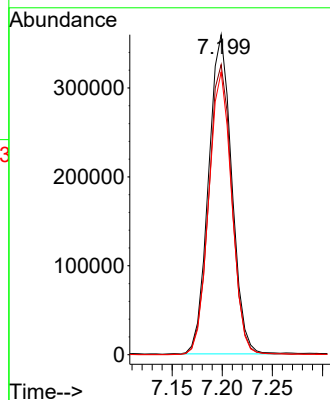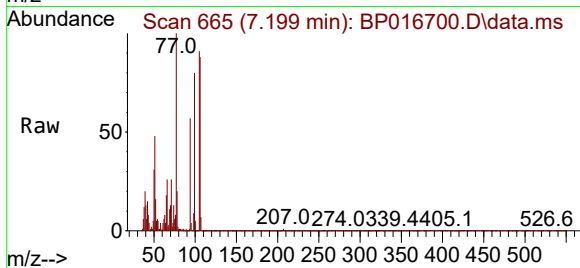

#8
Phenol
Concen: 38.587 ng/ul
RT: 7.217 min Scan# 668
Delta R.T. -0.006 min
Lab File: BP016700.D
Acq: 22 Aug 2023 12:52

Tgt Ion: 94 Resp: 1007945
Ion Ratio Lower Upper
94 100
65 28.7 22.3 33.5
66 37.6 28.7 43.1



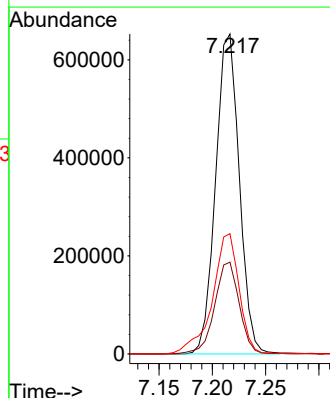
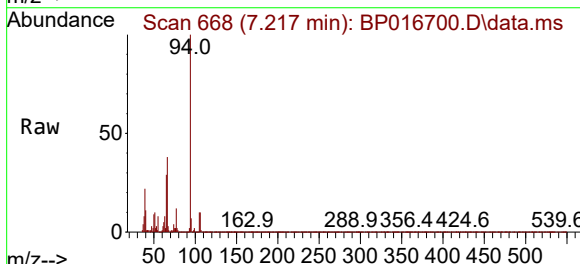


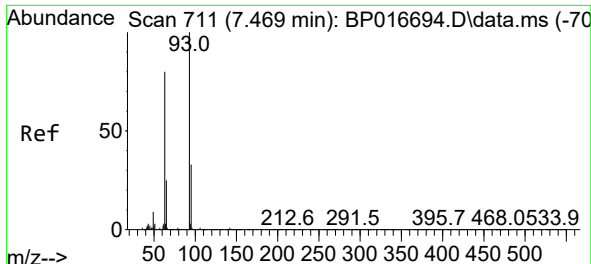

#10
Bis(2-Chloroethyl)ether
Concen: 37.015 ng/ul
RT: 7.475 min Scan# 711
Delta R.T. -0.006 min
Lab File: BP016700.D
Acq: 22 Aug 2023 12:52




Instrument :
BNA_P
ClientSampleId :
SLCS972


Tgt Ion: 93 Resp: 781028
Ion Ratio Lower Upper
93 100
63 77.4 60.1 90.1
95 32.7 25.4 38.2

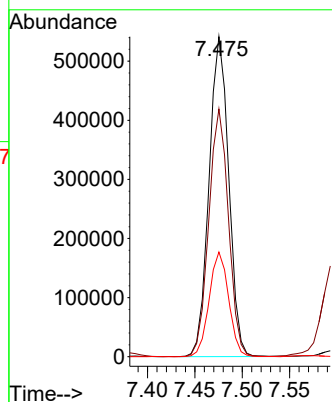

#12
2-Chlorophenol
Concen: 38.940 ng/ul
RT: 7.599 min Scan# 733
Delta R.T. -0.006 min
Lab File: BP016700.D
Acq: 22 Aug 2023 12:52

Tgt Ion:128 Resp: 719217
Ion Ratio Lower Upper
128 100
64 51.5 41.4 62.0
130 31.6 26.0 39.0



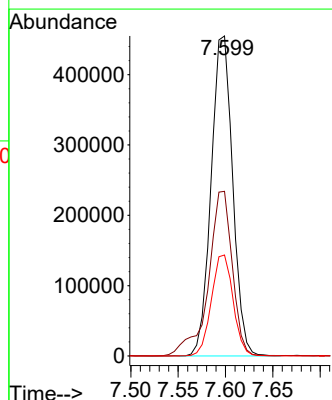
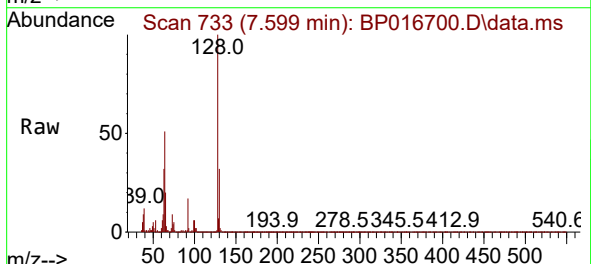




#13
2-Methylphenol
Concen: 38.959 ng/ul
RT: 8.481 min Scan# 882
Delta R.T. -0.006 min
Lab File: BP016700.D
Acq: 22 Aug 2023 12:52




Instrument :
BNA_P
ClientSampleId :
SLCS972


Tgt Ion:108 Resp: 739194
Ion Ratio Lower Upper
108 100
107 90.1 70.5 105.7

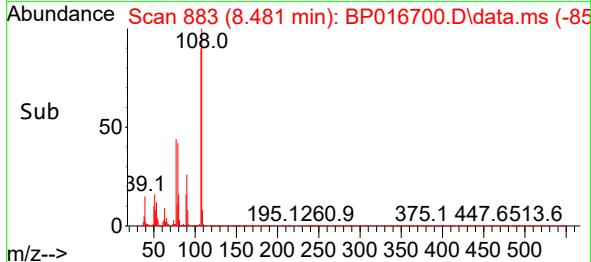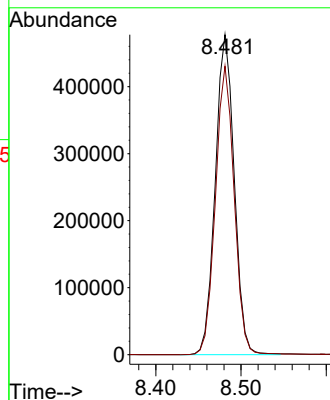

#14
2,2'-oxybis(1-Chloropropane)
Concen: 17.827 ng/ul
RT: 8.558 min Scan# 896
Delta R.T. -0.012 min
Lab File: BP016700.D
Acq: 22 Aug 2023 12:52

Tgt Ion: 45 Resp: 524253
Ion Ratio Lower Upper
45 100
77 15.7 12.1 18.1
79 10.9 8.2 12.4


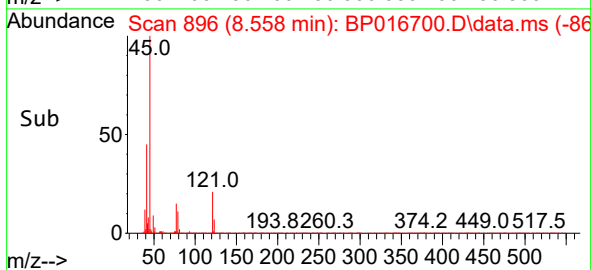
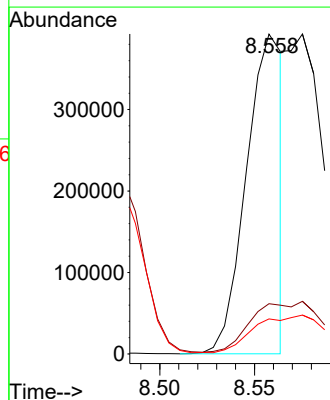
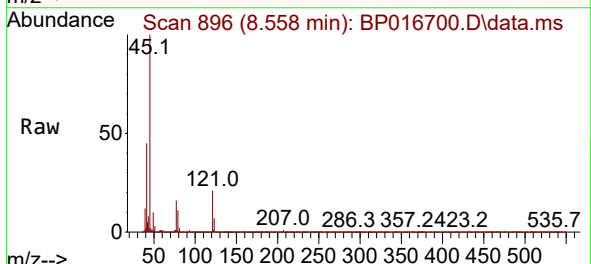




#18
4-Methylphenol
Concen: 38.912 ng/ul
RT: 8.816 min Scan# 940
Delta R.T. -0.006 min
Lab File: BP016700.D
Acq: 22 Aug 2023 12:52




Instrument :
BNA_P
ClientSampleId :
SLCS972


Tgt Ion:108 Resp: 811442
Ion Ratio Lower Upper
108 100
107 112.7 87.3 130.9

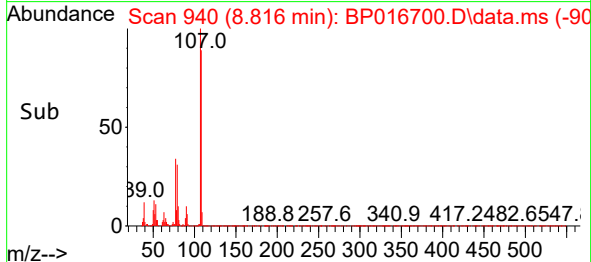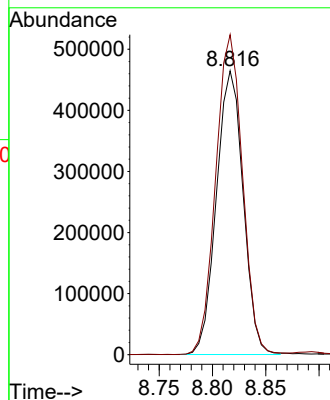

#19
Hexachloroethane
Concen: 36.944 ng/ul
RT: 9.116 min Scan# 991
Delta R.T. -0.012 min
Lab File: BP016700.D
Acq: 22 Aug 2023 12:52

Tgt Ion:117 Resp: 285081
Ion Ratio Lower Upper
117 100
201 90.5 71.8 107.6
199 55.6 45.2 67.8


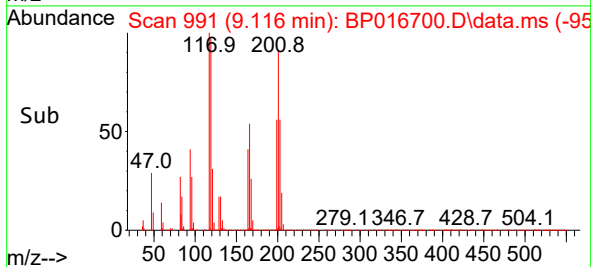
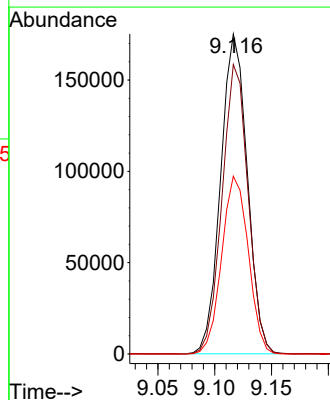
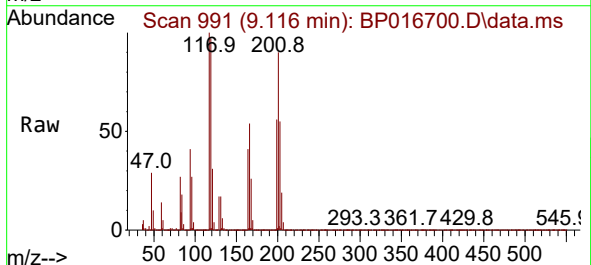




#22
Nitrobenzene
Concen: 40.442 ng/ul
RT: 9.287 min Scan# 1020
Delta R.T. -0.006 min
Lab File: BP016700.D
Acq: 22 Aug 2023 12:52




Instrument :
BNA_P
ClientSampleId :
SLCS972


Tgt Ion: 77 Resp: 956967
Ion Ratio Lower Upper
77 100
123 40.8 32.5 48.7
65 12.8 10.3 15.5

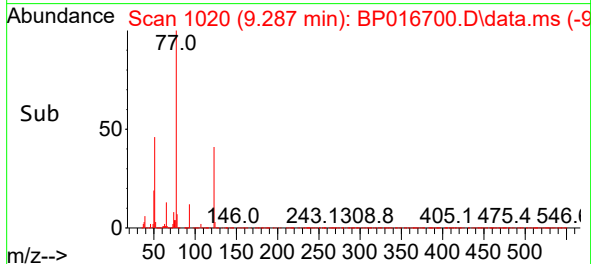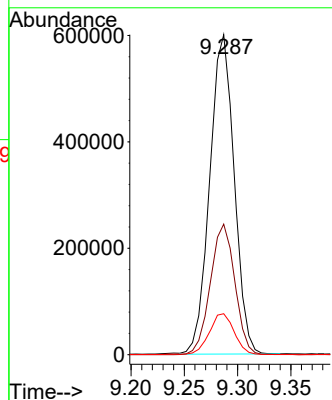

#23
Isophorone
Concen: 41.060 ng/ul
RT: 9.799 min Scan# 1107
Delta R.T. -0.006 min
Lab File: BP016700.D
Acq: 22 Aug 2023 12:52

Tgt Ion: 82 Resp: 1835099
Ion Ratio Lower Upper
82 100
95 6.9 5.3 7.9
138 15.3 12.7 19.1


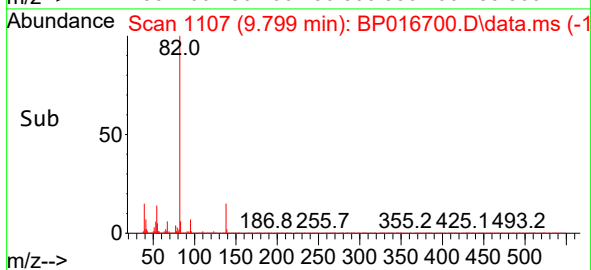
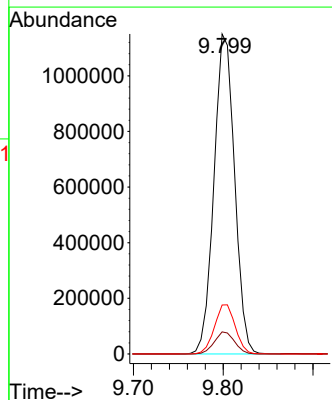
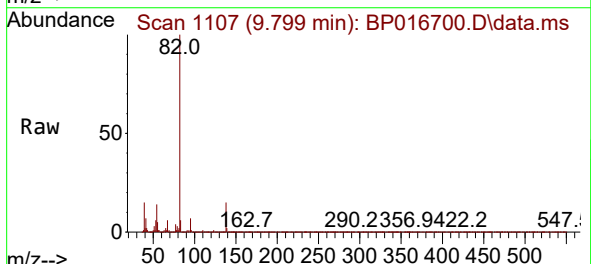




#25
2-Nitrophenol
Concen: 44.686 ng/ul
RT: 9.987 min Scan# 1139
Delta R.T. -0.012 min
Lab File: BP016700.D
Acq: 22 Aug 2023 12:52




Instrument :
BNA_P
ClientSampleId :
SLCS972


Tgt Ion:139 Resp: 410127
Ion Ratio Lower Upper
139 100
65 56.8 46.4 69.6
109 31.6 25.3 37.9

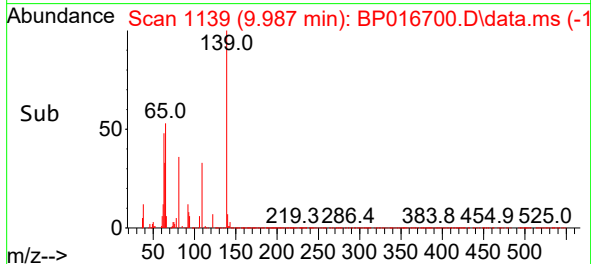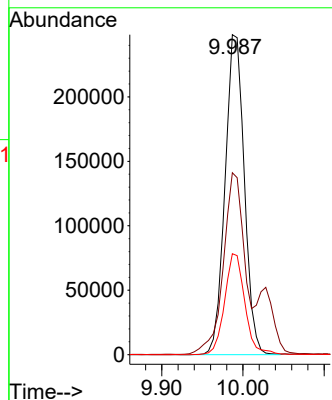

#26
2,4-Dimethylphenol
Concen: 40.187 ng/ul
RT: 10.028 min Scan# 1146
Delta R.T. -0.006 min
Lab File: BP016700.D
Acq: 22 Aug 2023 12:52

Tgt Ion:107 Resp: 869502
Ion Ratio Lower Upper
107 100
121 49.6 39.1 58.7
122 83.6 66.9 100.3


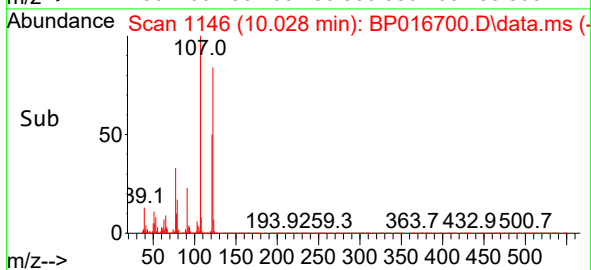
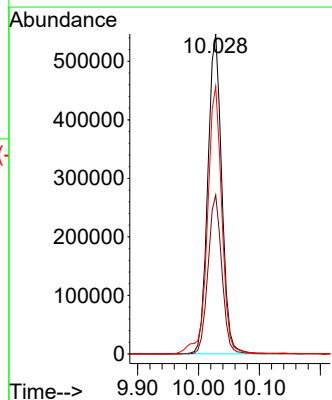
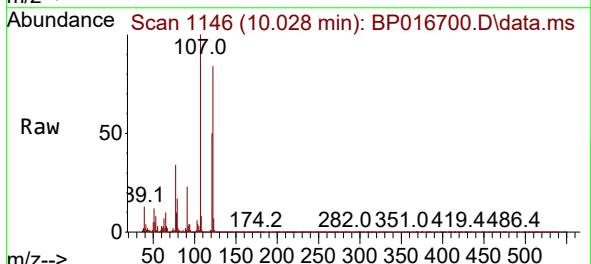


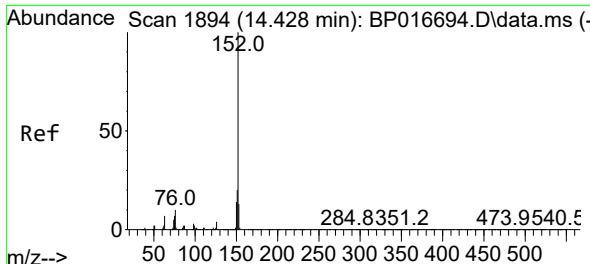

#50
Acenaphthylene
Concen: 36.391 ng/ul
RT: 14.422 min Scan# 1894
Delta R.T. -0.012 min
Lab File: BP016700.D
Acq: 22 Aug 2023 12:52




Instrument :
BNA_P
ClientSampleId :
SLCS972


Tgt Ion:152 Resp: 2595905
Ion Ratio Lower Upper
152 100
151 20.0 15.7 23.5
153 13.6 10.6 15.8

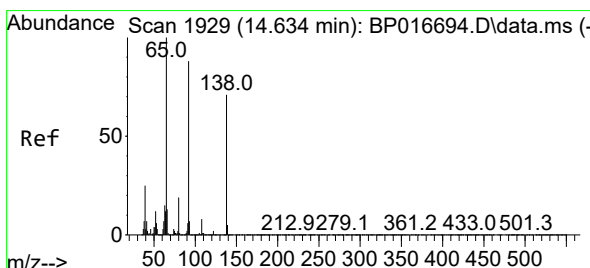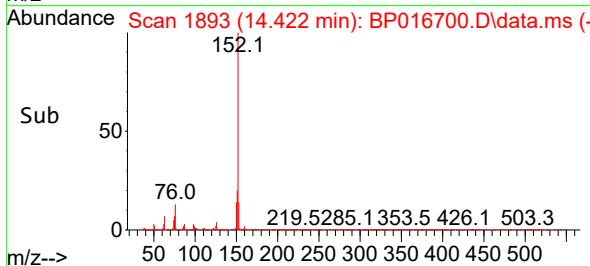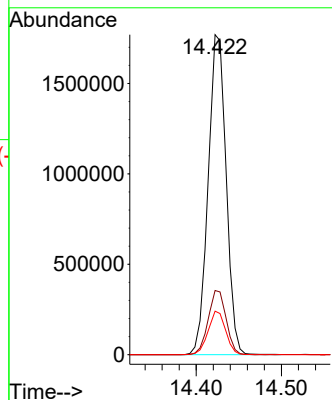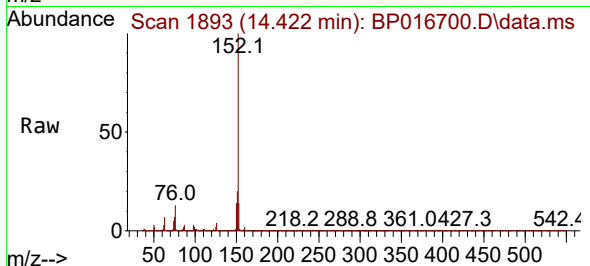

#51
3-Nitroaniline
Concen: 45.890 ng/ul
RT: 14.634 min Scan# 1929
Delta R.T. 0.000 min
Lab File: BP016700.D
Acq: 22 Aug 2023 12:52

Tgt Ion:138 Resp: 489010
Ion Ratio Lower Upper
138 100
108 11.1 10.9 16.3
92 128.0 105.0 157.6


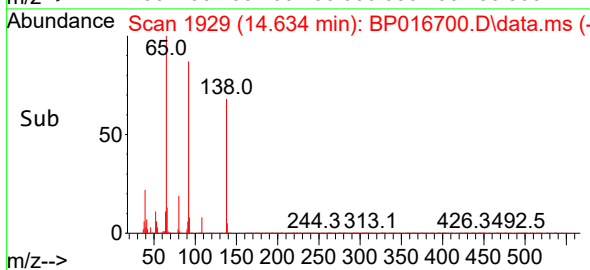
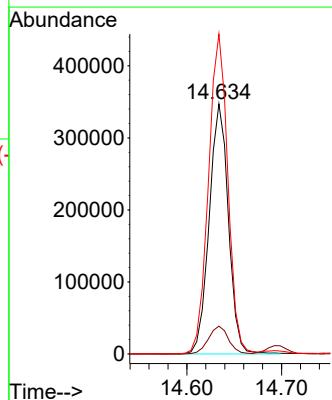
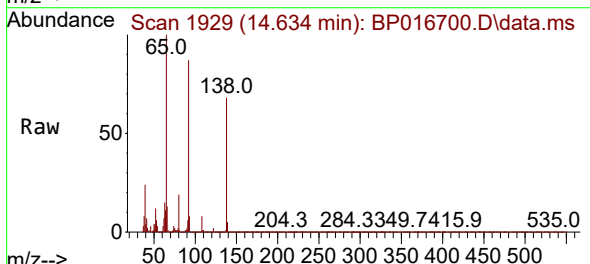




#55
4-Nitrophenol
Concen: 40.926 ng/ul
RT: 14.916 min Scan# 1977
Delta R.T. 0.000 min
Lab File: BP016700.D
Acq: 22 Aug 2023 12:52




Instrument :
BNA_P
ClientSampleId :
SLCS972


Tgt Ion:109 Resp: 363731
Ion Ratio Lower Upper
109 100
139 124.5 101.1 151.7
65 142.7 108.9 163.3

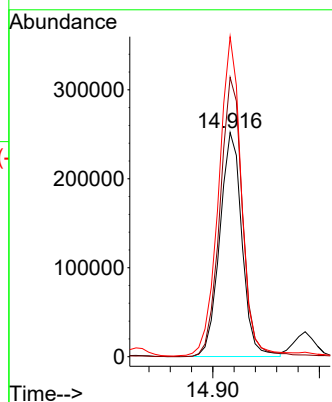

#56
Dibenzofuran
Concen: 37.680 ng/ul
RT: 15.098 min Scan# 2008
Delta R.T. -0.006 min
Lab File: BP016700.D
Acq: 22 Aug 2023 12:52

Tgt Ion:168 Resp: 2454878
Ion Ratio Lower Upper
168 100
139 38.4 31.4 47.0


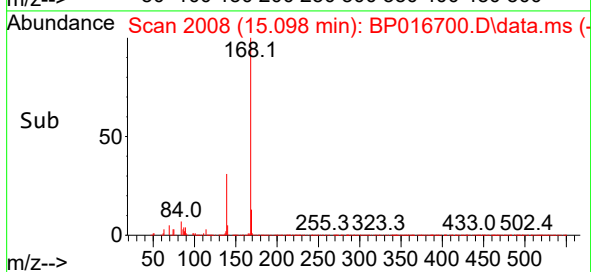
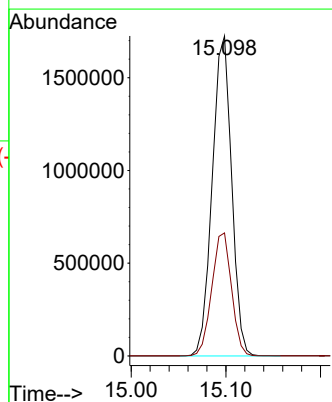





#62
4-Chlorophenyl-phenylether
Concen: 37.439 ng/ul
RT: 15.740 min Scan# 2117
Delta R.T. -0.006 min
Lab File: BP016700.D
Acq: 22 Aug 2023 12:52

Instrument :
BNA_P
ClientSampleId :
SLCS972

Tgt Ion:204 Resp: 938848
Ion Ratio Lower Upper
204 100
206 33.0 25.5 38.3
141 62.5 52.2 78.2

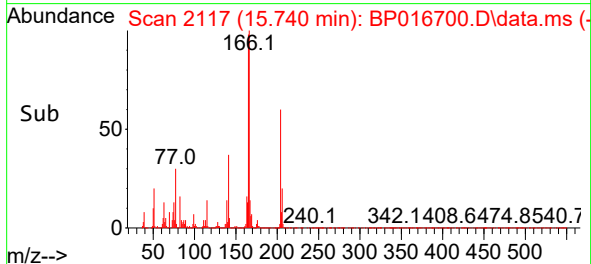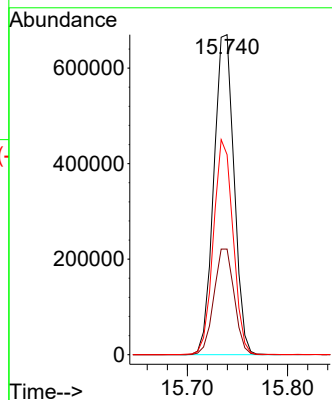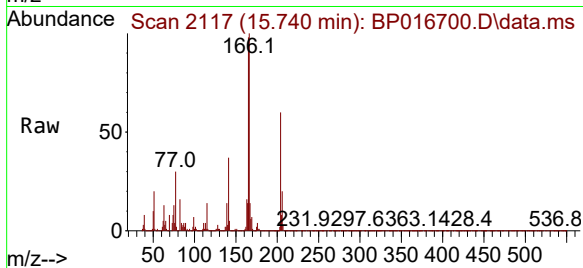

#63
4-Nitroaniline
Concen: 50.543 ng/ul
RT: 15.804 min Scan# 2128
Delta R.T. 0.000 min
Lab File: BP016700.D
Acq: 22 Aug 2023 12:52

Tgt Ion:138 Resp: 515430
Ion Ratio Lower Upper
138 100
92 58.7 46.7 70.1
108 97.3 73.7 110.5

