

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082223\
 Data File : BP016701.D
 Acq On : 22 Aug 2023 13:26
 Operator : MA/JU
 Sample : PB154937BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK937

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016701.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.387	13	17	31	rVB	142061	220049	2.17%	0.209%
2	3.822	87	91	108	rBV	1500263	2337289	23.07%	2.217%
3	4.140	140	145	156	rVB	195293	299246	2.95%	0.284%
4	7.181	655	662	675	rBV	1709228	2752551	27.17%	2.611%
5	7.381	686	696	705	rBV	1441112	2213832	21.85%	2.100%
6	7.563	719	727	738	rBV	1658870	2614601	25.80%	2.480%
7	8.046	799	809	817	rBV	1348340	2170558	21.42%	2.059%
8	8.745	919	928	943	rBV	2134283	3422871	33.78%	3.247%
9	9.240	1004	1012	1022	rBV	1714777	2738713	27.03%	2.598%
10	9.957	1123	1134	1143	rBV	1379091	2235450	22.06%	2.120%
11	10.481	1216	1223	1239	rBV	1967203	3333722	32.90%	3.162%
12	10.875	1281	1290	1299	rBV	2023188	3379814	33.36%	3.206%
13	11.028	1308	1316	1338	rBV	2177473	3726070	36.77%	3.534%
14	12.451	1552	1558	1566	rVB2	36688	62254	0.61%	0.059%
15	13.539	1738	1743	1749	rBV2	28700	45375	0.45%	0.043%
16	13.663	1759	1764	1768	rVB5	7001	12846	0.13%	0.012%
17	14.104	1832	1839	1852	rBV	4005411	5354988	52.85%	5.079%
18	14.392	1881	1888	1904	rBV	4312325	6324258	62.41%	5.998%
19	14.692	1932	1939	1948	rBV	3162267	4672811	46.12%	4.432%
20	14.804	1955	1958	1963	rVB7	6312	11983	0.12%	0.011%
21	14.898	1966	1974	1994	rBV	1768079	2899369	28.61%	2.750%
22	15.692	2101	2109	2119	rBV	5348578	7973476	78.69%	7.563%
23	15.810	2123	2129	2145	rVV	1602374	2245153	22.16%	2.129%
24	15.927	2145	2149	2153	rVB4	26168	37125	0.37%	0.035%
25	16.469	2238	2241	2246	rVB7	7938	10475	0.10%	0.010%
26	17.127	2348	2353	2362	rVB7	9991	26488	0.26%	0.025%
27	17.463	2403	2410	2420	rBV	4134490	5861588	57.85%	5.560%
28	17.563	2420	2427	2447	rVV2	6331269	8868852	87.53%	8.412%
29	18.298	2549	2552	2558	rBV8	23248	38373	0.38%	0.036%
30	19.363	2730	2733	2739	rVB2	75561	96959	0.96%	0.092%
31	19.433	2741	2745	2754	rVB	71575	107660	1.06%	0.102%
32	19.792	2800	2806	2819	rBV	7459758	10132703	100.00%	9.611%
33	21.557	3101	3106	3112	rBV	4235155	5660160	55.86%	5.369%
34	23.968	3507	3516	3527	rVB	3839322	8602197	84.90%	8.159%
35	24.133	3538	3544	3554	rVB	2306897	4942122	48.77%	4.687%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082223\
Data File : BP016701.D
Acq On : 22 Aug 2023 13:26
Operator : MA/JU
Sample : PB154937BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK937

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 105431981

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082223\
Data File : BP016701.D
Acq On : 22 Aug 2023 13:26
Operator : MA/JU
Sample : PB154937BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK937

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

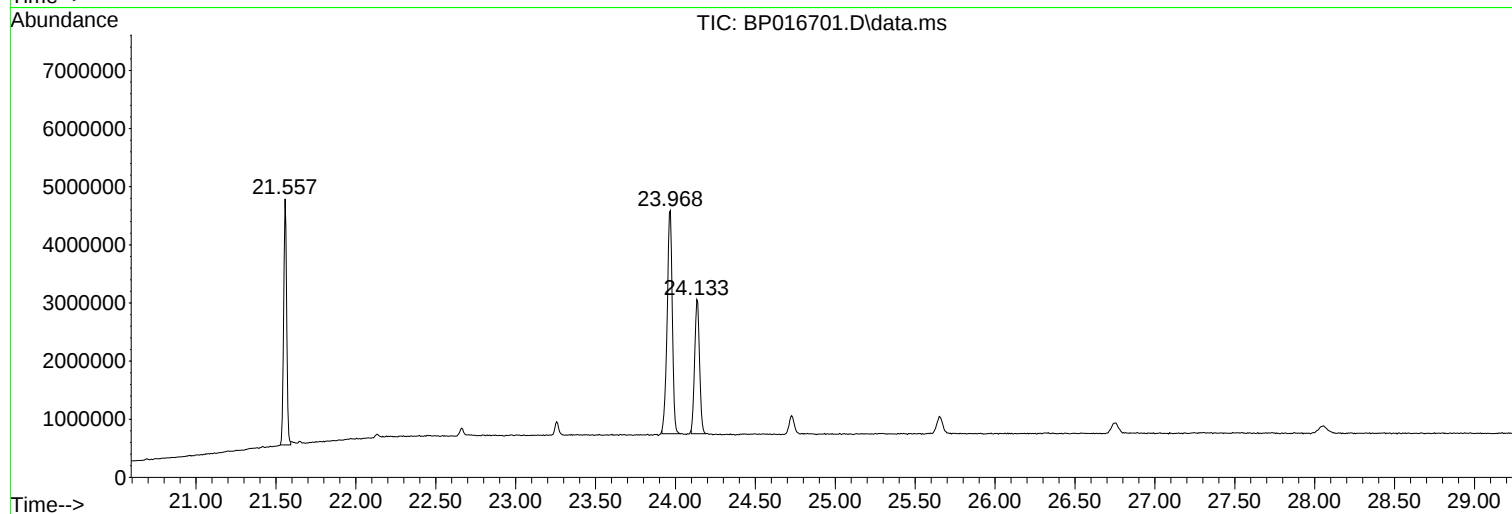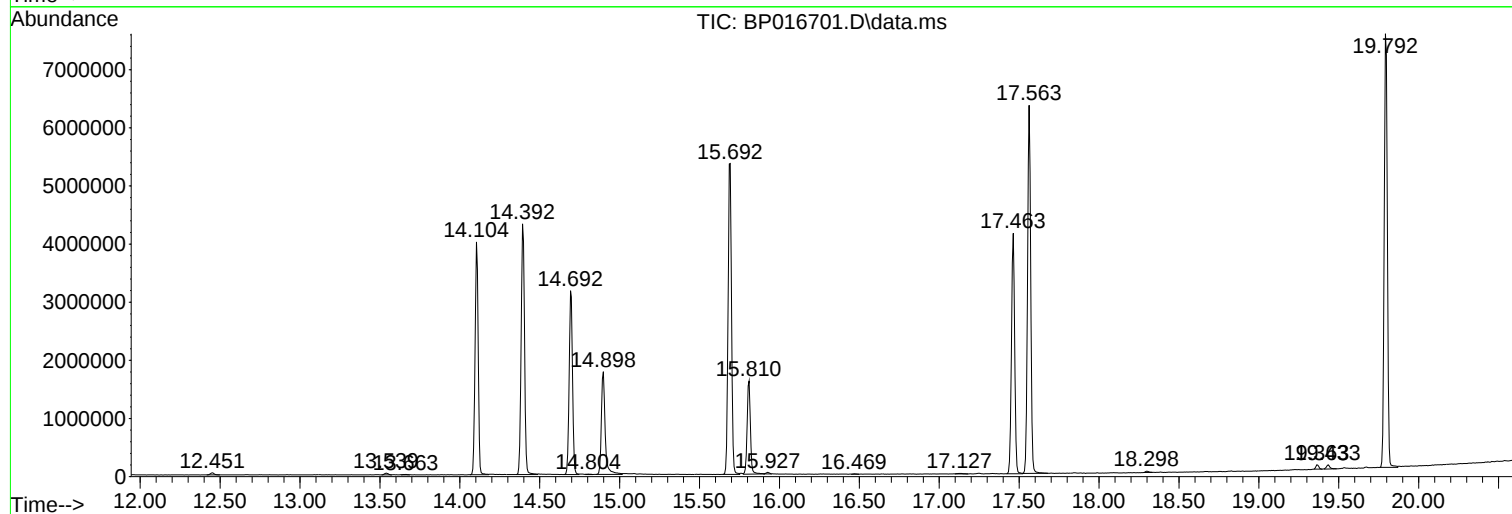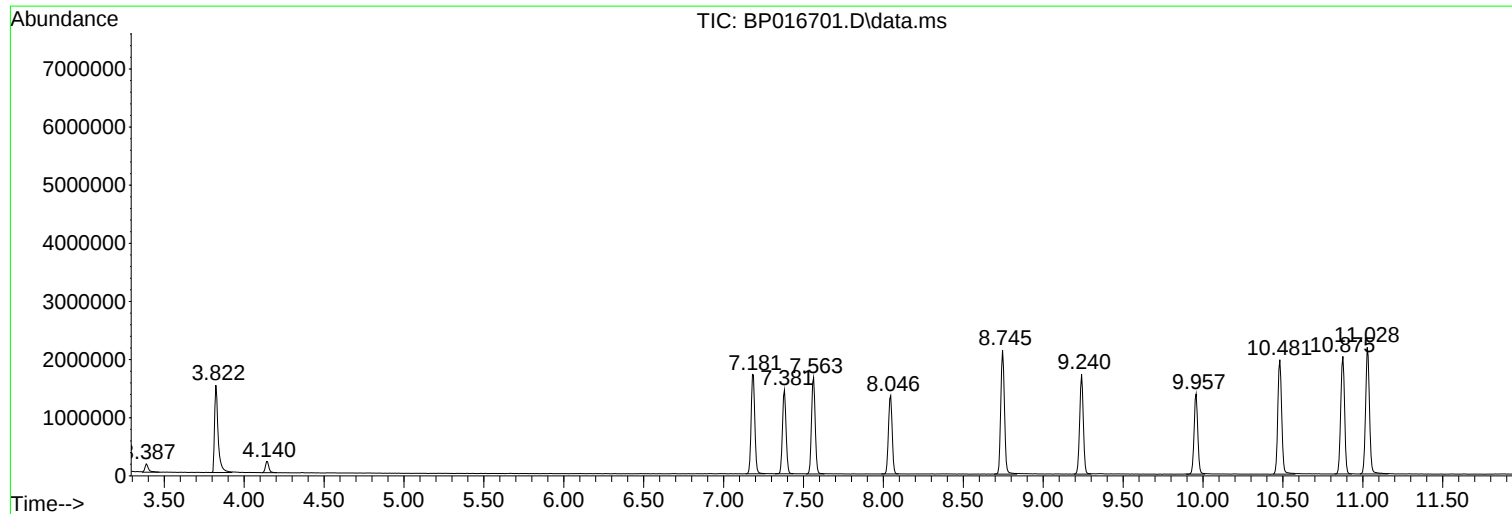

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082223\
Data File : BP016701.D
Acq On : 22 Aug 2023 13:26
Operator : MA/JU
Sample : PB154937BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK937










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Toluene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.140	2.76 ng/ul	299246	1,4-Dichlorobenzene-d4	8.046

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Toluene			92	C7H8	000108-88-3	94
2	Toluene			92	C7H8	000108-88-3	93
3	Toluene			92	C7H8	000108-88-3	93
4	Toluene			92	C7H8	000108-88-3	87
5	1,3,5-Cycloheptatriene			92	C7H8	000544-25-2	87

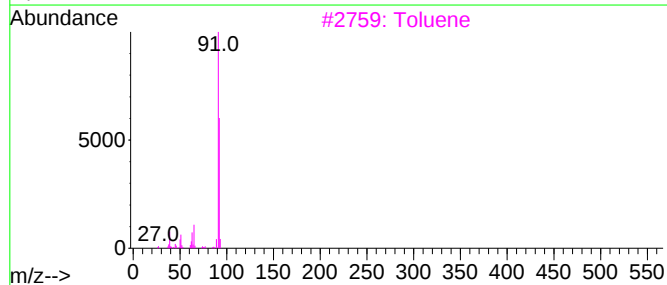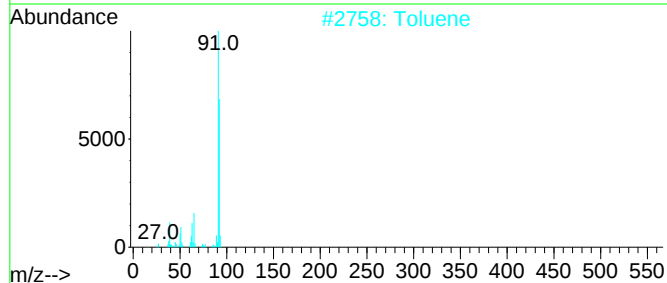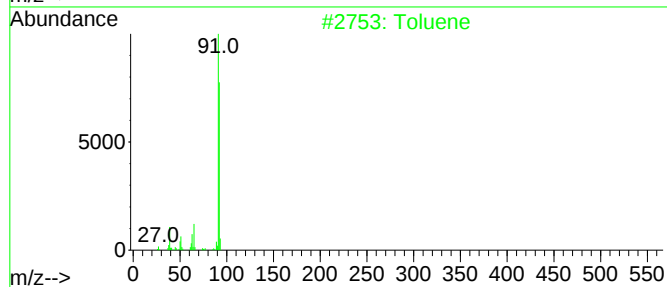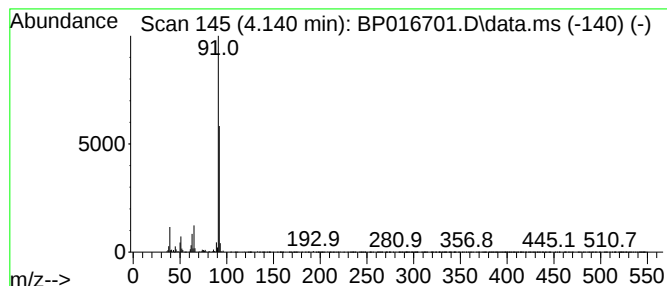

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082223\
Data File : BP016701.D
Acq On : 22 Aug 2023 13:26
Operator : MA/JU
Sample : PB154937BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK937

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Toluene	4.140	2.8	ng/ul	299246	1	8.046	2170560	20.0