

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082323\
 Data File : BP016717.D
 Acq On : 23 Aug 2023 16:24
 Operator : MA/JU
 Sample : 04105-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH8X7

Quant Time: Aug 23 18:38:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 17 01:38:34 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.040	152	366472	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.869	136	1622015	20.000	ng/u1	-0.02
38) Acenaphthene-d10	14.693	164	992664	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.463	188	2081647	20.000	ng/u1	0.00
79) Chrysene-d12	21.557	240	1352275	20.000	ng/u1	0.00
88) Perylene-d12	24.139	264	1321981	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	52028	5.395	ng/uL	0.00
4) Pyridine-d5	3.828	84	299604	10.211	ng/u1	0.00
7) Phenol-d5	7.181	99	201784	5.972	ng/u1	-0.01
9) Bis-(2-Chloroethyl)eth...	7.375	67	664864	29.878	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.558	132	546416	22.517	ng/u1	-0.01
15) 4-Methylphenol-d8	8.740	113	373082	13.888	ng/u1	-0.02
21) Nitrobenzene-d5	9.240	128	372274	32.618	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.952	143	368737	34.017	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.475	165	611483	28.665	ng/u1	-0.02
31) 4-Chloroaniline-d4	11.028	131	644820	17.617	ng/u1	-0.01
46) Dimethylphthalate-d6	14.104	166	2364166	32.928	ng/u1	0.00
49) Acenaphthylene-d8	14.393	160	2630437	32.459	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.898	143	53425	3.653	ng/u1	0.00
60) Fluorene-d10	15.687	176	2020641	33.012	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.804	200	274599	27.729	ng/u1	-0.01
73) Anthracene-d10	17.563	188	3197668	35.513	ng/u1	0.00
81) Pyrene-d10	19.792	212	3320470	46.862	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.963	264	2293724	36.205	ng/u1	-0.01
Target Compounds						Qvalue
2) 1,4-Dioxane	3.428	88	40300	3.800	ng/uL	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082323\
Data File : BP016717.D
Acq On : 23 Aug 2023 16:24
Operator : MA/JU
Sample : 04105-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH8X7

Quant Time: Aug 23 18:38:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 17 01:38:34 2023
Response via : Initial Calibration

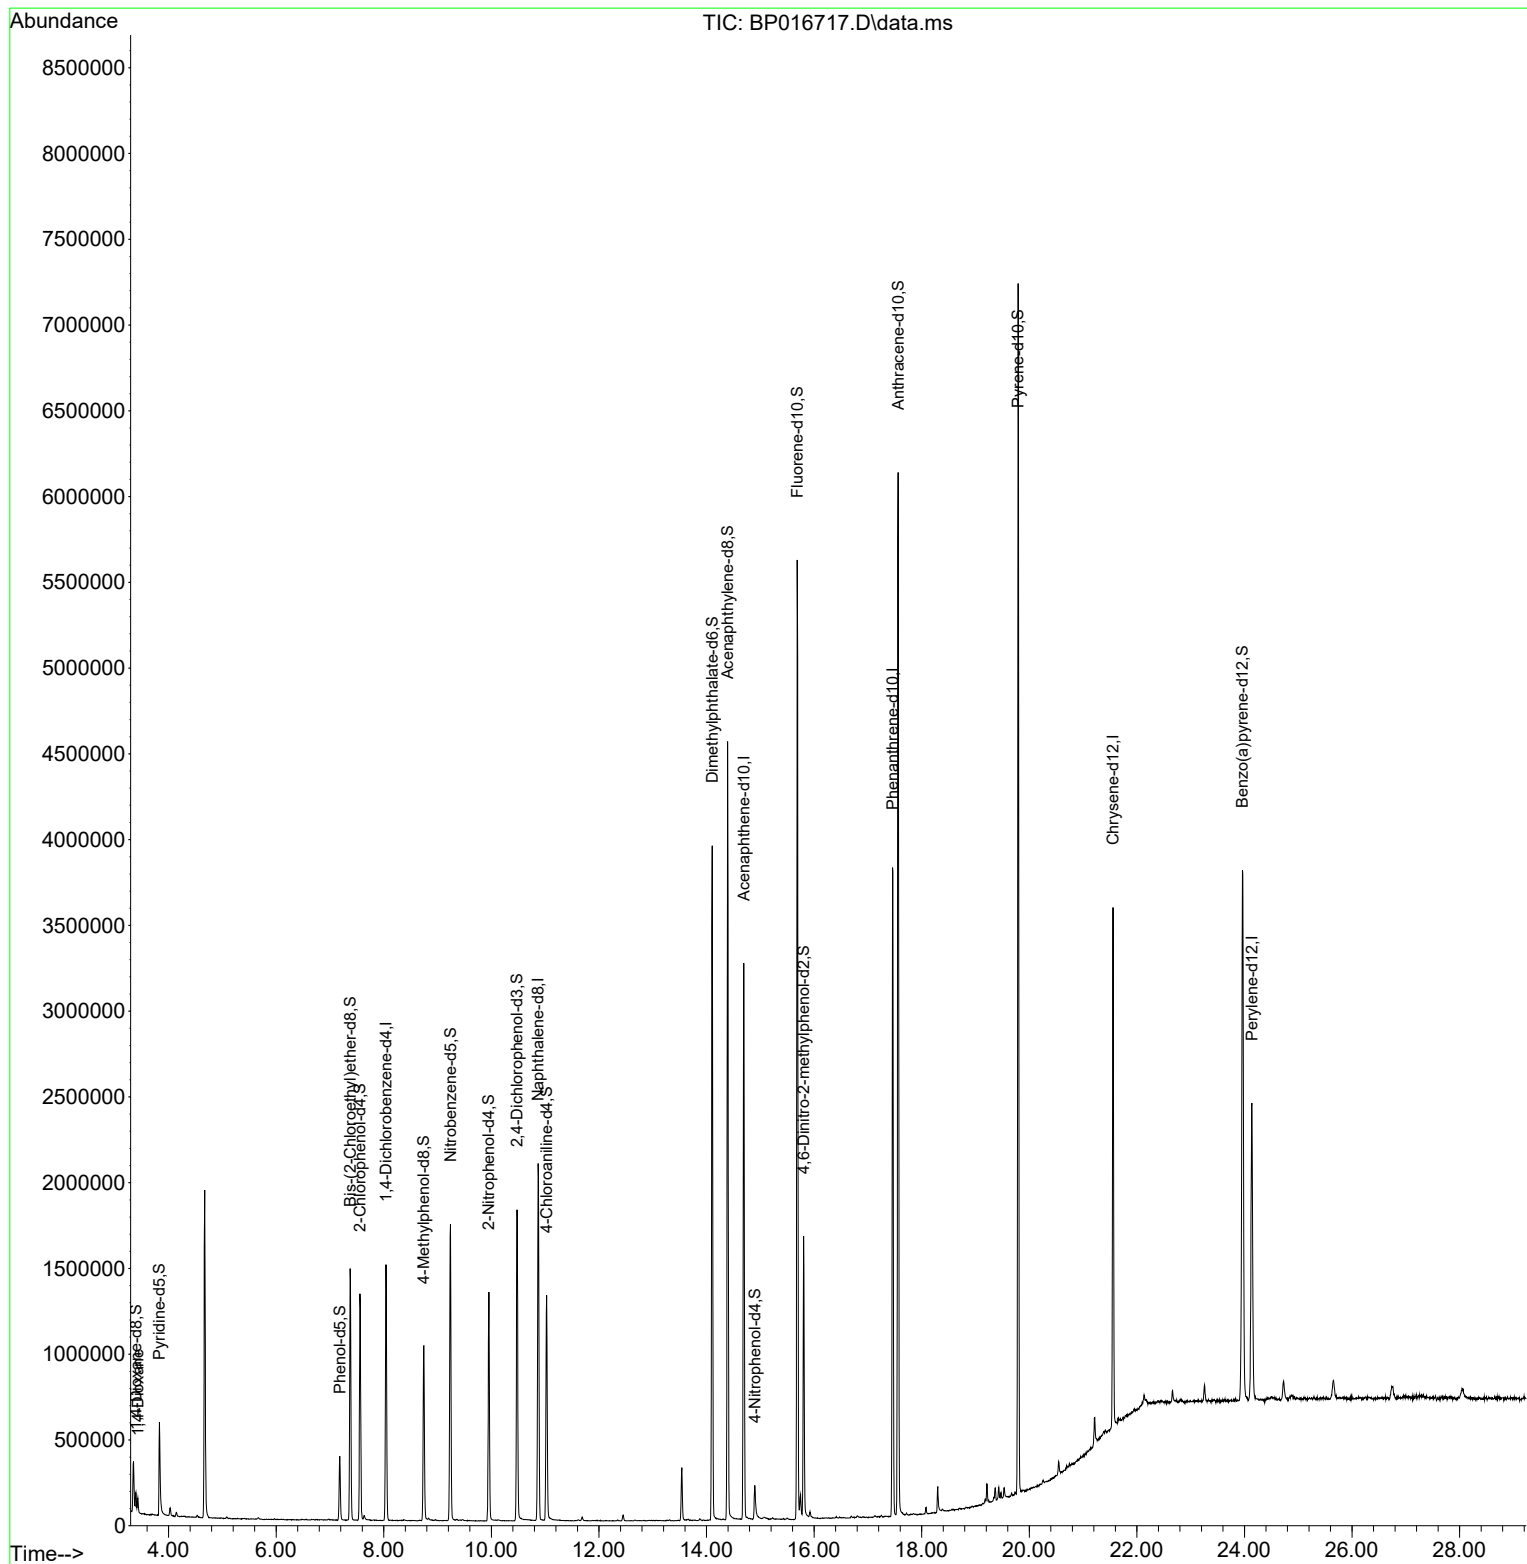

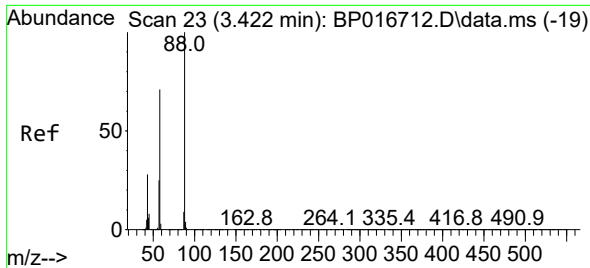

#2
 1,4-Dioxane
 Concen: 3.800 ng/uL
 RT: 3.428 min Scan# 24
 Delta R.T. 0.000 min
 Lab File: BP016717.D
 Acq: 23 Aug 2023 16:24

Instrument :
 BNA_P
 ClientSampleId :
 BH8X7

Tgt Ion: 88 Resp: 40300
 Ion Ratio Lower Upper
 88 100
 43 29.6 23.5 35.3
 58 76.3 57.1 85.7

