




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082323\
 Data File : BP016715.D
 Acq On : 23 Aug 2023 15:16
 Operator : MA/JU
 Sample : 04105-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH9F7

Manual IntegrationsAPPROVED

Quant Time: Aug 23 18:52:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 23 18:42:31 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/24/2023
 Supervised By :mohammad ahmed 08/24/2023

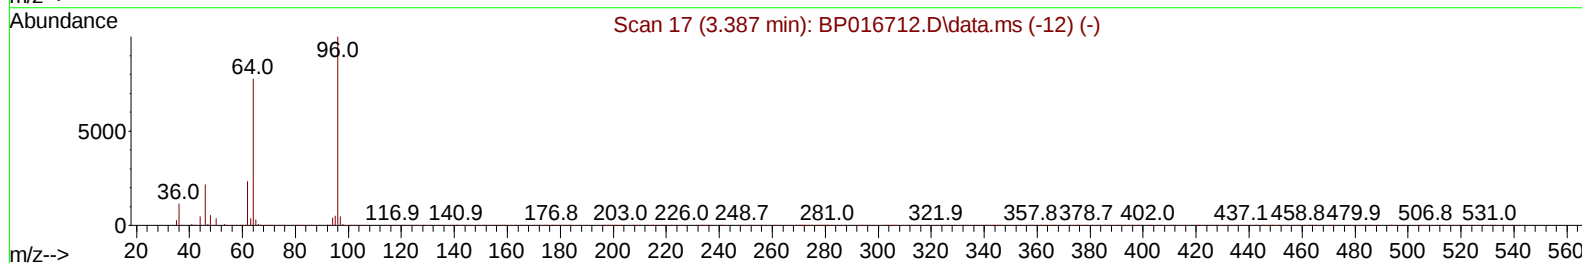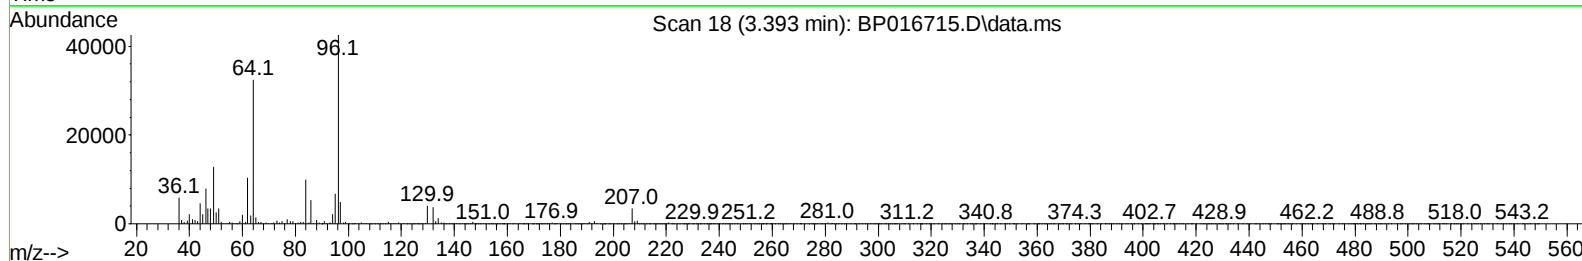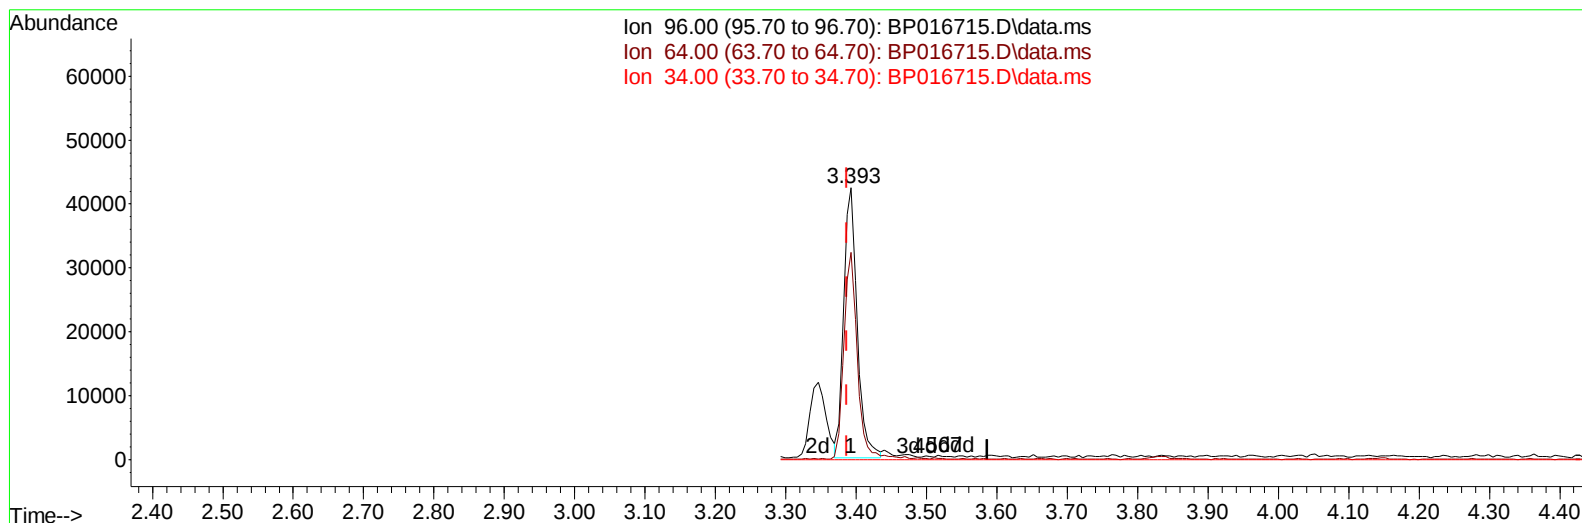

TIC: BP016715.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.393min (+ 0.006) 5.75 ng/uL

response 55928

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	79.70	76.16
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082323\
 Data File : BP016715.D
 Acq On : 23 Aug 2023 15:16
 Operator : MA/JU
 Sample : 04105-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH9F7

Manual IntegrationsAPPROVED

Quant Time: Aug 23 18:52:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 23 18:42:31 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/24/2023
 Supervised By :mohammad ahmed 08/24/2023

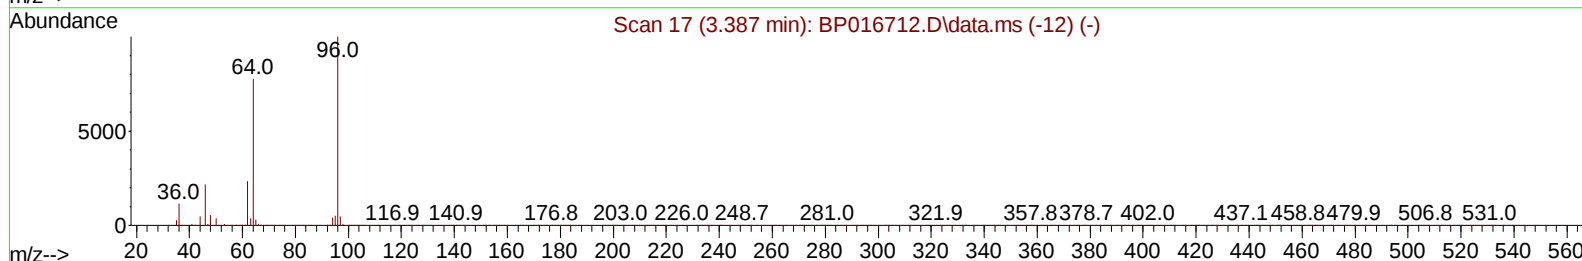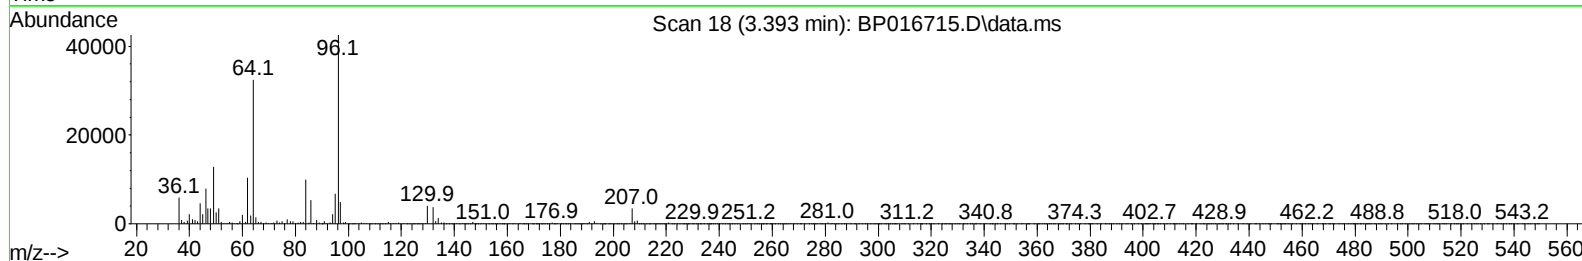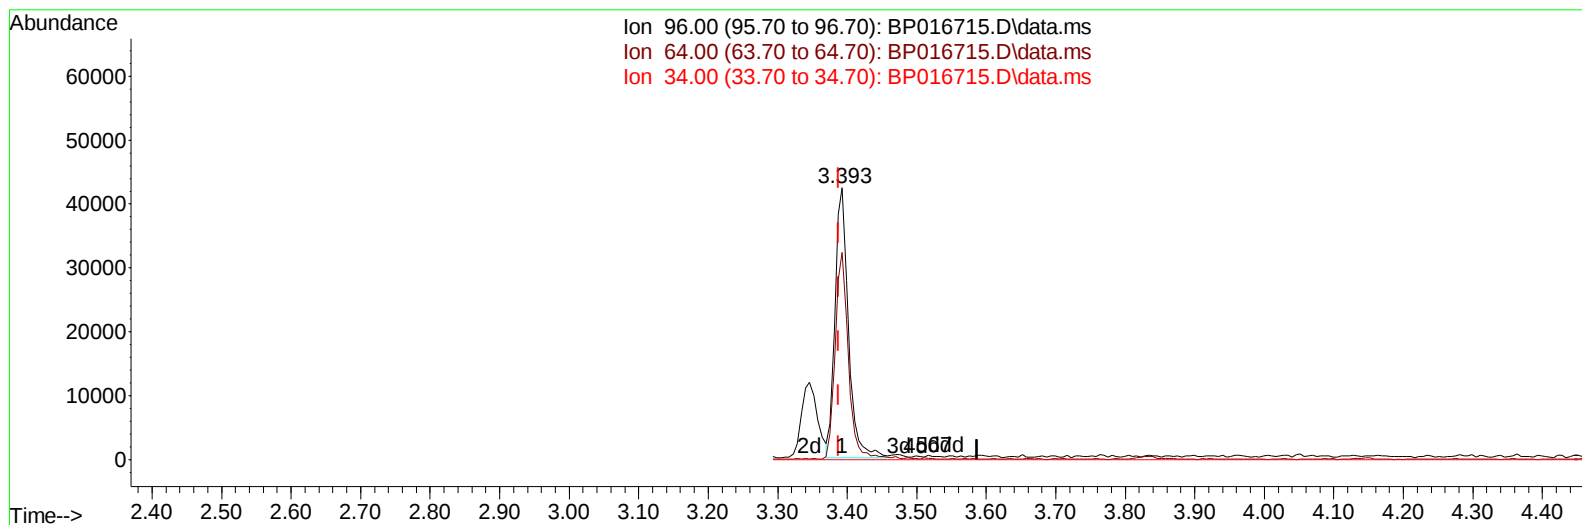

TIC: BP016715.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.393min (+ 0.006) 5.89 ng/uL m

response 57234

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	79.70	76.16
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082323\
 Data File : BP016715.D
 Acq On : 23 Aug 2023 15:16
 Operator : MA/JU
 Sample : 04105-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH9F7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/24/2023
 Supervised By :mohammad ahmed 08/24/2023

Quant Time: Aug 23 18:54:05 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 23 18:42:31 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.040	152	369449	20.000	ng/ul	0.00
20) Naphthalene-d8	10.869	136	1641298	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.692	164	987596	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.463	188	2037633	20.000	ng/ul	0.00
79) Chrysene-d12	21.557	240	1311446	20.000	ng/ul	0.00
88) Perylene-d12	24.133	264	1275993	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	57234m	5.887	ng/uL	0.00
4) Pyridine-d5	3.828	84	247616	8.371	ng/ul	0.00
7) Phenol-d5	7.181	99	203519	5.975	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.375	67	774369	34.518	ng/ul	0.00
11) 2-Chlorophenol-d4	7.557	132	612340	25.030	ng/ul	0.00
15) 4-Methylphenol-d8	8.746	113	401437	14.823	ng/ul	0.00
21) Nitrobenzene-d5	9.240	128	430252	37.256	ng/ul	0.00
24) 2-Nitrophenol-d4	9.951	143	419296	38.226	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.481	165	677754	31.398	ng/ul	0.00
31) 4-Chloroaniline-d4	11.028	131	975565	26.340	ng/ul	0.00
46) Dimethylphthalate-d6	14.104	166	2636783	36.913	ng/ul	0.00
49) Acenaphthylene-d8	14.392	160	2894761	35.904	ng/ul	0.00
54) 4-Nitrophenol-d4	14.898	143	44760	3.076	ng/ul	0.00
60) Fluorene-d10	15.686	176	2223022	36.505	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.810	200	293235	30.250	ng/ul	0.00
73) Anthracene-d10	17.563	188	3515079	39.882	ng/ul	0.00
81) Pyrene-d10	19.792	212	3605631	52.471	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.962	264	2512729	41.091	ng/ul	0.00
Target Compounds						
2) 1,4-Dioxane	3.428	88	36819	3.444	ng/uL	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082323\
Data File : BP016715.D
Acq On : 23 Aug 2023 15:16
Operator : MA/JU
Sample : 04105-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH9F7

Manual IntegrationsAPPROVED

Quant Time: Aug 23 18:54:05 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 23 18:42:31 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/24/2023
Supervised By :mohammad ahmed 08/24/2023

