

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082323\
 Data File : BP016713.D
 Acq On : 23 Aug 2023 14:08
 Operator : MA/JU
 Sample : PB155004BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK004

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016713.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	14	18	31	rVB	203334	288503	3.18%	0.259%
2	3.823	87	91	108	rBV	2086490	3040001	33.55%	2.729%
3	4.146	141	146	151	rVB	32904	50044	0.55%	0.045%
4	6.693	573	579	583	rBV6	4928	10380	0.11%	0.009%
5	7.181	655	662	681	rBV	2308576	3605874	39.79%	3.237%
6	7.381	688	696	706	rVB	1830666	2865886	31.62%	2.573%
7	7.558	719	726	737	rBV	2141914	3417656	37.71%	3.068%
8	8.040	800	808	816	rBV	1706188	2655051	29.30%	2.383%
9	8.746	920	928	942	rBV	2709714	4372912	48.25%	3.926%
10	9.240	1004	1012	1023	rBV	2175828	3502188	38.65%	3.144%
11	9.952	1125	1133	1146	rBV	1682869	2844969	31.39%	2.554%
12	10.475	1213	1222	1234	rBV	2489660	4228138	46.66%	3.796%
13	10.869	1281	1289	1304	rVB	2354782	4037282	44.55%	3.624%
14	11.028	1308	1316	1339	rBV	2696509	4556197	50.28%	4.090%
15	12.451	1550	1558	1566	rVB	44705	76446	0.84%	0.069%
16	13.540	1737	1743	1748	rVV2	27284	42941	0.47%	0.039%
17	13.657	1760	1763	1768	rVB5	8560	13057	0.14%	0.012%
18	14.104	1832	1839	1852	rBV	4637583	6272636	69.22%	5.631%
19	14.393	1881	1888	1905	rBV2	5076848	7590845	83.76%	6.814%
20	14.693	1932	1939	1956	rBV	3664639	5326269	58.77%	4.781%
21	14.893	1967	1973	1995	rBV	1495207	2588196	28.56%	2.323%
22	15.087	2004	2006	2010	rVB4	8884	9258	0.10%	0.008%
23	15.687	2101	2108	2122	rBV	6395850	9062434	100.00%	8.135%
24	15.804	2122	2128	2143	rVV	1476842	2088402	23.04%	1.875%
25	15.928	2145	2149	2155	rVB2	30004	49119	0.54%	0.044%
26	16.475	2238	2242	2246	rBV7	8560	12283	0.14%	0.011%
27	17.128	2348	2353	2360	rBV9	10706	19111	0.21%	0.017%
28	17.245	2370	2373	2379	rVB4	10003	17968	0.20%	0.016%
29	17.463	2403	2410	2420	rBV	3946515	5683917	62.72%	5.102%
30	17.563	2420	2427	2445	rVV	6300017	8909507	98.31%	7.998%
31	19.363	2730	2733	2738	rBV2	70772	91261	1.01%	0.082%
32	19.433	2741	2745	2749	rVV	52700	72156	0.80%	0.065%
33	19.792	2800	2806	2815	rBV	6550768	8376381	92.43%	7.519%
34	21.557	3101	3106	3115	rBV	2958254	3989412	44.02%	3.581%
35	23.963	3507	3515	3528	rVB2	3426368	7413285	81.80%	6.655%
36	24.133	3538	3544	3553	rVB	1978105	4216085	46.52%	3.785%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082323\
Data File : BP016713.D
Acq On : 23 Aug 2023 14:08
Operator : MA/JU
Sample : PB155004BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK004

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Title : SVOA CALIBRATION


Sum of corrected areas: 111396050

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082323\
Data File : BP016713.D
Acq On : 23 Aug 2023 14:08
Operator : MA/JU
Sample : PB155004BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK004

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

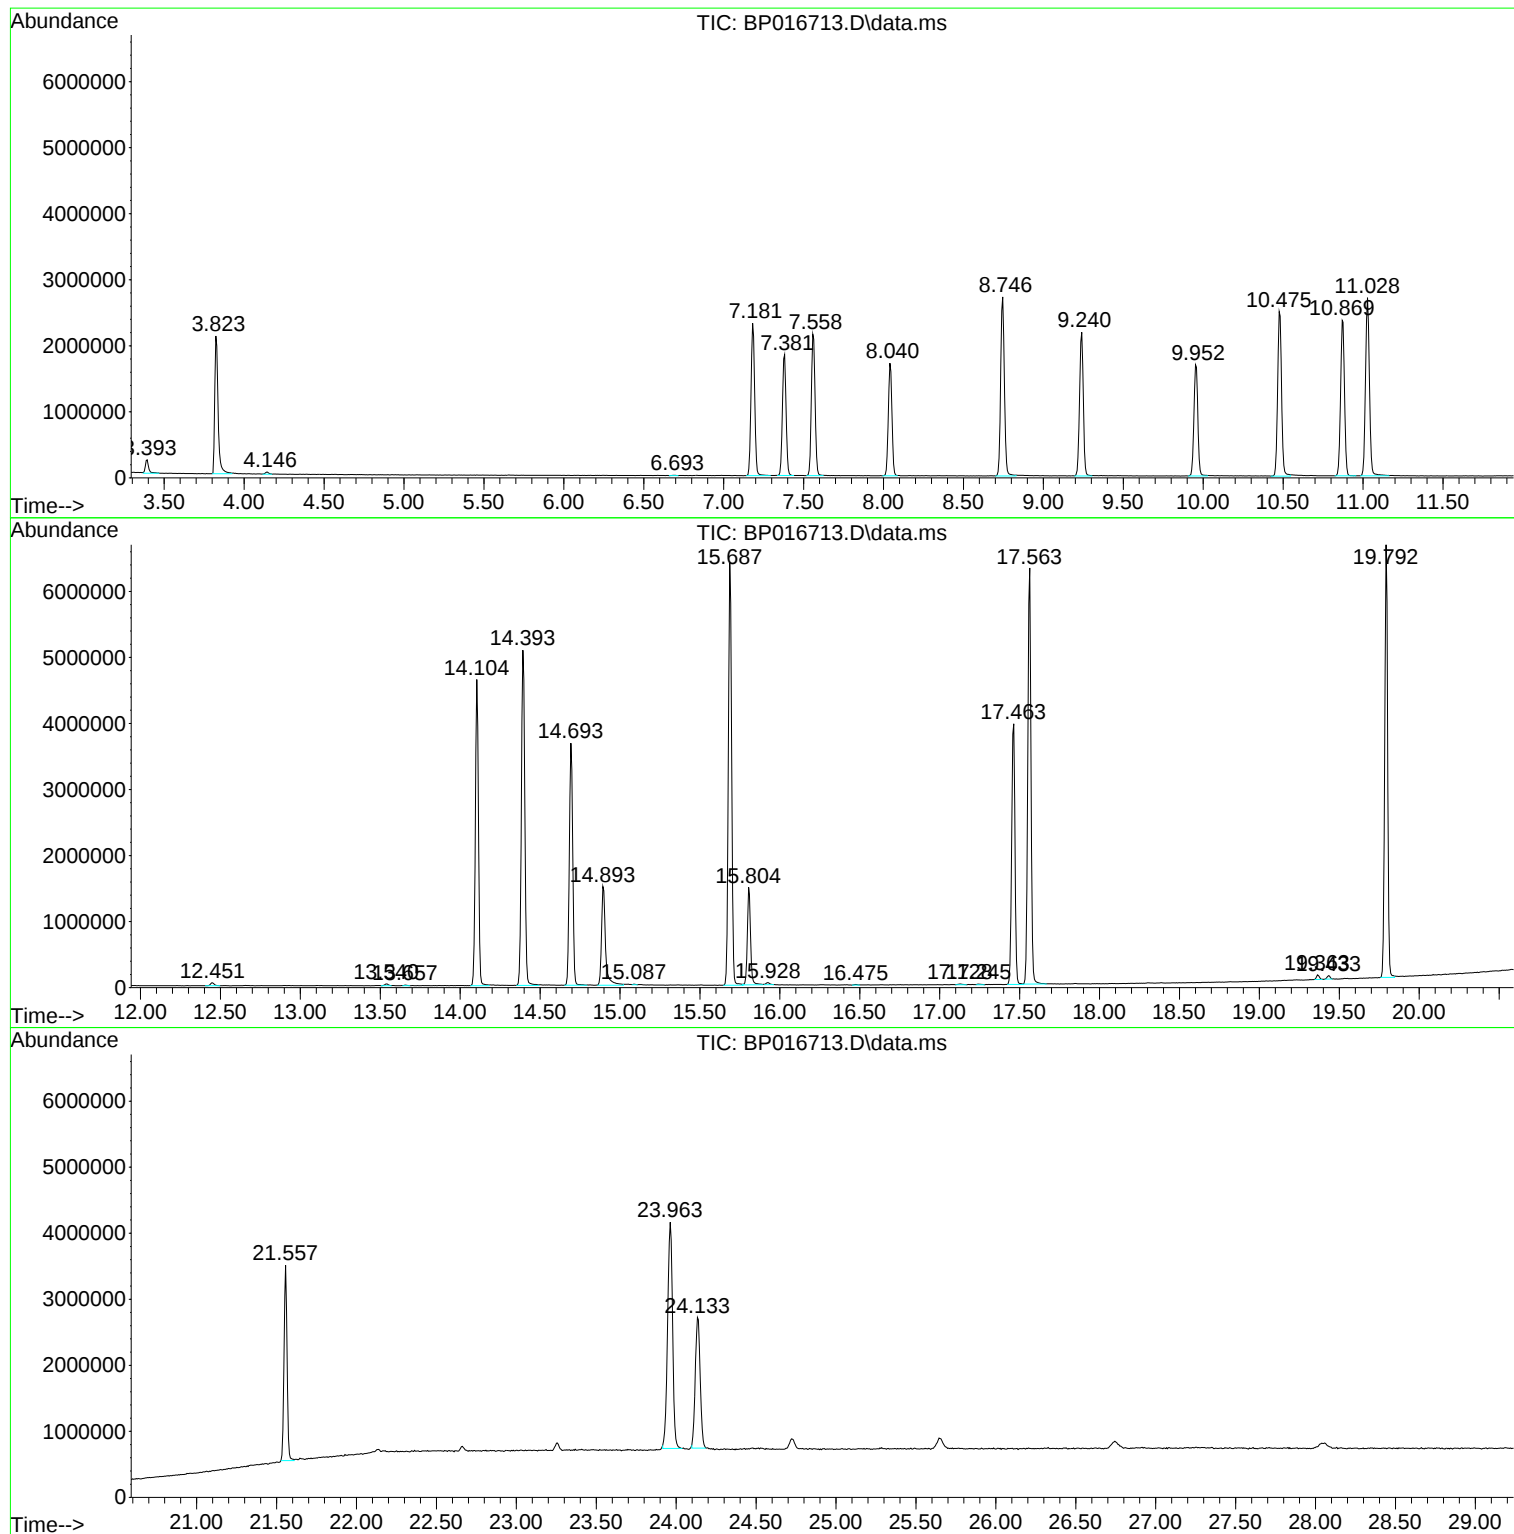

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082323\
Data File : BP016713.D
Acq On : 23 Aug 2023 14:08
Operator : MA/JU
Sample : PB155004BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK004

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082323\
Data File : BP016713.D
Acq On : 23 Aug 2023 14:08
Operator : MA/JU
Sample : PB155004BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK004

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc