

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082323\
 Data File : BP016717.D
 Acq On : 23 Aug 2023 16:24
 Operator : MA/JU
 Sample : 04105-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH8X7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016717.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.346	5	10	15	rBV	291547	459977	5.01%	0.488%
2	3.393	15	18	21	rVV	116503	155260	1.69%	0.165%
3	3.428	21	24	32	rVB	91155	122058	1.33%	0.130%
4	3.828	89	92	113	rBV	544218	843933	9.20%	0.896%
5	4.028	121	126	133	rVB2	48130	75025	0.82%	0.080%
6	4.140	141	145	150	rBV	24309	37662	0.41%	0.040%
7	4.528	208	211	216	rVB6	11637	15701	0.17%	0.017%
8	4.670	229	235	248	rVB	1909014	2875826	31.34%	3.054%
9	5.081	302	305	310	rVB3	9450	13590	0.15%	0.014%
10	5.670	400	405	410	rVB5	8497	16077	0.18%	0.017%
11	7.181	655	662	675	rBV	373771	592224	6.45%	0.629%
12	7.375	686	695	708	rVB	1466162	2291623	24.97%	2.433%
13	7.558	717	726	735	rBV	1320519	2085894	22.73%	2.215%
14	7.634	735	739	747	rVB	24358	45489	0.50%	0.048%
15	8.040	801	808	818	rBV	1491804	2301260	25.08%	2.444%
16	8.746	920	928	940	rBV	1020879	1695485	18.48%	1.800%
17	8.834	940	943	951	rVB6	11772	20274	0.22%	0.022%
18	9.240	1003	1012	1023	rBV	1727326	2832309	30.87%	3.008%
19	9.352	1027	1031	1038	rVB10	6511	13348	0.15%	0.014%
20	9.952	1125	1133	1144	rBV	1334851	2178070	23.74%	2.313%
21	10.122	1159	1162	1173	rVB	5452	12465	0.14%	0.013%
22	10.475	1214	1222	1233	rBV	1814745	3089926	33.67%	3.281%
23	10.869	1280	1289	1298	rBV	2080842	3498742	38.13%	3.715%
24	11.028	1308	1316	1327	rBV	1311041	2221405	24.21%	2.359%
25	11.687	1422	1428	1436	rVV2	20255	33694	0.37%	0.036%
26	12.452	1553	1558	1563	rBV	33539	53172	0.58%	0.056%
27	13.540	1735	1743	1754	rBV	309395	479677	5.23%	0.509%
28	13.663	1759	1764	1767	rVB7	7321	13658	0.15%	0.015%
29	13.875	1797	1800	1805	rBV5	9732	14242	0.16%	0.015%
30	14.104	1833	1839	1852	rBV	3931423	5370507	58.53%	5.703%
31	14.316	1869	1875	1879	rVB9	5280	10125	0.11%	0.011%
32	14.393	1881	1888	1908	rBV	4536958	6362398	69.34%	6.756%
33	14.693	1932	1939	1947	rBV	3242503	4625328	50.41%	4.912%
34	14.898	1968	1974	1994	rBV	196071	412106	4.49%	0.438%
35	15.069	1999	2003	2011	rVB9	7655	19093	0.21%	0.020%
36	15.228	2026	2030	2035	rVB6	8304	13230	0.14%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082323\
 Data File : BP016717.D
 Acq On : 23 Aug 2023 16:24
 Operator : MA/JU
 Sample : 04105-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH8X7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Title : SVOA CALIBRATION

37	15.498	2068	2076	2083	rBV7	8623	20548	0.22%	0.022%
38	15.687	2101	2108	2114	rBV	5591461	7914372	86.25%	8.404%
39	15.745	2114	2118	2123	rVV2	137881	237462	2.59%	0.252%
40	15.804	2123	2128	2144	rVV	1641572	2274138	24.78%	2.415%
41	15.922	2144	2148	2152	rVB2	28207	38400	0.42%	0.041%
42	16.692	2275	2279	2283	rBV	11498	18936	0.21%	0.020%
43	16.804	2295	2298	2303	rVB7	9082	13934	0.15%	0.015%
44	17.128	2350	2353	2360	rVB9	7817	15051	0.16%	0.016%
45	17.251	2369	2374	2379	rBV4	10316	17544	0.19%	0.019%
46	17.457	2403	2409	2420	rBV	3783080	5417743	59.04%	5.753%
47	17.563	2420	2427	2443	rVV	6079394	8775096	95.63%	9.318%
48	18.081	2511	2515	2520	rBV3	38471	48143	0.52%	0.051%
49	18.298	2548	2552	2562	rBV	151005	240814	2.62%	0.256%
50	19.210	2704	2707	2711	rBV	99134	111031	1.21%	0.118%
51	19.369	2730	2734	2737	rVB	71405	93113	1.01%	0.099%
52	19.434	2742	2745	2749	rVV	66541	80792	0.88%	0.086%
53	19.475	2749	2752	2756	rVB2	34562	36977	0.40%	0.039%
54	19.534	2759	2762	2769	rVB5	54076	79554	0.87%	0.084%
55	19.792	2800	2806	2814	rBV	7059363	9176274	100.00%	9.744%
56	21.216	3045	3048	3053	rVB	124098	165314	1.80%	0.176%
57	21.557	3101	3106	3114	rBV2	3022083	4092216	44.60%	4.345%
58	23.963	3508	3515	3526	rVB2	3070037	6637499	72.33%	7.048%
59	24.139	3538	3545	3555	rVB	1722041	3767297	41.05%	4.000%




Sum of corrected areas: 94173101

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082323\
Data File : BP016717.D
Acq On : 23 Aug 2023 16:24
Operator : MA/JU
Sample : 04105-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH8X7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

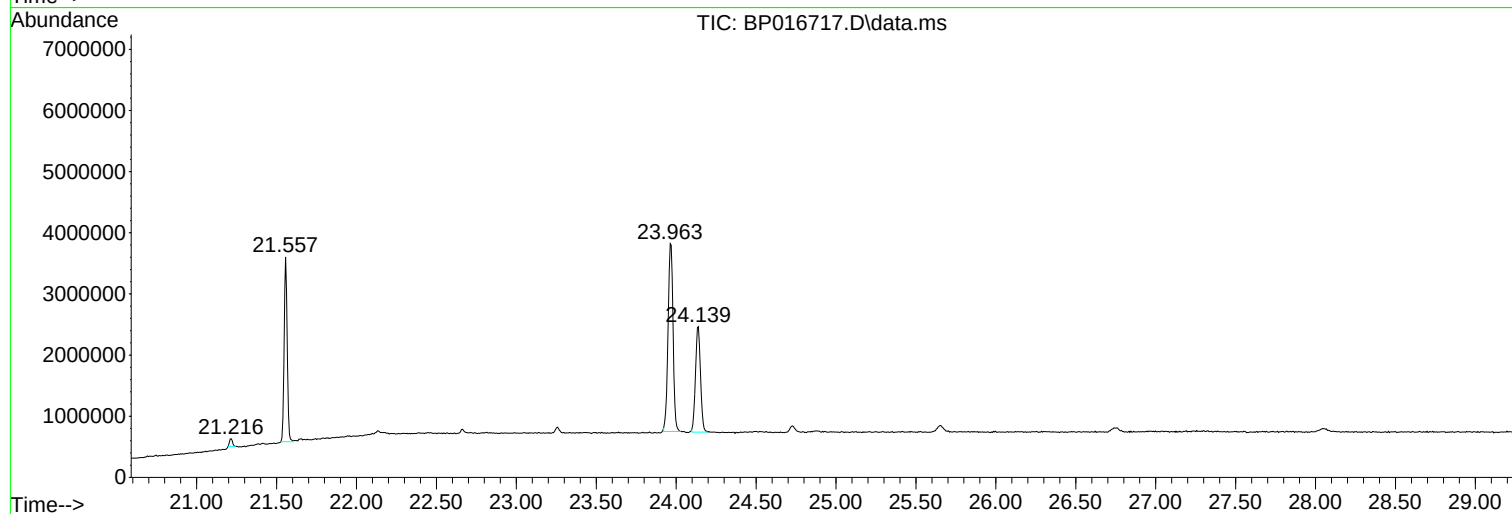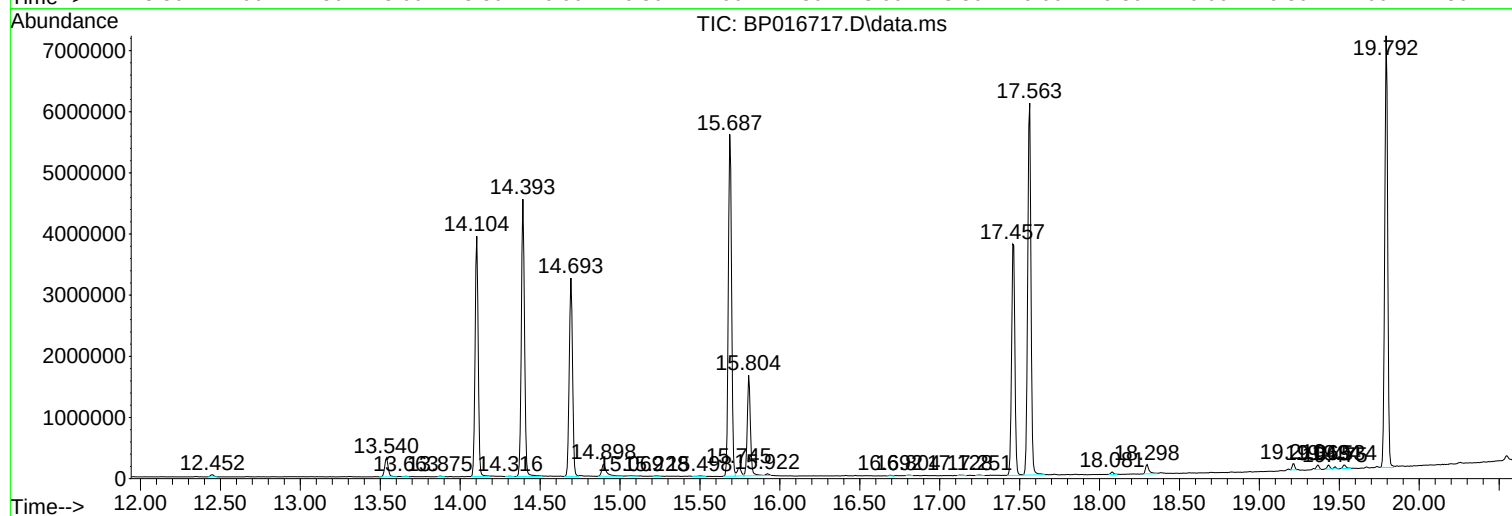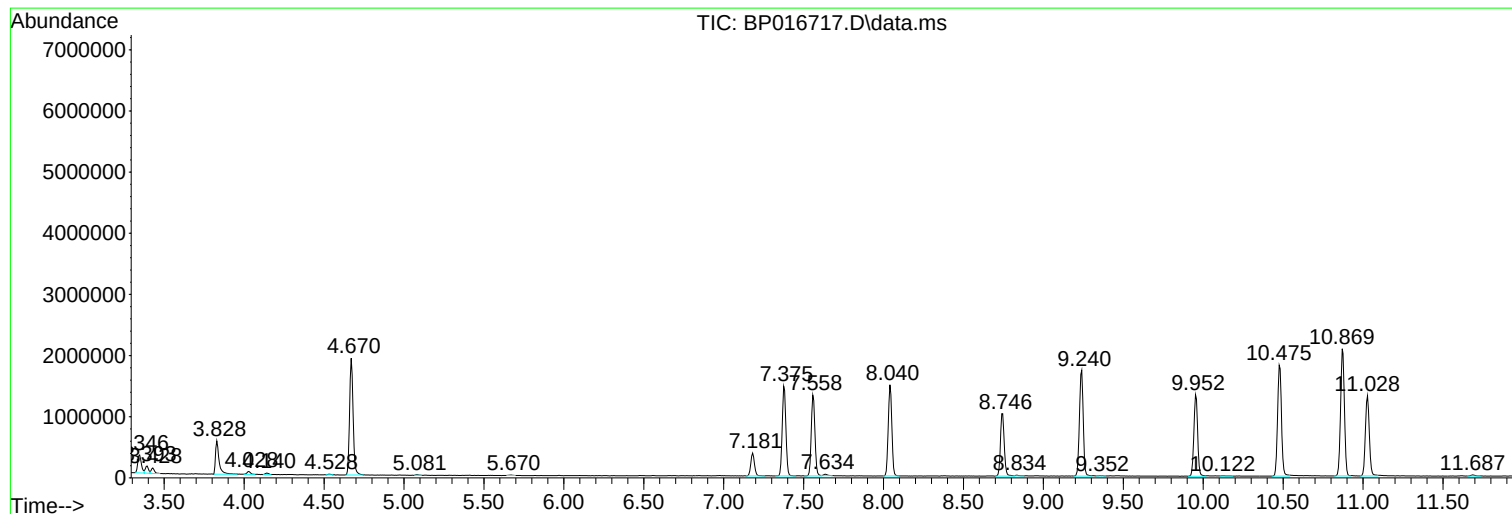

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082323\
Data File : BP016717.D
Acq On : 23 Aug 2023 16:24
Operator : MA/JU
Sample : 04105-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH8X7










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.670	24.99 ng/ul	2875830	1,4-Dichlorobenzene-d4	8.040

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	96
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	96
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	25

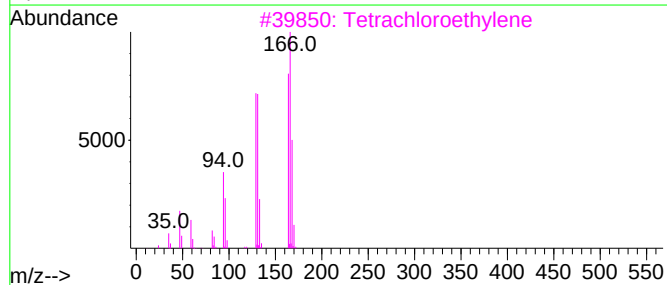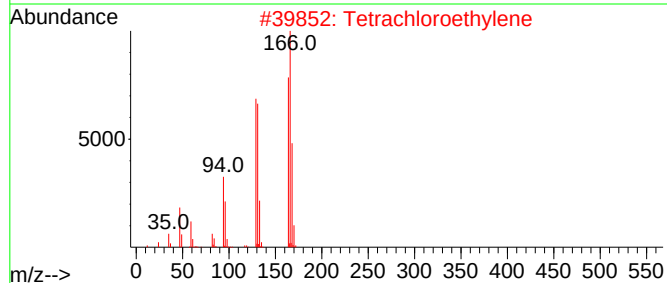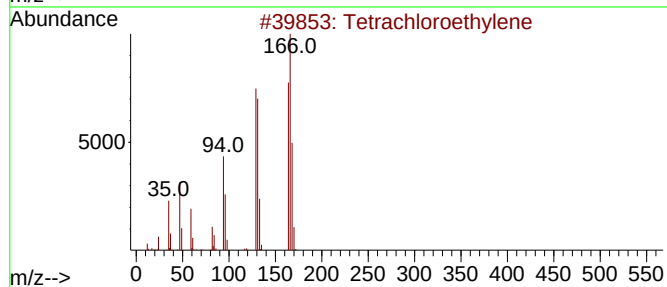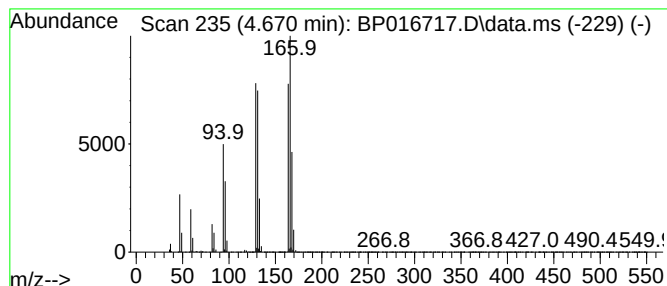

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082323\
Data File : BP016717.D
Acq On : 23 Aug 2023 16:24
Operator : MA/JU
Sample : 04105-04
Misc :
ALS Vial : 7 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
BH8X7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 2,4,7,9-Tetramethyl-5-decyn... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.	
13.540	2.07 ng/ul	479677	Acenaphthene-d10	14.693	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2,4,7,9-Tetramethyl-5-decyn-4,7-...	226	C14H26O2	000126-86-3	87
2	2,4,7,9-Tetramethyl-5-decyn-4,7-...	226	C14H26O2	000126-86-3	64
3	Pyridine, 2-butyl-, 1-oxide	151	C9H13NO	031396-32-4	53
4	Metacetamol	151	C8H9NO2	000621-42-1	47
5	Acetaminophen	151	C8H9NO2	000103-90-2	47

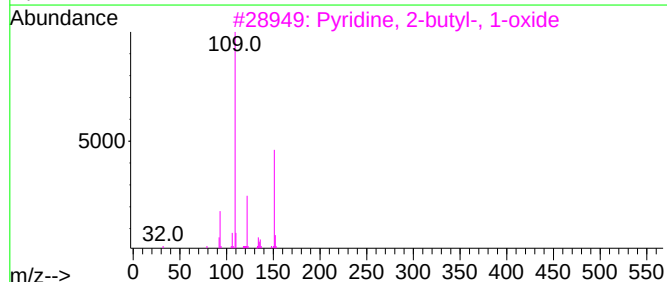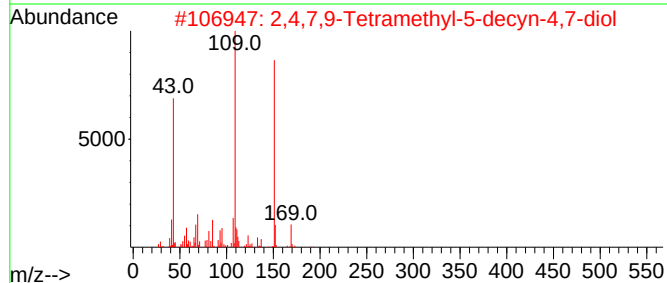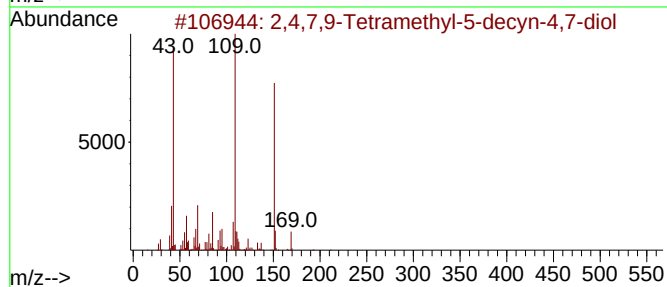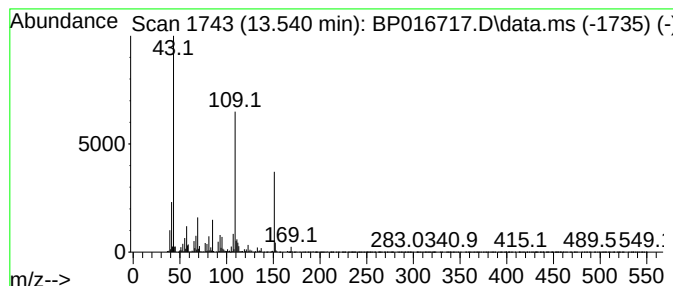

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082323\
Data File : BP016717.D
Acq On : 23 Aug 2023 16:24
Operator : MA/JU
Sample : 04105-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH8X7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.670	25.0	ng/u1	2875830	1	8.040	2301260	20.0
2,4,7,9-Tetrame...	13.540	2.1	ng/u1	479677	3	14.693	4625330	20.0