
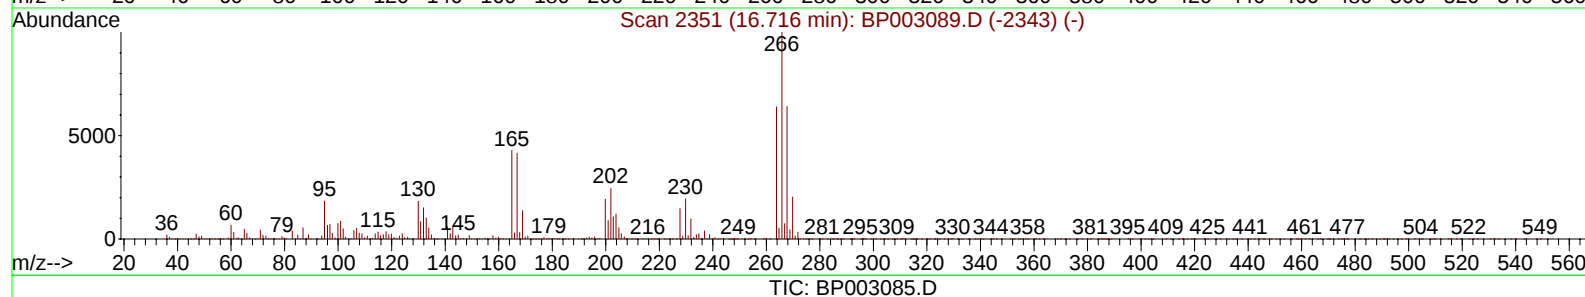
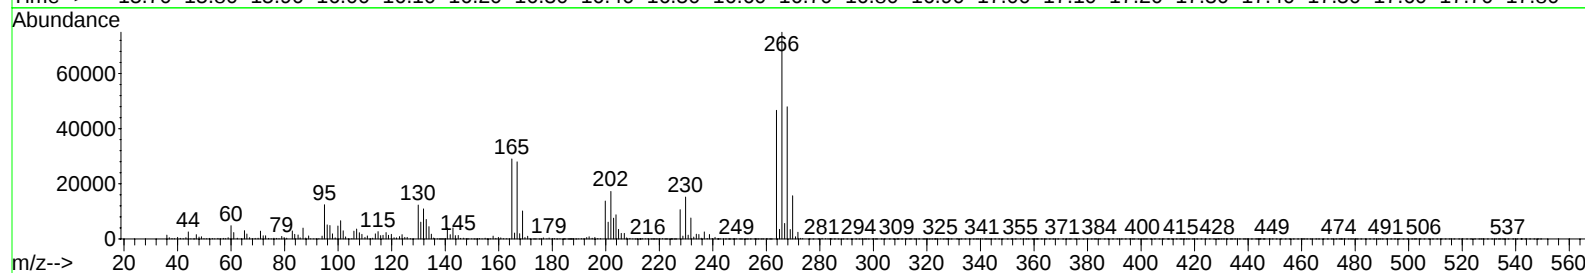


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP082420\
Data File : BP003085.D
Acq On : 24 Aug 2020 09:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 24 18:44:39 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP082420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 24 15:32:08 2020
Response via : Initial Calibration

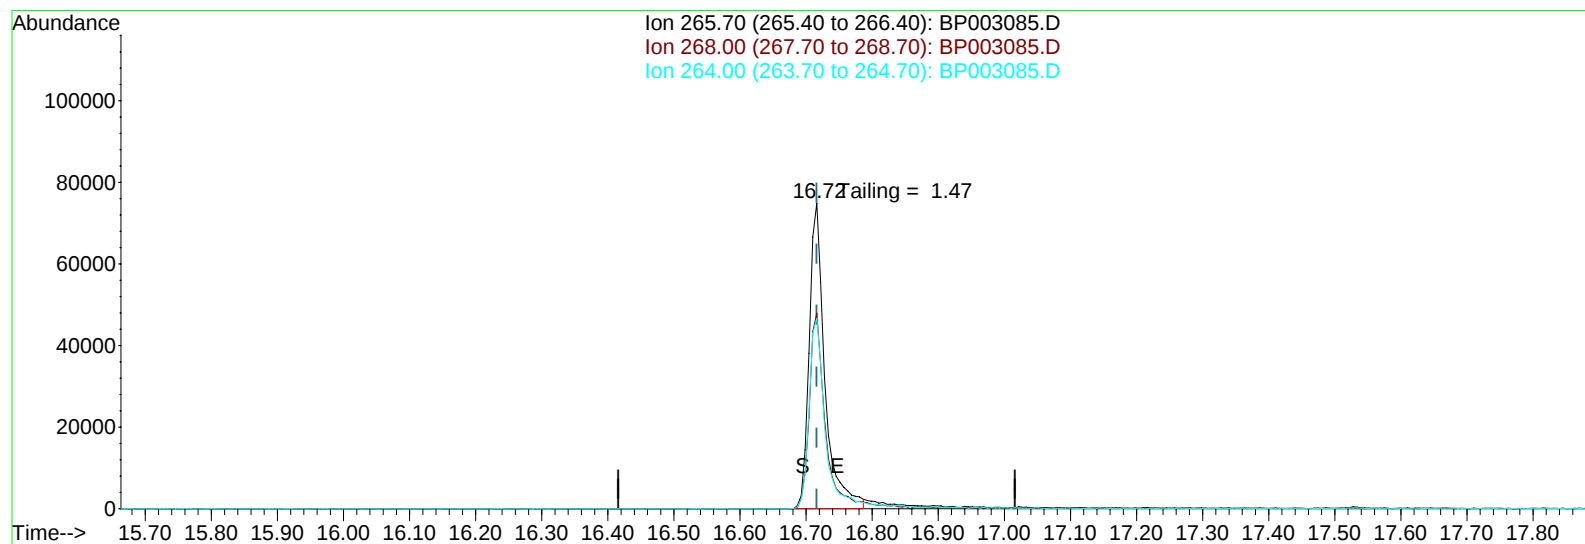

(70) Pentachlorophenol (C)




16.716min (+0.000) 609855.38ng

response 130286

Ion	Exp%	Act%
265.70	100	100
268.00	64.10	63.92
264.00	63.80	62.25
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP082420\
 Data File : BP003085.D
 Acq On : 24 Aug 2020 09:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 24 18:44:39 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP082420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 24 15:32:08 2020
 Response via : Initial Calibration

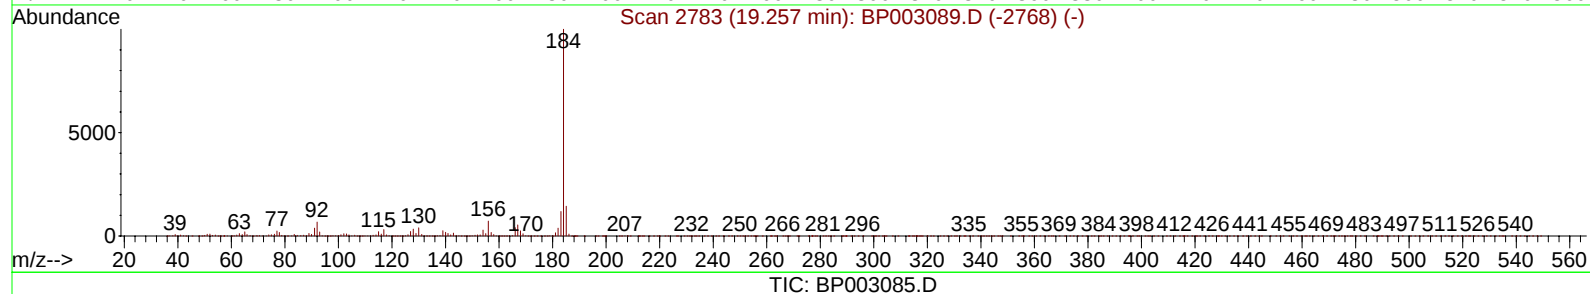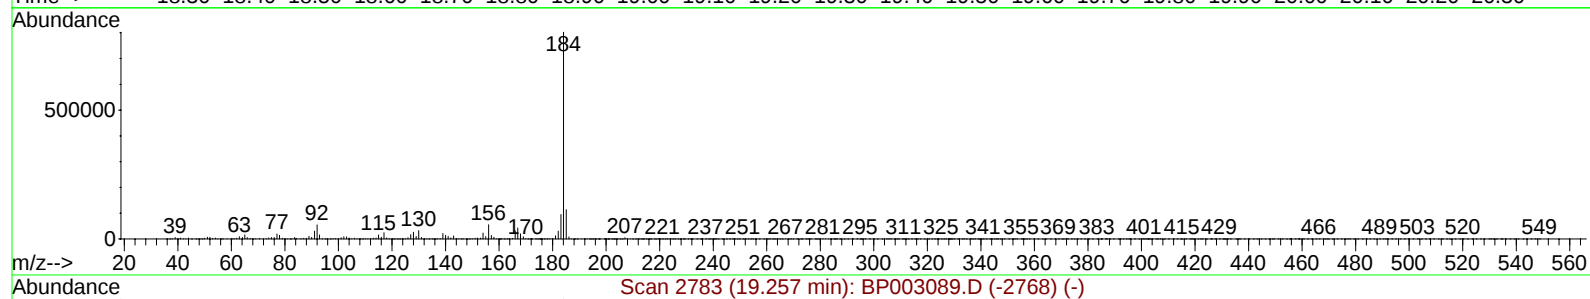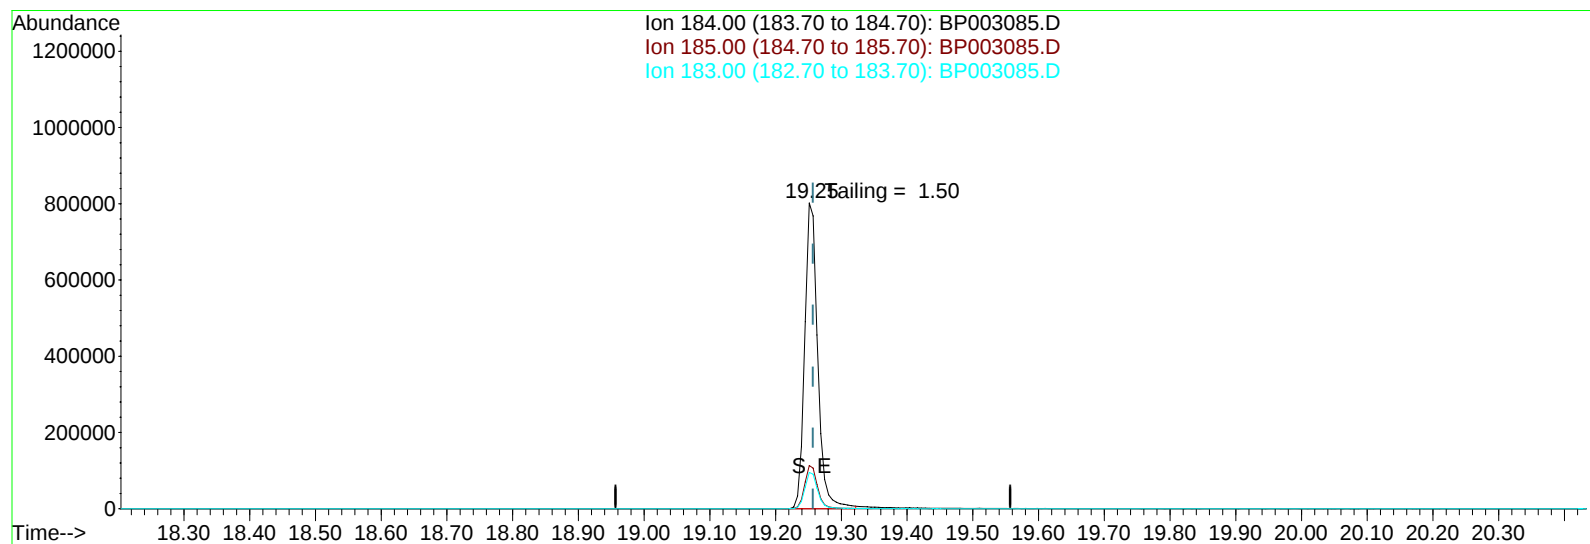

TIC: BP003085.D

(77) Benzidine

19.251min (-0.006) 5447994.75ng

response 1120623

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	14.16
183.00	11.80	11.87
0.00	0.00	0.00