


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082420\
 Data File : BP003085.D
 Acq On : 24 Aug 2020 09:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP082420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 24 15:32:08 2020

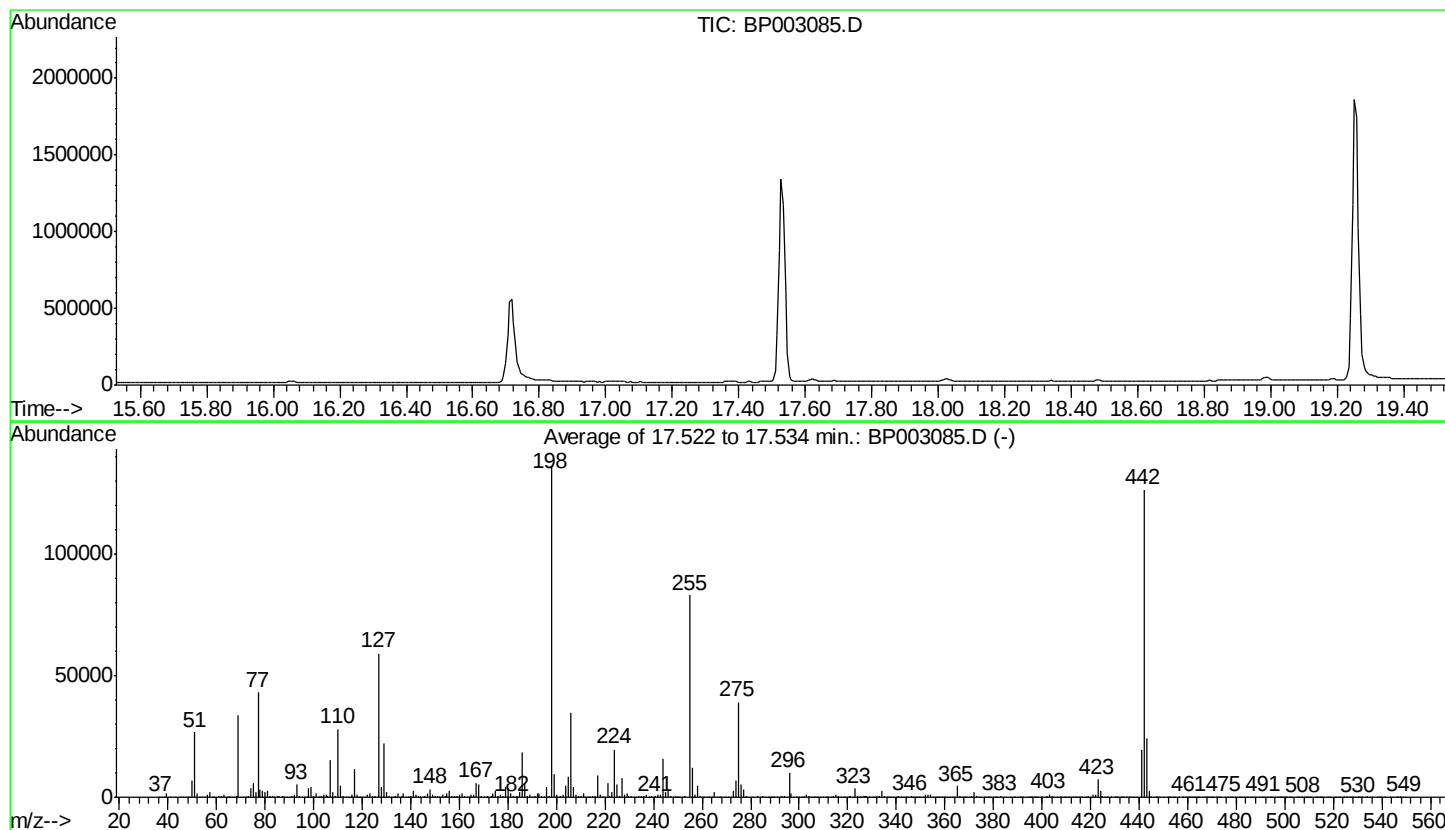

AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.6	26744	PASS
68	69	0.00	2	1.6	526	PASS
69	198	0.00	100	24.8	33717	PASS
70	69	0.00	2	0.1	18	PASS
127	198	10	80	43.3	59017	PASS
197	198	0.00	2	0.3	362	PASS
198	198	100	100	100.0	136158	PASS
199	198	5	9	7.0	9505	PASS
275	198	10	60	28.6	38915	PASS
365	198	1	100	3.4	4694	PASS
441	198	0.01	100	14.2	19304	PASS
442	198	50	100	92.8	126328	PASS
443	442	15	24	19.3	24375	PASS