

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082423\
 Data File : BP016730.D
 Acq On : 24 Aug 2023 16:13
 Operator : MA/JU
 Sample : SSTD04034
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD040634

Quant Time: Aug 25 00:55:14 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 25 00:53:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.040	152	403717	20.000	ng/u1	0.00
20) Naphthalene-d8	10.869	136	1772667	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.692	164	1098838	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.457	188	2422348	20.000	ng/u1	0.00
79) Chrysene-d12	21.557	240	2157689	20.000	ng/u1	0.00
88) Perylene-d12	24.127	264	1980429	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	169050	17.306	ng/uL	0.00
4) Pyridine-d5	3.822	84	1241385	41.586	ng/u1	0.00
7) Phenol-d5	7.181	99	1460387	40.681	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.375	67	933595	40.804	ng/u1	0.00
11) 2-Chlorophenol-d4	7.557	132	1143017	42.348	ng/u1	0.00
15) 4-Methylphenol-d8	8.746	113	1190088	40.610	ng/u1	0.00
21) Nitrobenzene-d5	9.240	128	581968	43.420	ng/u1	0.00
24) 2-Nitrophenol-d4	9.951	143	629279	44.542	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.481	165	1133814	43.048	ng/u1	0.00
31) 4-Chloroaniline-d4	11.028	131	1669746	41.339	ng/u1	0.00
46) Dimethylphthalate-d6	14.104	166	3427607	41.363	ng/u1	0.00
49) Acenaphthylene-d8	14.392	160	3979491	42.480	ng/u1	0.00
54) 4-Nitrophenol-d4	14.904	143	694505	40.548	ng/u1	0.00
60) Fluorene-d10	15.686	176	2882040	41.300	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.816	200	595701	41.294	ng/u1	0.00
73) Anthracene-d10	17.563	188	4475834	41.685	ng/u1	0.00
81) Pyrene-d10	19.792	212	5182345	43.731	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.962	264	4225276	42.593	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.422	88	178284	16.760	ng/uL	99
5) Pyridine	3.840	79	1274565	41.451	ng/u1	99
6) Benzaldehyde	7.193	77	835546	42.561	ng/u1	99
8) Phenol	7.210	94	1527164	40.649	ng/u1	100
10) Bis(2-Chloroethyl)ether	7.469	93	1243708	41.012	ng/u1	99
12) 2-Chlorophenol	7.593	128	1154736	41.855	ng/u1	98
13) 2-Methylphenol	8.475	108	1147823	40.730	ng/u1	100
14) 2,2'-oxybis(1-Chloropr...	8.551	45	1101029	24.888	ng/u1	98
16) Acetophenone	8.893	105	1868699	41.124	ng/u1	98
17) N-Nitroso-di-n-propyla...	8.869	70	1007820	42.085	ng/u1	99
18) 4-Methylphenol	8.816	108	1247712	40.658	ng/u1	98
19) Hexachloroethane	9.110	117	475885	41.456	ng/u1	99
22) Nitrobenzene	9.281	77	1444181	42.000	ng/u1	100
23) Isophorone	9.798	82	2825133	42.303	ng/u1	99
25) 2-Nitrophenol	9.987	139	682203	43.671	ng/u1	100
26) 2,4-Dimethylphenol	10.022	107	1315229	41.890	ng/u1	99
27) Bis(2-Chloroethoxy)met...	10.281	93	1715802	41.644	ng/u1	99
29) 2,4-Dichlorophenol	10.504	162	1120818	42.364	ng/u1	99
30) Naphthalene	10.922	128	3767683	41.030	ng/u1	100
32) 4-Chloroaniline	11.051	127	1637764	41.260	ng/u1	100
33) Hexachlorobutadiene	11.151	225	669433	41.077	ng/u1	98
34) Caprolactam	11.881	113	276291	28.079	ng/u1	97
35) 4-Chloro-3-methylphenol	12.145	107	1253636	42.255	ng/u1	99
36) 2-Methylnaphthalene	12.522	142	2613601	41.235	ng/u1	100

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082423\
 Data File : BP016730.D
 Acq On : 24 Aug 2023 16:13
 Operator : MA/JU
 Sample : SST04034
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SST040634


Quant Time: Aug 25 00:55:14 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 25 00:53:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.739	142	2628288	41.121	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.869	216	1315932	42.018	ng/ul	99
40) Hexachlorocyclopentadiene	12.822	237	830778	36.071	ng/ul	99
41) 2,4,6-Trichlorophenol	13.122	196	909915	43.507	ng/ul	99
42) 2,4,5-Trichlorophenol	13.187	196	983930	43.477	ng/ul	98
43) 1,1'-Biphenyl	13.528	154	3393241	41.533	ng/ul	99
44) 2-Chloronaphthalene	13.575	162	2692733	41.751	ng/ul	99
45) 2-Nitroaniline	13.804	65	858124	43.873	ng/ul	97
47) Dimethylphthalate	14.151	163	3440042	40.990	ng/ul	100
48) 2,6-Dinitrotoluene	14.292	165	728424	44.302	ng/ul	99
50) Acenaphthylene	14.422	152	4463411	41.628	ng/ul	100
51) 3-Nitroaniline	14.634	138	707969	41.344	ng/ul	97
52) Acenaphthene	14.757	153	2927258	41.267	ng/ul	99
53) 2,4-Dinitrophenol	14.828	184	416426	34.848	ng/ul	100
55) 4-Nitrophenol	14.916	109	524035	40.512	ng/ul	98
56) Dibenzofuran	15.092	168	3961950	40.706	ng/ul	99
57) 2,4-Dinitrotoluene	15.075	165	1054168	43.551	ng/ul	98
58) 2,3,4,6-Tetrachlorophenol	15.304	232	815653	42.335	ng/ul	99
59) Diethylphthalate	15.504	149	3482684	40.849	ng/ul	99
61) Fluorene	15.745	166	3298997	40.523	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.733	204	1635993	40.930	ng/ul	98
63) 4-Nitroaniline	15.804	138	673318	41.322	ng/ul	99
66) 4,6-Dinitro-2-methylph...	15.828	198	637235	40.972	ng/ul	99
67) N-Nitrosodiphenylamine	15.957	169	2788716	41.624	ng/ul	100
68) 4-Bromophenyl-phenylether	16.633	248	963038	41.467	ng/ul	93
69) Hexachlorobenzene	16.716	284	1057974	40.686	ng/ul	95
70) Atrazine	16.910	200	1073972	42.519	ng/ul	99
71) Pentachlorophenol	17.080	266	739357	38.303	ng/ul	100
72) Phenanthrene	17.504	178	5226205	40.982	ng/ul	99
74) Anthracene	17.598	178	5321310	41.268	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.481	216	1395600	43.028	ng/ul	99
76) Pentachlorobenzene	14.981	250	1210192	41.751	ng/ul	98
77) Carbazole	17.875	167	4868402	41.922	ng/ul	99
78) Di-n-butylphthalate	18.386	149	6118705	42.231	ng/ul	100
80) Fluoranthene	19.463	202	6250282	43.907	ng/ul	99
82) Pyrene	19.821	202	6321101	42.987	ng/ul	99
83) Butylbenzylphthalate	20.674	149	2855241	45.024	ng/ul	100
84) 3,3'-Dichlorobenzidine	21.474	252	1982423	42.985	ng/ul	99
85) Benzo(a)anthracene	21.539	228	6187433	41.632	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.410	149	4133193	44.636	ng/ul	100
87) Chrysene	21.598	228	5607046	41.532	ng/ul	99
89) Di-n-octyl phthalate	22.392	149	6865498	46.029	ng/ul	100
90) Benzo(b)fluoranthene	23.327	252	5330643	42.151	ng/ul	100
91) Benzo(k)fluoranthene	23.380	252	5478791	43.805	ng/ul	99
93) Benzo(a)pyrene	24.015	252	4879787	42.659	ng/ul	100
94) Indeno(1,2,3-cd)pyrene	26.868	276	4720869	40.387	ng/ul	99
95) Dibenzo(a,h)anthracene	26.898	278	3944189	40.626	ng/ul	99
96) Benzo(g,h,i)perylene	27.727	276	3572356	40.311	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Aug 25 00:55:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 25 00:53:07 2023
Response via : Initial Calibration







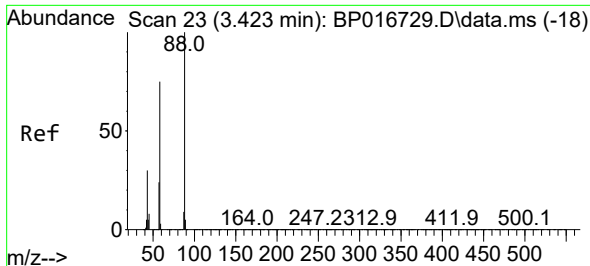

#2
1,4-Dioxane
Concen: 16.760 ng/uL
RT: 3.422 min Scan# 21
Delta R.T. -0.000 min
Lab File: BP016730.D
Acq: 24 Aug 2023 16:13




Instrument :
BNA_P
ClientSampleId :
SSTD040634


Tgt Ion: 88 Resp: 178284
Ion Ratio Lower Upper
88 100
43 29.3 24.0 36.0
58 73.9 59.8 89.8

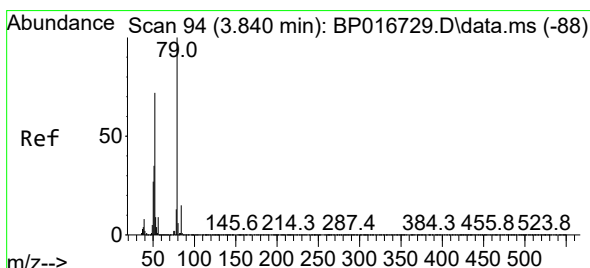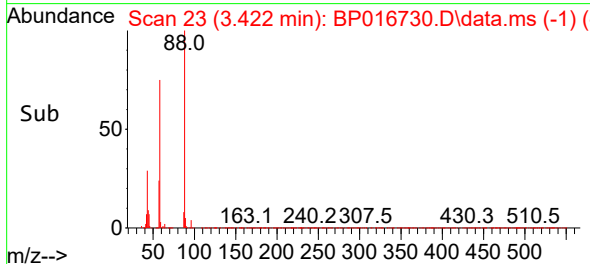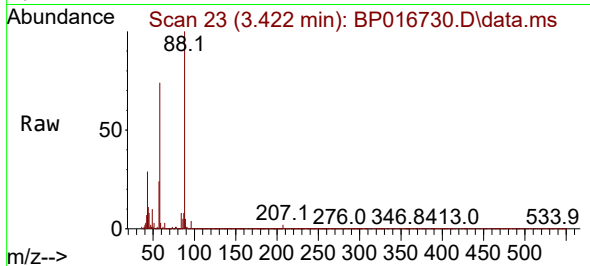

#5
Pyridine
Concen: 41.451 ng/uL
RT: 3.840 min Scan# 94
Delta R.T. -0.000 min
Lab File: BP016730.D
Acq: 24 Aug 2023 16:13

Tgt Ion: 79 Resp: 1274565
Ion Ratio Lower Upper
79 100
52 75.1 59.6 89.4
51 34.5 28.2 42.2


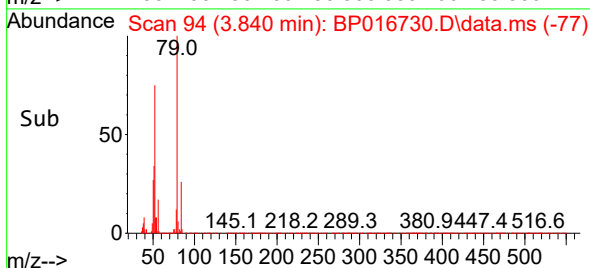
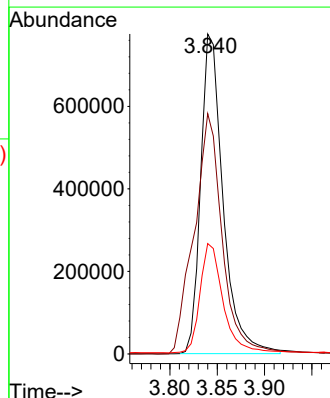
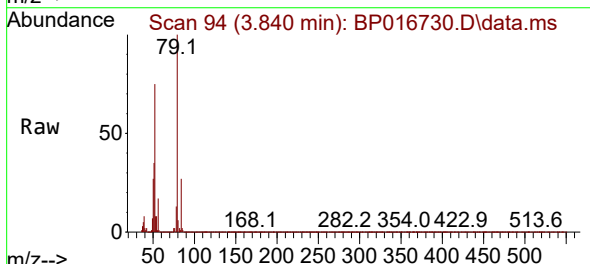




#6
Benzaldehyde
Concen: 42.561 ng/ul
RT: 7.193 min Scan# 664
Delta R.T. -0.000 min
Lab File: BP016730.D
Acq: 24 Aug 2023 16:13




Instrument :
BNA_P
ClientSampleId :
SSTD040634


Tgt Ion: 77 Resp: 835546
Ion Ratio Lower Upper
77 100
105 93.8 75.4 113.2
106 90.0 73.1 109.7

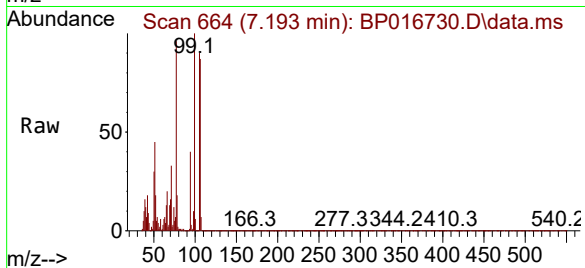

#8
Phenol
Concen: 40.649 ng/ul
RT: 7.210 min Scan# 667
Delta R.T. -0.000 min
Lab File: BP016730.D
Acq: 24 Aug 2023 16:13

Tgt Ion: 94 Resp: 1527164
Ion Ratio Lower Upper
94 100
65 28.2 22.4 33.6
66 35.9 28.6 42.8

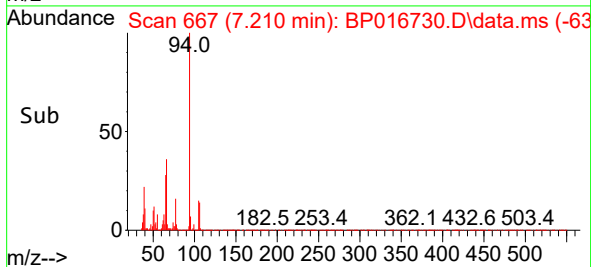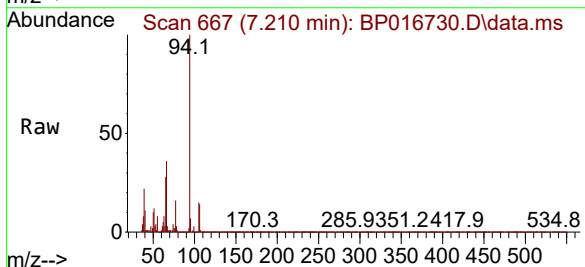







#10
Bis(2-Chloroethyl)ether
Concen: 41.012 ng/ul
RT: 7.469 min Scan# 711
Delta R.T. -0.000 min
Lab File: BP016730.D
Acq: 24 Aug 2023 16:13

Instrument :
BNA_P
ClientSampleId :
SSTD040634

Tgt Ion: 93 Resp: 1243708




Ion	Ratio	Lower	Upper
93	100		
63	77.6	62.9	94.3
95	32.2	26.3	39.5

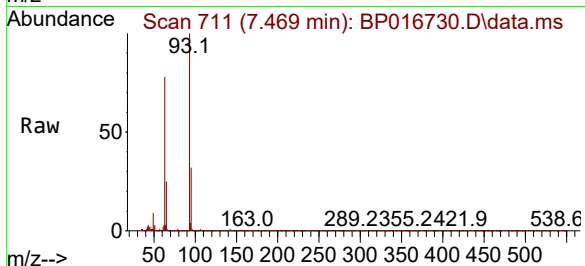


#12
2-Chlorophenol
Concen: 41.855 ng/ul
RT: 7.593 min Scan# 732
Delta R.T. -0.000 min
Lab File: BP016730.D
Acq: 24 Aug 2023 16:13

Tgt Ion: 128 Resp: 1154736

Ion	Ratio	Lower	Upper
128	100		
64	48.3	40.0	60.0
130	32.3	26.4	39.6

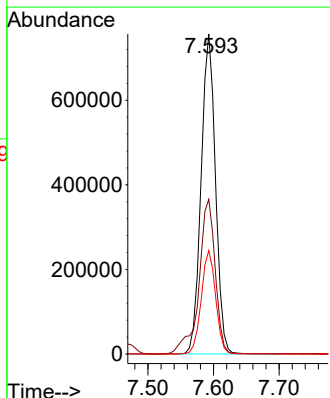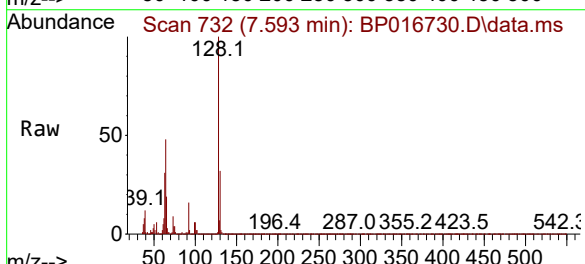



#13

2-Methylphenol

Concen: 40.730 ng/ul

RT: 8.475 min Scan# 882

Delta R.T. -0.000 min

Lab File: BP016730.D

Acq: 24 Aug 2023 16:13

Instrument :

BNA_P

ClientSampleId :





SSTD040634

Tgt Ion:108 Resp: 1147823

Ion Ratio Lower Upper

108 100

107 89.7 71.4 107.2

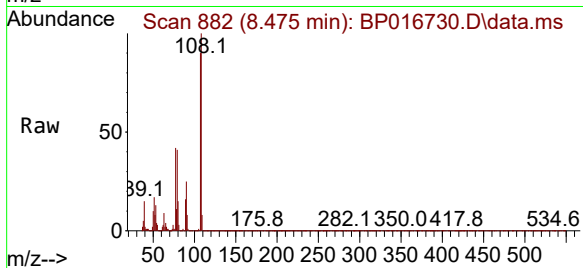

#14

2,2'-oxybis(1-Chloropropane)

Concen: 24.888 ng/ul

RT: 8.551 min Scan# 895

Delta R.T. -0.000 min

Lab File: BP016730.D

Acq: 24 Aug 2023 16:13




Tgt Ion: 45 Resp: 1101029


Ion Ratio Lower Upper

45 100

77 14.9 11.1 16.7

79 10.6 8.2 12.4




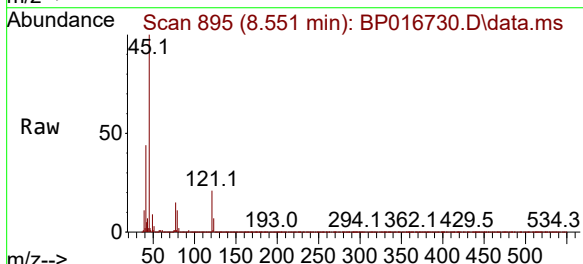




#16
Acetophenone
Concen: 41.124 ng/ul
RT: 8.893 min Scan# 91
Delta R.T. 0.006 min
Lab File: BP016730.D
Acq: 24 Aug 2023 16:13




Instrument :
BNA_P
ClientSampleId :
SSTD040634


Tgt Ion:105 Resp: 1868699
Ion Ratio Lower Upper
105 100
77 79.0 64.2 96.4
51 26.9 22.2 33.4



#17
N-Nitroso-di-n-propylamine
Concen: 42.085 ng/ul
RT: 8.869 min Scan# 949
Delta R.T. 0.006 min
Lab File: BP016730.D
Acq: 24 Aug 2023 16:13

Tgt Ion: 70 Resp: 1007820
Ion Ratio Lower Upper
70 100
42 56.5 46.0 69.0
101 9.5 7.6 11.4
130 20.6 16.1 24.1

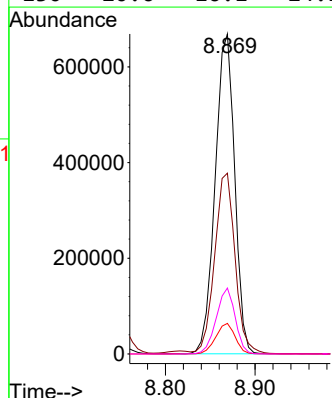



#18

4-Methylphenol

Concen: 40.658 ng/ul

RT: 8.816 min Scan# 940

Delta R.T. 0.006 min

Lab File: BP016730.D

Acq: 24 Aug 2023 16:13

Instrument :

BNA_P

ClientSampleId :





SSTD040634

Tgt Ion:108 Resp: 1247712

Ion Ratio Lower Upper

108 100

107 110.3 89.8 134.6

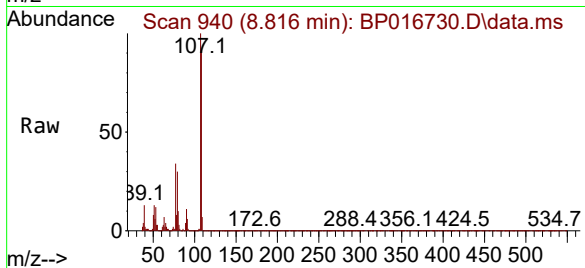

#19

Hexachloroethane

Concen: 41.456 ng/ul

RT: 9.110 min Scan# 990

Delta R.T. -0.000 min

Lab File: BP016730.D

Acq: 24 Aug 2023 16:13




Tgt Ion:117 Resp: 475885


Ion Ratio Lower Upper

117 100

201 95.5 75.4 113.2

199 60.8 47.8 71.6


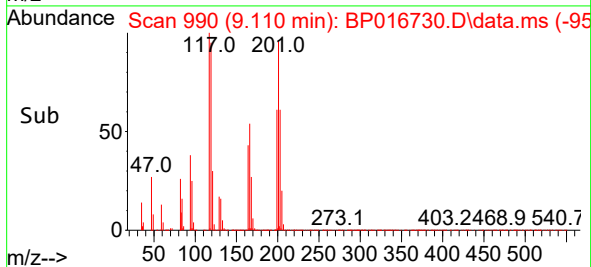

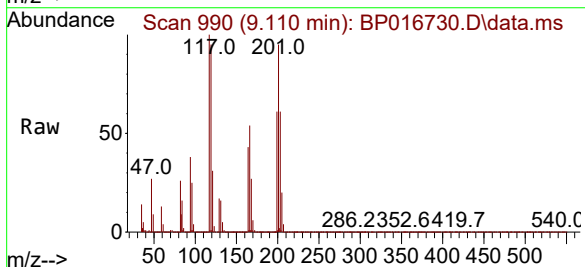




#22
Nitrobenzene
Concen: 42.000 ng/ul
RT: 9.281 min Scan# 1019
Delta R.T. -0.000 min
Lab File: BP016730.D
Acq: 24 Aug 2023 16:13




Instrument :
BNA_P
ClientSampleId :
SSTD040634


Tgt Ion: 77 Resp: 1444181
Ion Ratio Lower Upper
77 100
123 43.3 34.9 52.3
65 13.1 10.6 15.8



#23
Isophorone
Concen: 42.303 ng/ul
RT: 9.798 min Scan# 1107
Delta R.T. -0.000 min
Lab File: BP016730.D
Acq: 24 Aug 2023 16:13

Tgt Ion: 82 Resp: 2825133
Ion Ratio Lower Upper
82 100
95 6.8 5.4 8.0
138 16.6 13.5 20.3









#25
2-Nitrophenol
Concen: 43.671 ng/ul
RT: 9.987 min Scan# 1139
Delta R.T. -0.000 min
Lab File: BP016730.D
Acq: 24 Aug 2023 16:13




Instrument :
BNA_P
ClientSampleId :
SSTD040634


Tgt Ion:139 Resp: 682203
Ion Ratio Lower Upper
139 100
65 52.4 42.0 63.0
109 29.0 23.4 35.2



#26
2,4-Dimethylphenol
Concen: 41.890 ng/ul
RT: 10.022 min Scan# 1145
Delta R.T. -0.000 min
Lab File: BP016730.D
Acq: 24 Aug 2023 16:13

Tgt Ion:107 Resp: 1315229
Ion Ratio Lower Upper
107 100
121 49.9 40.7 61.1
122 85.9 69.7 104.5









#27
 Bis(2-Chloroethoxy)methane
 Concen: 41.644 ng/ul
 RT: 10.281 min Scan# 1189
 Delta R.T. -0.000 min
 Lab File: BP016730.D
 Acq: 24 Aug 2023 16:13

Instrument :
 BNA_P
 ClientSampleId :
 SSTD040634

Tgt Ion: 93 Resp: 1715802




Ion	Ratio	Lower	Upper
93	100		
95	32.2	26.3	39.5
123	10.9	8.8	13.2

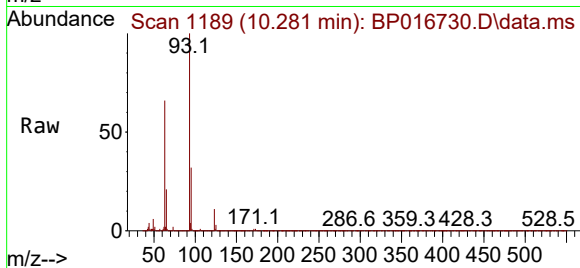


#29
 2,4-Dichlorophenol
 Concen: 42.364 ng/ul
 RT: 10.504 min Scan# 1227
 Delta R.T. -0.000 min
 Lab File: BP016730.D
 Acq: 24 Aug 2023 16:13

Tgt Ion: 162 Resp: 1120818

Ion	Ratio	Lower	Upper
162	100		
164	65.2	52.2	78.2
98	37.7	29.3	43.9




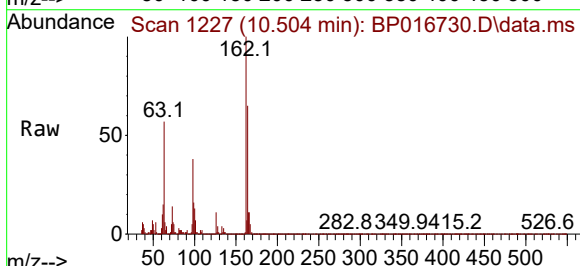




#30
Naphthalene
Concen: 41.030 ng/ul
RT: 10.922 min Scan# 1298
Delta R.T. -0.000 min
Lab File: BP016730.D
Acq: 24 Aug 2023 16:13




Instrument :
BNA_P
ClientSampleId :
SSTD040634


Tgt Ion:128 Resp: 3767683
Ion Ratio Lower Upper
128 100
129 11.0 8.8 13.2
127 13.2 10.3 15.5



#32
4-Chloroaniline
Concen: 41.260 ng/ul
RT: 11.051 min Scan# 1320
Delta R.T. -0.000 min
Lab File: BP016730.D
Acq: 24 Aug 2023 16:13

Tgt Ion:127 Resp: 1637764
Ion Ratio Lower Upper
127 100
129 32.2 25.9 38.9





#33

Hexachlorobutadiene

Concen: 41.077 ng/ul

RT: 11.151 min Scan# 11

Delta R.T. -0.000 min

Lab File: BP016730.D

Acq: 24 Aug 2023 16:13

Instrument :

BNA_P

ClientSampleId :

SSTD040634





Tgt Ion:225 Resp: 669433

Ion Ratio Lower Upper

225 100

223 62.6 51.0 76.4

227 63.8 52.5 78.7

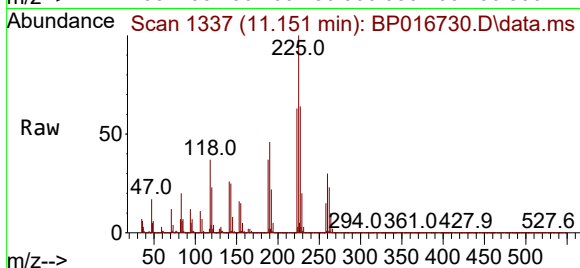

#34

Caprolactam

Concen: 28.079 ng/ul

RT: 11.881 min Scan# 1461

Delta R.T. 0.006 min

Lab File: BP016730.D

Acq: 24 Aug 2023 16:13




Tgt Ion:113 Resp: 276291


Ion Ratio Lower Upper

113 100

55 173.3 140.6 210.8

56 125.3 104.5 156.7




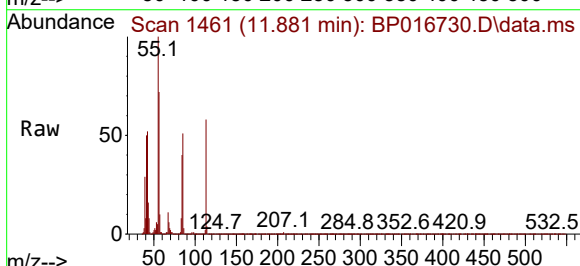




#35
4-Chloro-3-methylphenol
Concen: 42.255 ng/ul
RT: 12.145 min Scan# 1506
Delta R.T. -0.000 min
Lab File: BP016730.D
Acq: 24 Aug 2023 16:13




Instrument :
BNA_P
ClientSampleId :
SSTD040634


Tgt Ion:107 Resp: 1253636
Ion Ratio Lower Upper
107 100
144 25.3 20.6 31.0
142 79.3 63.7 95.5



#36
2-Methylnaphthalene
Concen: 41.235 ng/ul
RT: 12.522 min Scan# 1570
Delta R.T. -0.000 min
Lab File: BP016730.D
Acq: 24 Aug 2023 16:13

Tgt Ion:142 Resp: 2613601
Ion Ratio Lower Upper
142 100
141 88.9 71.4 107.0

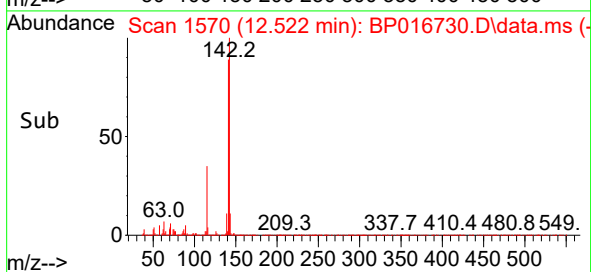



#37

1-Methylnaphthalene

Concen: 41.121 ng/ul

RT: 12.739 min Scan# 1

Delta R.T. -0.000 min

Lab File: BP016730.D

Acq: 24 Aug 2023 16:13

Instrument :

BNA_P

ClientSampleId :

SSTD040634





Tgt Ion:142 Resp: 2628288

Ion Ratio Lower Upper

142 100

141 92.2 73.0 109.4

116 3.9 3.1 4.7

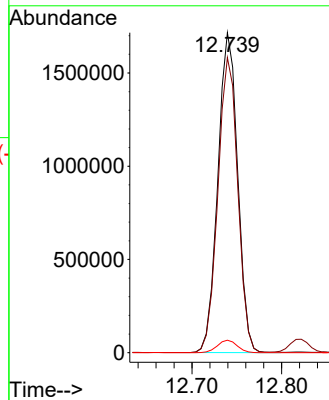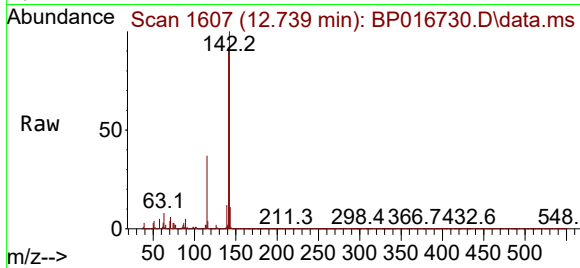

#39

1,2,4,5-Tetrachlorobenzene

Concen: 42.018 ng/ul

RT: 12.869 min Scan# 1629

Delta R.T. -0.000 min

Lab File: BP016730.D

Acq: 24 Aug 2023 16:13

Tgt Ion:216 Resp: 1315932




Ion Ratio Lower Upper


216 100

214 79.9 63.4 95.2

179 22.0 17.4 26.2

108 18.2 15.3 22.9


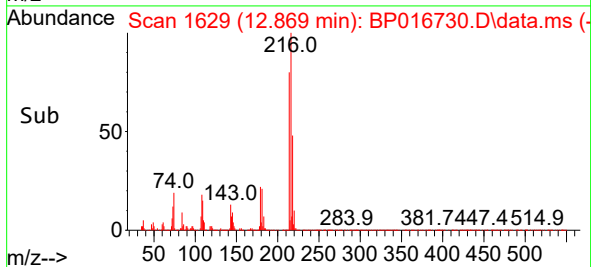
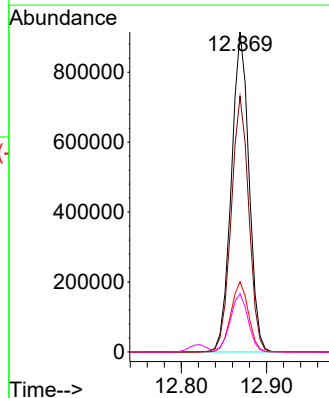
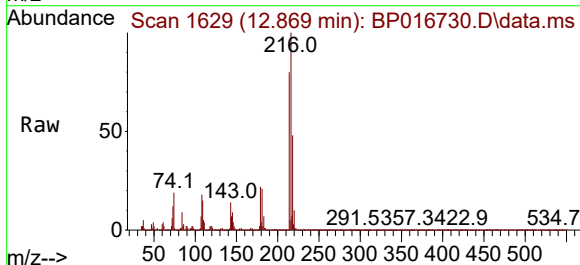




#40
Hexachlorocyclopentadiene
Concen: 36.071 ng/ul
RT: 12.822 min Scan# 1621
Delta R.T. -0.000 min
Lab File: BP016730.D
Acq: 24 Aug 2023 16:13




Instrument :
BNA_P
ClientSampleId :
SSTD040634


Tgt Ion:237 Resp: 830778
Ion Ratio Lower Upper
237 100
235 63.2 51.3 76.9
272 12.2 9.8 14.8



#41
2,4,6-Trichlorophenol
Concen: 43.507 ng/ul
RT: 13.122 min Scan# 1672
Delta R.T. -0.000 min
Lab File: BP016730.D
Acq: 24 Aug 2023 16:13

Tgt Ion:196 Resp: 909915
Ion Ratio Lower Upper
196 100
198 97.2 76.6 115.0
200 31.2 25.2 37.8









#42
2,4,5-Trichlorophenol
Concen: 43.477 ng/ul
RT: 13.187 min Scan# 1683
Delta R.T. -0.000 min
Lab File: BP016730.D
Acq: 24 Aug 2023 16:13




Instrument :
BNA_P
ClientSampleId :
SSTD040634


Tgt Ion:196 Resp: 983930
Ion Ratio Lower Upper
196 100
198 94.7 77.8 116.8
200 31.0 24.8 37.2

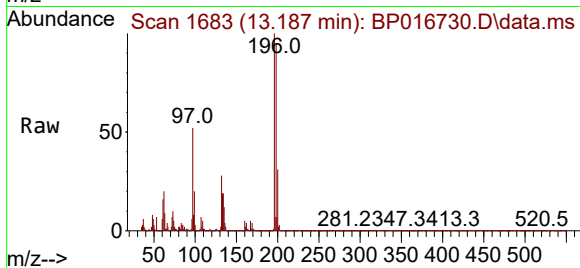

#43
1,1'-Biphenyl
Concen: 41.533 ng/ul
RT: 13.528 min Scan# 1741
Delta R.T. -0.000 min
Lab File: BP016730.D
Acq: 24 Aug 2023 16:13

Tgt Ion:154 Resp: 3393241
Ion Ratio Lower Upper
154 100
153 40.4 32.7 49.1
76 14.2 11.3 16.9

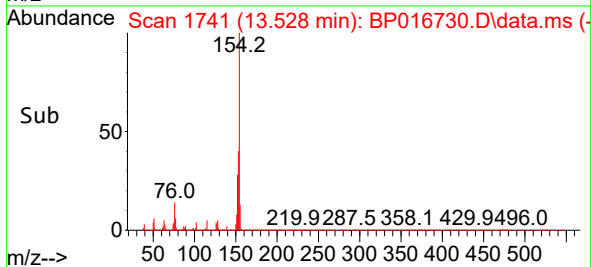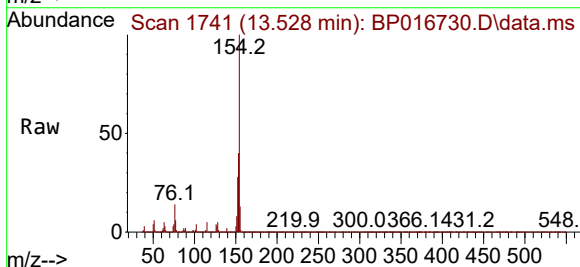



#44

2-Chloronaphthalene

Concen: 41.751 ng/ul

RT: 13.575 min Scan# 1749

Delta R.T. -0.000 min

Lab File: BP016730.D

Acq: 24 Aug 2023 16:13

Instrument :

BNA_P

ClientSampleId :

SSTD040634





Tgt Ion:162 Resp: 2692733

Ion Ratio Lower Upper

162 100

164 33.3 26.1 39.1

127 38.8 30.8 46.2

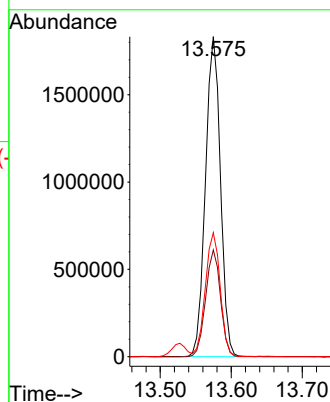

#45

2-Nitroaniline

Concen: 43.873 ng/ul

RT: 13.804 min Scan# 1788

Delta R.T. -0.000 min

Lab File: BP016730.D

Acq: 24 Aug 2023 16:13




Tgt Ion: 65 Resp: 858124


Ion Ratio Lower Upper

65 100

92 68.6 53.8 80.8

138 104.0 80.7 121.1









#47
Dimethylphthalate
Concen: 40.990 ng/ul
RT: 14.151 min Scan# 1847
Delta R.T. -0.000 min
Lab File: BP016730.D
Acq: 24 Aug 2023 16:13




Instrument :
BNA_P
ClientSampleId :
SSTD040634


Tgt Ion:163 Resp: 3440042
Ion Ratio Lower Upper
163 100
194 3.9 3.2 4.8
164 10.3 8.2 12.4

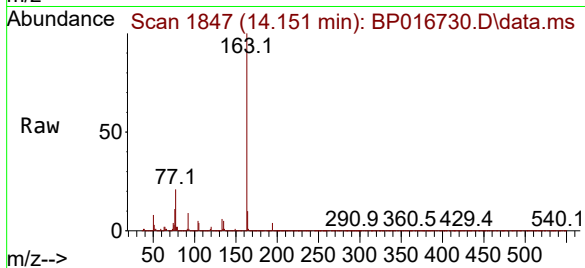

#48
2,6-Dinitrotoluene
Concen: 44.302 ng/ul
RT: 14.292 min Scan# 1871
Delta R.T. -0.000 min
Lab File: BP016730.D
Acq: 24 Aug 2023 16:13

Tgt Ion:165 Resp: 728424
Ion Ratio Lower Upper
165 100
89 59.5 48.0 72.0
121 21.1 16.9 25.3


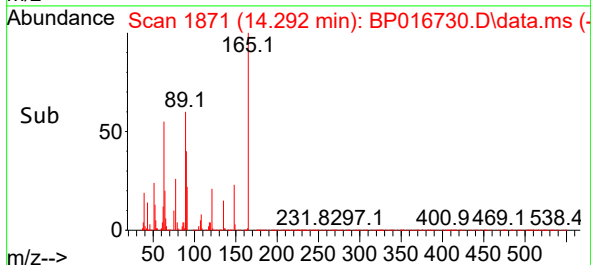
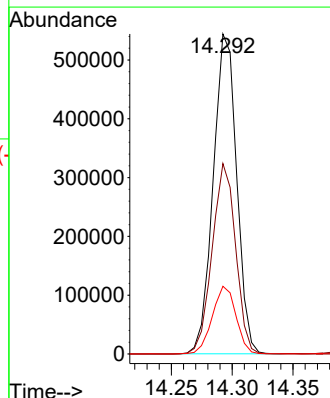
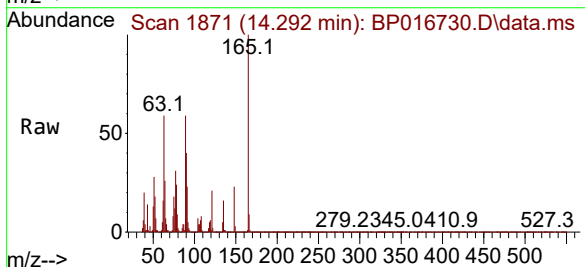




#50
Acenaphthylene
Concen: 41.628 ng/ul
RT: 14.422 min Scan# 1893
Delta R.T. -0.000 min
Lab File: BP016730.D
Acq: 24 Aug 2023 16:13




Instrument :
BNA_P
ClientSampleId :
SSTD040634


Tgt Ion:152 Resp: 4463411
Ion Ratio Lower Upper
152 100
151 20.2 16.1 24.1
153 13.4 10.6 15.8



#51
3-Nitroaniline
Concen: 41.344 ng/ul
RT: 14.634 min Scan# 1929
Delta R.T. -0.000 min
Lab File: BP016730.D
Acq: 24 Aug 2023 16:13

Tgt Ion:138 Resp: 707969
Ion Ratio Lower Upper
138 100
108 10.4 8.2 12.4
92 115.4 95.4 143.0

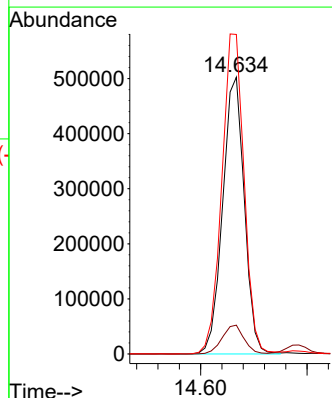



#52

Acenaphthene

Concen: 41.267 ng/ul

RT: 14.757 min Scan# 1950

Delta R.T. -0.000 min

Lab File: BP016730.D

Acq: 24 Aug 2023 16:13

Instrument :

BNA_P

ClientSampleId :

SSTD040634





Tgt Ion:153 Resp: 2927258

Ion Ratio Lower Upper

153 100

152 48.1 38.5 57.7

154 86.7 70.6 105.8



#53

2,4-Dinitrophenol

Concen: 34.848 ng/ul

RT: 14.828 min Scan# 1962

Delta R.T. -0.000 min

Lab File: BP016730.D

Acq: 24 Aug 2023 16:13




Tgt Ion:184 Resp: 416426


Ion Ratio Lower Upper

184 100

63 68.5 55.3 82.9

154 62.8 50.3 75.5


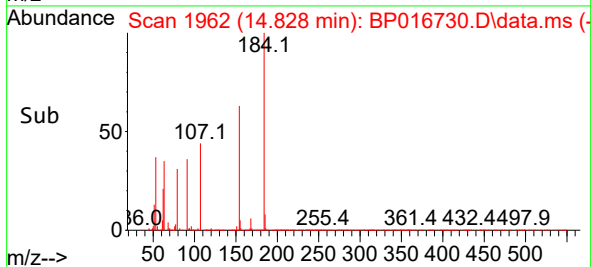

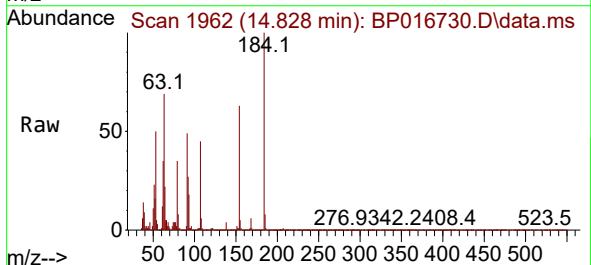




#55
4-Nitrophenol
Concen: 40.512 ng/ul
RT: 14.916 min Scan# 1977
Delta R.T. -0.000 min
Lab File: BP016730.D
Acq: 24 Aug 2023 16:13




Instrument :
BNA_P
ClientSampleId :
SSTD040634


Tgt Ion:109 Resp: 524035
Ion Ratio Lower Upper
109 100
139 134.5 108.6 163.0
65 137.1 107.8 161.6

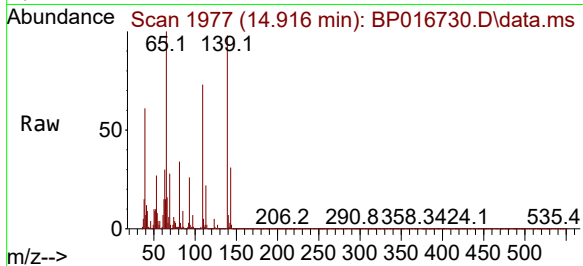

#56
Dibenzofuran
Concen: 40.706 ng/ul
RT: 15.092 min Scan# 2007
Delta R.T. -0.000 min
Lab File: BP016730.D
Acq: 24 Aug 2023 16:13

Tgt Ion:168 Resp: 3961950
Ion Ratio Lower Upper
168 100
139 37.3 29.2 43.8




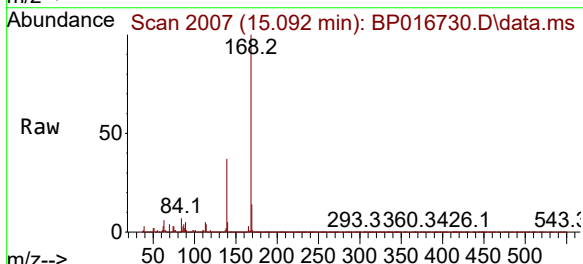




#57
2,4-Dinitrotoluene
Concen: 43.551 ng/ul
RT: 15.075 min Scan# 2004
Delta R.T. -0.000 min
Lab File: BP016730.D
Acq: 24 Aug 2023 16:13




Instrument :
BNA_P
ClientSampleId :
SSTD040634


Tgt Ion:165 Resp: 1054168
Ion Ratio Lower Upper
165 100
63 47.2 39.0 58.4
182 2.7 2.2 3.2

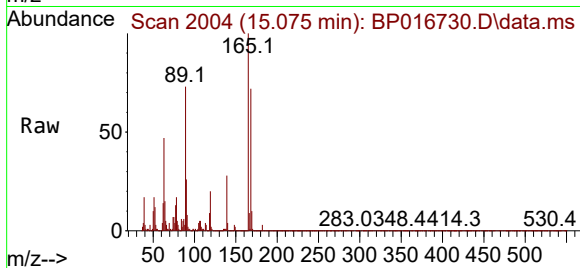

#58
2,3,4,6-Tetrachlorophenol
Concen: 42.335 ng/ul
RT: 15.304 min Scan# 2043
Delta R.T. -0.000 min
Lab File: BP016730.D
Acq: 24 Aug 2023 16:13

Tgt Ion:232 Resp: 815653
Ion Ratio Lower Upper
232 100
131 47.0 38.1 57.1
130 2.6 1.9 2.9
166 32.0 26.5 39.7




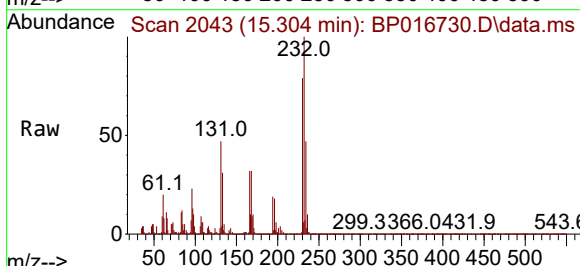




#59
Diethylphthalate
Concen: 40.849 ng/ul
RT: 15.504 min Scan# 2077
Delta R.T. -0.000 min
Lab File: BP016730.D
Acq: 24 Aug 2023 16:13




Instrument :
BNA_P
ClientSampleId :
SSTD040634


Tgt Ion:149 Resp: 3482684
Ion Ratio Lower Upper
149 100
177 22.2 17.3 25.9
150 12.7 10.2 15.2



#61
Fluorene
Concen: 40.523 ng/ul
RT: 15.745 min Scan# 2118
Delta R.T. -0.000 min
Lab File: BP016730.D
Acq: 24 Aug 2023 16:13

Tgt Ion:166 Resp: 3298997
Ion Ratio Lower Upper
166 100
165 99.0 78.8 118.2
167 13.3 10.9 16.3



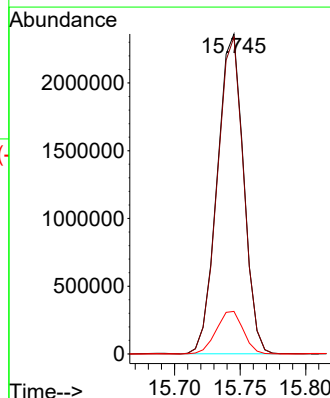





#62
4-Chlorophenyl-phenylether
Concen: 40.930 ng/ul
RT: 15.733 min Scan# 2116
Delta R.T. -0.000 min
Lab File: BP016730.D
Acq: 24 Aug 2023 16:13




Instrument :
BNA_P
ClientSampleId :
SSTD040634


Tgt Ion:204 Resp: 1635993
Ion Ratio Lower Upper
204 100
206 33.1 26.7 40.1
141 56.5 46.8 70.2

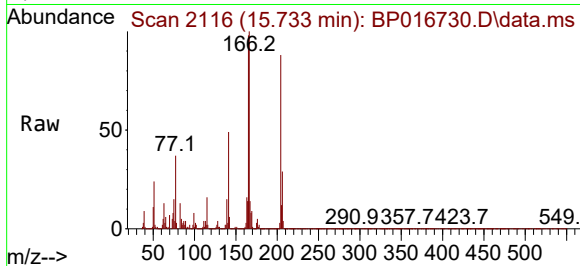

#63
4-Nitroaniline
Concen: 41.322 ng/ul
RT: 15.804 min Scan# 2128
Delta R.T. -0.000 min
Lab File: BP016730.D
Acq: 24 Aug 2023 16:13

Tgt Ion:138 Resp: 673318
Ion Ratio Lower Upper
138 100
92 53.5 41.6 62.4
108 93.4 74.9 112.3

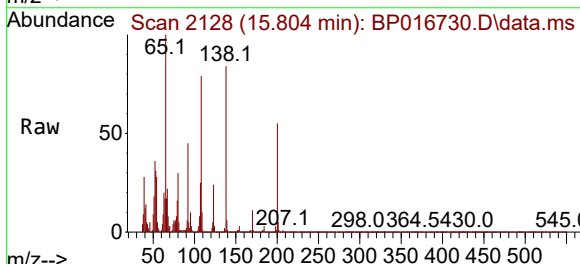




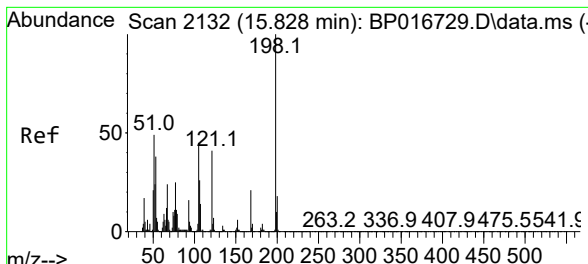


#66
 4,6-Dinitro-2-methylphenol
 Concen: 40.972 ng/ul
 RT: 15.828 min Scan# 2132
 Delta R.T. -0.000 min
 Lab File: BP016730.D
 Acq: 24 Aug 2023 16:13

Instrument :
 BNA_P
 ClientSampleId :
 SSTD040634

Tgt Ion:198 Resp: 637235




Ion	Ratio	Lower	Upper
198	100		
182	3.7	3.2	4.8
77	25.2	20.7	31.1

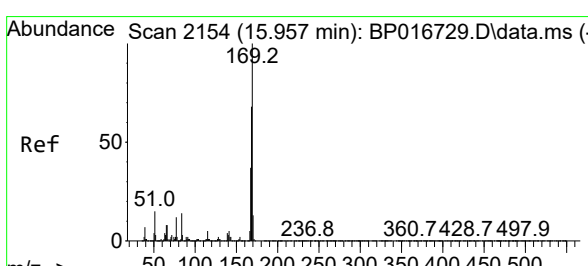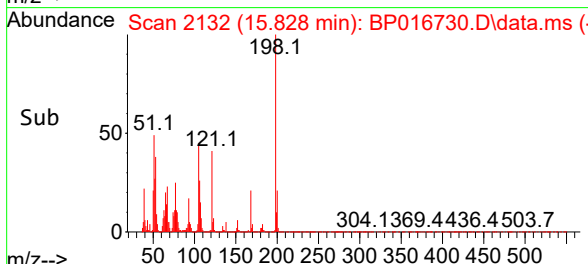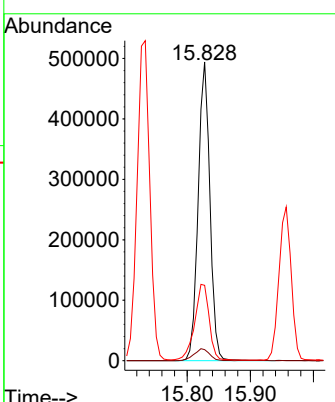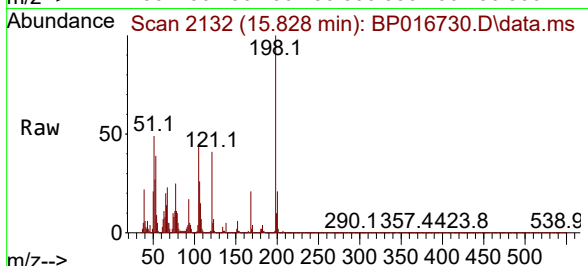


#67
 N-Nitrosodiphenylamine
 Concen: 41.624 ng/ul
 RT: 15.957 min Scan# 2154
 Delta R.T. -0.000 min
 Lab File: BP016730.D
 Acq: 24 Aug 2023 16:13

Tgt Ion:169 Resp: 2788716

Ion	Ratio	Lower	Upper
169	100		
168	67.8	54.2	81.2
167	37.3	29.4	44.2


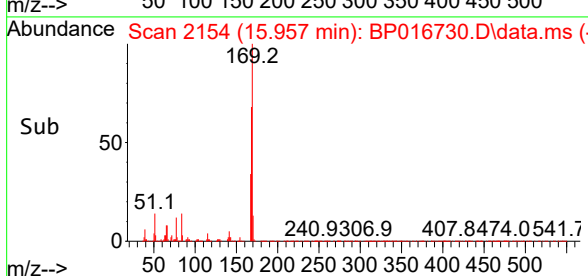
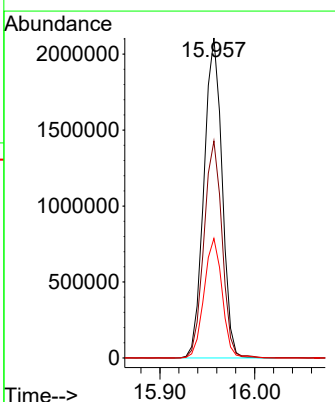
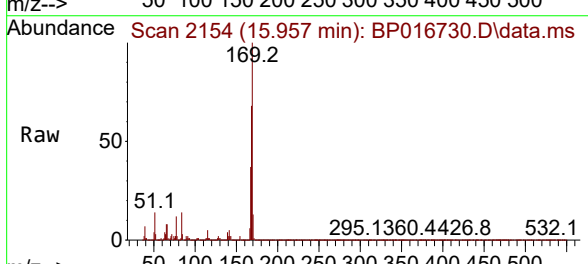




#68
4-Bromophenyl-phenylether
Concen: 41.467 ng/ul
RT: 16.633 min Scan# 21
Delta R.T. -0.006 min
Lab File: BP016730.D
Acq: 24 Aug 2023 16:13




Instrument :
BNA_P
ClientSampleId :
SSTD040634


Tgt Ion:248 Resp: 963038
Ion Ratio Lower Upper
248 100
250 99.5 75.4 113.2
141 80.7 58.7 88.1



#69
Hexachlorobenzene
Concen: 40.686 ng/ul
RT: 16.716 min Scan# 2283
Delta R.T. -0.006 min
Lab File: BP016730.D
Acq: 24 Aug 2023 16:13

Tgt Ion:284 Resp: 1057974
Ion Ratio Lower Upper
284 100
142 41.0 29.8 44.8
249 34.0 25.9 38.9





#70

Atrazine

Concen: 42.519 ng/ul

RT: 16.910 min Scan# 2316

Delta R.T. -0.000 min

Lab File: BP016730.D

Acq: 24 Aug 2023 16:13

Instrument :

BNA_P

ClientSampleId :

SSTD040634





Tgt Ion:200 Resp: 1073972

Ion Ratio Lower Upper

200 100

173 26.8 21.4 32.2

215 47.4 37.3 55.9



#71

Pentachlorophenol

Concen: 38.303 ng/ul

RT: 17.080 min Scan# 2345

Delta R.T. -0.000 min

Lab File: BP016730.D

Acq: 24 Aug 2023 16:13




Tgt Ion:266 Resp: 739357


Ion Ratio Lower Upper

266 100

264 62.8 50.7 76.1

268 63.7 50.8 76.2





#72

Phenanthrene

Concen: 40.982 ng/ul

RT: 17.504 min Scan# 2417

Delta R.T. -0.000 min

Lab File: BP016730.D

Acq: 24 Aug 2023 16:13

Instrument :

BNA_P

ClientSampleId :

SSTD040634





Tgt Ion:178 Resp: 5226205

Ion Ratio Lower Upper

178 100

179 15.8 12.4 18.6

176 20.1 15.6 23.4



#74

Anthracene

Concen: 41.268 ng/ul

RT: 17.598 min Scan# 2433

Delta R.T. -0.000 min

Lab File: BP016730.D

Acq: 24 Aug 2023 16:13




Tgt Ion:178 Resp: 5321310


Ion Ratio Lower Upper

178 100

179 15.4 12.4 18.6

176 19.2 15.3 22.9

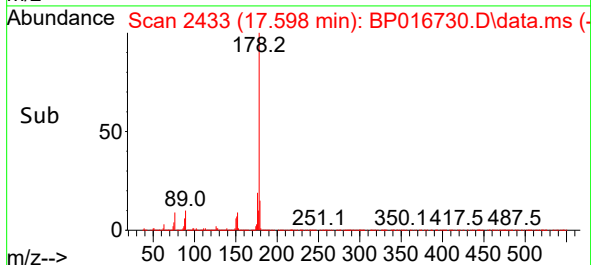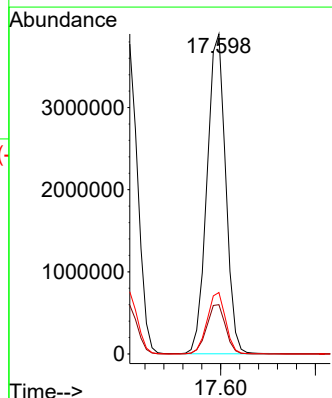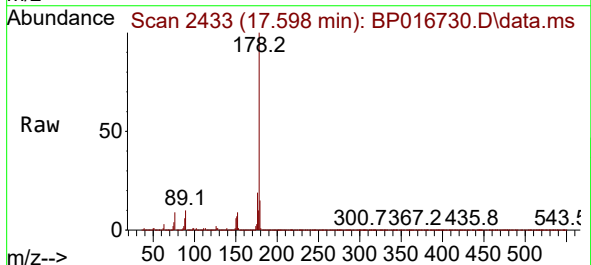



#75

1,2,3,4-Tetrachlorobenzene

Concen: 43.028 ng/uL

RT: 13.481 min Scan# 11

Delta R.T. -0.000 min

Lab File: BP016730.D

Acq: 24 Aug 2023 16:13

Instrument :

BNA_P

ClientSampleId :

SSTD040634





Tgt Ion:216 Resp: 1395600

Ion Ratio Lower Upper

216 100

214 80.1 64.0 96.0

218 48.7 38.2 57.2



#76

Pentachlorobenzene

Concen: 41.751 ng/uL

RT: 14.981 min Scan# 1988

Delta R.T. -0.006 min

Lab File: BP016730.D

Acq: 24 Aug 2023 16:13




Tgt Ion:250 Resp: 1210192


Ion Ratio Lower Upper

250 100

248 63.3 50.9 76.3

252 63.2 52.2 78.4

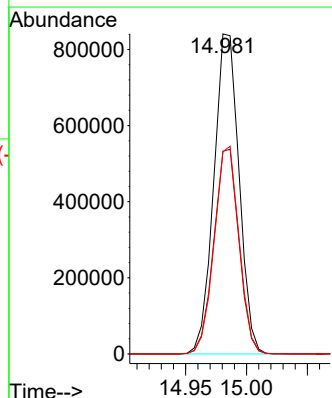



#77

Carbazole

Concen: 41.922 ng/ul

RT: 17.875 min Scan# 2480

Delta R.T. -0.000 min

Lab File: BP016730.D

Acq: 24 Aug 2023 16:13

Instrument :

BNA_P

ClientSampleId :

SSTD040634





Tgt Ion:167 Resp: 4868402

Ion Ratio Lower Upper

167 100

166 22.4 17.4 26.2

139 13.3 10.4 15.6



#78

Di-n-butylphthalate

Concen: 42.231 ng/ul

RT: 18.386 min Scan# 2567

Delta R.T. -0.000 min

Lab File: BP016730.D

Acq: 24 Aug 2023 16:13




Tgt Ion:149 Resp: 6118705


Ion Ratio Lower Upper

149 100

150 9.3 7.5 11.3

104 5.2 4.1 6.1

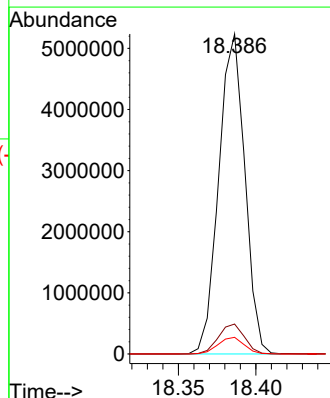



#80

Fluoranthene

Concen: 43.907 ng/ul

RT: 19.463 min Scan# 21

Delta R.T. -0.000 min

Lab File: BP016730.D

Acq: 24 Aug 2023 16:13

Instrument :

BNA_P

ClientSampleId :

SSTD040634





Tgt Ion:202 Resp: 6250282

Ion Ratio Lower Upper

202 100

101 11.8 9.7 14.5

100 9.0 7.4 11.2



#82

Pyrene

Concen: 42.987 ng/ul

RT: 19.821 min Scan# 2811

Delta R.T. -0.000 min

Lab File: BP016730.D

Acq: 24 Aug 2023 16:13




Tgt Ion:202 Resp: 6321101


Ion Ratio Lower Upper

202 100

101 14.7 11.4 17.2

100 11.8 9.4 14.2





#83

Butylbenzylphthalate

Concen: 45.024 ng/ul

RT: 20.674 min Scan# 2956

Delta R.T. -0.000 min

Lab File: BP016730.D

Acq: 24 Aug 2023 16:13

Instrument :

BNA_P

ClientSampleId :

SSTD040634





Tgt Ion:149 Resp: 2855241

Ion Ratio Lower Upper

149 100

91 73.0 58.5 87.7

206 20.9 16.1 24.1

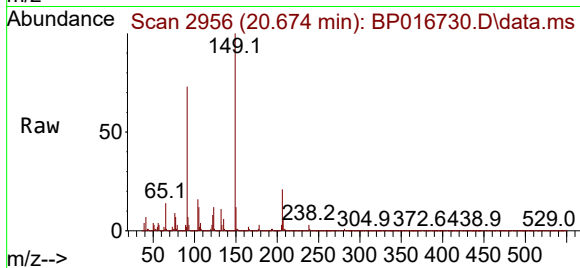

#84

3,3'-Dichlorobenzidine

Concen: 42.985 ng/ul

RT: 21.474 min Scan# 3092

Delta R.T. -0.000 min

Lab File: BP016730.D

Acq: 24 Aug 2023 16:13




Tgt Ion:252 Resp: 1982423


Ion Ratio Lower Upper

252 100

254 64.6 52.1 78.1

126 11.6 9.6 14.4

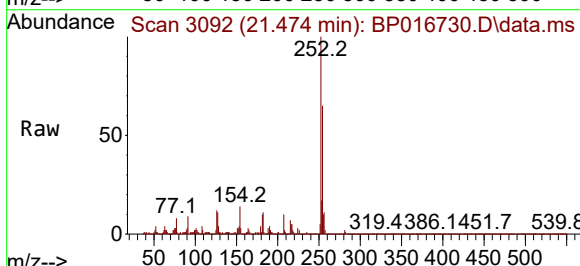



#85

Benzo(a)anthracene

Concen: 41.632 ng/ul

RT: 21.539 min Scan# 3103

Delta R.T. -0.000 min

Lab File: BP016730.D

Acq: 24 Aug 2023 16:13

Instrument :

BNA_P

ClientSampleId :

SSTD040634





Tgt Ion:228 Resp: 6187433

Ion Ratio Lower Upper

228 100

229 20.1 16.2 24.4

226 28.8 22.9 34.3



#86

Bis(2-ethylhexyl)phthalate

Concen: 44.636 ng/ul

RT: 21.410 min Scan# 3081

Delta R.T. -0.000 min

Lab File: BP016730.D

Acq: 24 Aug 2023 16:13




Tgt Ion:149 Resp: 4133193


Ion Ratio Lower Upper

149 100

167 27.6 22.1 33.1

279 3.6 3.0 4.4









#87
Chrysene
Concen: 41.532 ng/ul
RT: 21.598 min Scan# 3113
Delta R.T. -0.000 min
Lab File: BP016730.D
Acq: 24 Aug 2023 16:13




Instrument :
BNA_P
ClientSampleId :
SSTD040634


Tgt Ion:228 Resp: 5607046
Ion Ratio Lower Upper
228 100
226 32.0 25.0 37.4
229 20.3 16.0 24.0



#89
Di-n-octyl phthalate
Concen: 46.029 ng/ul
RT: 22.392 min Scan# 3248
Delta R.T. -0.006 min
Lab File: BP016730.D
Acq: 24 Aug 2023 16:13

Tgt Ion:149 Resp: 6865498

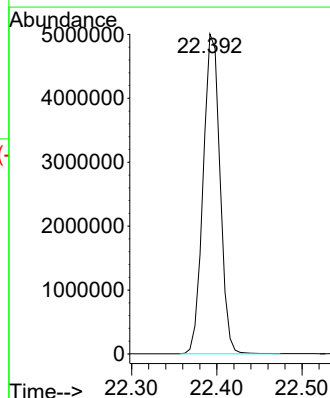



#90

Benzo(b)fluoranthene

Concen: 42.151 ng/ul

RT: 23.327 min Scan# 3407

Delta R.T. -0.000 min

Lab File: BP016730.D

Acq: 24 Aug 2023 16:13

Instrument :

BNA_P

ClientSampleId :

SSTD040634





Tgt Ion:252 Resp: 5330643

Ion Ratio Lower Upper

252 100

253 22.1 17.7 26.5

125 11.1 9.0 13.4



#91

Benzo(k)fluoranthene

Concen: 43.805 ng/ul

RT: 23.380 min Scan# 3416

Delta R.T. -0.000 min

Lab File: BP016730.D

Acq: 24 Aug 2023 16:13




Tgt Ion:252 Resp: 5478791


Ion Ratio Lower Upper

252 100

253 22.3 18.1 27.1

125 11.5 8.9 13.3





#93

Benzo(a)pyrene

Concen: 42.659 ng/ul

RT: 24.015 min Scan# 3

Delta R.T. -0.000 min

Lab File: BP016730.D

Acq: 24 Aug 2023 16:13

Instrument :

BNA_P

ClientSampleId :

SSTD040634





Tgt Ion:252 Resp: 4879787

Ion Ratio Lower Upper

252 100

253 22.3 17.8 26.8

125 12.5 9.9 14.9

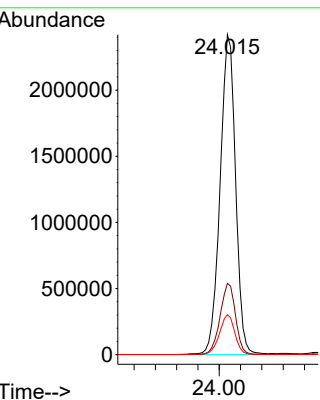

#94

Indeno(1,2,3-cd)pyrene

Concen: 40.387 ng/ul

RT: 26.868 min Scan# 4009

Delta R.T. -0.006 min

Lab File: BP016730.D

Acq: 24 Aug 2023 16:13




Tgt Ion:276 Resp: 4720869


Ion Ratio Lower Upper

276 100

138 25.4 20.9 31.3

277 24.9 19.8 29.6

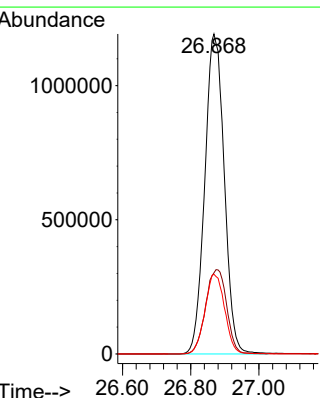



#95

Dibenzo(a,h)anthracene

Concen: 40.626 ng/ul

RT: 26.898 min Scan# 4014

Delta R.T. -0.000 min

Lab File: BP016730.D

Acq: 24 Aug 2023 16:13

Instrument :

BNA_P

ClientSampleId :

SSTD040634





Tgt Ion:278 Resp: 3944189

Ion Ratio Lower Upper

278 100

139 18.0 15.0 22.6

279 23.7 19.4 29.2



#96

Benzo(g,h,i)perylene

Concen: 40.311 ng/ul

RT: 27.727 min Scan# 4155

Delta R.T. -0.000 min

Lab File: BP016730.D

Acq: 24 Aug 2023 16:13

Tgt Ion:276 Resp: 3572356

Ion Ratio Lower Upper

276 100

138 24.4 20.2 30.4

277 24.1 19.3 28.9

