

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082423\
 Data File : BM041488.D
 Acq On : 25 Aug 2023 08:46
 Operator : MA/JU
 Sample : PB155029BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK029

Quant Time: Aug 26 00:16:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 24 18:34:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.110	152	15440	0.400	ng/ul	0.00
4) Naphthalene-d8	10.944	136	44917	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.754	164	22255	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.510	188	44947	0.400	ng/ul	0.00
17) Chrysene-d12	21.708	240	15548	0.400	ng/ul	0.00
23) Perylene-d12	24.281	264	20456	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.444	96	126941	6.496	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.517	152	15414	0.260	ng/ul	-0.01
18) Fluoranthene-d10	19.534	212	21924	0.320	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.749	166	6747	0.065	ng/ul#	12
20) Pyrene	19.905	202	6655	0.046	ng/ul#	1
26) Benzo(a)pyrene	24.120	252	13109	0.114	ng/ul#	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082423\
Data File : BM041488.D
Acq On : 25 Aug 2023 08:46
Operator : MA/JU
Sample : PB155029BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK029

Quant Time: Aug 26 00:16:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 24 18:34:12 2023
Response via : Initial Calibration




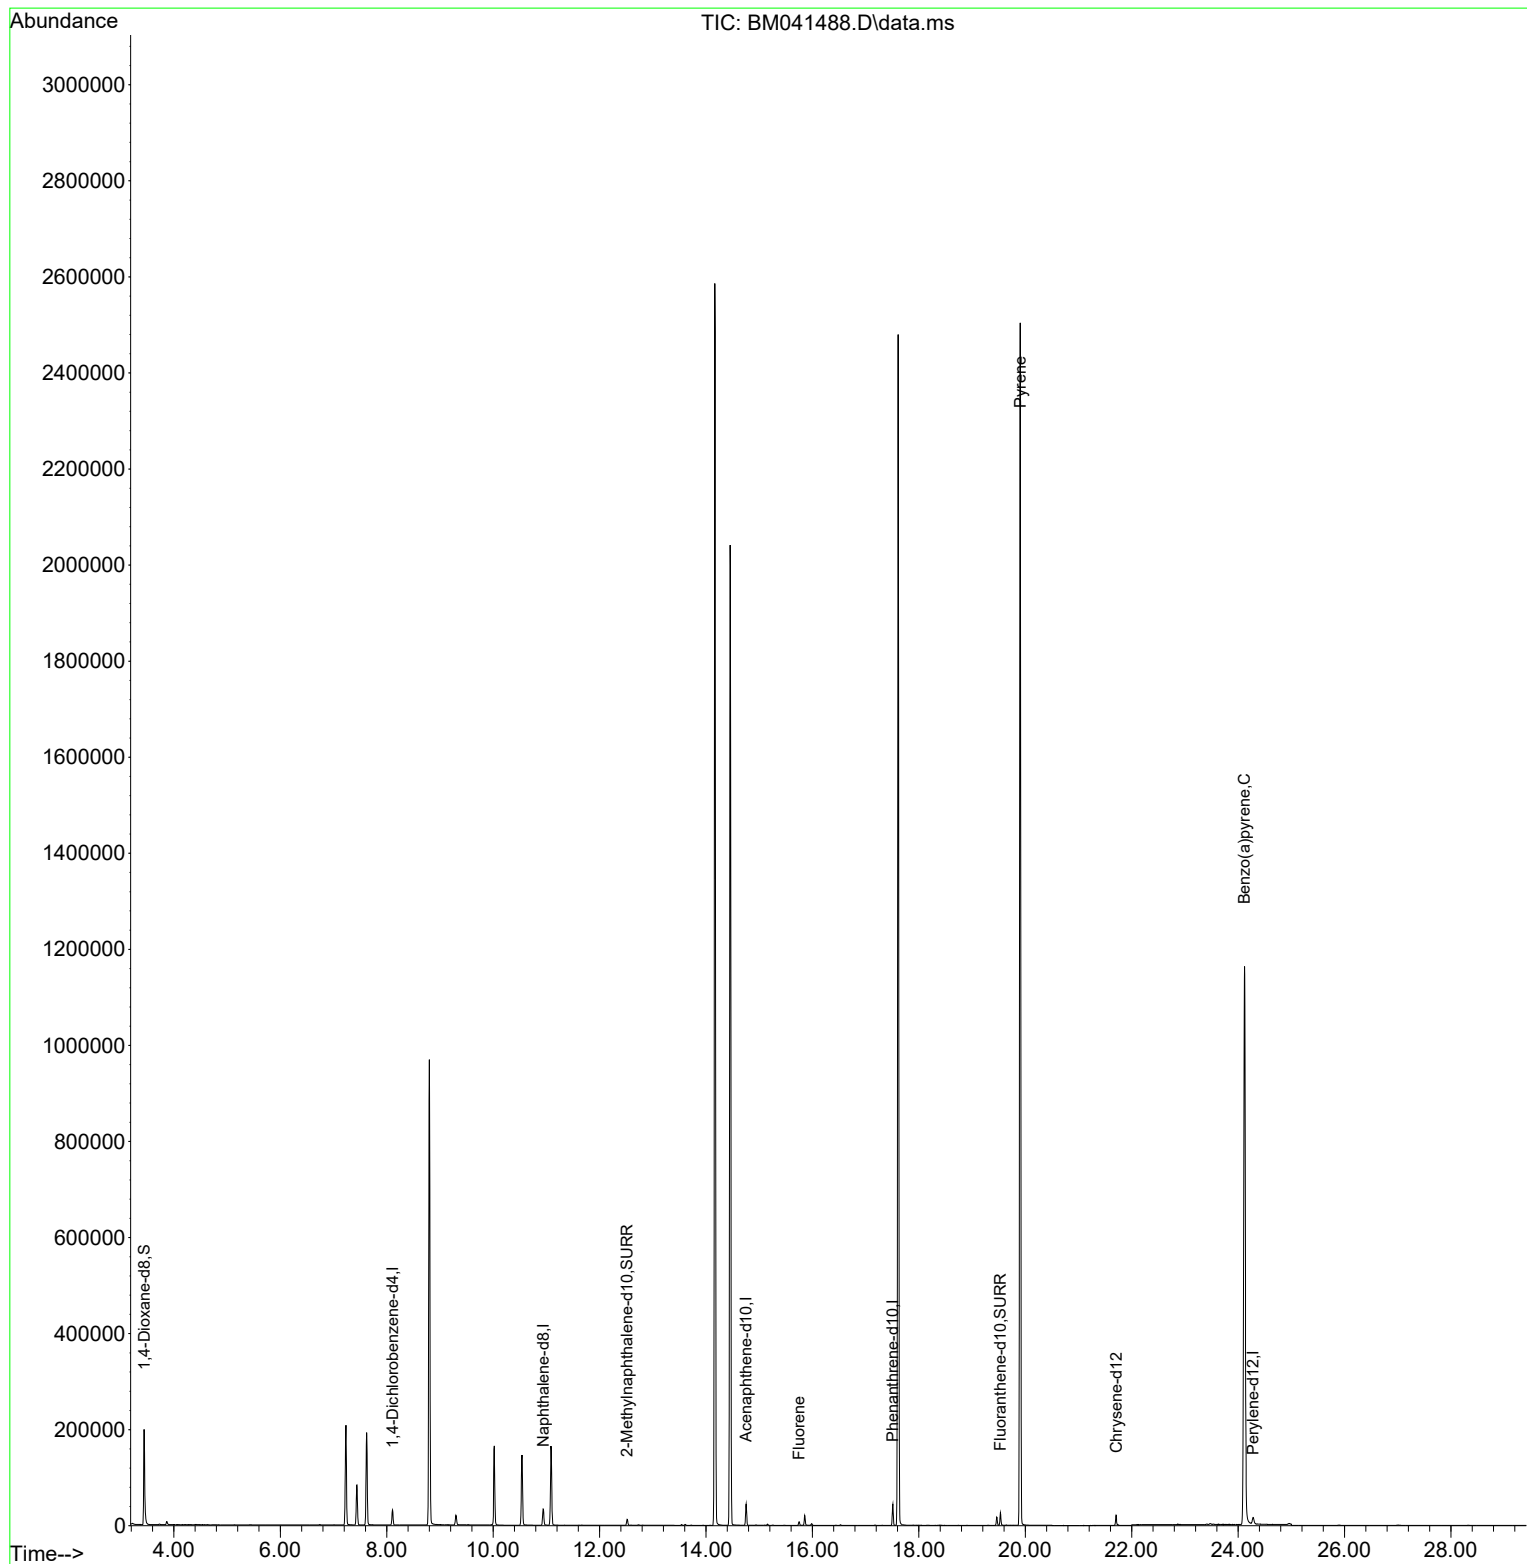


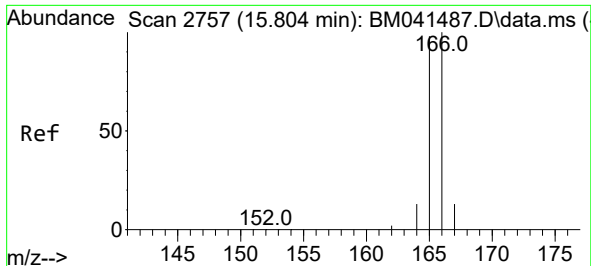

#12
Fluorene
Concen: 0.065 ng/ul
RT: 15.749 min Scan# 21
Delta R.T. -0.056 min
Lab File: BM041488.D
Acq: 25 Aug 2023 08:46




Instrument :
BNA_P
ClientSampleId :
SBLK029


Tgt Ion:166 Resp: 6747
Ion Ratio Lower Upper
166 100
165 5.8 79.4 119.2#
167 31.5 11.0 16.6#

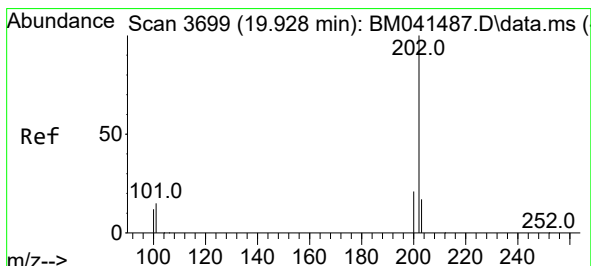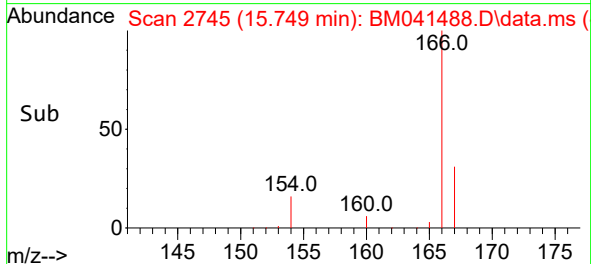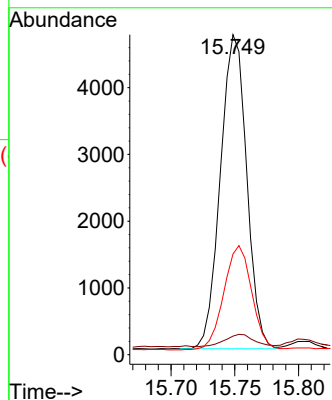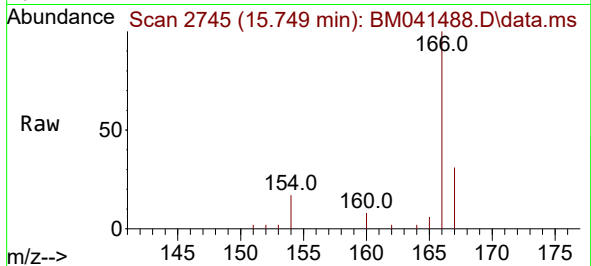

#20
Pyrene
Concen: 0.046 ng/ul
RT: 19.905 min Scan# 3694
Delta R.T. -0.028 min
Lab File: BM041488.D
Acq: 25 Aug 2023 08:46


Tgt Ion:202 Resp: 6655
Ion Ratio Lower Upper
202 100
101 157.6 12.2 18.2#
100 1177.6 9.8 14.8#

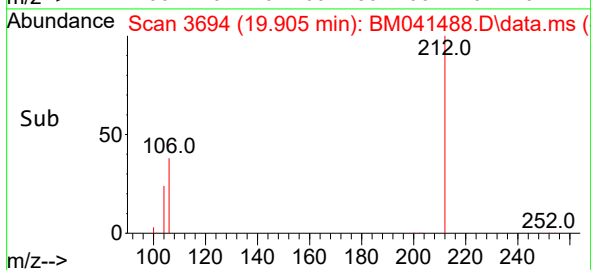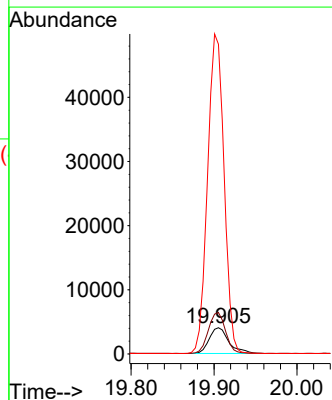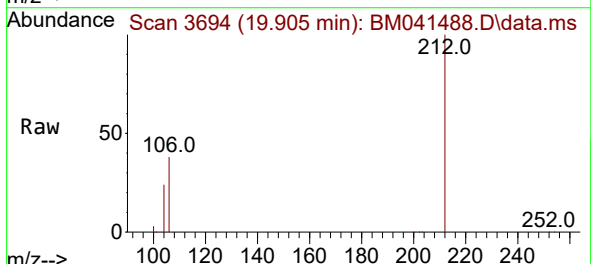

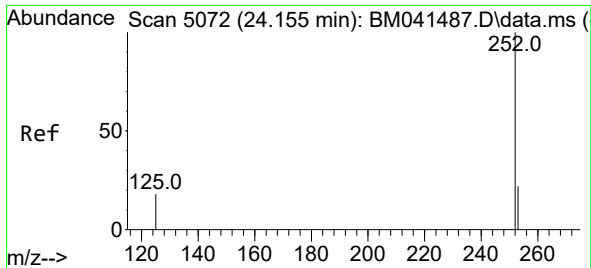

#26
Benzo(a)pyrene
Concen: 0.114 ng/ul
RT: 24.120 min Scan# 5072
Delta R.T. -0.044 min
Lab File: BM041488.D
Acq: 25 Aug 2023 08:46

Instrument :
BNA_P
ClientSampleId :
SBLK029

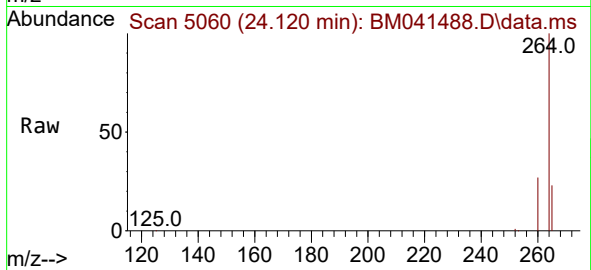

Tgt Ion:252 Resp: 13109
Ion Ratio Lower Upper
252 100
253 33.0 19.5 29.3#
125 29.3 16.0 24.0#

