

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082523\
 Data File : BP016739.D
 Acq On : 25 Aug 2023 09:12
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020702

Quant Time: Aug 25 22:24:59 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 25 01:47:30 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.034	152	357394	20.000	ng/u1	0.00
20) Naphthalene-d8	10.863	136	1622540	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.687	164	1037348	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.457	188	2308159	20.000	ng/u1	0.00
79) Chrysene-d12	21.551	240	2277069	20.000	ng/u1	0.00
88) Perylene-d12	24.127	264	2404033	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	73461	8.495	ng/uL	0.00
4) Pyridine-d5	3.817	84	540818	20.465	ng/u1	0.00
7) Phenol-d5	7.175	99	622873	19.600	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.369	67	418668	20.670	ng/u1	0.00
11) 2-Chlorophenol-d4	7.552	132	494976	20.715	ng/u1	0.00
15) 4-Methylphenol-d8	8.740	113	514581	19.835	ng/u1	0.00
21) Nitrobenzene-d5	9.234	128	246927	20.128	ng/u1	0.00
24) 2-Nitrophenol-d4	9.946	143	260581	20.151	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.469	165	481703	19.981	ng/u1	0.00
31) 4-Chloroaniline-d4	11.022	131	733663	19.845	ng/u1	0.00
46) Dimethylphthalate-d6	14.098	166	1539127	19.674	ng/u1	0.00
49) Acenaphthylene-d8	14.387	160	1788618	20.225	ng/u1	0.00
54) 4-Nitrophenol-d4	14.892	143	301147	18.624	ng/u1	0.00
60) Fluorene-d10	15.681	176	1303265	19.783	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.804	200	239535	17.426	ng/u1	0.00
73) Anthracene-d10	17.557	188	2063723	20.171	ng/u1	0.00
81) Pyrene-d10	19.786	212	2455724	19.636	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.957	264	2420610	20.101	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.422	88	76432	8.116	ng/uL	97
5) Pyridine	3.840	79	558928	20.533	ng/u1	98
6) Benzaldehyde	7.187	77	414157	23.831	ng/u1	99
8) Phenol	7.205	94	662236	19.912	ng/u1	98
10) Bis(2-Chloroethyl)ether	7.463	93	544737	20.291	ng/u1	100
12) 2-Chlorophenol	7.587	128	502612	20.579	ng/u1	98
13) 2-Methylphenol	8.469	108	490654	19.667	ng/u1	99
14) 2,2'-oxybis(1-Chloropr...	8.546	45	505045	12.897	ng/u1	99
16) Acetophenone	8.881	105	832348	20.691	ng/u1	99
17) N-Nitroso-di-n-propyla...	8.852	70	449892	21.222	ng/u1	99
18) 4-Methylphenol	8.805	108	536760	19.758	ng/u1	99
19) Hexachloroethane	9.105	117	208130	20.481	ng/u1	95
22) Nitrobenzene	9.275	77	648558	20.607	ng/u1	98
23) Isophorone	9.787	82	1235094	20.205	ng/u1	99
25) 2-Nitrophenol	9.981	139	291280	20.371	ng/u1	99
26) 2,4-Dimethylphenol	10.016	107	576064	20.045	ng/u1	99
27) Bis(2-Chloroethoxy)met...	10.275	93	765491	20.298	ng/u1	99
29) 2,4-Dichlorophenol	10.499	162	486512	20.090	ng/u1	99
30) Naphthalene	10.916	128	1701083	20.239	ng/u1	100
32) 4-Chloroaniline	11.046	127	719936	19.815	ng/u1	99
33) Hexachlorobutadiene	11.152	225	289710	19.422	ng/u1	96
34) Caprolactam	11.863	113	167772	18.786	ng/u1	98
35) 4-Chloro-3-methylphenol	12.140	107	554535	20.420	ng/u1	100
36) 2-Methylnaphthalene	12.516	142	1167166	20.118	ng/u1	99

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082523\
 Data File : BP016739.D
 Acq On : 25 Aug 2023 09:12
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020702

Quant Time: Aug 25 22:24:59 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 25 01:47:30 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.734	142	1191323	20.363	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.863	216	568619	19.232	ng/ul	99
40) Hexachlorocyclopentadiene	12.816	237	332177	15.278	ng/ul	100
41) 2,4,6-Trichlorophenol	13.116	196	384283	19.464	ng/ul	99
42) 2,4,5-Trichlorophenol	13.181	196	410973	19.236	ng/ul	98
43) 1,1'-Biphenyl	13.522	154	1544231	20.022	ng/ul	99
44) 2-Chloronaphthalene	13.569	162	1217120	19.990	ng/ul	99
45) 2-Nitroaniline	13.798	65	375886	20.357	ng/ul	99
47) Dimethylphthalate	14.145	163	1556275	19.643	ng/ul	100
48) 2,6-Dinitrotoluene	14.287	165	300713	19.370	ng/ul	97
50) Acenaphthylene	14.416	152	2048943	20.242	ng/ul	100
51) 3-Nitroaniline	14.628	138	319805	19.783	ng/ul	98
52) Acenaphthene	14.751	153	1345143	20.087	ng/ul	100
53) 2,4-Dinitrophenol	14.822	184	168016	14.894	ng/ul	97
55) 4-Nitrophenol	14.910	109	235029	19.247	ng/ul	99
56) Dibenzofuran	15.087	168	1836934	19.992	ng/ul	97
57) 2,4-Dinitrotoluene	15.069	165	456303	19.969	ng/ul	100
58) 2,3,4,6-Tetrachlorophenol	15.298	232	348653	19.169	ng/ul	96
59) Diethylphthalate	15.498	149	1598107	19.855	ng/ul	99
61) Fluorene	15.740	166	1527767	19.879	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.728	204	730883	19.370	ng/ul	96
63) 4-Nitroaniline	15.792	138	317009	20.608	ng/ul	95
66) 4,6-Dinitro-2-methylph...	15.822	198	264014	17.815	ng/ul	96
67) N-Nitrosodiphenylamine	15.951	169	1282123	20.084	ng/ul	99
68) 4-Bromophenyl-phenylether	16.634	248	428391	19.358	ng/ul	95
69) Hexachlorobenzene	16.716	284	471660	19.036	ng/ul	97
70) Atrazine	16.904	200	479126	19.907	ng/ul	99
71) Pentachlorophenol	17.081	266	305341	16.601	ng/ul	99
72) Phenanthrene	17.498	178	2450478	20.166	ng/ul	99
74) Anthracene	17.592	178	2495469	20.310	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.475	216	606340	19.619	ng/ul	98
76) Pentachlorobenzene	14.981	250	544852	19.727	ng/ul	99
77) Carbazole	17.875	167	2300805	20.792	ng/ul	100
78) Di-n-butylphthalate	18.381	149	2830202	20.500	ng/ul	100
80) Fluoranthene	19.457	202	2909337	19.366	ng/ul	98
82) Pyrene	19.816	202	3057847	19.705	ng/ul	99
83) Butylbenzylphthalate	20.675	149	1317761	19.690	ng/ul	99
84) 3,3'-Dichlorobenzidine	21.474	252	945879	19.434	ng/ul	99
85) Benzo(a)anthracene	21.533	228	3147099	20.065	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.410	149	1956163	20.018	ng/ul	99
87) Chrysene	21.592	228	2902324	20.371	ng/ul	100
89) Di-n-octyl phthalate	22.392	149	3371519	18.623	ng/ul	100
90) Benzo(b)fluoranthene	23.321	252	3041403	19.812	ng/ul	99
91) Benzo(k)fluoranthene	23.380	252	2943087	19.385	ng/ul	99
93) Benzo(a)pyrene	24.010	252	2786793	20.069	ng/ul	100
94) Indeno(1,2,3-cd)pyrene	26.862	276	2968715	20.922	ng/ul	100
95) Dibenzo(a,h)anthracene	26.886	278	2475721	21.007	ng/ul	99
96) Benzo(g,h,i)perylene	27.721	276	2279114	21.186	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082523\
 Data File : BP016739.D
 Acq On : 25 Aug 2023 09:12
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020702

Quant Time: Aug 25 22:24:59 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 25 01:47:30 2023
 Response via : Initial Calibration




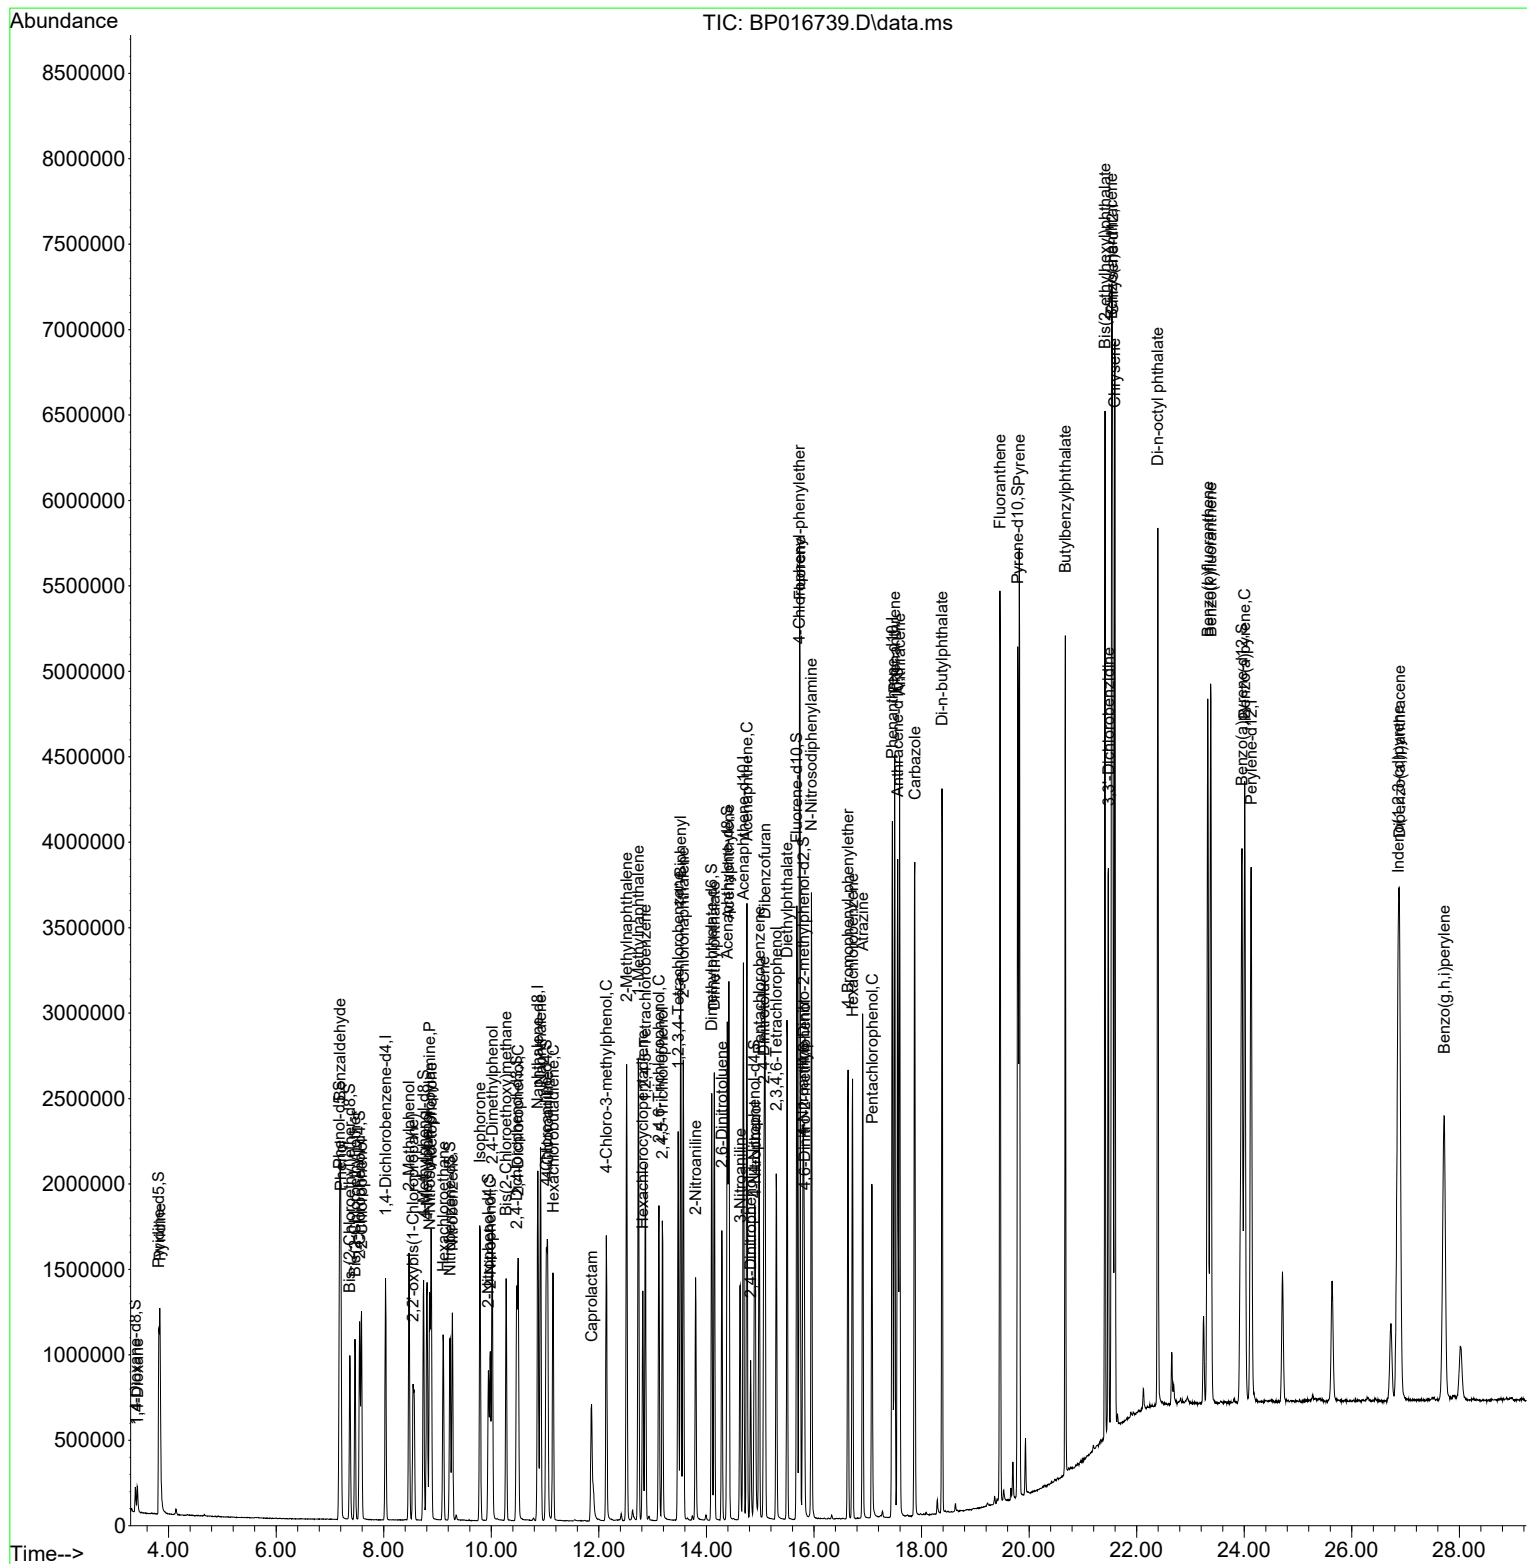


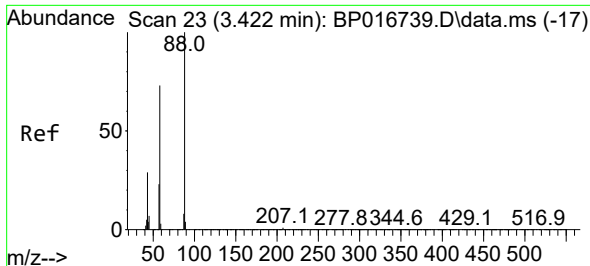

#2
1,4-Dioxane
Concen: 8.116 ng/uL
RT: 3.422 min Scan# 21
Delta R.T. -0.001 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12




Instrument :
BNA_P
ClientSampleId :
SSTD020702


Tgt Ion: 88 Resp: 76432
Ion Ratio Lower Upper
88 100
43 29.4 24.0 36.0
58 71.4 59.8 89.8

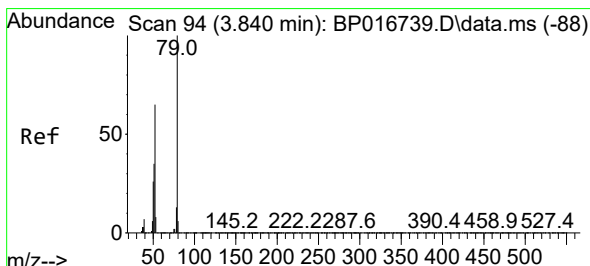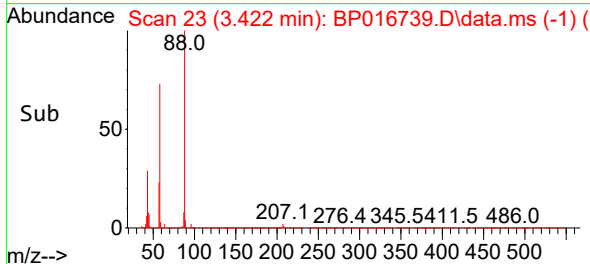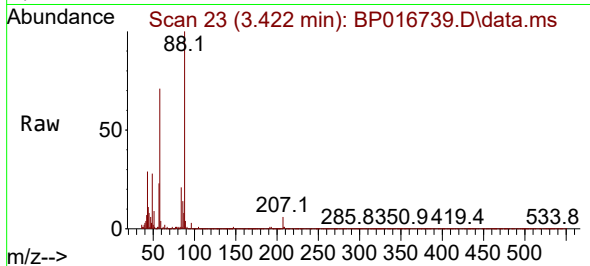

#5
Pyridine
Concen: 20.533 ng/uL
RT: 3.840 min Scan# 94
Delta R.T. -0.000 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12

Tgt Ion: 79 Resp: 558928
Ion Ratio Lower Upper
79 100
52 72.4 59.6 89.4
51 36.2 28.2 42.2


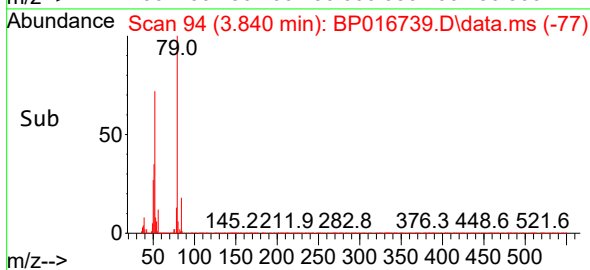

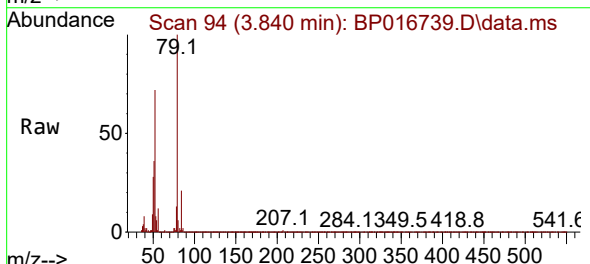




#6
Benzaldehyde
Concen: 23.831 ng/ul
RT: 7.187 min Scan# 663
Delta R.T. -0.006 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12




Instrument :
BNA_P
ClientSampleId :
SSTD020702


Tgt Ion: 77 Resp: 414157
Ion Ratio Lower Upper
77 100
105 94.6 75.4 113.2
106 89.7 73.1 109.7



#8
Phenol
Concen: 19.912 ng/ul
RT: 7.205 min Scan# 666
Delta R.T. -0.006 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12

Tgt Ion: 94 Resp: 662236
Ion Ratio Lower Upper
94 100
65 28.7 22.4 33.6
66 37.4 28.6 42.8









#10
Bis(2-Chloroethyl)ether
Concen: 20.291 ng/ul
RT: 7.463 min Scan# 710
Delta R.T. -0.006 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12




Instrument :
BNA_P
ClientSampleId :
SSTD020702


Tgt Ion: 93 Resp: 544737
Ion Ratio Lower Upper
93 100
63 78.7 62.9 94.3
95 33.1 26.3 39.5



#12
2-Chlorophenol
Concen: 20.579 ng/ul
RT: 7.587 min Scan# 731
Delta R.T. -0.006 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12

Tgt Ion: 128 Resp: 502612
Ion Ratio Lower Upper
128 100
64 48.6 40.0 60.0
130 32.0 26.4 39.6









#13
2-Methylphenol
Concen: 19.667 ng/ul
RT: 8.469 min Scan# 881
Delta R.T. -0.006 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12




Instrument :
BNA_P
ClientSampleId :
SSTD020702


Tgt Ion:108 Resp: 490654
Ion Ratio Lower Upper
108 100
107 90.4 71.4 107.2

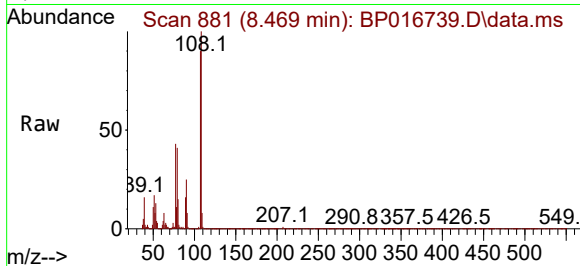

#14
2,2'-oxybis(1-Chloropropane)
Concen: 12.897 ng/ul
RT: 8.546 min Scan# 894
Delta R.T. -0.006 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12

Tgt Ion: 45 Resp: 505045
Ion Ratio Lower Upper
45 100
77 14.3 11.1 16.7
79 10.5 8.2 12.4




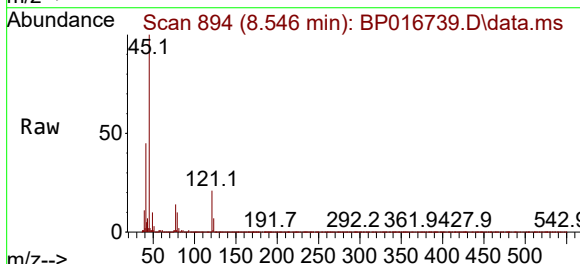




#16
Acetophenone
Concen: 20.691 ng/ul
RT: 8.881 min Scan# 91
Delta R.T. -0.006 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12




Instrument :
BNA_P
ClientSampleId :
SSTD020702


Tgt Ion:105 Resp: 832348
Ion Ratio Lower Upper
105 100
77 80.5 64.2 96.4
51 28.7 22.2 33.4



#17
N-Nitroso-di-n-propylamine
Concen: 21.222 ng/ul
RT: 8.852 min Scan# 946
Delta R.T. -0.012 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12

Tgt Ion: 70 Resp: 449892
Ion Ratio Lower Upper
70 100
42 58.0 46.0 69.0
101 9.4 7.6 11.4
130 19.7 16.1 24.1









#18
4-Methylphenol
Concen: 19.758 ng/ul
RT: 8.805 min Scan# 91
Delta R.T. -0.006 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12




Instrument :
BNA_P
ClientSampleId :
SSTD020702


Tgt Ion:108 Resp: 536760
Ion Ratio Lower Upper
108 100
107 113.6 89.8 134.6



#19
Hexachloroethane
Concen: 20.481 ng/ul
RT: 9.105 min Scan# 989
Delta R.T. -0.006 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12

Tgt Ion:117 Resp: 208130
Ion Ratio Lower Upper
117 100
201 90.3 75.4 113.2
199 54.7 47.8 71.6









#22
Nitrobenzene
Concen: 20.607 ng/ul
RT: 9.275 min Scan# 1018
Delta R.T. -0.006 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12




Instrument :
BNA_P
ClientSampleId :
SSTD020702


Tgt Ion: 77 Resp: 648558
Ion Ratio Lower Upper
77 100
123 42.3 34.9 52.3
65 12.9 10.6 15.8



#23
Isophorone
Concen: 20.205 ng/ul
RT: 9.787 min Scan# 1105
Delta R.T. -0.012 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12

Tgt Ion: 82 Resp: 1235094
Ion Ratio Lower Upper
82 100
95 6.8 5.4 8.0
138 16.2 13.5 20.3









#25
2-Nitrophenol
Concen: 20.371 ng/ul
RT: 9.981 min Scan# 1138
Delta R.T. -0.006 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12




Instrument :
BNA_P
ClientSampleId :
SSTD020702


Tgt Ion:139 Resp: 291280
Ion Ratio Lower Upper
139 100
65 52.7 42.0 63.0
109 30.6 23.4 35.2



#26
2,4-Dimethylphenol
Concen: 20.045 ng/ul
RT: 10.016 min Scan# 1144
Delta R.T. -0.006 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12

Tgt Ion:107 Resp: 576064
Ion Ratio Lower Upper
107 100
121 51.4 40.7 61.1
122 86.6 69.7 104.5









#27
 Bis(2-Chloroethoxy)methane
 Concen: 20.298 ng/ul
 RT: 10.275 min Scan# 1188
 Delta R.T. -0.006 min
 Lab File: BP016739.D
 Acq: 25 Aug 2023 09:12




Instrument :
 BNA_P
 ClientSampleId :
 SSTD020702


Tgt Ion: 93 Resp: 765491
 Ion Ratio Lower Upper
 93 100
 95 32.5 26.3 39.5
 123 10.9 8.8 13.2

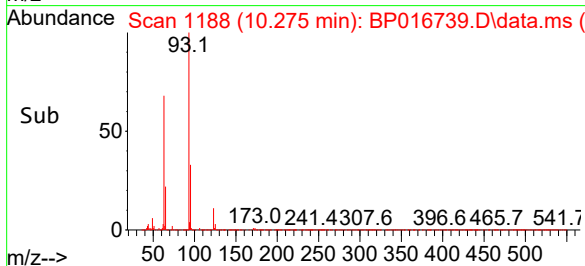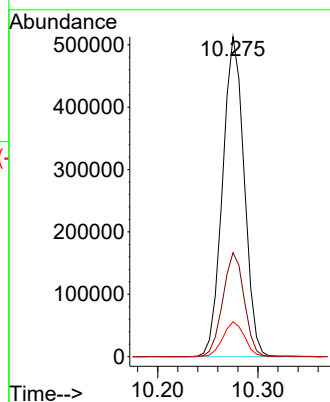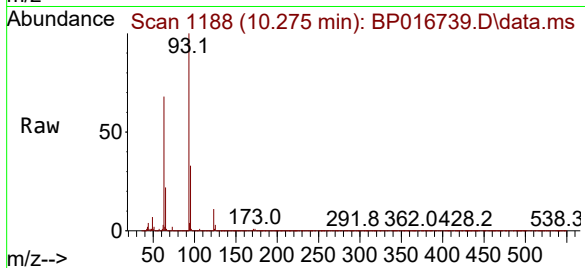

#29
 2,4-Dichlorophenol
 Concen: 20.090 ng/ul
 RT: 10.499 min Scan# 1226
 Delta R.T. -0.006 min
 Lab File: BP016739.D
 Acq: 25 Aug 2023 09:12

Tgt Ion: 162 Resp: 486512
 Ion Ratio Lower Upper
 162 100
 164 65.0 52.2 78.2
 98 37.5 29.3 43.9




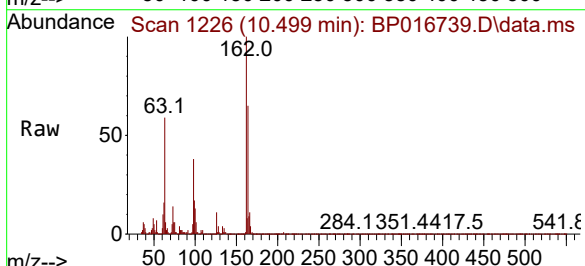




#30
Naphthalene
Concen: 20.239 ng/ul
RT: 10.916 min Scan# 1297
Delta R.T. -0.006 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12




Instrument :
BNA_P
ClientSampleId :
SSTD020702


Tgt Ion:128 Resp: 1701083
Ion Ratio Lower Upper
128 100
129 11.0 8.8 13.2
127 13.0 10.3 15.5

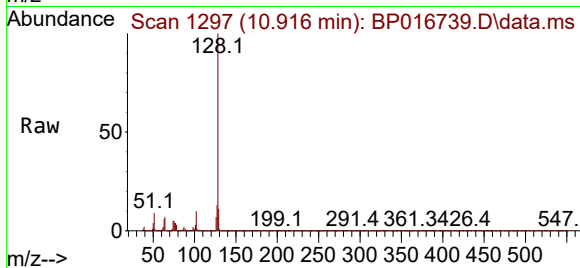

#32
4-Chloroaniline
Concen: 19.815 ng/ul
RT: 11.046 min Scan# 1319
Delta R.T. -0.006 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12

Tgt Ion:127 Resp: 719936
Ion Ratio Lower Upper
127 100
129 32.1 25.9 38.9

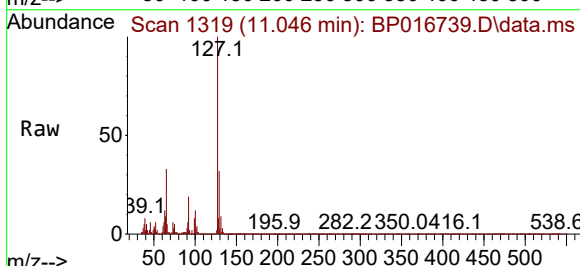



#33

Hexachlorobutadiene

Concen: 19.422 ng/ul

RT: 11.152 min Scan# 11

Delta R.T. -0.000 min

Lab File: BP016739.D

Acq: 25 Aug 2023 09:12

Instrument :

BNA_P

ClientSampleId :

SSTD020702





Tgt Ion:225 Resp: 289710

Ion Ratio Lower Upper

225 100

223 61.1 51.0 76.4

227 61.9 52.5 78.7



#34

Caprolactam

Concen: 18.786 ng/ul

RT: 11.863 min Scan# 1458

Delta R.T. -0.012 min

Lab File: BP016739.D

Acq: 25 Aug 2023 09:12




Tgt Ion:113 Resp: 167772


Ion Ratio Lower Upper

113 100

55 179.5 140.6 210.8

56 130.0 104.5 156.7









#35
4-Chloro-3-methylphenol
Concen: 20.420 ng/ul
RT: 12.140 min Scan# 1505
Delta R.T. -0.006 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12




Instrument :
BNA_P
ClientSampleId :
SSTD020702


Tgt Ion:107 Resp: 554535
Ion Ratio Lower Upper
107 100
144 25.7 20.6 31.0
142 79.3 63.7 95.5



#36
2-Methylnaphthalene
Concen: 20.118 ng/ul
RT: 12.516 min Scan# 1569
Delta R.T. -0.006 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12

Tgt Ion:142 Resp: 1167166
Ion Ratio Lower Upper
142 100
141 89.8 71.4 107.0









#37
1-Methylnaphthalene
Concen: 20.363 ng/ul
RT: 12.734 min Scan# 1606
Delta R.T. -0.006 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12




Instrument :
BNA_P
ClientSampleId :
SSTD020702


Tgt Ion:142 Resp: 1191323
Ion Ratio Lower Upper
142 100
141 92.4 73.0 109.4
116 4.1 3.1 4.7

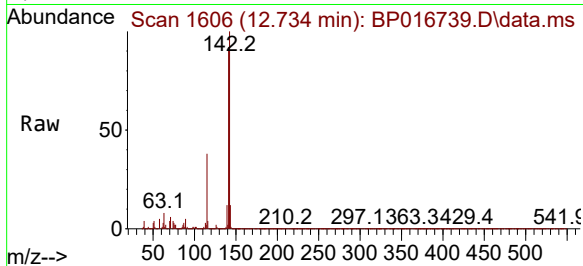

#39
1,2,4,5-Tetrachlorobenzene
Concen: 19.232 ng/ul
RT: 12.863 min Scan# 1628
Delta R.T. -0.006 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12

Tgt Ion:216 Resp: 568619
Ion Ratio Lower Upper
216 100
214 78.6 63.4 95.2
179 22.8 17.4 26.2
108 19.4 15.3 22.9

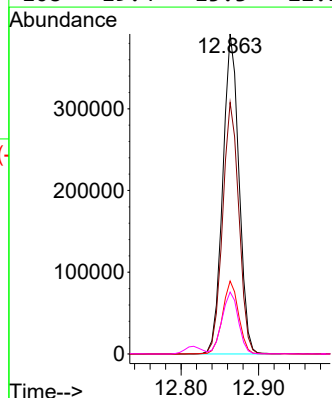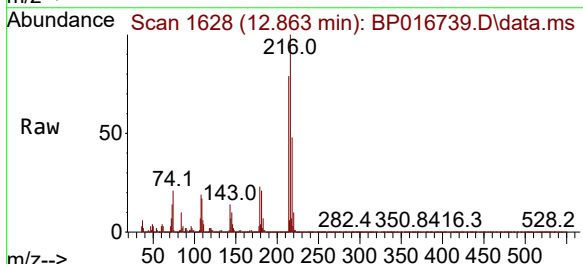



#40

Hexachlorocyclopentadiene

Concen: 15.278 ng/ul

RT: 12.816 min Scan# 1620

Delta R.T. -0.006 min

Lab File: BP016739.D

Acq: 25 Aug 2023 09:12

Instrument :

BNA_P

ClientSampleId :

SSTD020702





Tgt Ion:237 Resp: 332177

Ion Ratio Lower Upper

237 100

235 64.3 51.3 76.9

272 12.1 9.8 14.8



#41

2,4,6-Trichlorophenol

Concen: 19.464 ng/ul

RT: 13.116 min Scan# 1671

Delta R.T. -0.006 min

Lab File: BP016739.D

Acq: 25 Aug 2023 09:12




Tgt Ion:196 Resp: 384283


Ion Ratio Lower Upper

196 100

198 95.1 76.6 115.0

200 30.9 25.2 37.8









#42
2,4,5-Trichlorophenol
Concen: 19.236 ng/ul
RT: 13.181 min Scan# 1682
Delta R.T. -0.006 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12




Instrument :
BNA_P
ClientSampleId :
SSTD020702


Tgt Ion:196 Resp: 410973
Ion Ratio Lower Upper
196 100
198 95.7 77.8 116.8
200 30.0 24.8 37.2



#43
1,1'-Biphenyl
Concen: 20.022 ng/ul
RT: 13.522 min Scan# 1740
Delta R.T. -0.006 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12

Tgt Ion:154 Resp: 1544231
Ion Ratio Lower Upper
154 100
153 40.1 32.7 49.1
76 14.5 11.3 16.9









#44
2-Chloronaphthalene
Concen: 19.990 ng/ul
RT: 13.569 min Scan# 1748
Delta R.T. -0.006 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12




Instrument :
BNA_P
ClientSampleId :
SSTD020702


Tgt Ion:162 Resp: 1217120
Ion Ratio Lower Upper
162 100
164 32.4 26.1 39.1
127 39.3 30.8 46.2



#45
2-Nitroaniline
Concen: 20.357 ng/ul
RT: 13.798 min Scan# 1787
Delta R.T. -0.006 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12

Tgt Ion: 65 Resp: 375886
Ion Ratio Lower Upper
65 100
92 67.7 53.8 80.8
138 99.5 80.7 121.1



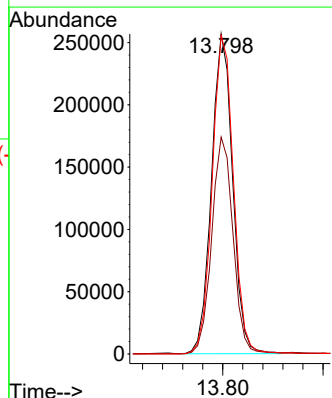



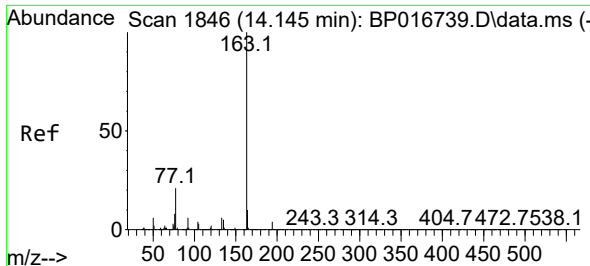

#47
Dimethylphthalate
Concen: 19.643 ng/ul
RT: 14.145 min Scan# 1846
Delta R.T. -0.006 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12




Instrument :
BNA_P
ClientSampleId :
SSTD020702


Tgt Ion:163 Resp: 1556275
Ion Ratio Lower Upper
163 100
194 3.9 3.2 4.8
164 10.3 8.2 12.4

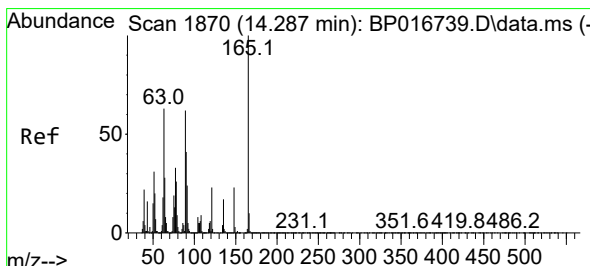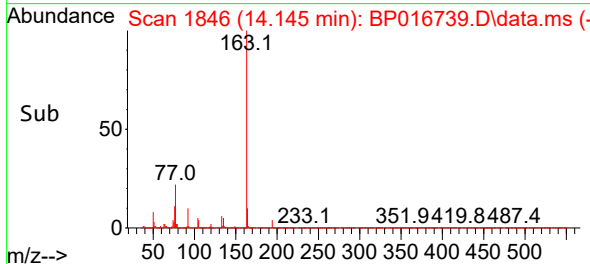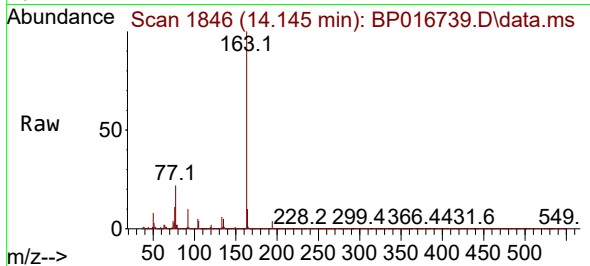

#48
2,6-Dinitrotoluene
Concen: 19.370 ng/ul
RT: 14.287 min Scan# 1870
Delta R.T. -0.006 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12

Tgt Ion:165 Resp: 300713
Ion Ratio Lower Upper
165 100
89 62.1 48.0 72.0
121 23.5 16.9 25.3


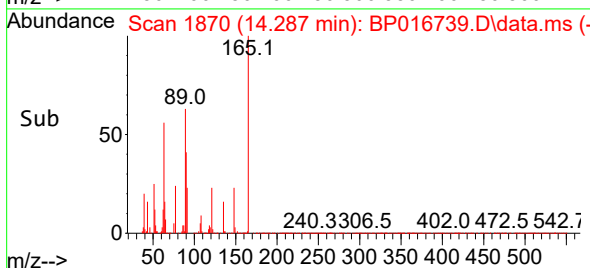
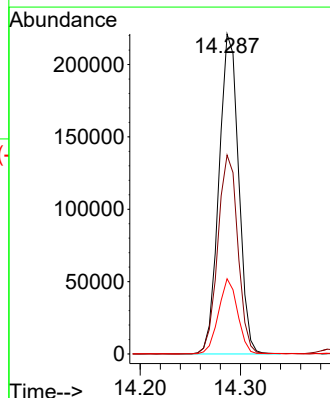
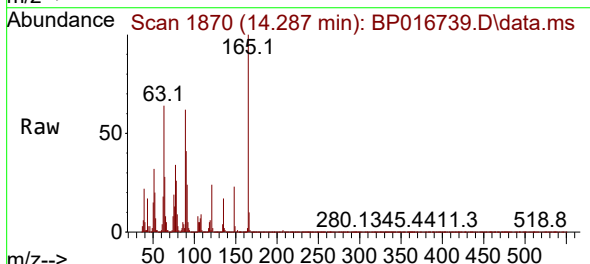




#50
Acenaphthylene
Concen: 20.242 ng/ul
RT: 14.416 min Scan# 1892
Delta R.T. -0.006 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12




Instrument :
BNA_P
ClientSampleId :
SSTD020702


Tgt Ion:152 Resp: 2048943
Ion Ratio Lower Upper
152 100
151 19.8 16.1 24.1
153 13.2 10.6 15.8



#51
3-Nitroaniline
Concen: 19.783 ng/ul
RT: 14.628 min Scan# 1928
Delta R.T. -0.006 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12

Tgt Ion:138 Resp: 319805
Ion Ratio Lower Upper
138 100
108 11.1 8.2 12.4
92 121.3 95.4 143.0









#52
Acenaphthene
Concen: 20.087 ng/ul
RT: 14.751 min Scan# 1949
Delta R.T. -0.006 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12




Instrument :
BNA_P
ClientSampleId :
SSTD020702


Tgt Ion:153 Resp: 1345143
Ion Ratio Lower Upper
153 100
152 48.2 38.5 57.7
154 87.8 70.6 105.8

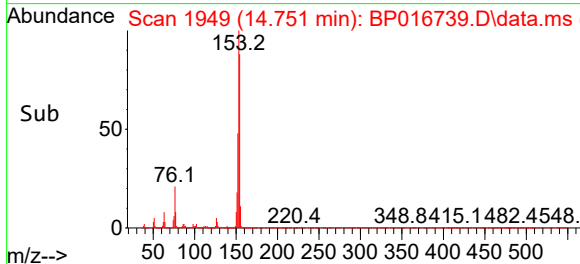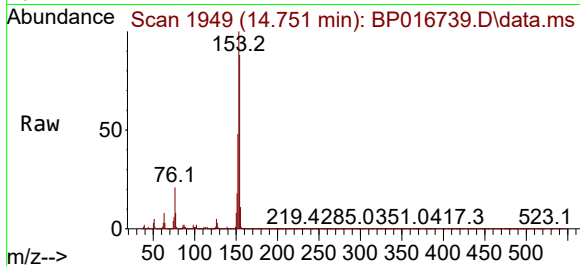

#53
2,4-Dinitrophenol
Concen: 14.894 ng/ul
RT: 14.822 min Scan# 1961
Delta R.T. -0.006 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12

Tgt Ion:184 Resp: 168016
Ion Ratio Lower Upper
184 100
63 71.7 55.3 82.9
154 65.8 50.3 75.5


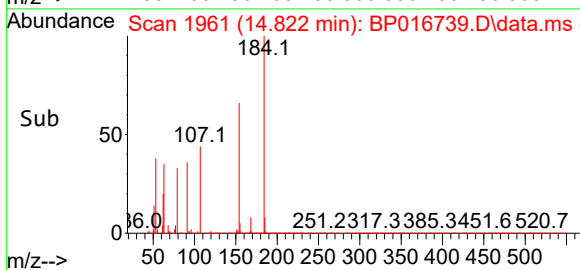

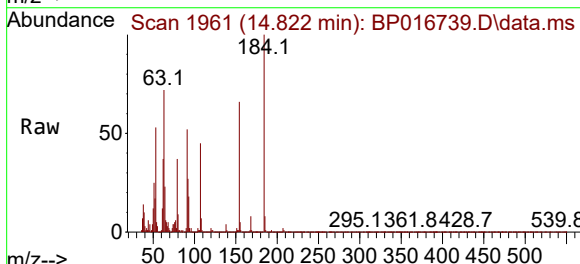




#55
4-Nitrophenol
Concen: 19.247 ng/ul
RT: 14.910 min Scan# 1976
Delta R.T. -0.006 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12




Instrument :
BNA_P
ClientSampleId :
SSTD020702


Tgt Ion:109 Resp: 235029
Ion Ratio Lower Upper
109 100
139 135.7 108.6 163.0
65 136.1 107.8 161.6

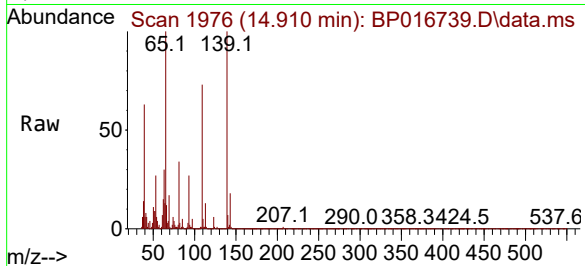

#56
Dibenzofuran
Concen: 19.992 ng/ul
RT: 15.087 min Scan# 2006
Delta R.T. -0.006 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12

Tgt Ion:168 Resp: 1836934
Ion Ratio Lower Upper
168 100
139 38.2 29.2 43.8

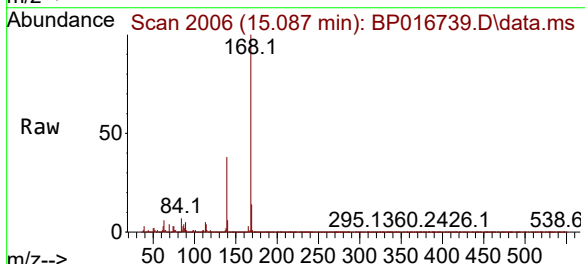



#57

2,4-Dinitrotoluene

Concen: 19.969 ng/ul

RT: 15.069 min Scan# 2003

Delta R.T. -0.006 min

Lab File: BP016739.D

Acq: 25 Aug 2023 09:12

Instrument :

BNA_P

ClientSampleId :

SSTD020702





Tgt Ion:165 Resp: 456303

Ion Ratio Lower Upper

165 100

63 48.5 39.0 58.4

182 2.7 2.2 3.2

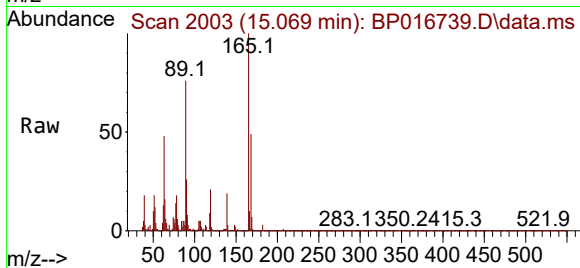

#58

2,3,4,6-Tetrachlorophenol

Concen: 19.169 ng/ul

RT: 15.298 min Scan# 2042

Delta R.T. -0.006 min

Lab File: BP016739.D

Acq: 25 Aug 2023 09:12

Tgt Ion:232 Resp: 348653




Ion Ratio Lower Upper


232 100

131 51.6 38.1 57.1

130 2.7 1.9 2.9

166 33.9 26.5 39.7



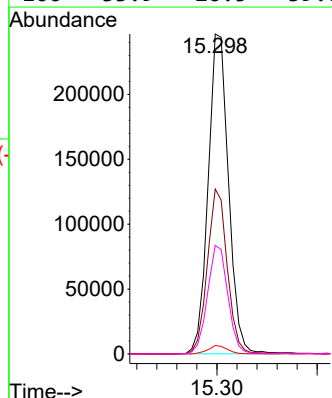
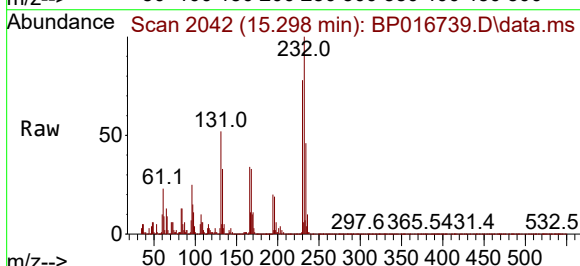




#59
Diethylphthalate
Concen: 19.855 ng/ul
RT: 15.498 min Scan# 2076
Delta R.T. -0.006 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12




Instrument :
BNA_P
ClientSampleId :
SSTD020702


Tgt Ion:149 Resp: 1598107
Ion Ratio Lower Upper
149 100
177 21.1 17.3 25.9
150 12.5 10.2 15.2

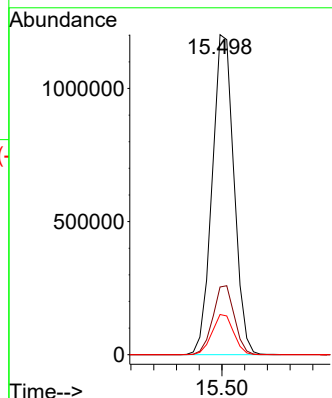

#61
Fluorene
Concen: 19.879 ng/ul
RT: 15.740 min Scan# 2117
Delta R.T. -0.006 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12

Tgt Ion:166 Resp: 1527767
Ion Ratio Lower Upper
166 100
165 99.1 78.8 118.2
167 13.8 10.9 16.3



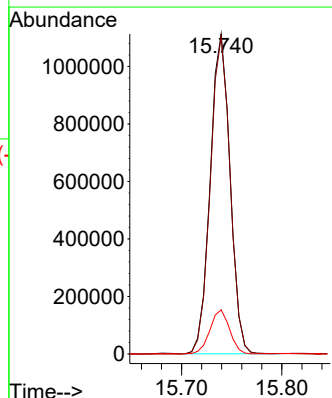





#62
4-Chlorophenyl-phenylether
Concen: 19.370 ng/ul
RT: 15.728 min Scan# 2115
Delta R.T. -0.006 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12




Instrument :
BNA_P
ClientSampleId :
SSTD020702


Tgt Ion:204 Resp: 730883
Ion Ratio Lower Upper
204 100
206 32.7 26.7 40.1
141 62.4 46.8 70.2

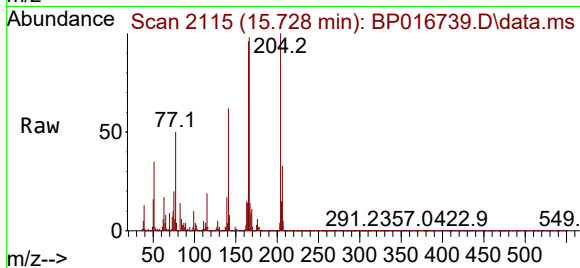

#63
4-Nitroaniline
Concen: 20.608 ng/ul
RT: 15.792 min Scan# 2126
Delta R.T. -0.012 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12

Tgt Ion:138 Resp: 317009
Ion Ratio Lower Upper
138 100
92 55.0 41.6 62.4
108 88.4 74.9 112.3




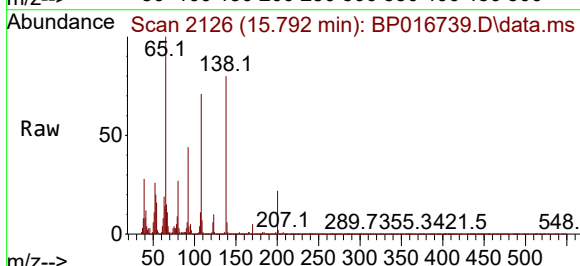




#66
4,6-Dinitro-2-methylphenol
Concen: 17.815 ng/ul
RT: 15.822 min Scan# 2131
Delta R.T. -0.006 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12




Instrument :
BNA_P
ClientSampleId :
SSTD020702


Tgt Ion:198 Resp: 264014
Ion Ratio Lower Upper
198 100
182 4.6 3.2 4.8
77 28.0 20.7 31.1



#67
N-Nitrosodiphenylamine
Concen: 20.084 ng/ul
RT: 15.951 min Scan# 2153
Delta R.T. -0.006 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12

Tgt Ion:169 Resp: 1282123
Ion Ratio Lower Upper
169 100
168 66.4 54.2 81.2
167 37.1 29.4 44.2


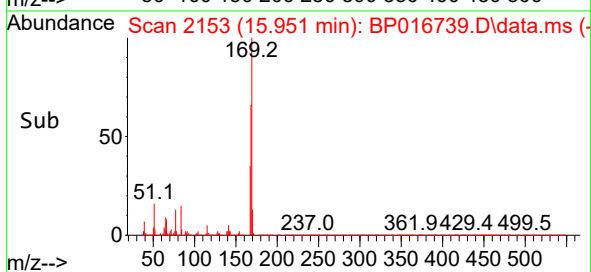






#68
4-Bromophenyl-phenylether
Concen: 19.358 ng/ul
RT: 16.634 min Scan# 2269
Delta R.T. -0.006 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12




Instrument :
BNA_P
ClientSampleId :
SSTD020702


Tgt Ion:248 Resp: 428391
Ion Ratio Lower Upper
248 100
250 97.1 75.4 113.2
141 79.2 58.7 88.1

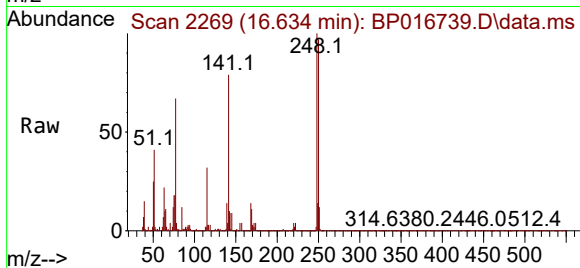

#69
Hexachlorobenzene
Concen: 19.036 ng/ul
RT: 16.716 min Scan# 2283
Delta R.T. -0.006 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12

Tgt Ion:284 Resp: 471660
Ion Ratio Lower Upper
284 100
142 40.4 29.8 44.8
249 32.5 25.9 38.9

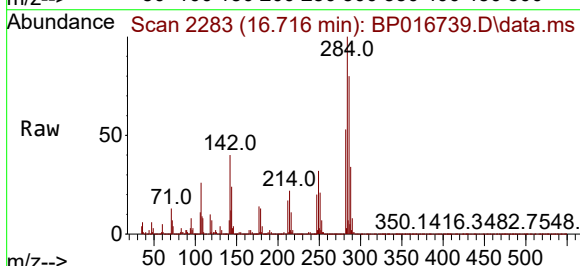



#70

Atrazine

Concen: 19.907 ng/ul

RT: 16.904 min Scan# 2315

Delta R.T. -0.006 min

Lab File: BP016739.D

Acq: 25 Aug 2023 09:12

Instrument :

BNA_P

ClientSampleId :

SSTD020702





Tgt Ion:200 Resp: 479126

Ion Ratio Lower Upper

200 100

173 27.2 21.4 32.2

215 45.9 37.3 55.9

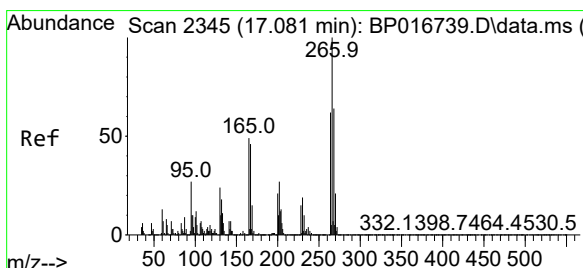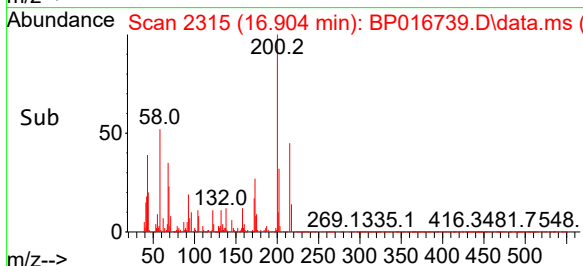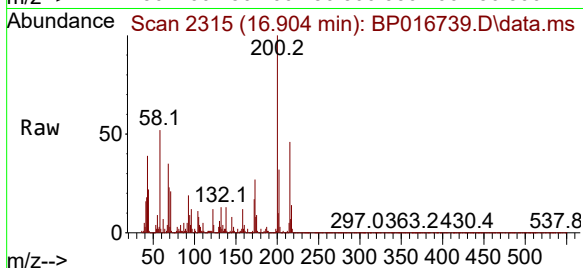

#71

Pentachlorophenol

Concen: 16.601 ng/ul

RT: 17.081 min Scan# 2345

Delta R.T. -0.000 min

Lab File: BP016739.D

Acq: 25 Aug 2023 09:12




Tgt Ion:266 Resp: 305341


Ion Ratio Lower Upper

266 100

264 62.4 50.7 76.1

268 63.8 50.8 76.2

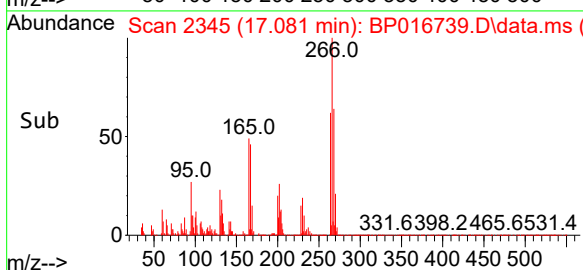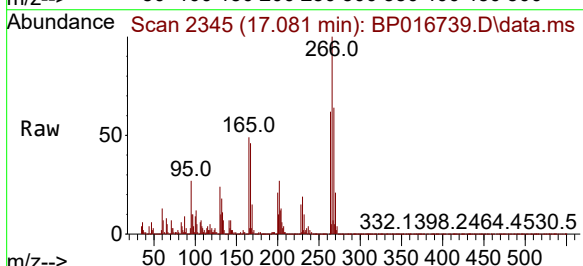



#72

Phenanthrene

Concen: 20.166 ng/ul

RT: 17.498 min Scan# 2416

Delta R.T. -0.006 min

Lab File: BP016739.D

Acq: 25 Aug 2023 09:12

Instrument :

BNA_P

ClientSampleId :

SSTD020702





Tgt Ion:178 Resp: 2450478

Ion Ratio Lower Upper

178 100

179 15.8 12.4 18.6

176 19.8 15.6 23.4



#74

Anthracene

Concen: 20.310 ng/ul

RT: 17.592 min Scan# 2432

Delta R.T. -0.006 min

Lab File: BP016739.D

Acq: 25 Aug 2023 09:12




Tgt Ion:178 Resp: 2495469


Ion Ratio Lower Upper

178 100

179 15.4 12.4 18.6

176 19.1 15.3 22.9


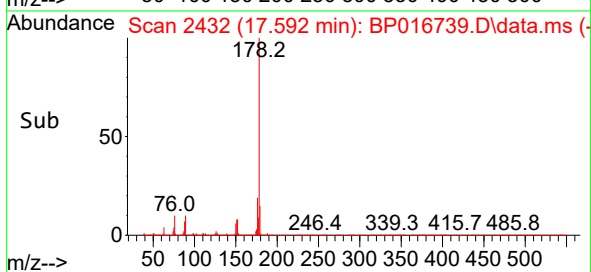






#75
1,2,3,4-Tetrachlorobenzene
Concen: 19.619 ng/uL
RT: 13.475 min Scan# 1732
Delta R.T. -0.006 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12




Instrument :
BNA_P
ClientSampleId :
SSTD020702


Tgt Ion:216 Resp: 606340
Ion Ratio Lower Upper
216 100
214 77.8 64.0 96.0
218 47.6 38.2 57.2

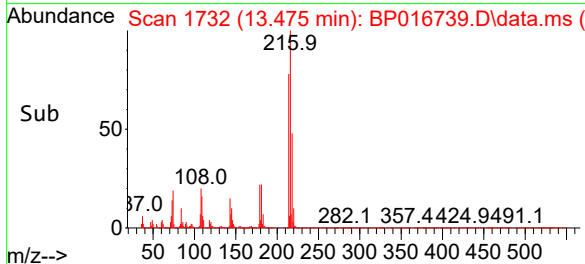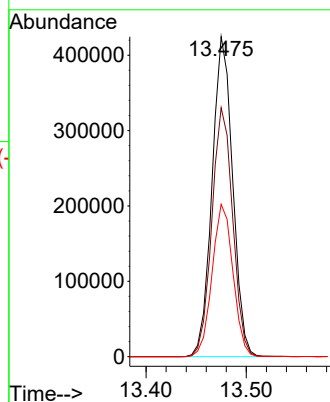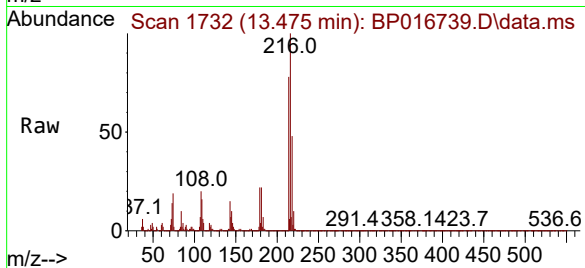

#76
Pentachlorobenzene
Concen: 19.727 ng/uL
RT: 14.981 min Scan# 1988
Delta R.T. -0.006 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12

Tgt Ion:250 Resp: 544852
Ion Ratio Lower Upper
250 100
248 64.2 50.9 76.3
252 64.4 52.2 78.4

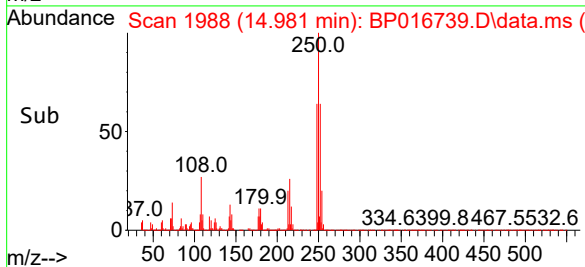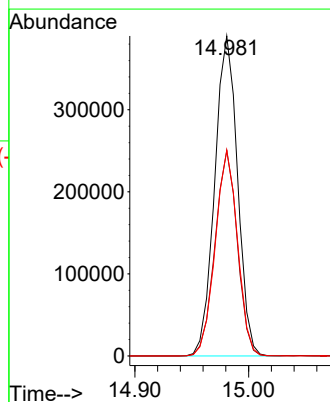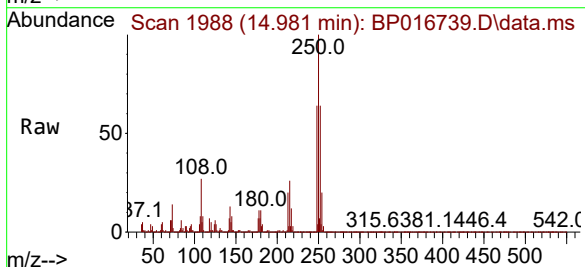

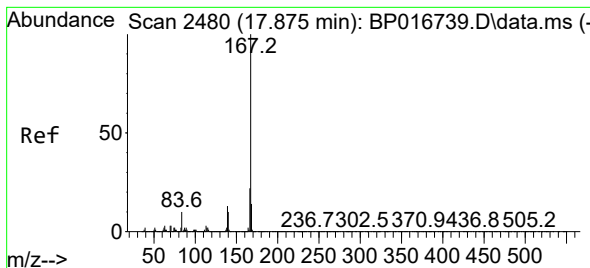

#77

Carbazole

Concen: 20.792 ng/ul

RT: 17.875 min Scan# 2480

Delta R.T. -0.000 min

Lab File: BP016739.D

Acq: 25 Aug 2023 09:12

Instrument :

BNA_P

ClientSampleId :

SSTD020702





Tgt Ion:167 Resp: 2300805

Ion Ratio Lower Upper

167 100

166 21.6 17.4 26.2

139 12.9 10.4 15.6

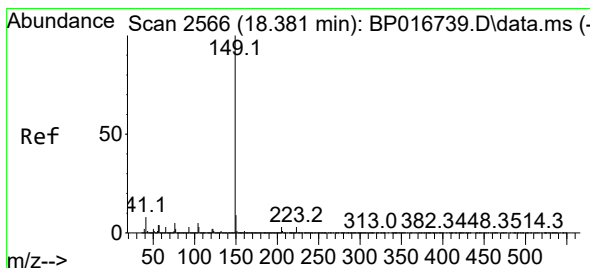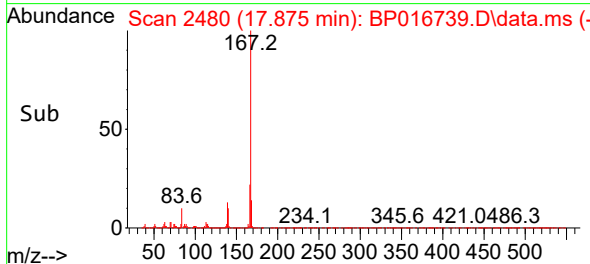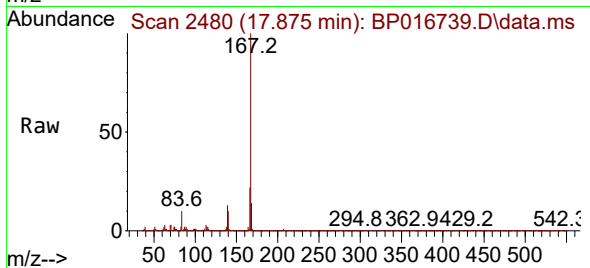

#78

Di-n-butylphthalate

Concen: 20.500 ng/ul

RT: 18.381 min Scan# 2566

Delta R.T. -0.006 min

Lab File: BP016739.D

Acq: 25 Aug 2023 09:12




Tgt Ion:149 Resp: 2830202


Ion Ratio Lower Upper

149 100

150 9.3 7.5 11.3

104 5.3 4.1 6.1

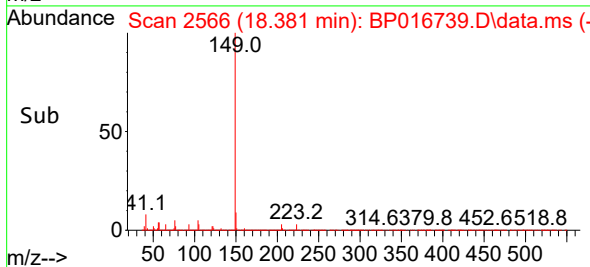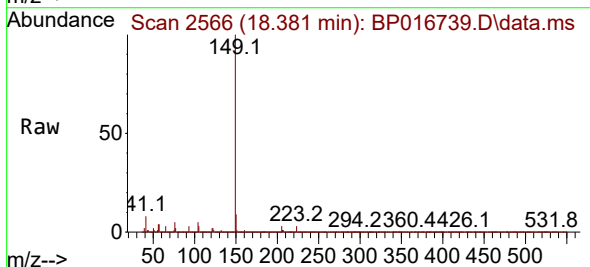



#80

Fluoranthene

Concen: 19.366 ng/ul

RT: 19.457 min Scan# 21

Delta R.T. -0.006 min

Lab File: BP016739.D

Acq: 25 Aug 2023 09:12

Instrument :

BNA_P

ClientSampleId :

SSTD020702





Tgt Ion:202 Resp: 2909337

Ion Ratio Lower Upper

202 100

101 12.9 9.7 14.5

100 10.2 7.4 11.2



#82

Pyrene

Concen: 19.705 ng/ul

RT: 19.816 min Scan# 2810

Delta R.T. -0.006 min

Lab File: BP016739.D

Acq: 25 Aug 2023 09:12




Tgt Ion:202 Resp: 3057847


Ion Ratio Lower Upper

202 100

101 14.7 11.4 17.2

100 12.4 9.4 14.2









#83
Butylbenzylphthalate
Concen: 19.690 ng/ul
RT: 20.675 min Scan# 2956
Delta R.T. -0.000 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12




Instrument :
BNA_P
ClientSampleId :
SSTD020702


Tgt Ion:149 Resp: 1317761
Ion Ratio Lower Upper
149 100
91 71.8 58.5 87.7
206 20.0 16.1 24.1

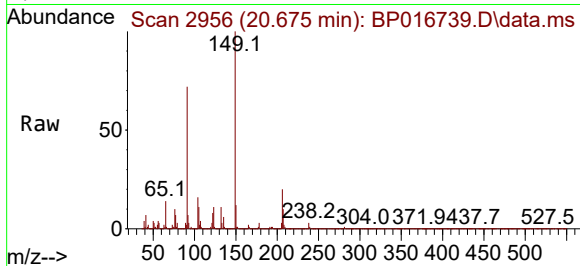

#84
3,3'-Dichlorobenzidine
Concen: 19.434 ng/ul
RT: 21.474 min Scan# 3092
Delta R.T. -0.000 min
Lab File: BP016739.D
Acq: 25 Aug 2023 09:12

Tgt Ion:252 Resp: 945879
Ion Ratio Lower Upper
252 100
254 64.3 52.1 78.1
126 11.9 9.6 14.4

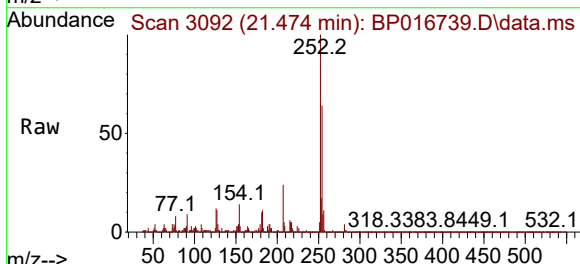

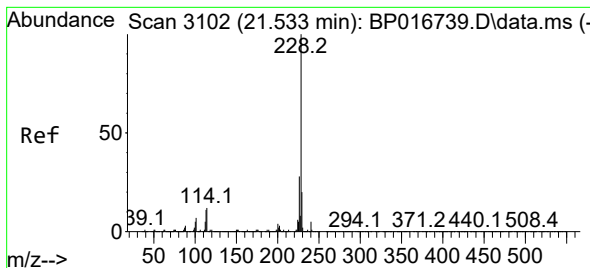

#85

Benzo(a)anthracene

Concen: 20.065 ng/ul

RT: 21.533 min Scan# 3102

Delta R.T. -0.006 min

Lab File: BP016739.D

Acq: 25 Aug 2023 09:12

Instrument :

BNA_P

ClientSampleId :

SSTD020702





Tgt Ion:228 Resp: 3147099

Ion Ratio Lower Upper

228 100

229 19.8 16.2 24.4

226 27.7 22.9 34.3

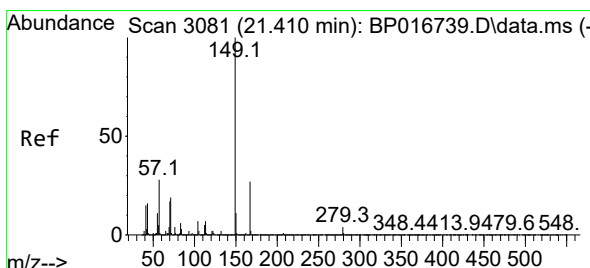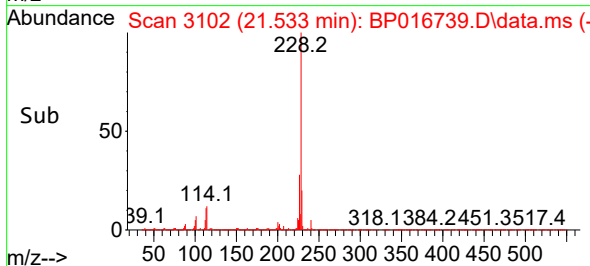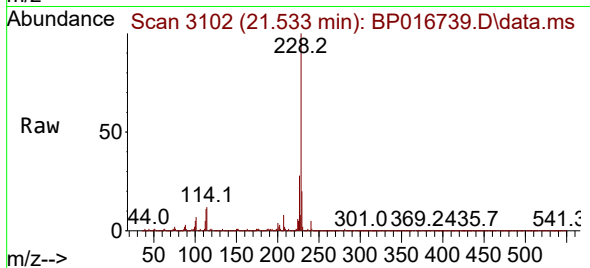

#86

Bis(2-ethylhexyl)phthalate

Concen: 20.018 ng/ul

RT: 21.410 min Scan# 3081

Delta R.T. -0.000 min

Lab File: BP016739.D

Acq: 25 Aug 2023 09:12




Tgt Ion:149 Resp: 1956163


Ion Ratio Lower Upper

149 100

167 27.3 22.1 33.1

279 3.6 3.0 4.4

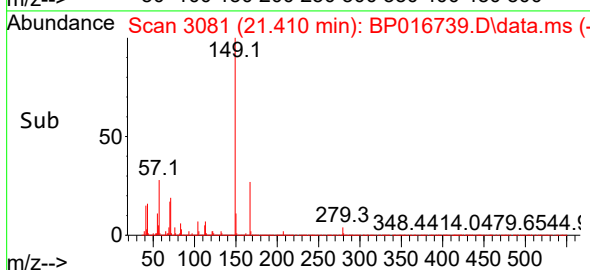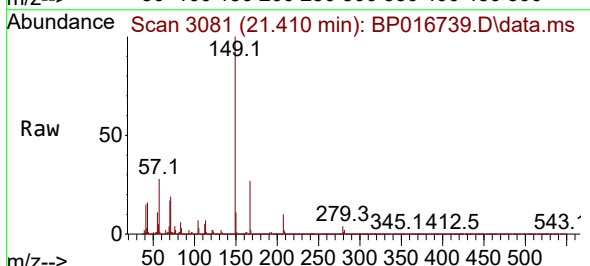



#87

Chrysene

Concen: 20.371 ng/ul

RT: 21.592 min Scan# 3112

Delta R.T. -0.006 min

Lab File: BP016739.D

Acq: 25 Aug 2023 09:12

Instrument :

BNA_P

ClientSampleId :

SSTD020702





Tgt Ion:228 Resp: 2902324

Ion Ratio Lower Upper

228 100

226 31.3 25.0 37.4

229 19.9 16.0 24.0



#89

Di-n-octyl phthalate

Concen: 18.623 ng/ul




RT: 22.392 min Scan# 3248


Delta R.T. -0.006 min

Lab File: BP016739.D

Acq: 25 Aug 2023 09:12

Tgt Ion:149 Resp: 3371519





#90

Benzo(b)fluoranthene

Concen: 19.812 ng/ul

RT: 23.321 min Scan# 3406

Delta R.T. -0.006 min

Lab File: BP016739.D

Acq: 25 Aug 2023 09:12

Instrument :

BNA_P

ClientSampleId :

SSTD020702





Tgt Ion:252 Resp: 3041403

Ion Ratio Lower Upper

252 100

253 22.0 17.7 26.5

125 11.7 9.0 13.4



#91

Benzo(k)fluoranthene

Concen: 19.385 ng/ul

RT: 23.380 min Scan# 3416

Delta R.T. -0.000 min

Lab File: BP016739.D

Acq: 25 Aug 2023 09:12




Tgt Ion:252 Resp: 2943087


Ion Ratio Lower Upper

252 100

253 21.9 18.1 27.1

125 10.8 8.9 13.3





#93

Benzo(a)pyrene

Concen: 20.069 ng/ul

RT: 24.010 min Scan# 3523

Delta R.T. -0.006 min

Lab File: BP016739.D

Acq: 25 Aug 2023 09:12

Instrument :

BNA_P

ClientSampleId :

SSTD020702





Tgt Ion:252 Resp: 2786793

Ion Ratio Lower Upper

252 100

253 22.2 17.8 26.8

125 12.4 9.9 14.9



#94

Indeno(1,2,3-cd)pyrene

Concen: 20.922 ng/ul

RT: 26.862 min Scan# 4008

Delta R.T. -0.012 min

Lab File: BP016739.D

Acq: 25 Aug 2023 09:12




Tgt Ion:276 Resp: 2968715


Ion Ratio Lower Upper

276 100

138 25.7 20.9 31.3

277 24.7 19.8 29.6

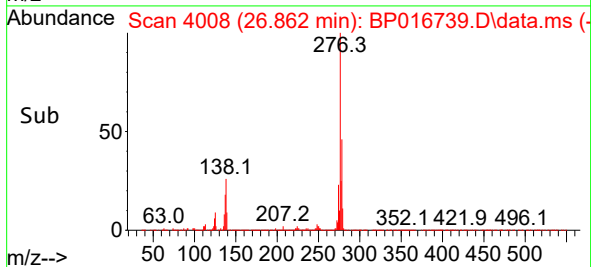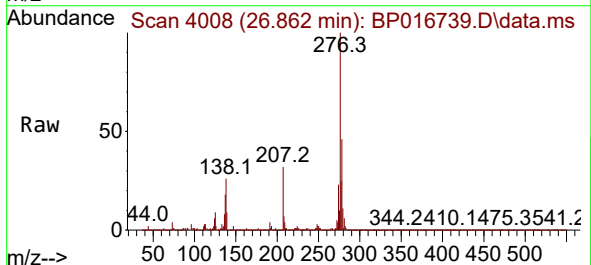



#95

Dibenzo(a,h)anthracene

Concen: 21.007 ng/ul

RT: 26.886 min Scan# 4012

Delta R.T. -0.012 min

Lab File: BP016739.D

Acq: 25 Aug 2023 09:12

Instrument :

BNA_P

ClientSampleId :

SSTD020702





Tgt Ion:278 Resp: 2475721

Ion Ratio Lower Upper

278 100

139 18.4 15.0 22.6

279 23.8 19.4 29.2



#96

Benzo(g,h,i)perylene

Concen: 21.186 ng/ul

RT: 27.721 min Scan# 4154

Delta R.T. -0.006 min

Lab File: BP016739.D

Acq: 25 Aug 2023 09:12

Tgt Ion:276 Resp: 2279114

Ion Ratio Lower Upper

276 100

138 24.9 20.2 30.4

277 23.2 19.3 28.9

