

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082523\
 Data File : BP016745.D
 Acq On : 25 Aug 2023 13:29
 Operator : MA/JU
 Sample : 04037-10
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYJ4

Quant Time: Aug 25 22:26:38 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 25 01:47:30 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.034	152	393207	20.000	ng/ul	0.00
20) Naphthalene-d8	10.863	136	1713331	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.687	164	1093304	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.457	188	2414018	20.000	ng/ul	0.00
79) Chrysene-d12	21.551	240	1982701	20.000	ng/ul	0.00
88) Perylene-d12	24.122	264	1755668	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	40194	4.225	ng/uL	0.00
4) Pyridine-d5	3.834	84	24965	0.859	ng/ul	0.01
7) Phenol-d5	7.175	99	531709	15.207	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.375	67	377019	16.919	ng/ul	0.00
11) 2-Chlorophenol-d4	7.552	132	339190	12.903	ng/ul	0.00
15) 4-Methylphenol-d8	8.734	113	373773	13.095	ng/ul	-0.01
21) Nitrobenzene-d5	9.234	128	223636	17.263	ng/ul	0.00
24) 2-Nitrophenol-d4	9.946	143	136960	10.030	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.469	165	250181	9.828	ng/ul	0.00
31) 4-Chloroaniline-d4	11.022	131	563746	14.440	ng/ul	0.00
46) Dimethylphthalate-d6	14.099	166	1451930	17.610	ng/ul	0.00
49) Acenaphthylene-d8	14.387	160	1613874	17.315	ng/ul	0.00
54) 4-Nitrophenol-d4	14.893	143	20945	1.229	ng/ul	0.00
60) Fluorene-d10	15.681	176	1266228	18.237	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.804	200	12374	0.861	ng/ul	0.00
73) Anthracene-d10	17.557	188	1934065	18.075	ng/ul	0.00
81) Pyrene-d10	19.787	212	2327241	21.372	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.951	264	1688236	19.197	ng/ul	-0.01
Target Compounds						
					Qvalue	
16) Acetophenone	8.887	105	55850	1.262	ng/ul	95
80) Fluoranthene	19.457	202	145471	1.112	ng/ul	100
82) Pyrene	19.816	202	183445	1.358	ng/ul	100
87) Chrysene	21.592	228	165244	1.332	ng/ul	98
90) Benzo(b)fluoranthene	23.322	252	214436	1.913	ng/ul#	96
96) Benzo(g,h,i)perylene	27.704	276	83340	1.061	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082523\
Data File : BP016745.D
Acq On : 25 Aug 2023 13:29
Operator : MA/JU
Sample : 04037-10
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYJ4

Quant Time: Aug 25 22:26:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 25 01:47:30 2023
Response via : Initial Calibration




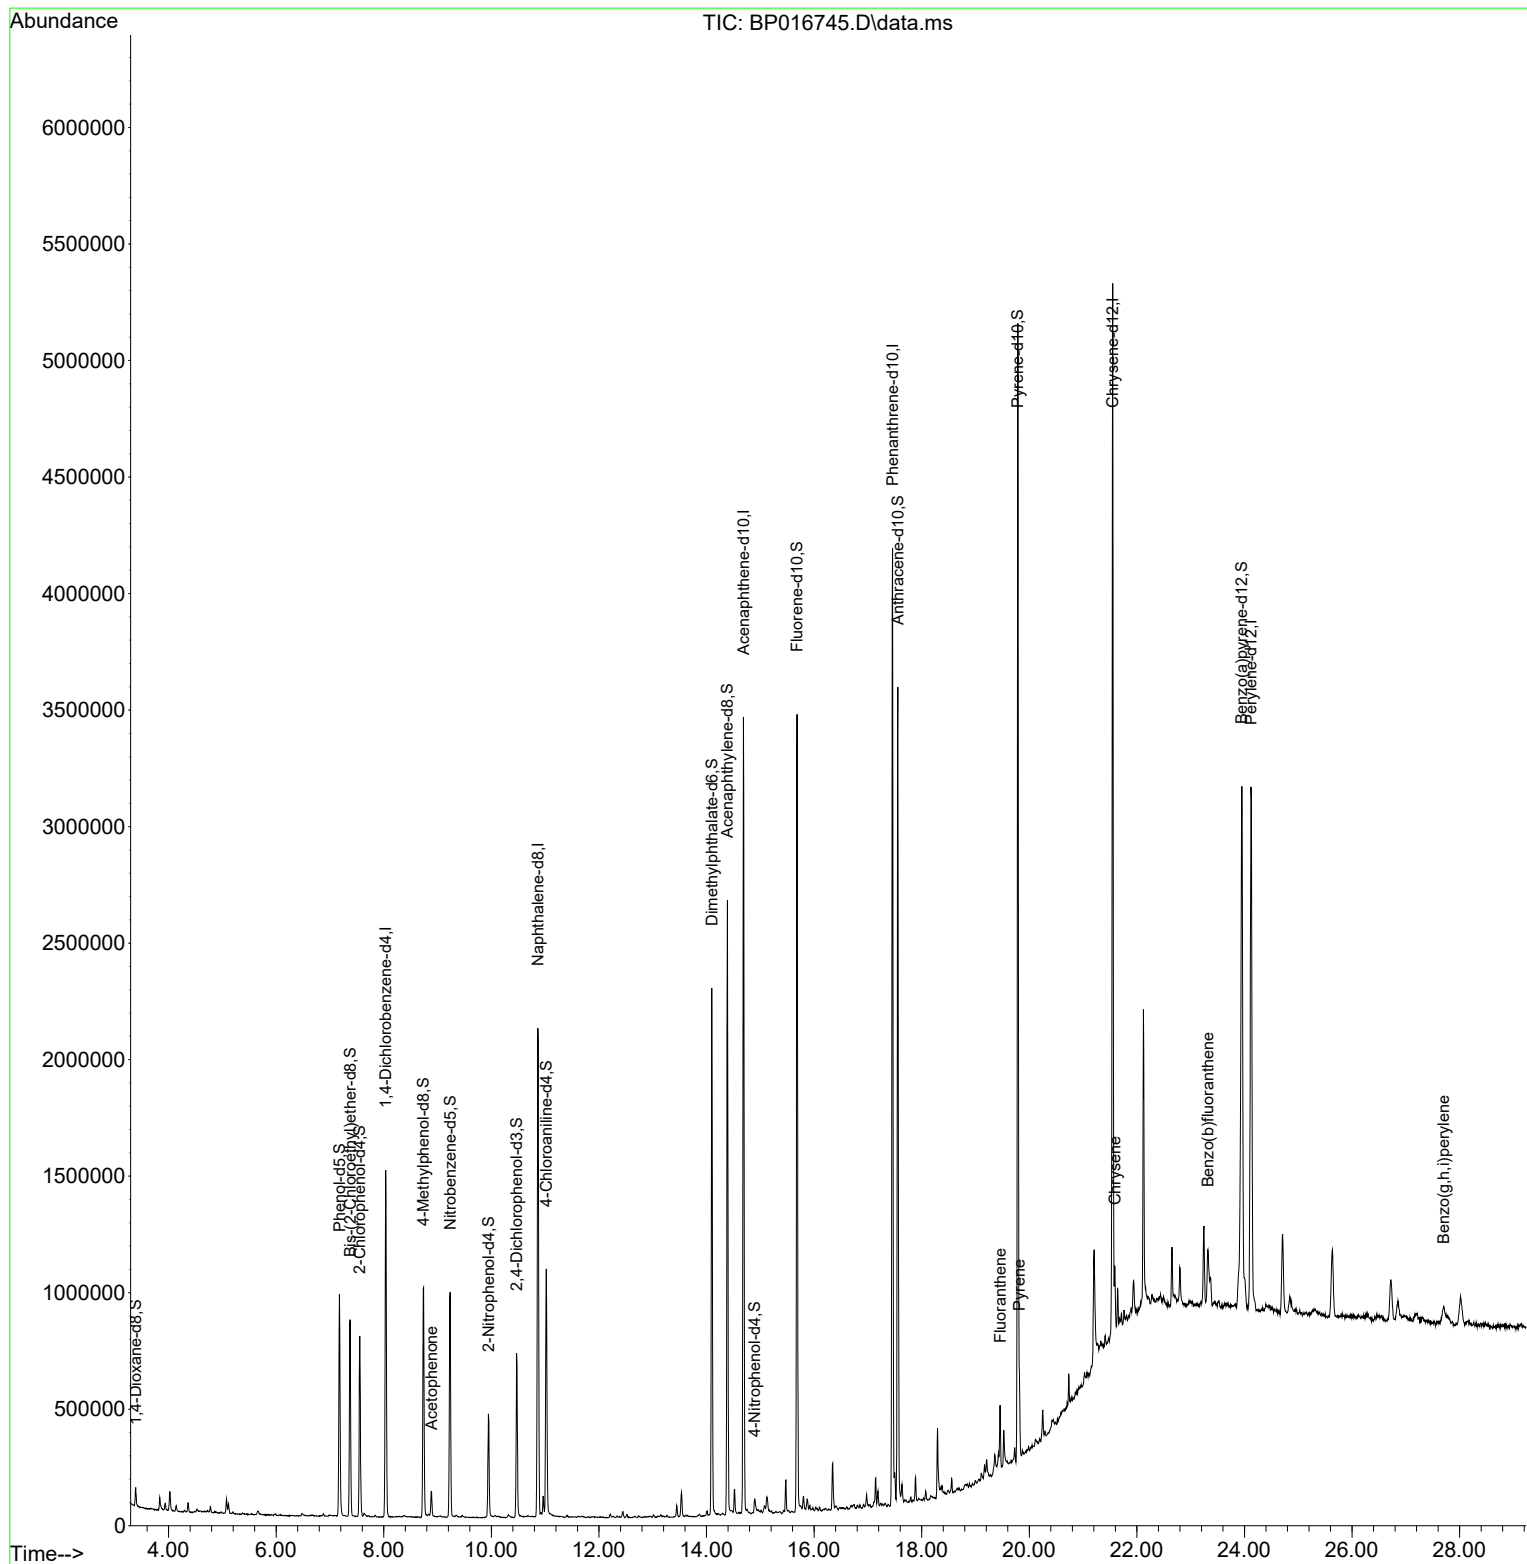


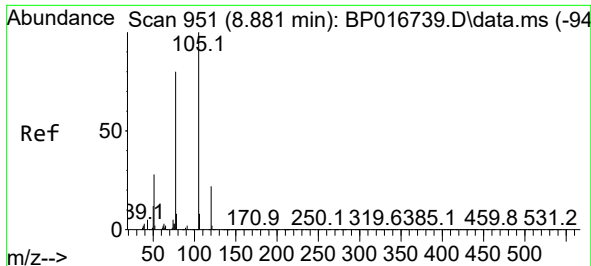

#16
Acetophenone
Concen: 1.262 ng/ul
RT: 8.887 min Scan# 91
Delta R.T. 0.000 min
Lab File: BP016745.D
Acq: 25 Aug 2023 13:29




Instrument :
BNA_P
ClientSampleId :
EZYJ4


Tgt Ion:105 Resp: 55850
Ion Ratio Lower Upper
105 100
77 74.8 64.2 96.4
51 27.4 22.2 33.4

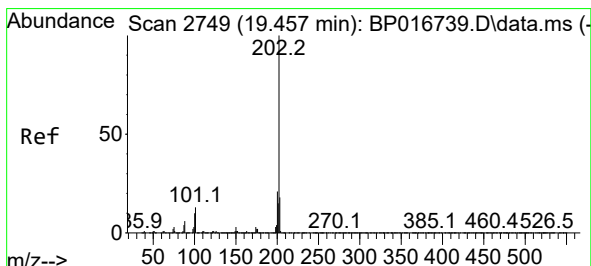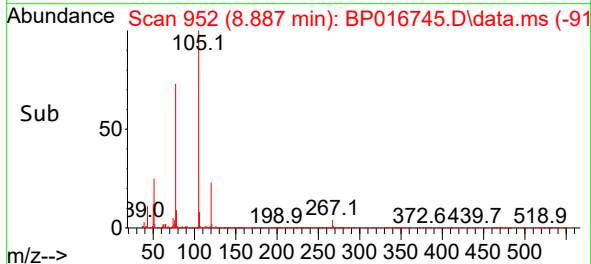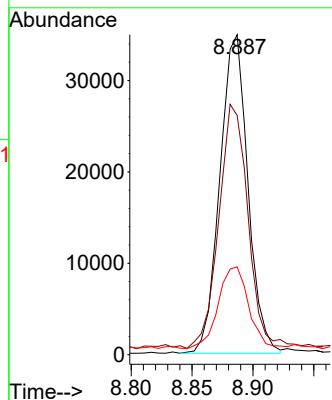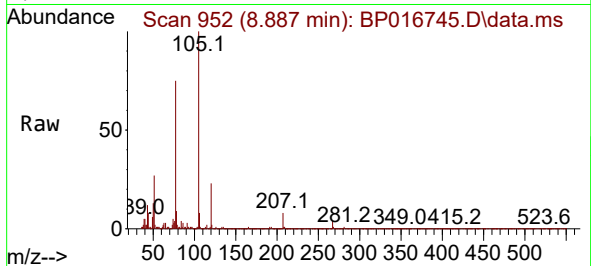

#80
Fluoranthene
Concen: 1.112 ng/ul
RT: 19.457 min Scan# 2749
Delta R.T. -0.006 min
Lab File: BP016745.D
Acq: 25 Aug 2023 13:29

Tgt Ion:202 Resp: 145471
Ion Ratio Lower Upper
202 100
101 12.2 9.7 14.5
100 9.3 7.4 11.2

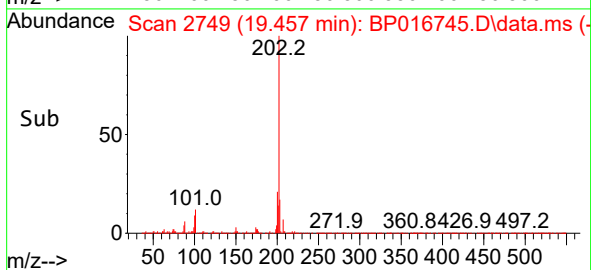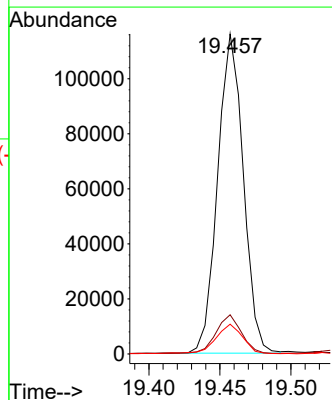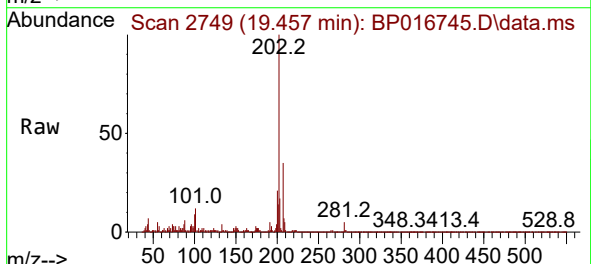

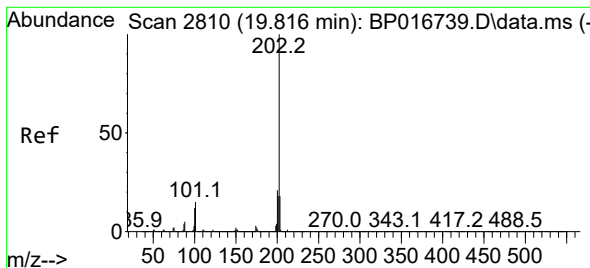

#82

Pyrene

Concen: 1.358 ng/ul

RT: 19.816 min Scan# 21

Delta R.T. -0.006 min

Lab File: BP016745.D

Acq: 25 Aug 2023 13:29

Instrument :

BNA_P

ClientSampleId :

EZYJ4





Tgt Ion:202 Resp: 183445

Ion Ratio Lower Upper

202 100

101 14.3 11.4 17.2

100 11.8 9.4 14.2

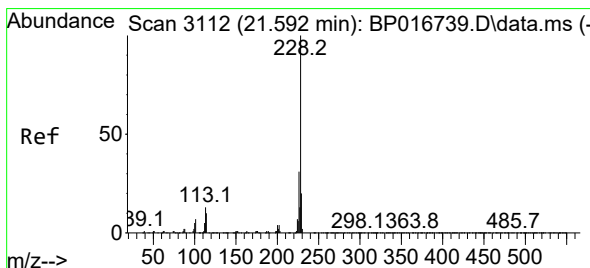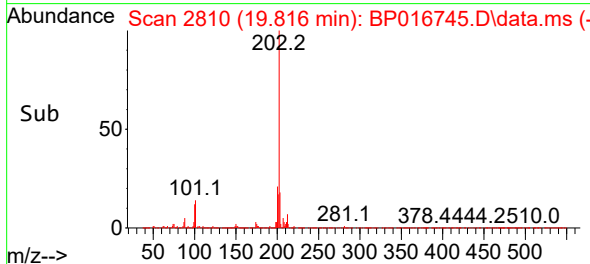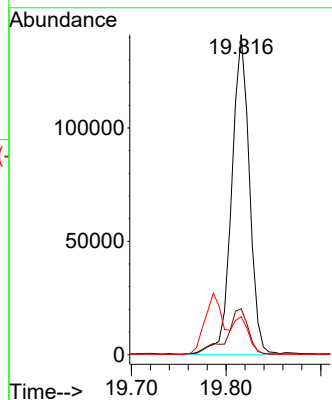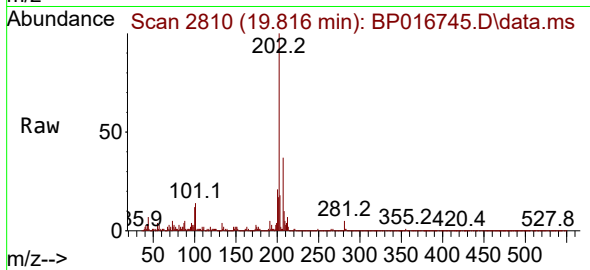

#87

Chrysene

Concen: 1.332 ng/ul

RT: 21.592 min Scan# 3112

Delta R.T. -0.006 min

Lab File: BP016745.D

Acq: 25 Aug 2023 13:29




Tgt Ion:228 Resp: 165244


Ion Ratio Lower Upper

228 100

226 32.0 25.0 37.4

229 21.6 16.0 24.0

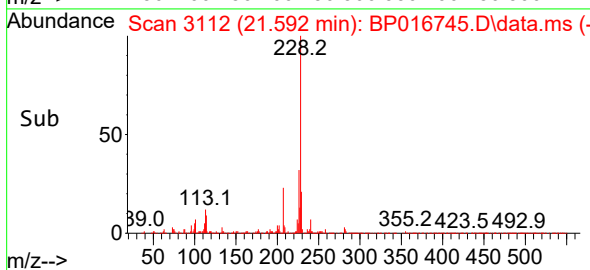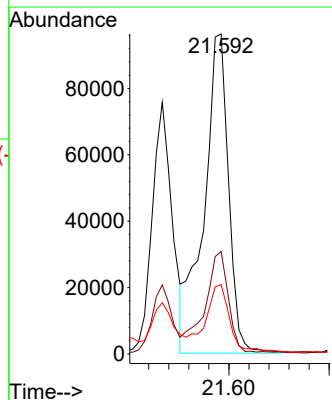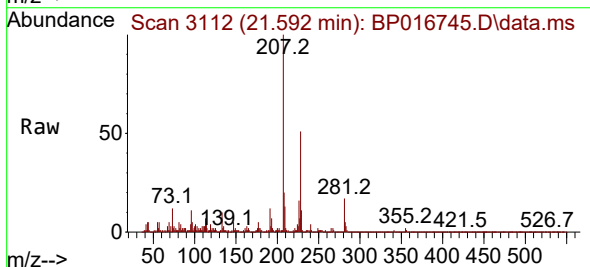

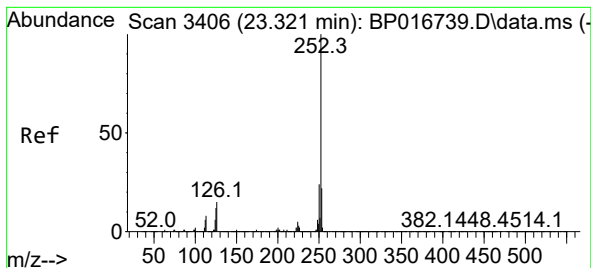

#90

Benzo(b)fluoranthene

Concen: 1.913 ng/ul

RT: 23.322 min Scan# 3406

Delta R.T. -0.006 min

Lab File: BP016745.D

Acq: 25 Aug 2023 13:29

Instrument :

BNA_P

ClientSampleId :

EZYJ4





Tgt Ion:252 Resp: 214436

Ion Ratio Lower Upper

252 100

253 23.0 17.7 26.5

125 14.8 9.0 13.4#

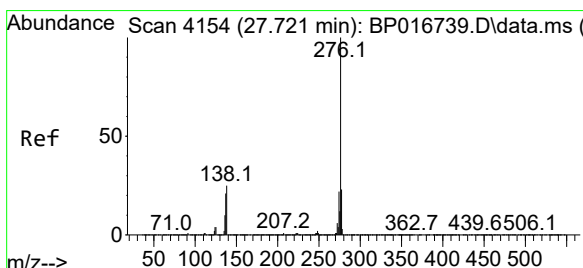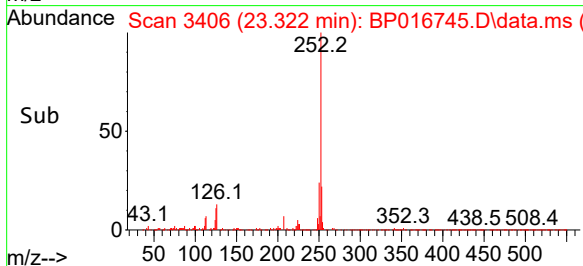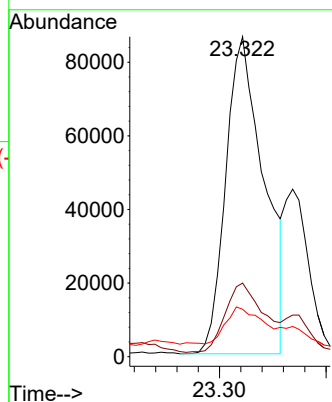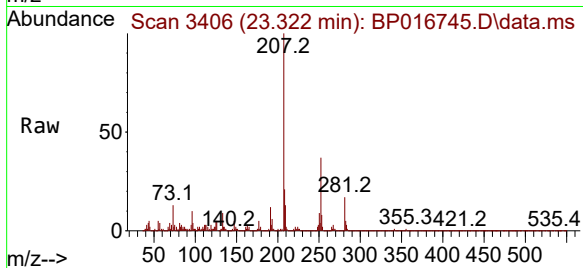

#96

Benzo(g,h,i)perylene

Concen: 1.061 ng/ul

RT: 27.704 min Scan# 4151

Delta R.T. -0.023 min

Lab File: BP016745.D

Acq: 25 Aug 2023 13:29

Tgt Ion:276 Resp: 83340

Ion Ratio Lower Upper

276 100

138 21.6 20.2 30.4

277 24.6 19.3 28.9

