

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082523\
 Data File : BP016747.D
 Acq On : 25 Aug 2023 15:27
 Operator : MA/JU
 Sample : 04037-12
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYH1

Quant Time: Aug 25 22:27:02 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 25 01:47:30 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.034	152	366049	20.000	ng/ul	0.00
20) Naphthalene-d8	10.863	136	1616693	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.687	164	993570	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.457	188	2155051	20.000	ng/ul	0.00
79) Chrysene-d12	21.551	240	1635993	20.000	ng/ul	0.00
88) Perylene-d12	24.127	264	1410927	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	41360	4.670	ng/uL	0.00
4) Pyridine-d5	3.834	84	26582	0.982	ng/ul	0.01
7) Phenol-d5	7.175	99	620655	19.068	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.369	67	409332	19.731	ng/ul	0.00
11) 2-Chlorophenol-d4	7.552	132	482386	19.711	ng/ul	0.00
15) 4-Methylphenol-d8	8.734	113	421640	15.868	ng/ul	-0.01
21) Nitrobenzene-d5	9.234	128	240692	19.690	ng/ul	0.00
24) 2-Nitrophenol-d4	9.946	143	243352	18.887	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.469	165	438842	18.269	ng/ul	0.00
31) 4-Chloroaniline-d4	11.022	131	585397	15.891	ng/ul	0.00
46) Dimethylphthalate-d6	14.098	166	1512255	20.183	ng/ul	0.00
49) Acenaphthylene-d8	14.387	160	1765504	20.843	ng/ul	0.00
54) 4-Nitrophenol-d4	14.892	143	82798	5.346	ng/ul	0.00
60) Fluorene-d10	15.681	176	1379805	21.867	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.804	200	39176	3.053	ng/ul	0.00
73) Anthracene-d10	17.557	188	2091429	21.894	ng/ul	0.00
81) Pyrene-d10	19.786	212	2404283	26.758	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.957	264	1594114	22.556	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.881	105	47443	1.151	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082523\
Data File : BP016747.D
Acq On : 25 Aug 2023 15:27
Operator : MA/JU
Sample : 04037-12
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYH1

Quant Time: Aug 25 22:27:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 25 01:47:30 2023
Response via : Initial Calibration

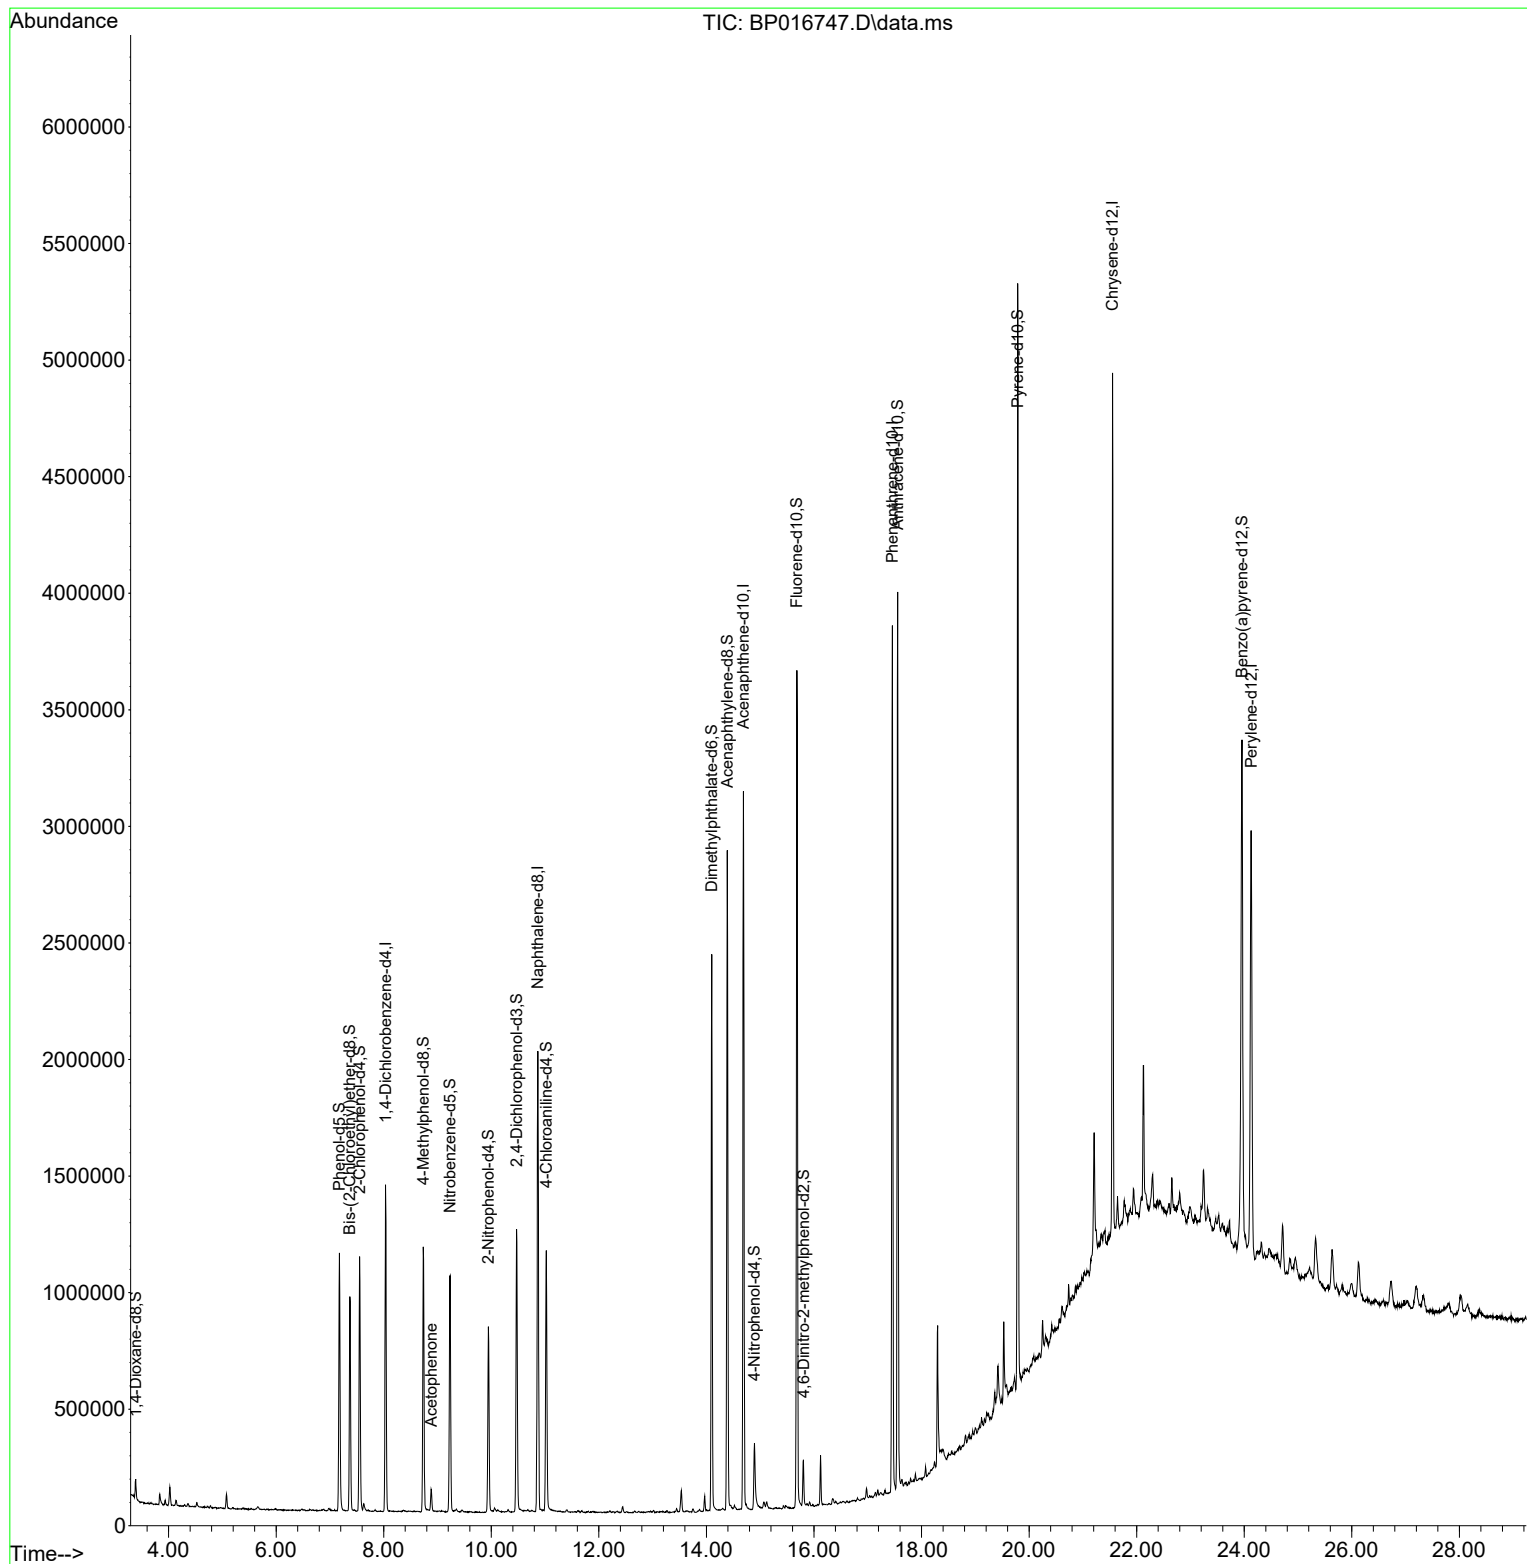

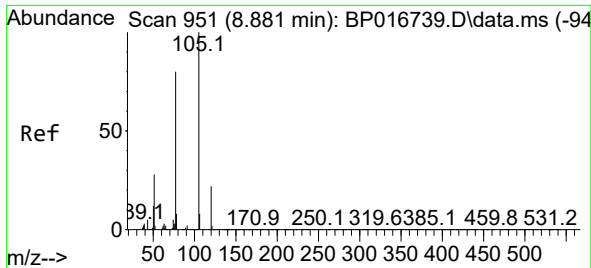

#16
 Acetophenone
 Concen: 1.151 ng/ul
 RT: 8.881 min Scan# 91
 Delta R.T. -0.006 min
 Lab File: BP016747.D
 Acq: 25 Aug 2023 15:27

Instrument :
 BNA_P
 ClientSampleId :
 EZYH1

Tgt Ion:	105	Resp:	47443
Ion	Ratio	Lower	Upper
105	100		
77	82.7	64.2	96.4
51	30.2	22.2	33.4

