




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082523\
 Data File : BP016765.D
 Acq On : 26 Aug 2023 02:18
 Operator : MA/JU
 Sample : 04105-10
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH960

Manual IntegrationsAPPROVED

Quant Time: Aug 26 02:55:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 25 01:47:30 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/26/2023
 Supervised By :mohammad ahmed 08/26/2023

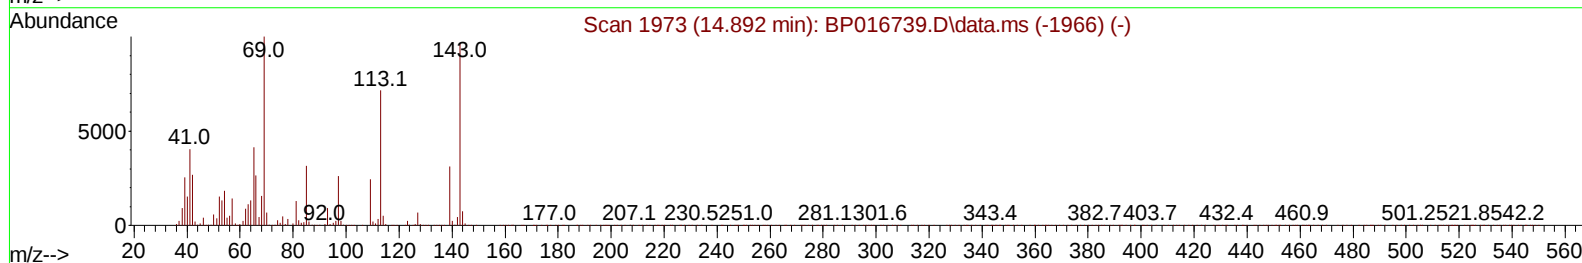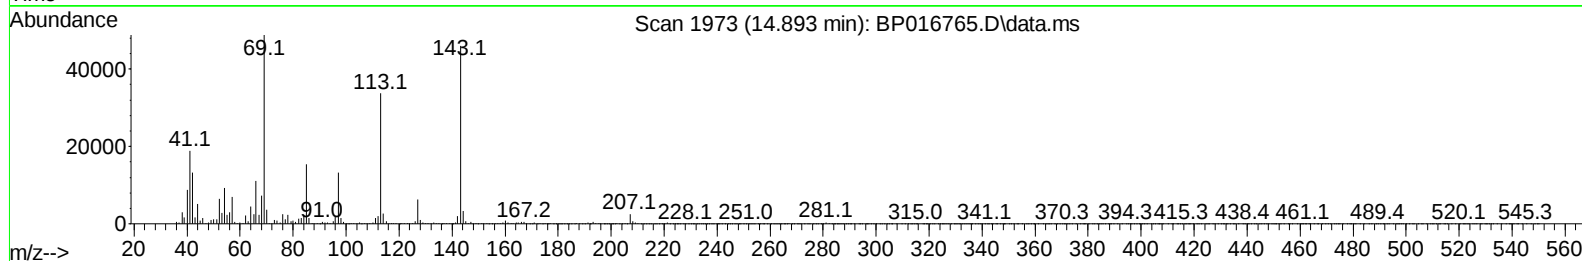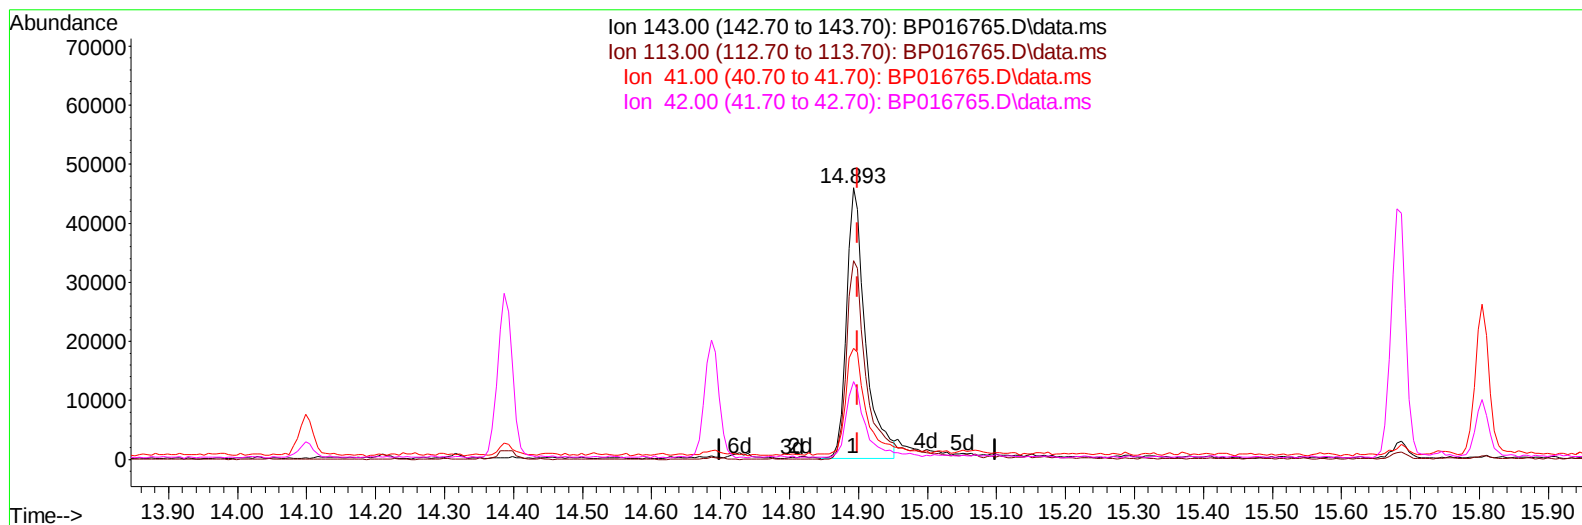

TIC: BP016765.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.893min (-0.006) 5.64 ng/u1

response 86446

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	71.70	73.28
41.00	40.70	41.01
42.00	27.10	28.62




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082523\
 Data File : BP016765.D
 Acq On : 26 Aug 2023 02:18
 Operator : MA/JU
 Sample : 04105-10
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH960

Manual IntegrationsAPPROVED

Quant Time: Aug 26 02:55:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 25 01:47:30 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/26/2023
 Supervised By :mohammad ahmed 08/26/2023

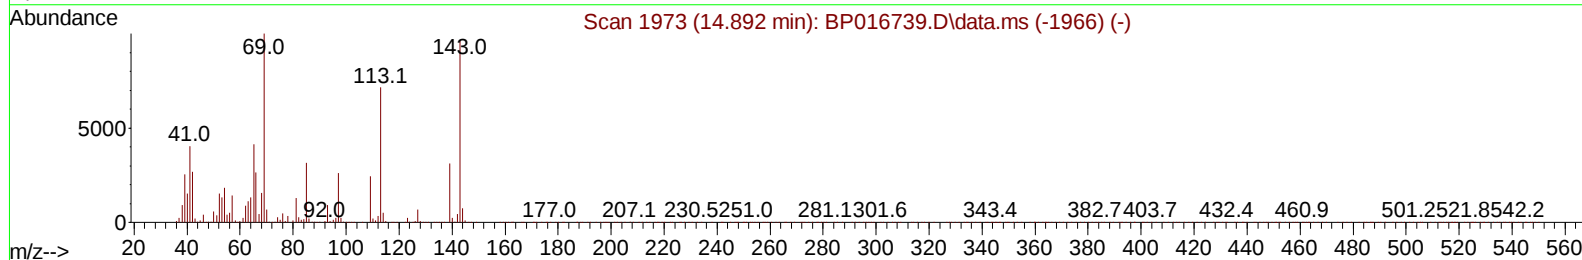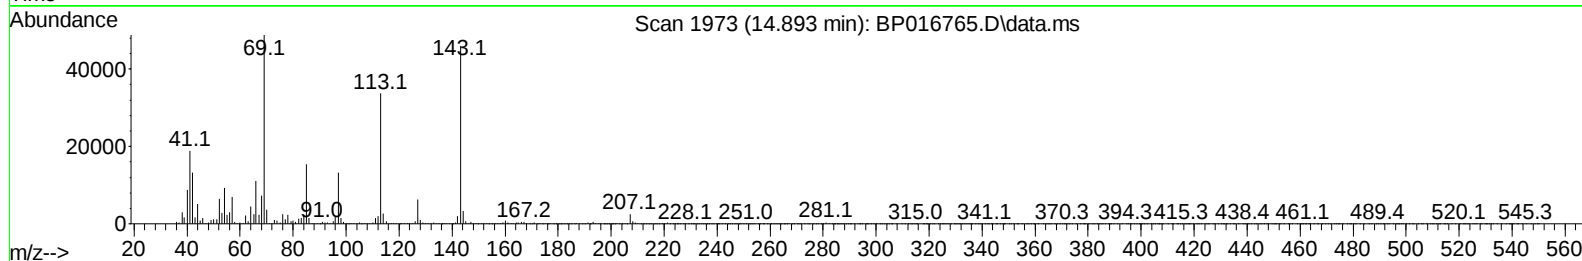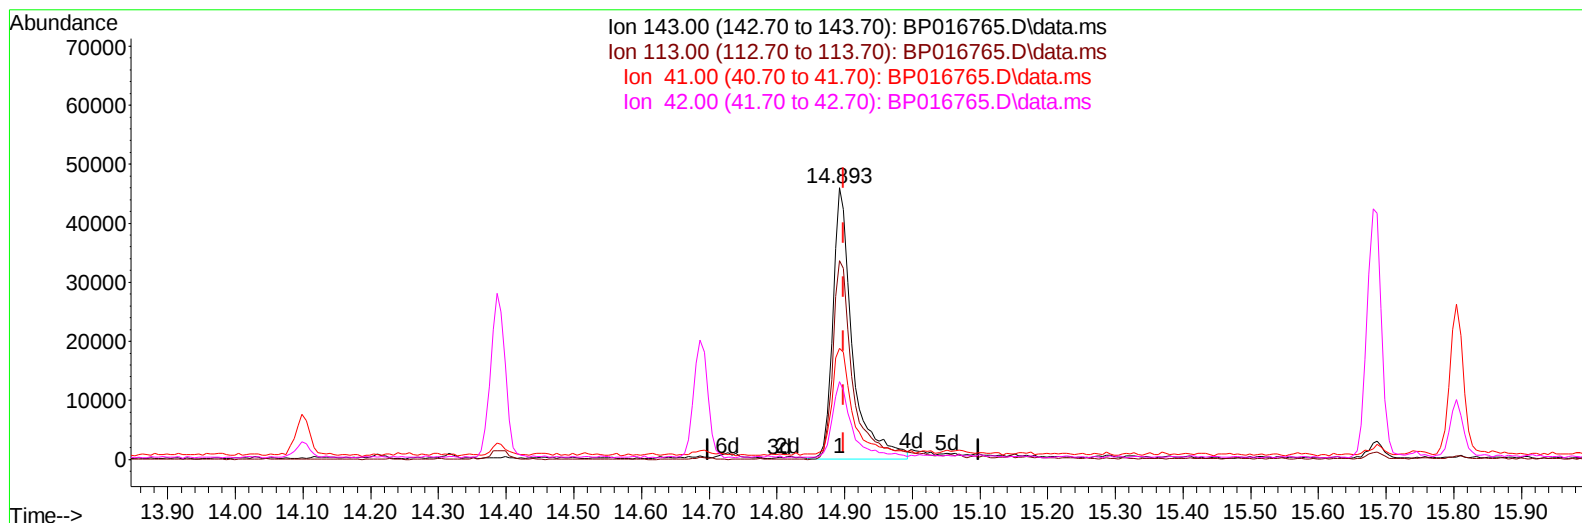

TIC: BP016765.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.893min (-0.006) 6.02 ng/ul m

response 92313

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	71.70	73.28
41.00	40.70	41.01
42.00	27.10	28.62

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082523\
 Data File : BP016765.D
 Acq On : 26 Aug 2023 02:18
 Operator : MA/JU
 Sample : 04105-10
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH960

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/26/2023
 Supervised By :mohammad ahmed 08/26/2023

Quant Time: Aug 26 02:56:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 25 01:47:30 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.034	152	368559	20.000	ng/ul	0.00
20) Naphthalene-d8	10.863	136	1598978	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.687	164	983009	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.457	188	2042903	20.000	ng/ul	0.00
79) Chrysene-d12	21.551	240	1168507	20.000	ng/ul	0.00
88) Perylene-d12	24.121	264	1105298	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	57927	6.496	ng/uL	0.00
4) Pyridine-d5	3.823	84	379873	13.940	ng/ul	0.00
7) Phenol-d5	7.175	99	296975	9.062	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.369	67	810794	38.817	ng/ul	0.00
11) 2-Chlorophenol-d4	7.552	132	787990	31.979	ng/ul	0.00
15) 4-Methylphenol-d8	8.740	113	535638	20.021	ng/ul	0.00
21) Nitrobenzene-d5	9.234	128	509497	42.143	ng/ul	0.00
24) 2-Nitrophenol-d4	9.952	143	529742	41.569	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.475	165	874223	36.797	ng/ul	0.00
31) 4-Chloroaniline-d4	11.022	131	1153793	31.668	ng/ul	0.00
46) Dimethylphthalate-d6	14.098	166	3108102	41.926	ng/ul	0.00
49) Acenaphthylene-d8	14.387	160	3547889	42.336	ng/ul	0.00
54) 4-Nitrophenol-d4	14.893	143	92313m	6.025	ng/ul	0.00
60) Fluorene-d10	15.687	176	2674068	42.835	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.804	200	408162	33.549	ng/ul	0.00
73) Anthracene-d10	17.557	188	4185046	46.217	ng/ul	0.00
81) Pyrene-d10	19.786	212	4140629	64.519	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.951	264	2542348	45.919	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082523\
Data File : BP016765.D
Acq On : 26 Aug 2023 02:18
Operator : MA/JU
Sample : 04105-10
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH960

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/26/2023
Supervised By :mohammad ahmed 08/26/2023

Quant Time: Aug 26 02:56:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 25 01:47:30 2023
Response via : Initial Calibration

