




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082523\
 Data File : BP016777.D
 Acq On : 26 Aug 2023 09:39
 Operator : MA/JU
 Sample : 04105-17
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHAA2

Manual IntegrationsAPPROVED

Quant Time: Aug 26 13:24:44 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 25 01:47:30 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/28/2023
 Supervised By :mohammad ahmed 08/28/2023

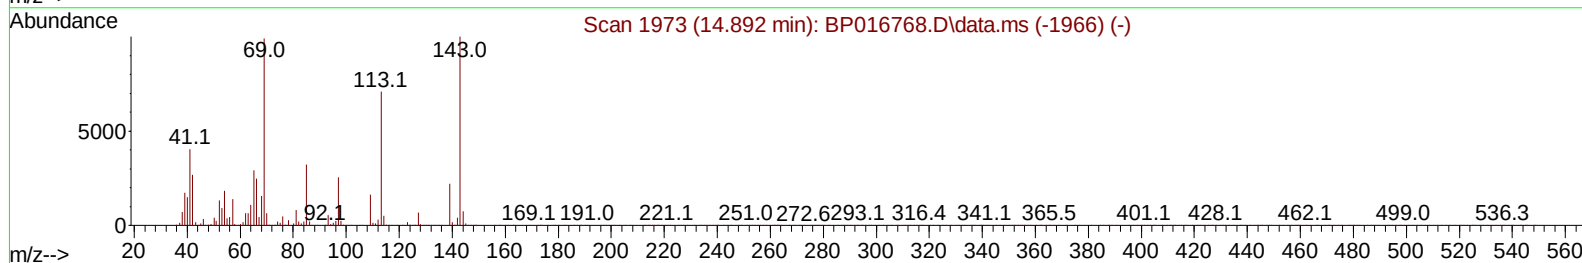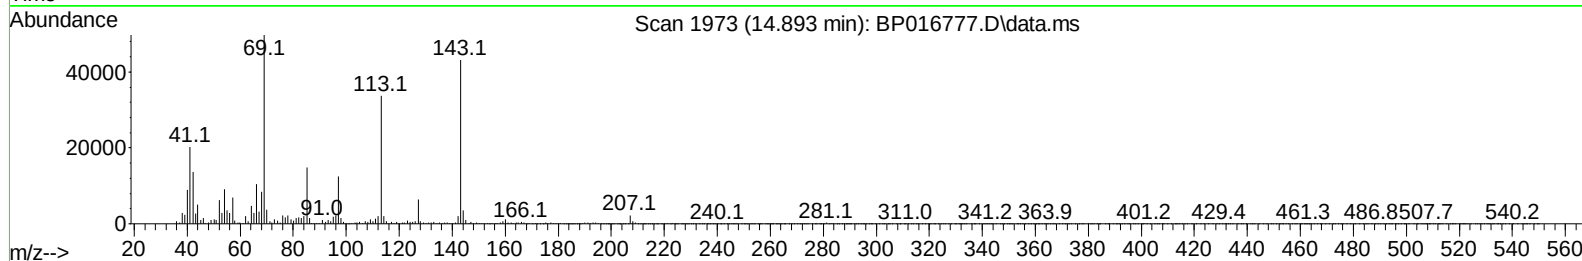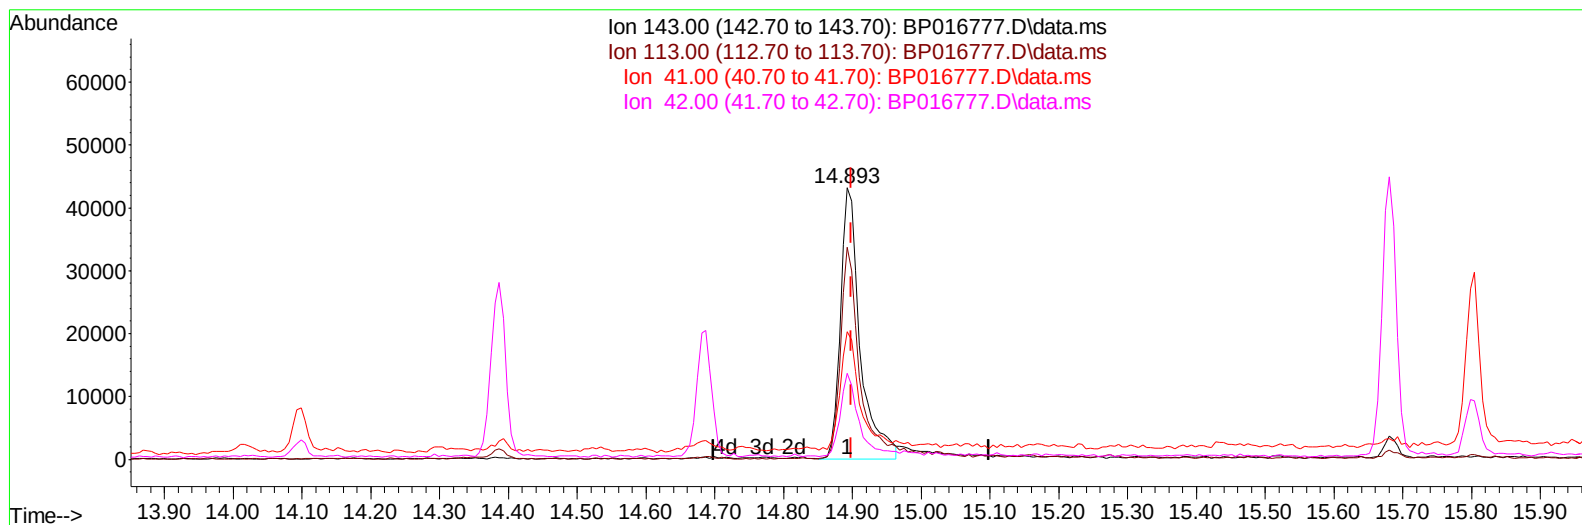

TIC: BP016777.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.893min (-0.006) 5.70 ng/ul

response 85931

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	71.70	78.08
41.00	40.70	47.03
42.00	27.10	31.65




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082523\
Data File : BP016777.D
Acq On : 26 Aug 2023 09:39
Operator : MA/JU
Sample : 04105-17
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAA2

Manual IntegrationsAPPROVED

Quant Time: Aug 26 13:24:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 25 01:47:30 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/28/2023
Supervised By :mohammad ahmed 08/28/2023

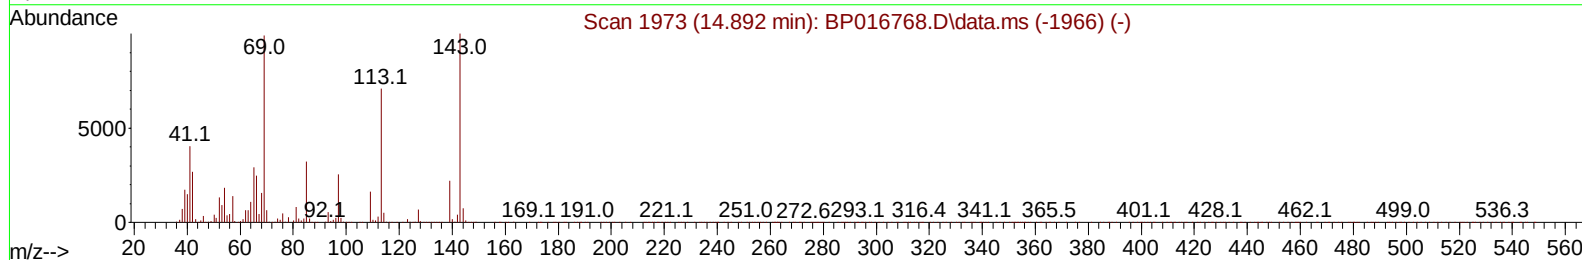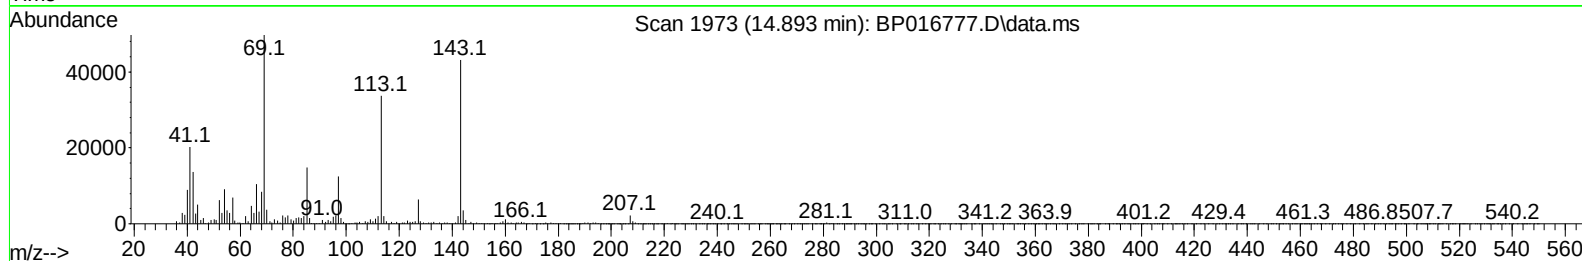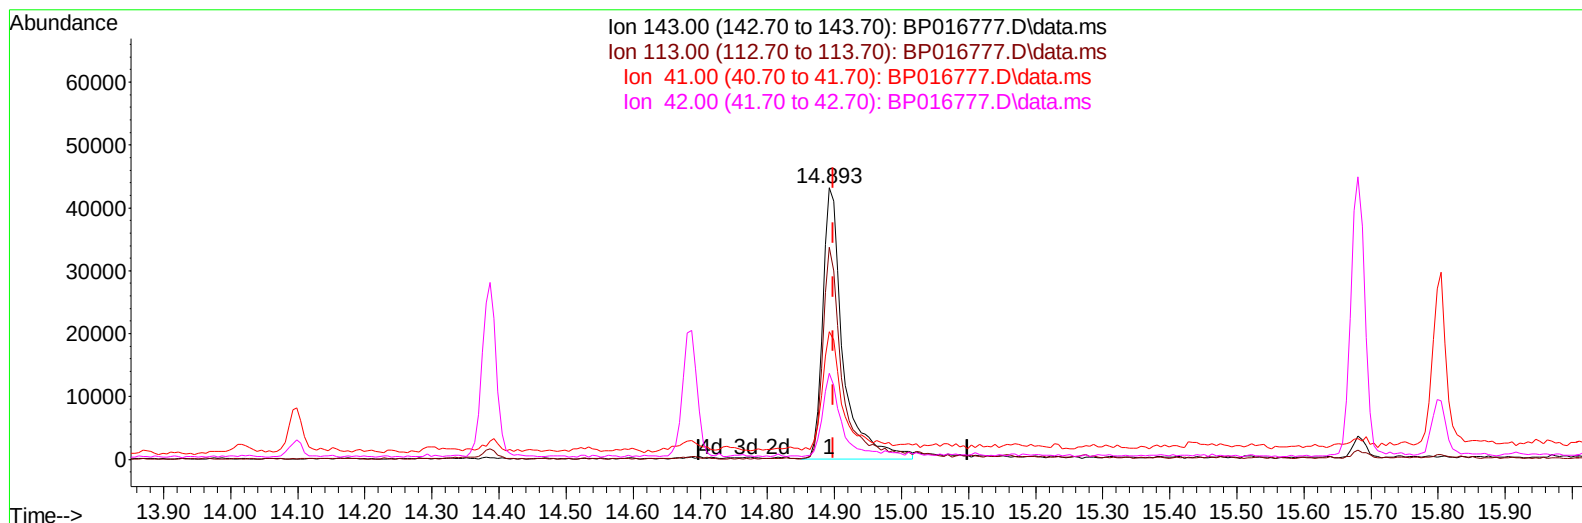

TIC: BP016777.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.893min (-0.006) 6.00 ng/ul m

response 90503

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	71.70	78.08
41.00	40.70	47.03
42.00	27.10	31.65

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082523\
 Data File : BP016777.D
 Acq On : 26 Aug 2023 09:39
 Operator : MA/JU
 Sample : 04105-17
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHAA2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/28/2023
 Supervised By :mohammad ahmed 08/28/2023

Quant Time: Aug 26 15:32:51 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 25 01:47:30 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.034	152	348542	20.000	ng/ul	0.00
20) Naphthalene-d8	10.863	136	1550999	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.687	164	967163	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.457	188	2133101	20.000	ng/ul	0.00
79) Chrysene-d12	21.551	240	1741295	20.000	ng/ul	0.00
88) Perylene-d12	24.127	264	1510677	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	50438	5.981	ng/uL	0.00
4) Pyridine-d5	3.823	84	348533	13.524	ng/ul	0.00
7) Phenol-d5	7.175	99	255808	8.254	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.369	67	753167	38.129	ng/ul	0.00
11) 2-Chlorophenol-d4	7.552	132	715395	30.701	ng/ul	0.00
15) 4-Methylphenol-d8	8.734	113	484924	19.167	ng/ul	-0.01
21) Nitrobenzene-d5	9.228	128	483394	41.220	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.946	143	502488	40.650	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.469	165	845359	36.683	ng/ul	0.00
31) 4-Chloroaniline-d4	11.022	131	1137425	32.185	ng/ul	0.00
46) Dimethylphthalate-d6	14.099	166	3045679	41.757	ng/ul	0.00
49) Acenaphthylene-d8	14.387	160	3503951	42.496	ng/ul	0.00
54) 4-Nitrophenol-d4	14.893	143	90503m	6.003	ng/ul	0.00
60) Fluorene-d10	15.681	176	2678638	43.611	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.804	200	412638	32.483	ng/ul	0.00
73) Anthracene-d10	17.557	188	4280819	45.275	ng/ul	0.00
81) Pyrene-d10	19.792	212	4912353	51.366	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.957	264	3518473	46.497	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082523\
Data File : BP016777.D
Acq On : 26 Aug 2023 09:39
Operator : MA/JU
Sample : 04105-17
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAA2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/28/2023
Supervised By :mohammad ahmed 08/28/2023

Quant Time: Aug 26 15:32:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 25 01:47:30 2023
Response via : Initial Calibration

