

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082523\
 Data File : BP016748.D
 Acq On : 25 Aug 2023 16:01
 Operator : MA/JU
 Sample : 04037-17
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYD7

Quant Time: Aug 25 23:09:14 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 25 01:47:30 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.034	152	288173	20.000	ng/ul	0.00
20) Naphthalene-d8	10.863	136	1283504	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.687	164	805900	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.457	188	1757540	20.000	ng/ul	0.00
79) Chrysene-d12	21.557	240	1548456	20.000	ng/ul	0.00
88) Perylene-d12	24.127	264	1561581	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	35920	5.152	ng/uL	0.00
4) Pyridine-d5	3.834	84	24005	1.127	ng/ul	0.01
7) Phenol-d5	7.175	99	570465	22.262	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.370	67	373191	22.851	ng/ul	0.00
11) 2-Chlorophenol-d4	7.552	132	446359	23.168	ng/ul	0.00
15) 4-Methylphenol-d8	8.734	113	403716	19.300	ng/ul	-0.01
21) Nitrobenzene-d5	9.234	128	225444	23.231	ng/ul	0.00
24) 2-Nitrophenol-d4	9.946	143	242294	23.686	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.469	165	445755	23.374	ng/ul	0.00
31) 4-Chloroaniline-d4	11.022	131	594845	20.340	ng/ul	0.00
46) Dimethylphthalate-d6	14.099	166	1701718	28.000	ng/ul	0.00
49) Acenaphthylene-d8	14.387	160	1901955	27.683	ng/ul	0.00
54) 4-Nitrophenol-d4	14.893	143	190152	15.137	ng/ul	0.00
60) Fluorene-d10	15.681	176	1515444	29.610	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.804	200	173710	16.596	ng/ul	0.00
73) Anthracene-d10	17.557	188	2410628	30.944	ng/ul	0.00
81) Pyrene-d10	19.792	212	2828471	33.259	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.957	264	2464656	31.509	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.881	105	49183	1.516	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082523\
Data File : BP016748.D
Acq On : 25 Aug 2023 16:01
Operator : MA/JU
Sample : 04037-17
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYD7


Quant Time: Aug 25 23:09:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 25 01:47:30 2023
Response via : Initial Calibration

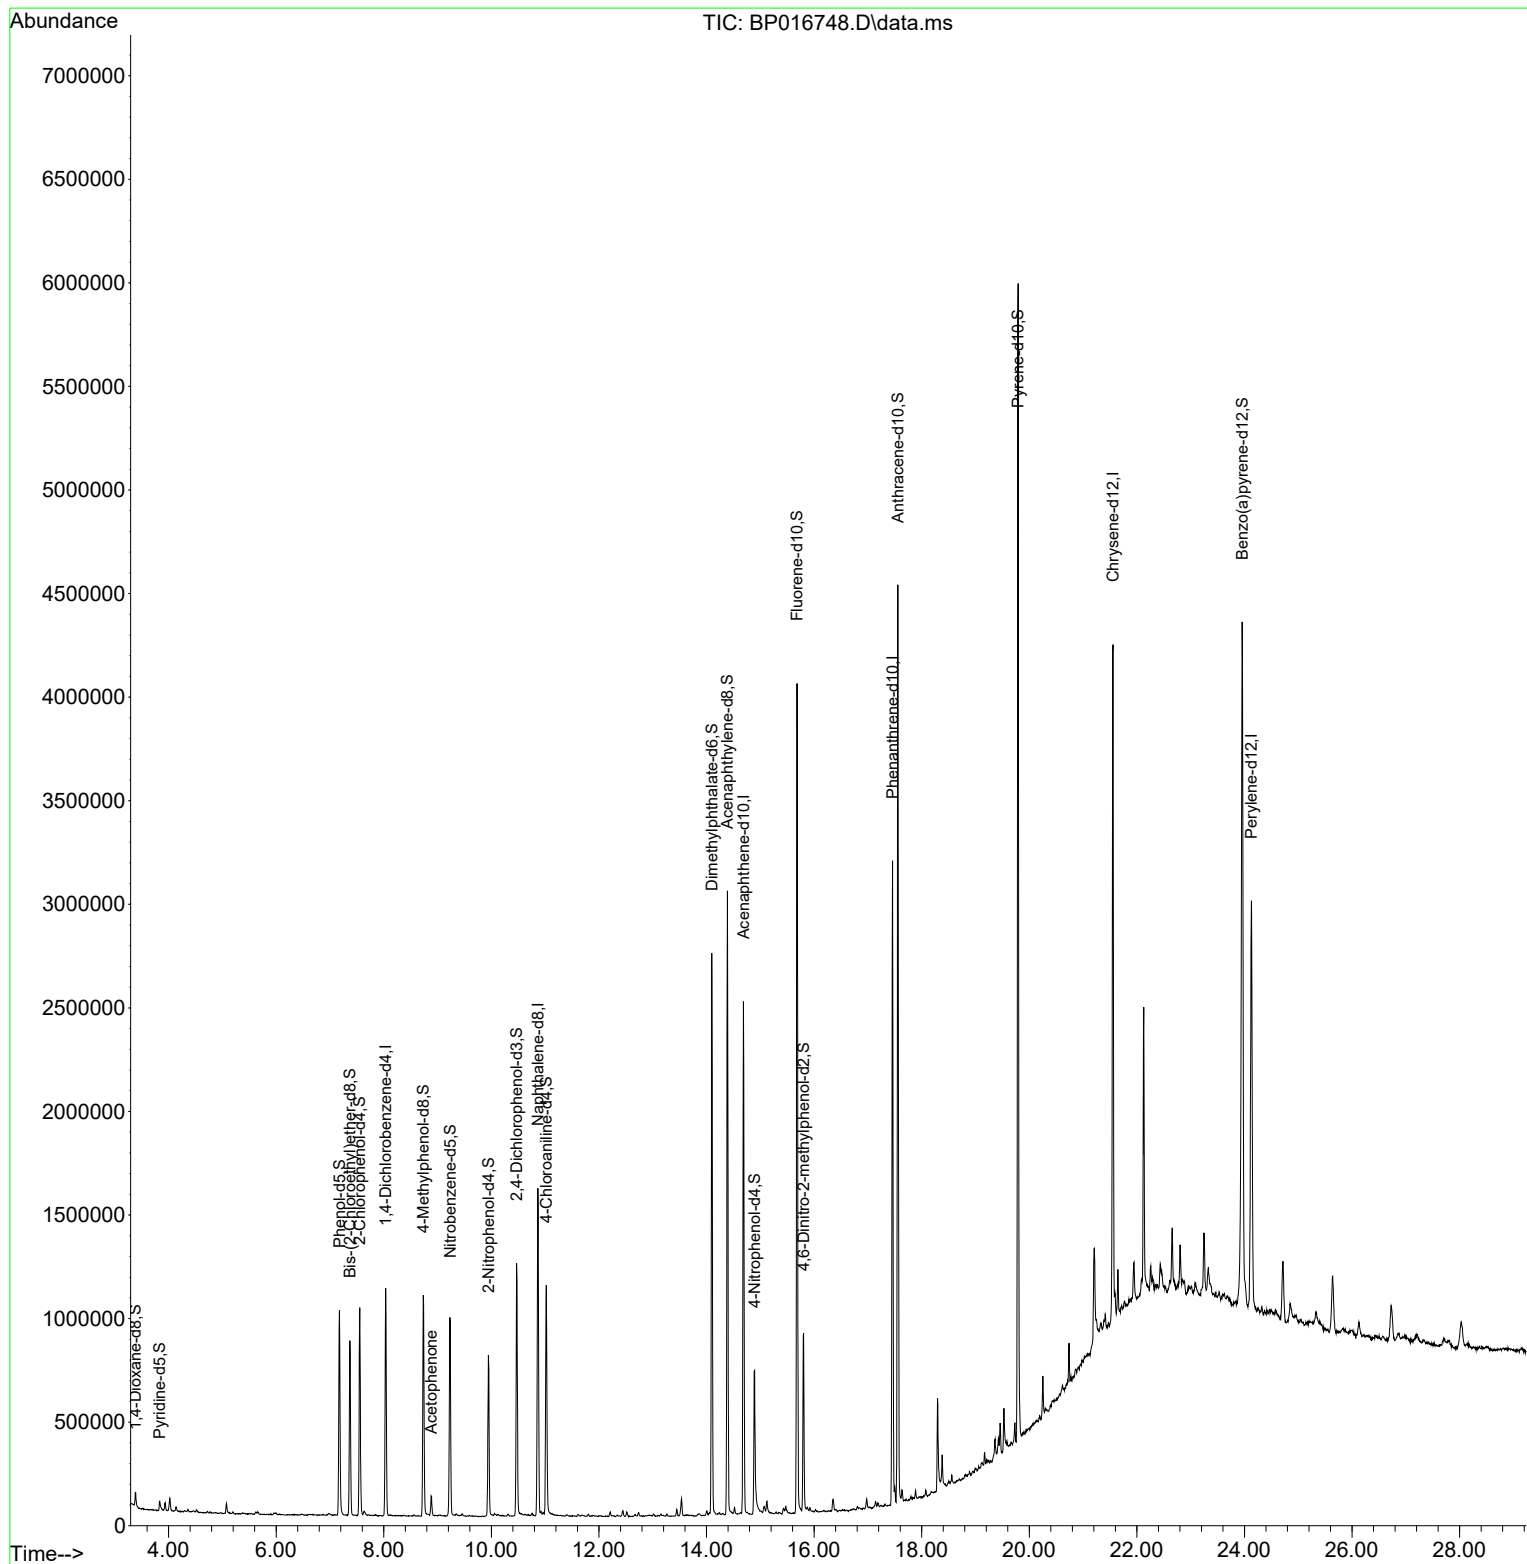

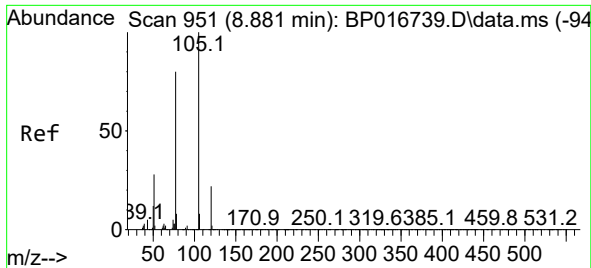

#16
Acetophenone
Concen: 1.516 ng/ul
RT: 8.881 min Scan# 91
Delta R.T. -0.006 min
Lab File: BP016748.D
Acq: 25 Aug 2023 16:01

Instrument :
BNA_P
ClientSampleId :
EZYD7

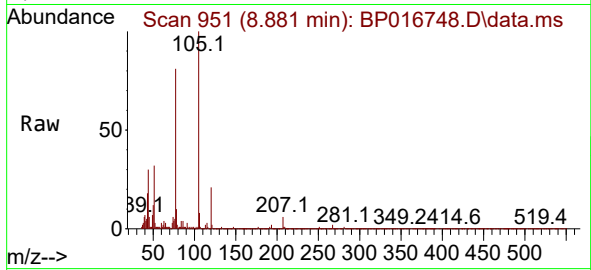

Tgt Ion:	105	Resp:	49183
Ion	Ratio	Lower	Upper
105	100		
77	80.8	64.2	96.4
51	31.5	22.2	33.4

