

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082523\
 Data File : BP016761.D
 Acq On : 26 Aug 2023 00:02
 Operator : MA/JU
 Sample : 04105-06
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHAR9

Quant Time: Aug 26 01:36:32 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 25 01:47:30 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.040	152	386672	20.000	ng/ul	0.00
20) Naphthalene-d8	10.869	136	1702554	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.693	164	1054117	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.457	188	2255726	20.000	ng/ul	0.00
79) Chrysene-d12	21.551	240	1585160	20.000	ng/ul	0.00
88) Perylene-d12	24.127	264	1386793	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	68096	7.278	ng/uL	0.00
4) Pyridine-d5	3.822	84	382392	13.375	ng/ul	0.00
7) Phenol-d5	7.175	99	298749	8.689	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.375	67	821800	37.501	ng/ul	0.00
11) 2-Chlorophenol-d4	7.558	132	802543	31.044	ng/ul	0.00
15) 4-Methylphenol-d8	8.740	113	537176	19.138	ng/ul	0.00
21) Nitrobenzene-d5	9.234	128	522492	40.588	ng/ul	0.00
24) 2-Nitrophenol-d4	9.952	143	537167	39.588	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.475	165	908822	35.927	ng/ul	0.00
31) 4-Chloroaniline-d4	11.022	131	1272764	32.808	ng/ul	0.00
46) Dimethylphthalate-d6	14.104	166	3192057	40.154	ng/ul	0.00
49) Acenaphthylene-d8	14.393	160	3739737	41.615	ng/ul	0.00
54) 4-Nitrophenol-d4	14.898	143	95914	5.837	ng/ul	0.00
60) Fluorene-d10	15.687	176	2798653	41.806	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.810	200	384893	28.652	ng/ul	0.00
73) Anthracene-d10	17.557	188	4491041	44.917	ng/ul	0.00
81) Pyrene-d10	19.792	212	4757620	54.648	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.957	264	3038665	43.743	ng/ul	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.423	88	23576	2.314 ng/uL#	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082523\
Data File : BP016761.D
Acq On : 26 Aug 2023 00:02
Operator : MA/JU
Sample : 04105-06
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAR9

Quant Time: Aug 26 01:36:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 25 01:47:30 2023
Response via : Initial Calibration

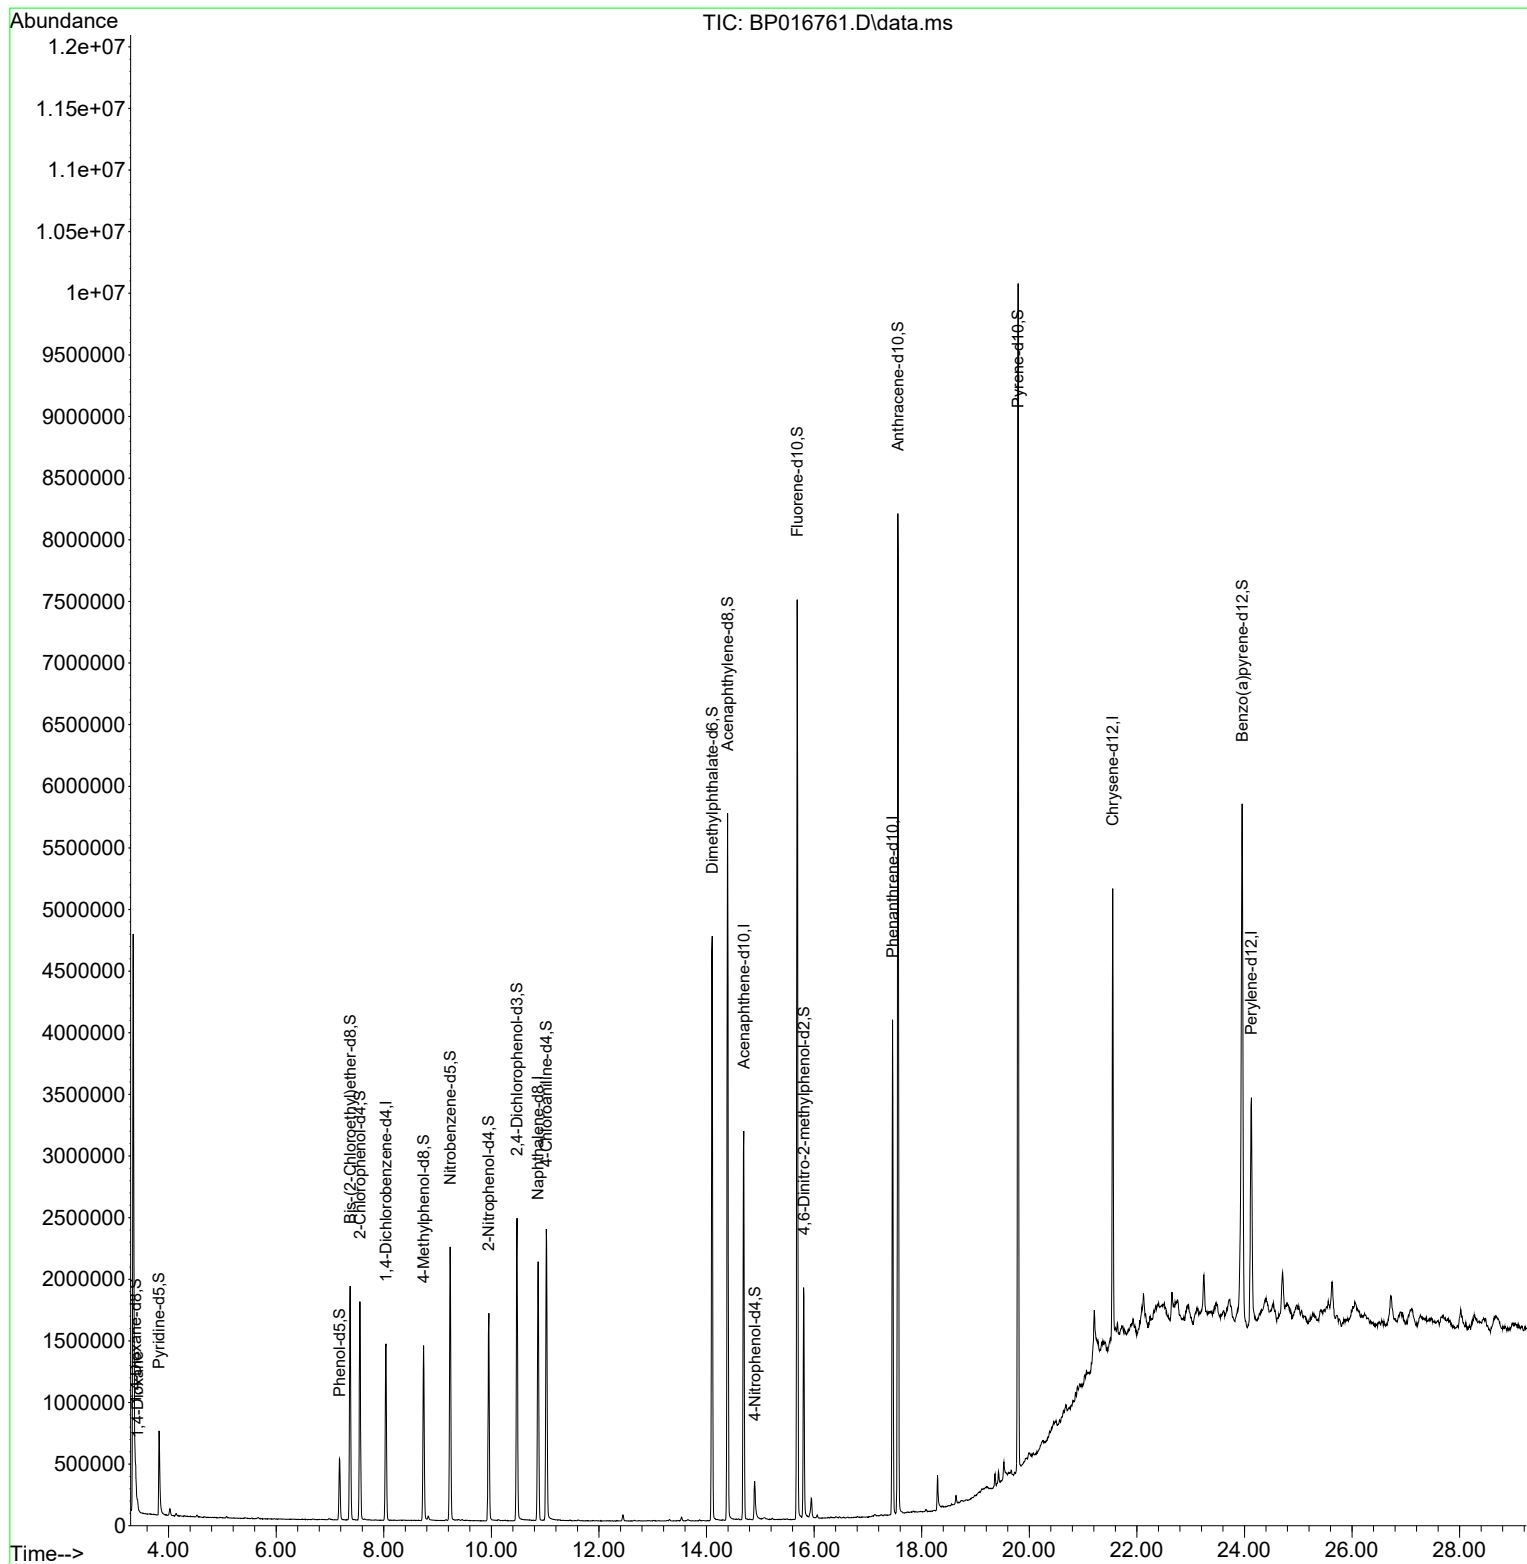

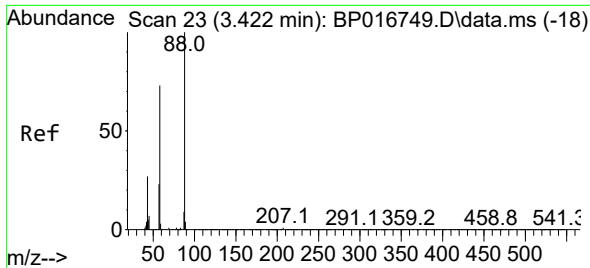

#2
 1,4-Dioxane
 Concen: 2.314 ng/uL
 RT: 3.423 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BP016761.D
 Acq: 26 Aug 2023 00:02

Instrument :
 BNA_P
 ClientSampleId :
 BHAR9

Tgt Ion: 88 Resp: 23576
 Ion Ratio Lower Upper
 88 100
 43 43.9 24.0 36.0#
 58 73.5 59.8 89.8

