

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082523\
 Data File : BP016761.D
 Acq On : 26 Aug 2023 00:02
 Operator : MA/JU
 Sample : 04105-06
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHAR9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016761.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	4	9	34	rVB	4696350	8116834	64.77%	6.659%
2	3.823	87	91	106	rBV	683090	1059559	8.46%	0.869%
3	4.023	121	125	132	rVB	55948	89888	0.72%	0.074%
4	4.140	140	145	150	rBV	22915	41197	0.33%	0.034%
5	4.528	208	211	215	rVB6	14732	20806	0.17%	0.017%
6	5.081	301	305	309	rVB	12006	15759	0.13%	0.013%
7	5.664	400	404	408	rVB5	8879	15868	0.13%	0.013%
8	6.681	571	577	584	rBV9	6417	18419	0.15%	0.015%
9	6.981	624	628	633	rBV5	7691	14711	0.12%	0.012%
10	7.175	655	661	674	rBV	494669	809724	6.46%	0.664%
11	7.375	688	695	704	rBV	1895050	2898387	23.13%	2.378%
12	7.558	718	726	738	rBV	1773892	2829145	22.58%	2.321%
13	7.640	738	740	751	rVB	7987	17717	0.14%	0.015%
14	8.040	800	808	818	rBV	1432165	2284523	18.23%	1.874%
15	8.740	918	927	937	rBV	1419480	2309780	18.43%	1.895%
16	8.828	937	942	954	rVB	33265	68074	0.54%	0.056%
17	9.234	1003	1011	1023	rBV	2219708	3569974	28.49%	2.929%
18	9.399	1034	1039	1044	rVB8	7296	14889	0.12%	0.012%
19	9.952	1123	1133	1144	rBV	1685561	2767328	22.08%	2.270%
20	10.475	1214	1222	1245	rBV	2453420	4102554	32.74%	3.366%
21	10.869	1281	1289	1303	rBV	2099091	3485862	27.82%	2.860%
22	11.022	1307	1315	1328	rBV	2363068	4071691	32.49%	3.340%
23	11.616	1411	1416	1423	rVB10	6370	12720	0.10%	0.010%
24	12.446	1549	1557	1563	rBV2	49096	82506	0.66%	0.068%
25	13.310	1700	1704	1709	rVB	12529	17377	0.14%	0.014%
26	13.534	1737	1742	1748	rBV	31280	47454	0.38%	0.039%
27	13.657	1758	1763	1772	rVB6	10433	22193	0.18%	0.018%
28	14.104	1832	1839	1852	rBV	4741614	6710955	53.55%	5.505%
29	14.393	1880	1888	1904	rBV	5738004	8590025	68.55%	7.047%
30	14.693	1932	1939	1947	rBV	3152888	4627720	36.93%	3.796%
31	14.893	1965	1973	1990	rBV	314270	653361	5.21%	0.536%
32	15.081	1997	2005	2010	rBV10	10404	26476	0.21%	0.022%
33	15.687	2101	2108	2122	rBV	7463190	10525631	84.00%	8.635%
34	15.804	2122	2128	2144	rVV	1873519	2691284	21.48%	2.208%
35	15.945	2144	2152	2162	rVB2	159864	316902	2.53%	0.260%
36	16.057	2167	2171	2178	rVB3	24951	37749	0.30%	0.031%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082523\
 Data File : BP016761.D
 Acq On : 26 Aug 2023 00:02
 Operator : MA/JU
 Sample : 04105-06
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHAR9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

37	16.404	2227	2230	2238	rVV6	9544	17816	0.14%	0.015%
38	16.469	2238	2241	2247	rVB8	9392	16096	0.13%	0.013%
39	17.128	2349	2353	2355	rBV4	12466	20164	0.16%	0.017%
40	17.457	2403	2409	2419	rBV	4014301	5530798	44.14%	4.537%
41	17.557	2420	2426	2442	rVB	8112189	11574480	92.37%	9.495%
42	18.292	2547	2551	2563	rBV	284332	502537	4.01%	0.412%
43	18.639	2606	2610	2617	rBV2	66014	97769	0.78%	0.080%
44	19.363	2730	2733	2737	rVB3	95929	112147	0.89%	0.092%
45	19.428	2741	2744	2749	rVV	94773	124661	0.99%	0.102%
46	19.528	2758	2761	2765	rBV	120757	175566	1.40%	0.144%
47	19.792	2800	2806	2812	rBV	9635063	12531176	100.00%	10.280%
48	21.551	3100	3105	3111	rBV	3650379	4788663	38.21%	3.928%
49	23.957	3508	3514	3530	rVB2	4252014	9463581	75.52%	7.763%
50	24.127	3537	3543	3555	rVB	1798741	3958811	31.59%	3.248%




Sum of corrected areas: 121899307

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082523\
Data File : BP016761.D
Acq On : 26 Aug 2023 00:02
Operator : MA/JU
Sample : 04105-06
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAR9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

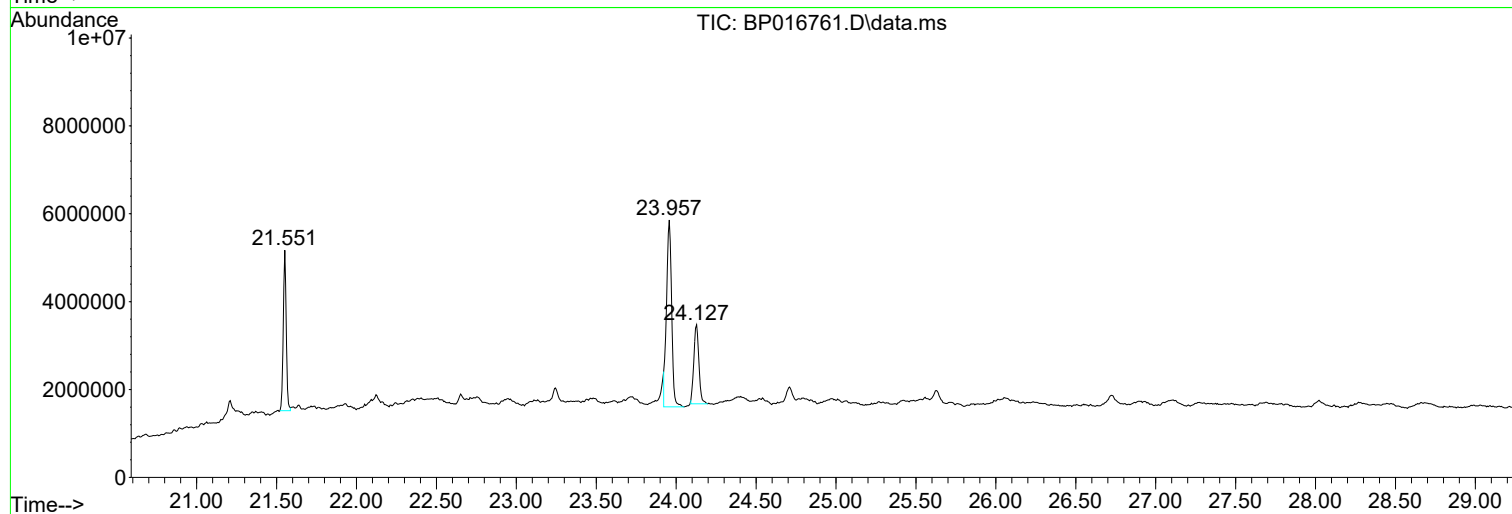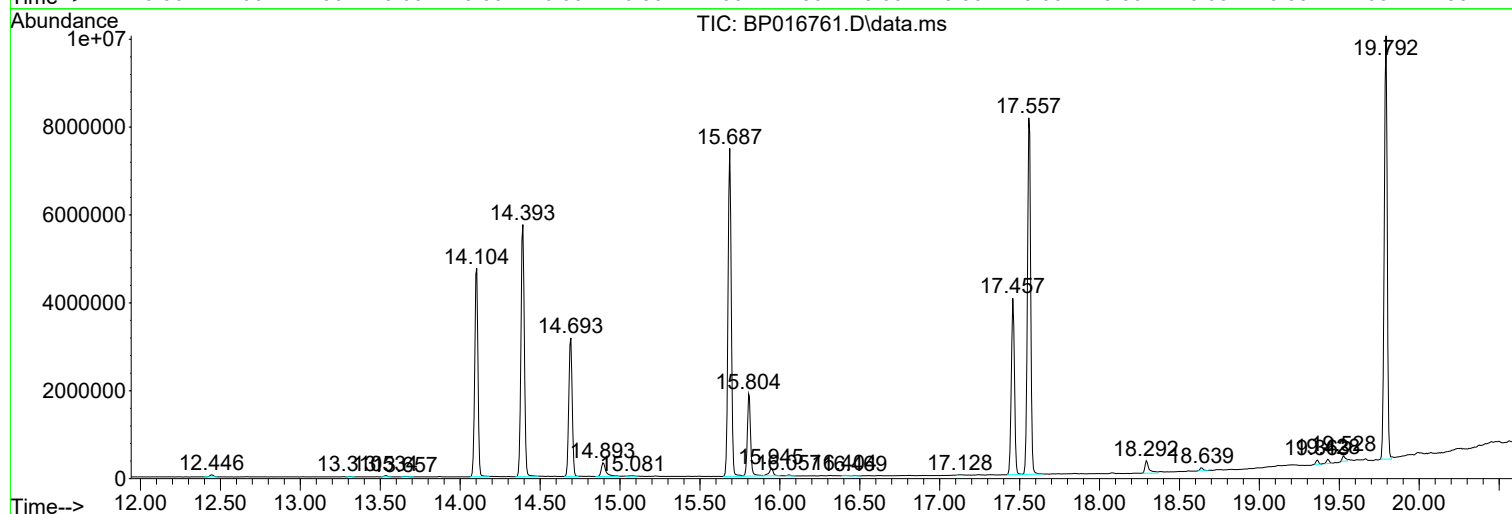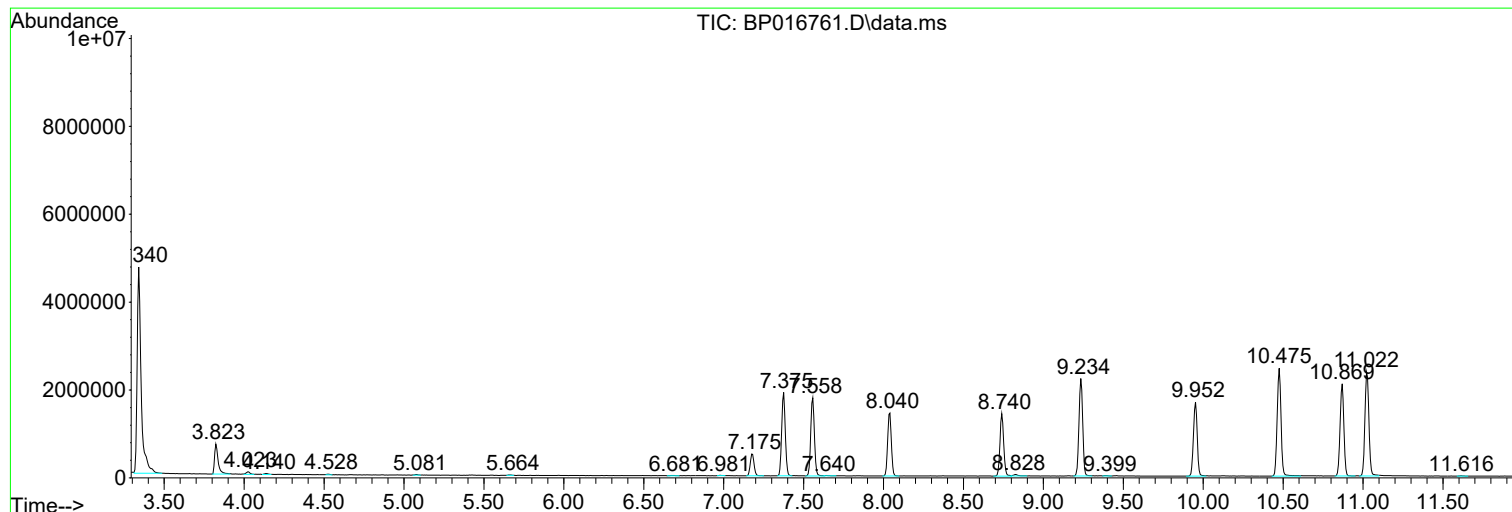

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082523\
Data File : BP016761.D
Acq On : 26 Aug 2023 00:02
Operator : MA/JU
Sample : 04105-06
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAR9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082523\
Data File : BP016761.D
Acq On : 26 Aug 2023 00:02
Operator : MA/JU
Sample : 04105-06
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAR9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------