

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082523\
 Data File : BP016764.D
 Acq On : 26 Aug 2023 01:44
 Operator : MA/JU
 Sample : 04105-09
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHAB1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016764.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	6	9	13	rVB2	19029	20931	0.20%	0.022%
2	3.381	13	16	21	rBV	87227	108356	1.05%	0.114%
3	3.823	87	91	108	rBV	443059	713587	6.92%	0.748%
4	4.023	121	125	131	rVB	46756	73519	0.71%	0.077%
5	4.134	141	144	154	rVB	22483	36339	0.35%	0.038%
6	4.528	207	211	214	rBV5	9913	15069	0.15%	0.016%
7	4.664	228	234	245	rBV	834408	1248052	12.10%	1.308%
8	5.075	301	304	309	rVB	10483	14976	0.15%	0.016%
9	5.658	399	403	414	rVB6	11307	27887	0.27%	0.029%
10	7.175	655	661	677	rVB	427515	688038	6.67%	0.721%
11	7.375	688	695	707	rVB	1419221	2258211	21.89%	2.367%
12	7.552	717	725	736	rBV	1364172	2201585	21.34%	2.307%
13	8.034	800	807	817	rBV	1305453	2067981	20.05%	2.167%
14	8.740	920	927	938	rBV	1122615	1851942	17.95%	1.941%
15	9.234	1001	1011	1023	rBV	1711092	2773663	26.89%	2.907%
16	9.458	1043	1049	1055	rVB	39895	61270	0.59%	0.064%
17	9.946	1124	1132	1143	rBV	1290767	2162127	20.96%	2.266%
18	10.475	1213	1222	1238	rBV	1866843	3219673	31.21%	3.374%
19	10.863	1281	1288	1297	rBV	1863449	3156509	30.60%	3.308%
20	11.022	1307	1315	1339	rBV	2005692	3467533	33.62%	3.634%
21	11.610	1410	1415	1421	rVB10	7157	12124	0.12%	0.013%
22	11.952	1465	1473	1481	rVB	77463	118586	1.15%	0.124%
23	12.446	1549	1557	1564	rBV	36340	64693	0.63%	0.068%
24	13.534	1735	1742	1749	rVB3	33956	56829	0.55%	0.060%
25	13.657	1758	1763	1767	rVB4	7093	12426	0.12%	0.013%
26	13.940	1805	1811	1815	rBV	28829	43980	0.43%	0.046%
27	14.098	1831	1838	1852	rBV	3789977	5195271	50.37%	5.445%
28	14.387	1880	1887	1902	rBV	4491276	6600967	63.99%	6.918%
29	14.522	1908	1910	1919	rVB10	5572	10749	0.10%	0.011%
30	14.687	1931	1938	1948	rBV	2848598	4297469	41.66%	4.504%
31	14.893	1967	1973	1990	rBV	238242	523362	5.07%	0.549%
32	15.498	2068	2076	2085	rBV9	14238	23830	0.23%	0.025%
33	15.687	2101	2108	2122	rBV	5518338	8117988	78.70%	8.508%
34	15.804	2122	2128	2137	rVV	1540437	2073024	20.10%	2.173%
35	15.922	2144	2148	2160	rVB3	31230	59242	0.57%	0.062%
36	17.239	2370	2372	2379	rVB5	9723	13734	0.13%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082523\
 Data File : BP016764.D
 Acq On : 26 Aug 2023 01:44
 Operator : MA/JU
 Sample : 04105-09
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHAB1

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

37	17.457	2402	2409	2419	rBV	3774140	5200303	50.41%	5.450%
38	17.557	2420	2426	2444	rVB2	6389667	9136515	88.58%	9.576%
39	18.292	2547	2551	2561	rBV	143004	243967	2.37%	0.256%
40	19.363	2729	2733	2737	rBV	79395	107242	1.04%	0.112%
41	19.428	2741	2744	2748	rVB	75523	100072	0.97%	0.105%
42	19.528	2757	2761	2766	rBV2	105340	166631	1.62%	0.175%
43	19.792	2800	2806	2814	rBV	7908234	10315004	100.00%	10.811%
44	21.551	3100	3105	3111	rBV	3643402	4803112	46.56%	5.034%
45	23.957	3507	3514	3531	rVB2	3516347	7916894	76.75%	8.297%
46	24.121	3536	3542	3554	rVB	1854494	4033456	39.10%	4.227%




Sum of corrected areas: 95414718

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082523\
Data File : BP016764.D
Acq On : 26 Aug 2023 01:44
Operator : MA/JU
Sample : 04105-09
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAB1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

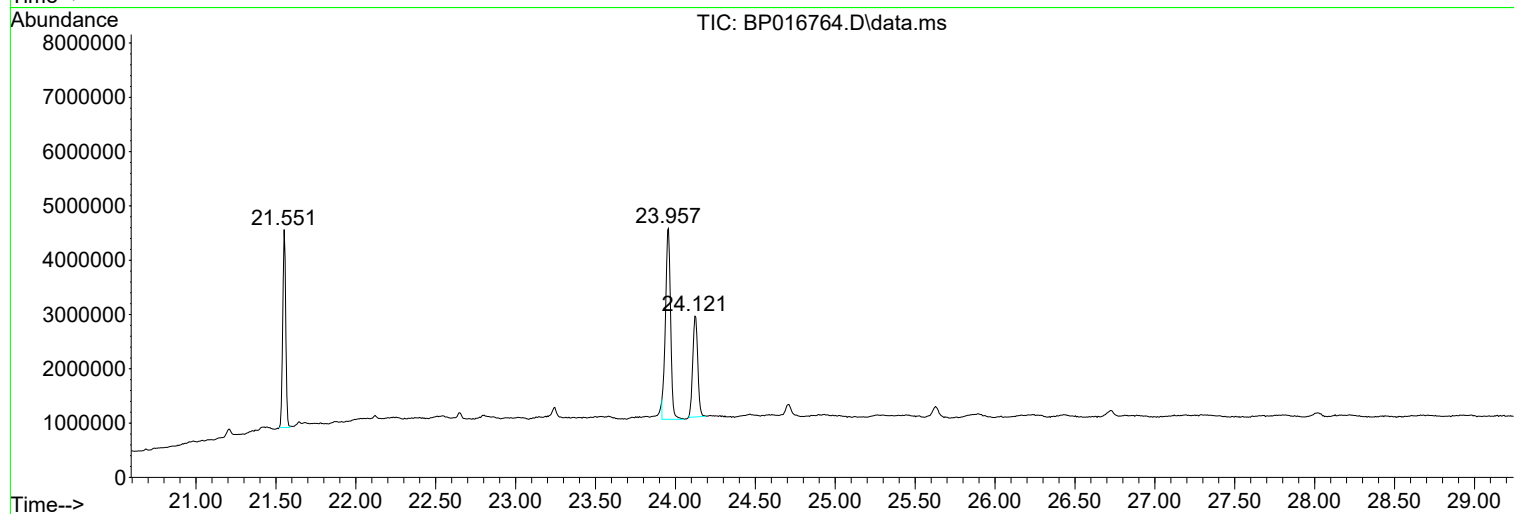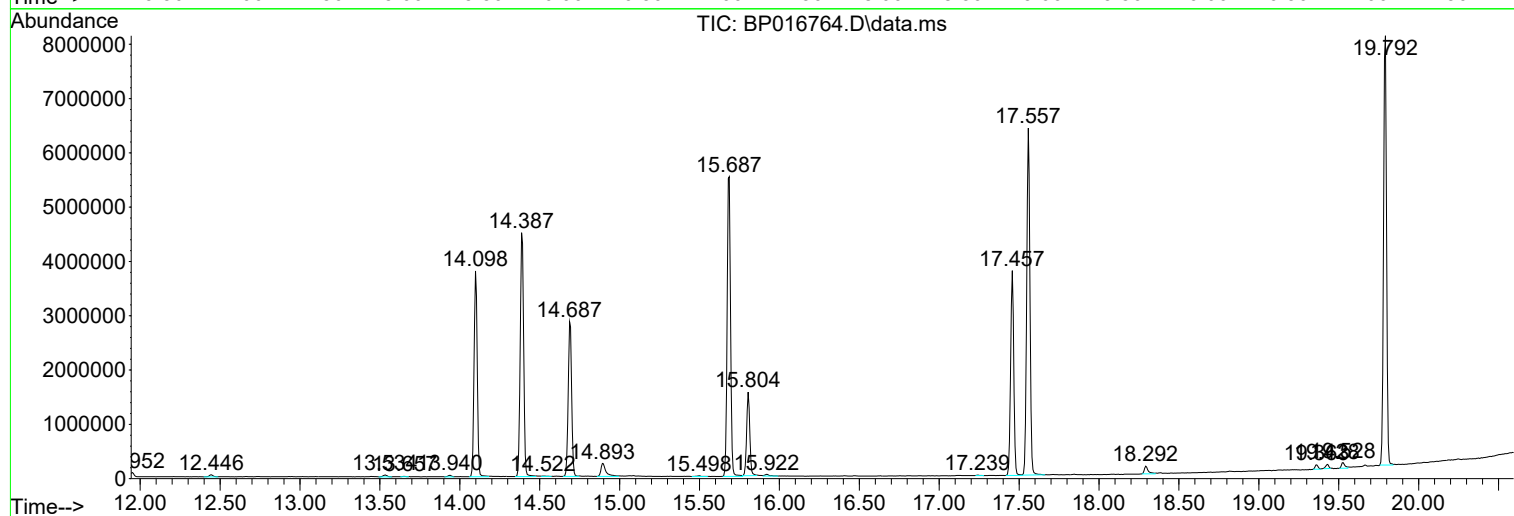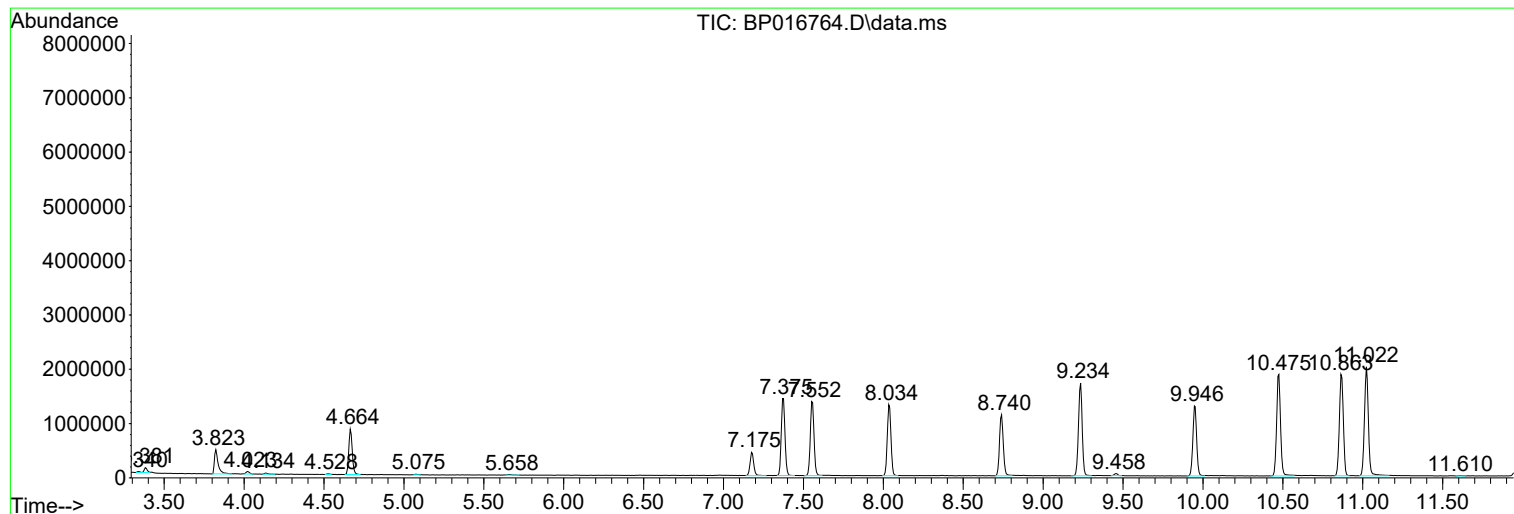

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082523\
Data File : BP016764.D
Acq On : 26 Aug 2023 01:44
Operator : MA/JU
Sample : 04105-09
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAB1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.664	12.07 ng/ul	1248050	1,4-Dichlorobenzene-d4	8.034

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	99
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	94
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	35

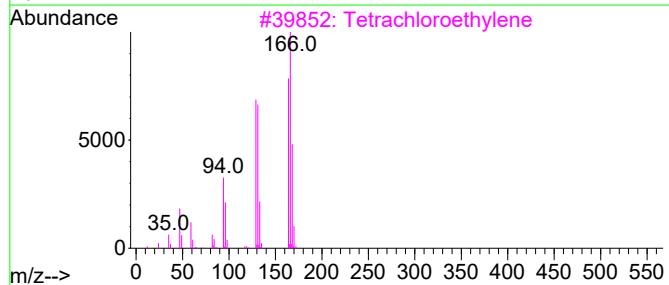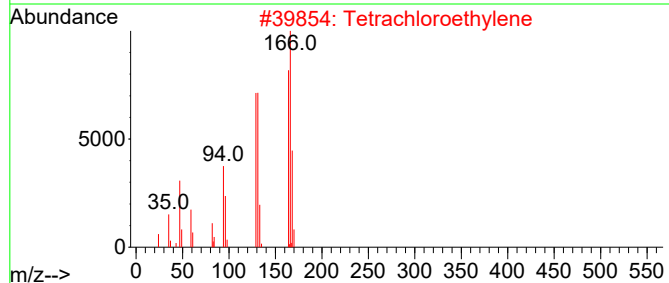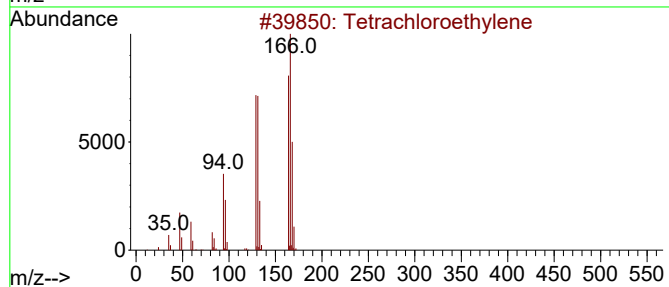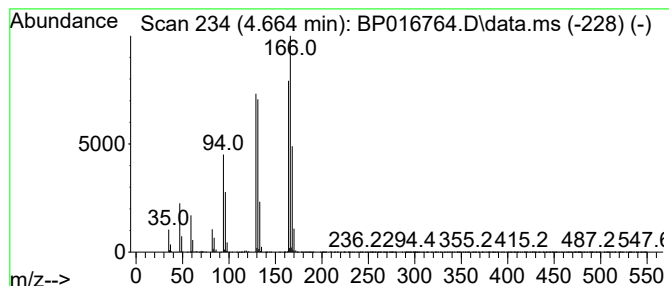

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082523\
Data File : BP016764.D
Acq On : 26 Aug 2023 01:44
Operator : MA/JU
Sample : 04105-09
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAB1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.664	12.1	ng/ul	1248050	1	8.034	2067980	20.0