

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082523\
 Data File : BP016771.D
 Acq On : 26 Aug 2023 06:16
 Operator : MA/JU
 Sample : 04105-11
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH962

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016771.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	12	16	29	rVB	107560	187842	1.58%	0.181%
2	3.822	87	91	108	rBV	600891	992389	8.34%	0.954%
3	4.022	121	125	132	rVB	49802	80930	0.68%	0.078%
4	4.134	141	144	150	rVB	18436	25965	0.22%	0.025%
5	4.522	207	210	218	rVB5	16352	26123	0.22%	0.025%
6	5.081	301	305	308	rVB2	9716	13548	0.11%	0.013%
7	5.658	397	403	407	rBV4	11381	21059	0.18%	0.020%
8	6.981	623	628	633	rBV6	7260	13256	0.11%	0.013%
9	7.175	653	661	672	rBV	464657	740377	6.22%	0.712%
10	7.369	687	694	709	rVB	1707975	2648553	22.26%	2.546%
11	7.552	718	725	739	rBV	1602761	2539601	21.35%	2.441%
12	8.034	800	807	819	rBV	1284385	2018727	16.97%	1.941%
13	8.734	919	926	939	rBV	1277187	2102544	17.67%	2.021%
14	9.234	1003	1011	1022	rBV	1977337	3270502	27.49%	3.144%
15	9.946	1124	1132	1142	rBV	1560728	2554975	21.48%	2.456%
16	10.469	1212	1221	1234	rBV	2220689	3710348	31.19%	3.567%
17	10.863	1280	1288	1299	rBV	1848007	3095018	26.02%	2.975%
18	11.022	1306	1315	1337	rBV	2015884	3505780	29.47%	3.370%
19	12.440	1551	1556	1564	rVB	45352	72956	0.61%	0.070%
20	13.440	1723	1726	1732	rBV5	5719	12437	0.10%	0.012%
21	13.528	1735	1741	1748	rVB2	22429	37966	0.32%	0.036%
22	14.098	1828	1838	1851	rBV	4500335	6037581	50.75%	5.804%
23	14.387	1880	1887	1898	rBV	5219539	7619672	64.05%	7.325%
24	14.469	1899	1901	1905	rVV5	18987	30314	0.25%	0.029%
25	14.504	1905	1907	1914	rVB8	11716	22827	0.19%	0.022%
26	14.687	1931	1938	1946	rBV	2880046	4156856	34.94%	3.996%
27	14.810	1954	1959	1963	rBV8	12190	20891	0.18%	0.020%
28	14.892	1967	1973	1995	rBV	266071	549624	4.62%	0.528%
29	15.292	2036	2041	2048	rVB9	9130	17296	0.15%	0.017%
30	15.681	2100	2107	2114	rBV	6587887	9424258	79.22%	9.060%
31	15.804	2122	2128	2142	rBV	1890267	2581249	21.70%	2.481%
32	15.922	2144	2148	2155	rVB2	33096	51130	0.43%	0.049%
33	16.463	2238	2240	2248	rVB9	9862	15642	0.13%	0.015%
34	17.122	2348	2352	2354	rBV5	9122	13474	0.11%	0.013%
35	17.239	2367	2372	2377	rBV2	10506	17872	0.15%	0.017%
36	17.451	2402	2408	2419	rBV	3483405	5007692	42.10%	4.814%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082523\
Data File : BP016771.D
Acq On : 26 Aug 2023 06:16
Operator : MA/JU
Sample : 04105-11
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH962

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Title : SVOA CALIBRATION

37	17.557	2419	2426	2441	rVV	7399883	10472588	88.04%	10.068%
38	18.292	2546	2551	2562	rBV	131000	242970	2.04%	0.234%
39	19.357	2729	2732	2737	rBV2	86736	107210	0.90%	0.103%
40	19.428	2740	2744	2748	rVB	84877	109123	0.92%	0.105%
41	19.522	2757	2760	2767	rBV3	98565	148885	1.25%	0.143%
42	19.786	2799	2805	2815	rBV	9237753	11895793	100.00%	11.436%
43	21.551	3100	3105	3111	rBV	3683442	4729390	39.76%	4.547%
44	23.951	3505	3513	3529	rVB2	4097109	9171793	77.10%	8.817%
45	24.121	3536	3542	3553	rVB	1809112	3906195	32.84%	3.755%




Sum of corrected areas: 104021221

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082523\
Data File : BP016771.D
Acq On : 26 Aug 2023 06:16
Operator : MA/JU
Sample : 04105-11
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH962

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

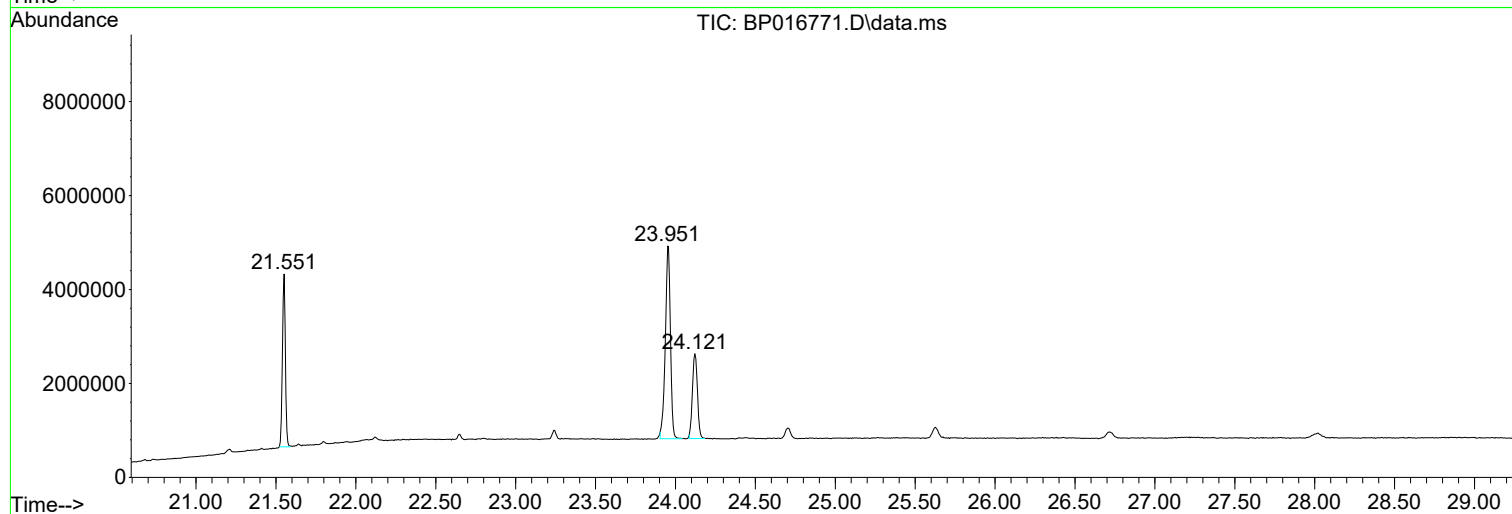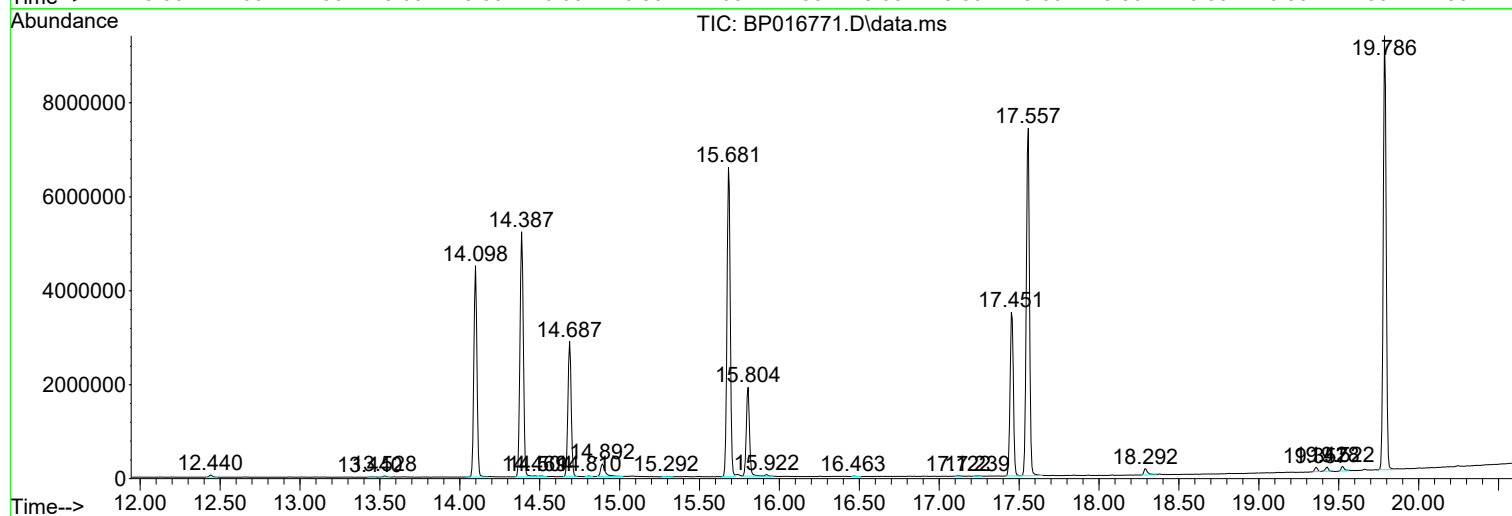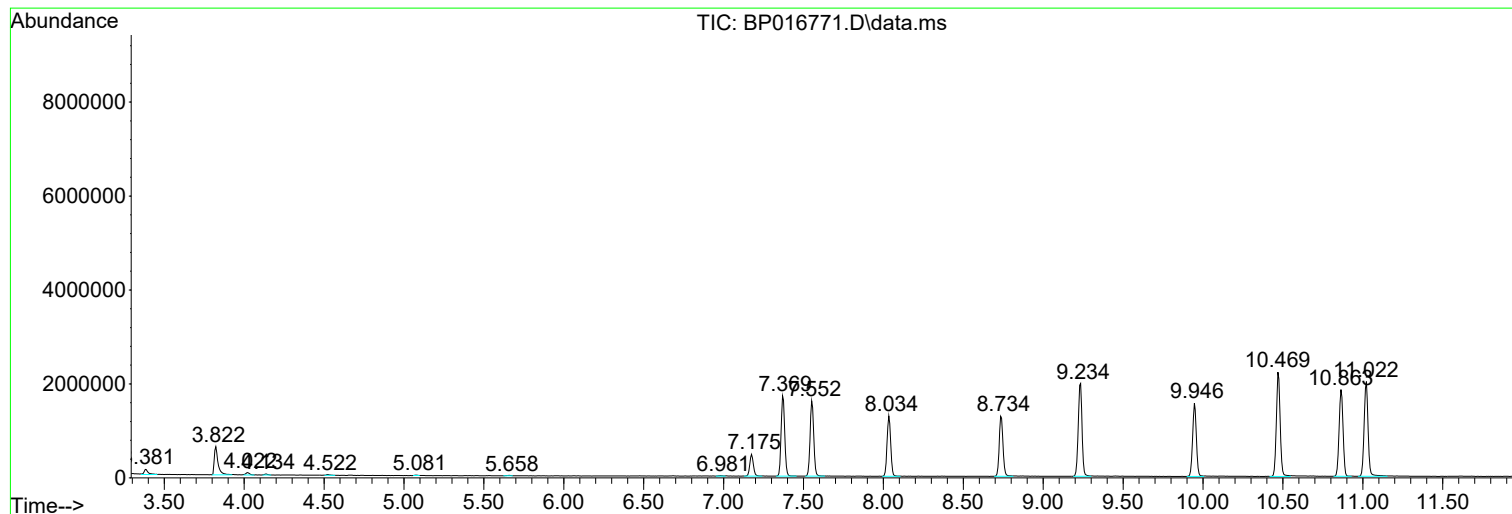

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082523\
Data File : BP016771.D
Acq On : 26 Aug 2023 06:16
Operator : MA/JU
Sample : 04105-11
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH962

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082523\
Data File : BP016771.D
Acq On : 26 Aug 2023 06:16
Operator : MA/JU
Sample : 04105-11
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH962

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc