

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082523\
 Data File : BP016773.D
 Acq On : 26 Aug 2023 07:24
 Operator : MA/JU
 Sample : 04105-13
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH926

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016773.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	12	16	27	rVB	98245	153957	1.28%	0.146%
2	3.822	87	91	106	rBV	479843	789331	6.55%	0.747%
3	4.022	121	125	132	rVB	44949	73904	0.61%	0.070%
4	4.134	141	144	148	rBV	19078	26637	0.22%	0.025%
5	4.664	229	234	242	rBV2	35014	55213	0.46%	0.052%
6	5.075	301	304	309	rVB4	10111	15410	0.13%	0.015%
7	5.658	397	403	409	rBV5	12401	25059	0.21%	0.024%
8	6.975	623	627	630	rBV3	8421	12590	0.10%	0.012%
9	7.175	655	661	674	rBV	477644	758500	6.30%	0.718%
10	7.369	687	694	705	rBV	1604308	2465689	20.47%	2.334%
11	7.552	718	725	733	rBV	1566589	2440197	20.26%	2.310%
12	8.034	799	807	818	rBV	1316787	2054103	17.06%	1.945%
13	8.363	858	863	869	rBV10	7021	16096	0.13%	0.015%
14	8.734	918	926	940	rBV	1320546	2163438	17.96%	2.048%
15	8.869	946	949	956	rVB8	8064	16199	0.13%	0.015%
16	9.110	982	990	994	rBV4	13415	23149	0.19%	0.022%
17	9.228	1001	1010	1023	rBV	1830618	3063613	25.44%	2.900%
18	9.328	1023	1027	1034	rVV7	12111	26053	0.22%	0.025%
19	9.404	1035	1040	1044	rVV2	44402	78953	0.66%	0.075%
20	9.452	1044	1048	1055	rVB	100589	151759	1.26%	0.144%
21	9.699	1082	1090	1097	rBV	18292	34868	0.29%	0.033%
22	9.887	1117	1122	1125	rBV5	15872	29461	0.24%	0.028%
23	9.946	1125	1132	1148	rVB	1499518	2407899	19.99%	2.280%
24	10.204	1170	1176	1181	rBV	18819	39243	0.33%	0.037%
25	10.246	1181	1183	1190	rVB7	10720	15774	0.13%	0.015%
26	10.469	1213	1221	1230	rBV	2196105	3593638	29.84%	3.402%
27	10.716	1259	1263	1269	rVB6	22143	36141	0.30%	0.034%
28	10.863	1277	1288	1296	rBV	1908973	3207958	26.64%	3.037%
29	11.022	1306	1315	1327	rBV	1500137	2646620	21.98%	2.506%
30	11.234	1349	1351	1360	rVB10	11424	19978	0.17%	0.019%
31	11.393	1372	1378	1382	rVB7	11113	23590	0.20%	0.022%
32	11.516	1395	1399	1403	rBV5	8349	14217	0.12%	0.013%
33	11.610	1411	1415	1418	rBV6	10845	17210	0.14%	0.016%
34	11.681	1423	1427	1433	rVB5	14576	23745	0.20%	0.022%
35	11.798	1444	1447	1454	rVB9	6745	12545	0.10%	0.012%
36	11.904	1457	1465	1467	rVV7	14811	36747	0.31%	0.035%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082523\
 Data File : BP016773.D
 Acq On : 26 Aug 2023 07:24
 Operator : MA/JU
 Sample : 04105-13
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH926

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Title : SVOA CALIBRATION

37	11.946	1467	1472	1480	rVV2	83213	169192	1.40%	0.160%
38	12.010	1480	1483	1490	rVB7	21311	37049	0.31%	0.035%
39	12.128	1495	1503	1510	rBV2	89181	163992	1.36%	0.155%
40	12.210	1514	1517	1523	rVB4	17624	28646	0.24%	0.027%
41	12.275	1524	1528	1531	rBV3	14053	21187	0.18%	0.020%
42	12.316	1531	1535	1541	rVB3	24811	44762	0.37%	0.042%
43	12.440	1551	1556	1562	rVB2	49565	84788	0.70%	0.080%
44	12.716	1599	1603	1609	rVB7	8196	18377	0.15%	0.017%
45	12.816	1618	1620	1624	rVB5	11925	15025	0.12%	0.014%
46	12.928	1636	1639	1643	rBV6	12205	16083	0.13%	0.015%
47	13.145	1672	1676	1682	rVB2	58914	93839	0.78%	0.089%
48	13.228	1684	1690	1694	rBV2	34043	64858	0.54%	0.061%
49	13.357	1708	1712	1717	rVB5	28868	40564	0.34%	0.038%
50	13.528	1737	1741	1751	rVB6	28546	58745	0.49%	0.056%
51	13.681	1759	1767	1770	rBV4	49066	100770	0.84%	0.095%
52	13.798	1783	1787	1795	rVB5	34396	65792	0.55%	0.062%
53	13.934	1807	1810	1813	rVB2	22805	27170	0.23%	0.026%
54	14.016	1820	1824	1830	rVB6	30833	53475	0.44%	0.051%
55	14.098	1831	1838	1845	rBV	4444008	5986841	49.71%	5.668%
56	14.310	1869	1874	1878	rBV3	41127	74036	0.61%	0.070%
57	14.387	1880	1887	1896	rVV	5115634	7382279	61.30%	6.989%
58	14.687	1930	1938	1945	rBV	2883244	4315256	35.83%	4.085%
59	14.892	1968	1973	1990	rVB	336916	649387	5.39%	0.615%
60	15.398	2053	2059	2063	rBV8	30476	58936	0.49%	0.056%
61	15.439	2063	2066	2071	rBV6	29096	43266	0.36%	0.041%
62	15.681	2100	2107	2113	rBV	6606510	9316585	77.36%	8.820%
63	15.739	2113	2117	2122	rVV	129358	189567	1.57%	0.179%
64	15.804	2122	2128	2138	rVV	1911720	2677807	22.23%	2.535%
65	15.969	2154	2156	2163	rVB6	32265	46417	0.39%	0.044%
66	16.781	2292	2294	2301	rVB6	49962	77990	0.65%	0.074%
67	17.251	2371	2374	2381	rVB4	35569	54125	0.45%	0.051%
68	17.451	2403	2408	2417	rBV	3476208	5108530	42.42%	4.836%
69	17.557	2419	2426	2435	rBV	7327137	10544173	87.55%	9.983%
70	18.292	2547	2551	2555	rBV	206469	294641	2.45%	0.279%
71	19.357	2729	2732	2737	rVB	93621	114596	0.95%	0.108%
72	19.522	2757	2760	2767	rBV	137366	213584	1.77%	0.202%
73	19.786	2800	2805	2815	rBV	9181270	12043592	100.00%	11.402%
74	21.551	3100	3105	3112	rBV	3824264	4994599	41.47%	4.729%
75	23.957	3505	3514	3524	rVB2	4343196	9611816	79.81%	9.100%
76	24.121	3536	3542	3552	rVB	1985264	4154618	34.50%	3.933%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082523\
Data File : BP016773.D
Acq On : 26 Aug 2023 07:24
Operator : MA/JU
Sample : 04105-13
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH926

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Title : SVOA CALIBRATION



Sum of corrected areas: 105626439

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082523\
Data File : BP016773.D
Acq On : 26 Aug 2023 07:24
Operator : MA/JU
Sample : 04105-13
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH926

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

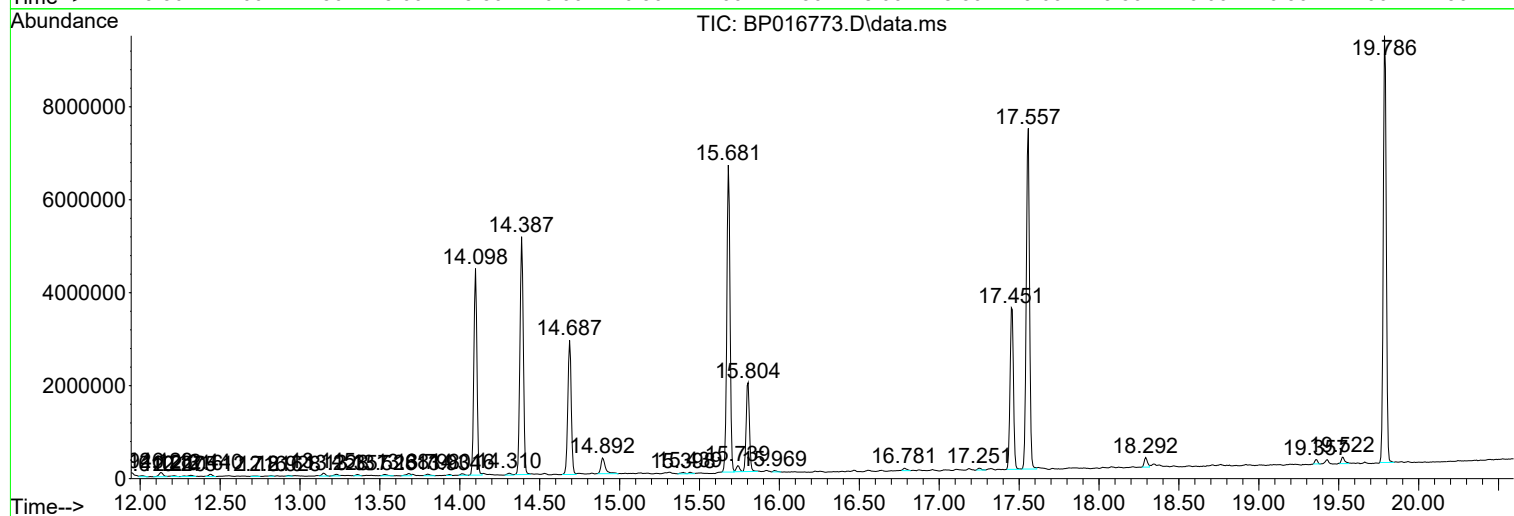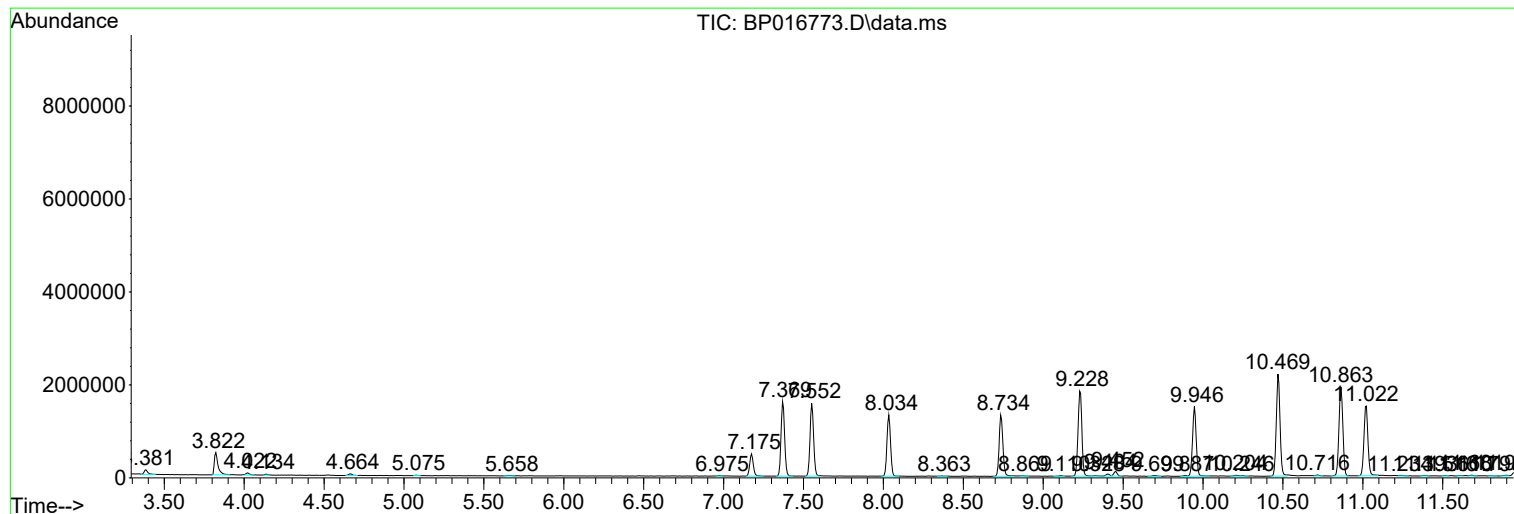

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082523\
Data File : BP016773.D
Acq On : 26 Aug 2023 07:24
Operator : MA/JU
Sample : 04105-13
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH926

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082523\
Data File : BP016773.D
Acq On : 26 Aug 2023 07:24
Operator : MA/JU
Sample : 04105-13
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH926

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------