

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082525\
 Data File : BP025569.D
 Acq On : 25 Aug 2025 17:48
 Operator : CG/JU
 Sample : Q2909-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 4065

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 08/26/2025
 Supervised By :Jagrut Upadhyay 08/26/2025

Quant Time: Aug 25 18:09:45 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 14 18:14:31 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.778	152	210562	20.000	ng	-0.02
21) Naphthalene-d8	10.548	136	656869	20.000	ng	-0.01
39) Acenaphthene-d10	14.389	164	1739904m	20.000	ng	-0.02
64) Phenanthrene-d10	17.189	188	1042522	20.000	ng	-0.01
76) Chrysene-d12	21.642	240	1046560	20.000	ng	0.00
86) Perylene-d12	25.006	264	1153898	20.000	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.402	112	1505998	118.778	ng	0.00
7) Phenol-d6	6.966	99	1827548	112.425	ng	0.00
23) Nitrobenzene-d5	8.919	82	1323801	101.946	ng	-0.02
42) 2,4,6-Tribromophenol	15.907	330	897769	38.335	ng	0.00
45) 2-Fluorobiphenyl	13.007	172	2981819	23.422	ng	-0.01
79) Terphenyl-d14	19.913	244	4362770	76.269	ng	0.00
Target Compounds						
32) Benzoic acid	10.548	122	23706968m	3135.157	ng	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082525\
Data File : BP025569.D
Acq On : 25 Aug 2025 17:48
Operator : CG/JU
Sample : Q2909-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
4065

Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 08/26/2025
Supervised By :Jagrut Upadhyay 08/26/2025


Quant Time: Aug 25 18:09:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

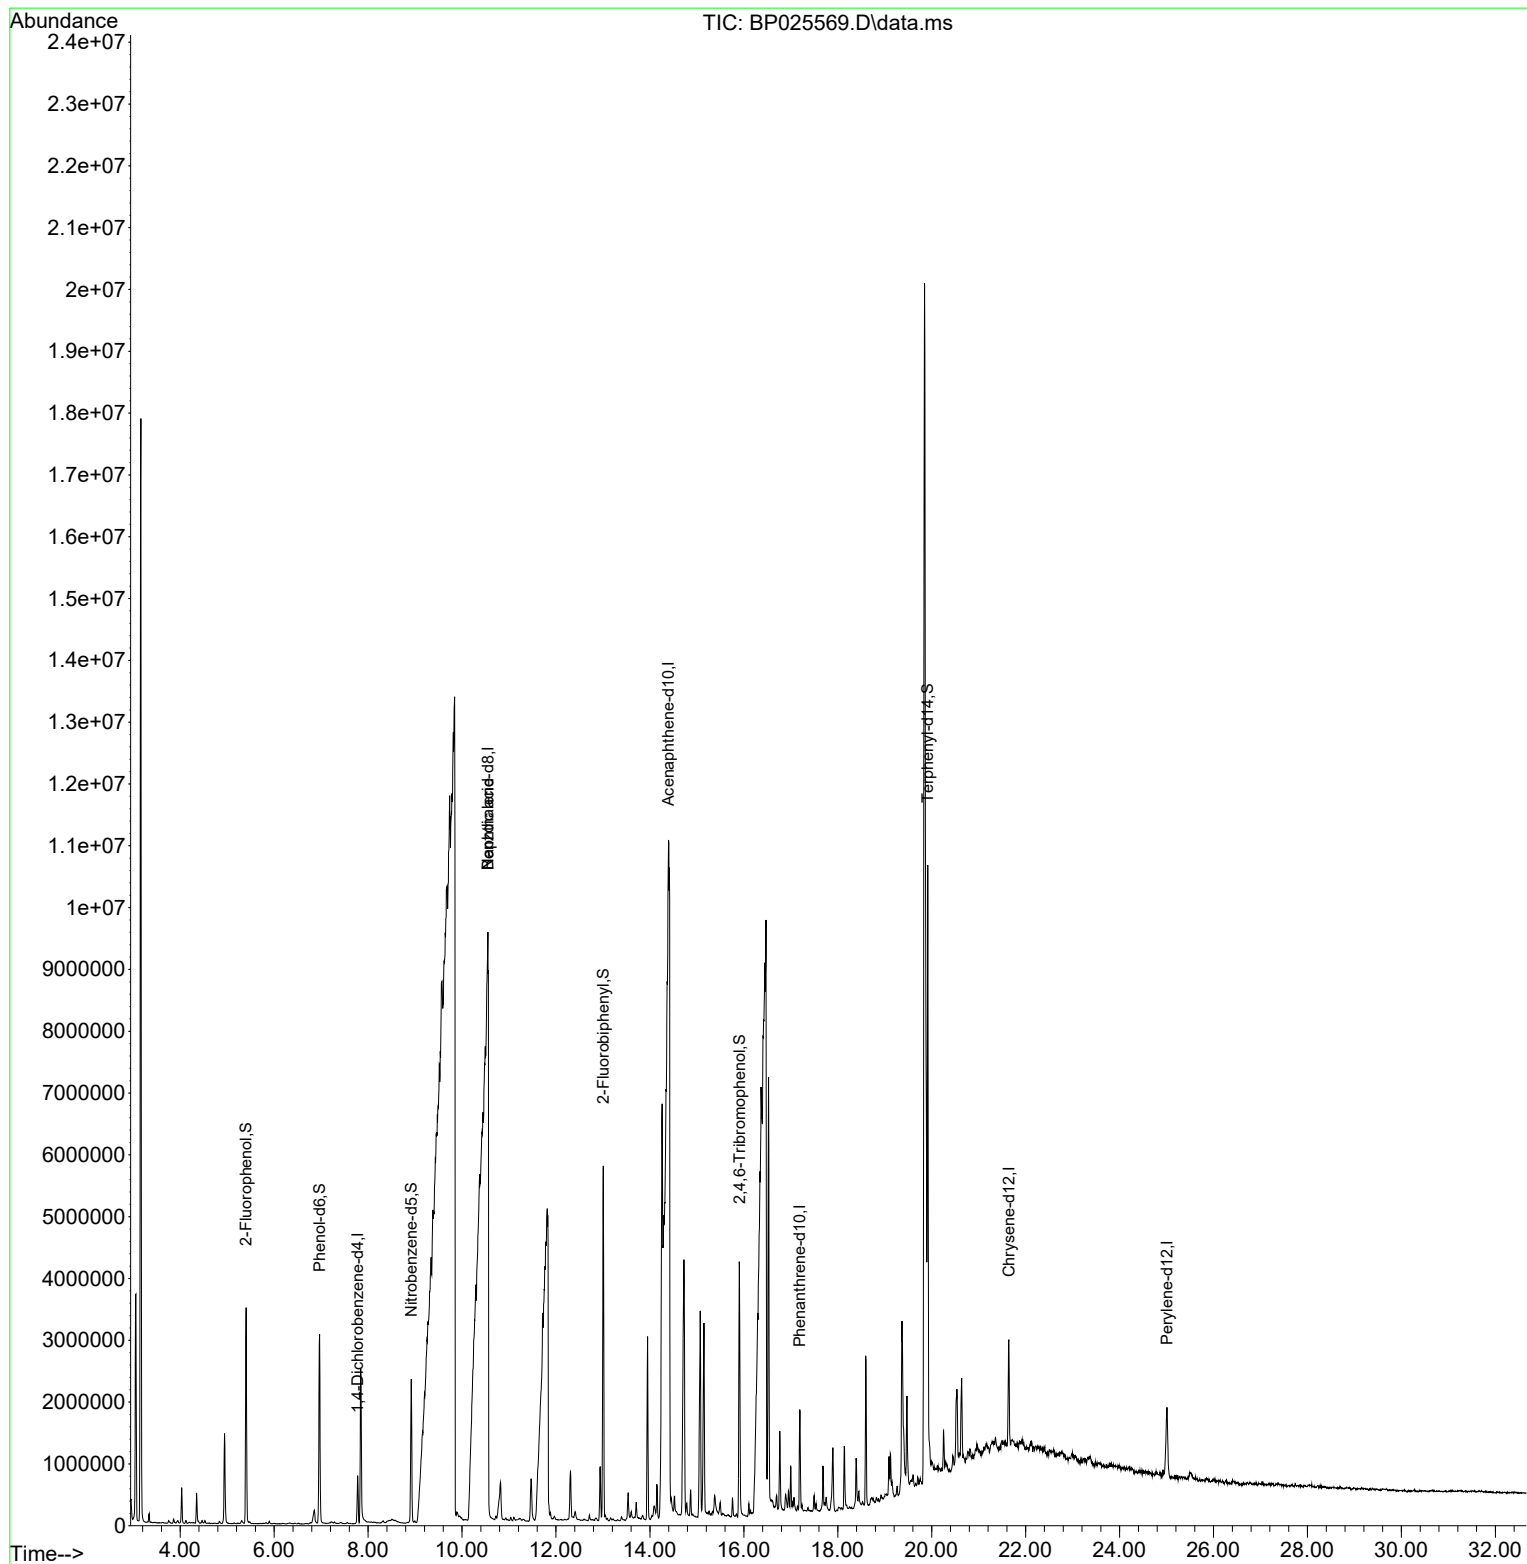



#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.778 min Scan# 81
Delta R.T. -0.018 min
Lab File: BP025569.D
Acq: 25 Aug 2025 17:48




Instrument :
BNA_P
ClientSampleId :
4065




Tgt Ion:152 Resp: 210562
Ion Ratio Lower Upper
152 100
150 154.3 125.9 188.9
115 60.7 48.5 72.7

Manual Integrations
APPROVED



Reviewed By :Rahul Chavli 08/26/2025
Supervised By :Jagrut Upadhyay 08/26/2025

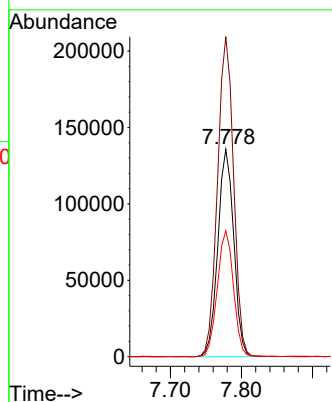


#5
2-Fluorophenol
Concen: 118.778 ng
RT: 5.402 min Scan# 419
Delta R.T. -0.006 min
Lab File: BP025569.D
Acq: 25 Aug 2025 17:48




Tgt Ion:112 Resp: 1505998
Ion Ratio Lower Upper
112 100
64 56.1 43.8 65.8
63 29.7 22.7 34.1

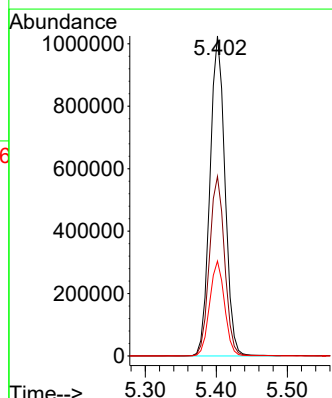



#7
Phenol-d6
Concen: 112.425 ng
RT: 6.966 min Scan# 685
Delta R.T. -0.000 min
Lab File: BP025569.D
Acq: 25 Aug 2025 17:48




Instrument :
BNA_P
ClientSampleId :
4065




Tgt Ion: 99 Resp: 1827548
Ion Ratio Lower Upper
99 100
42 17.4 13.7 20.5
71 34.1 28.2 42.4

Manual Integrations
APPROVED



Reviewed By :Rahul Chavli 08/26/2025
Supervised By :Jagrut Upadhyay 08/26/2025

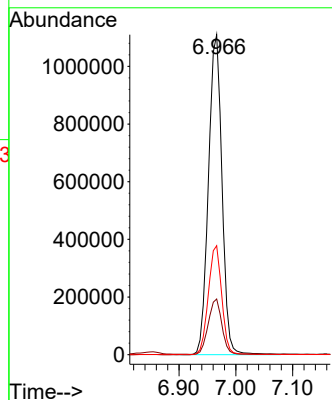


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.548 min Scan# 1294
Delta R.T. -0.012 min
Lab File: BP025569.D
Acq: 25 Aug 2025 17:48

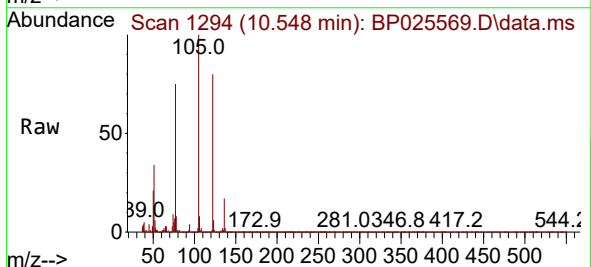


Tgt Ion:136 Resp: 656869
Ion Ratio Lower Upper
136 100
137 10.6 9.2 13.8
54 8.2 6.0 9.0
68 5.7 4.3 6.5

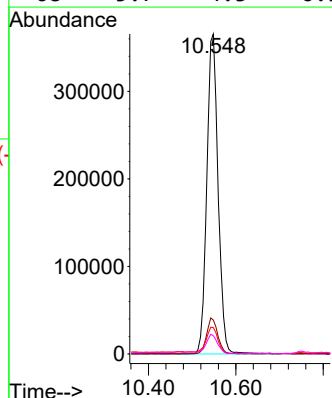



#23
Nitrobenzene-d5
Concen: 101.946 ng
RT: 8.919 min Scan# 1017
Delta R.T. -0.018 min
Lab File: BP025569.D
Acq: 25 Aug 2025 17:48




Instrument :
BNA_P
ClientSampleId :
4065



Tgt Ion: 82 Resp: 132380
Ion Ratio Lower Upper
82 100
128 46.5 37.7 56.5
54 51.0 39.8 59.6




Manual Integrations
APPROVED


Reviewed By :Rahul Chavli 08/26/2025
Supervised By :Jagrut Upadhyay 08/26/2025

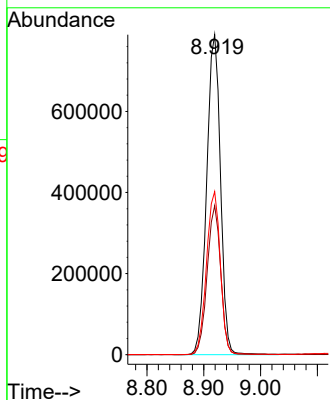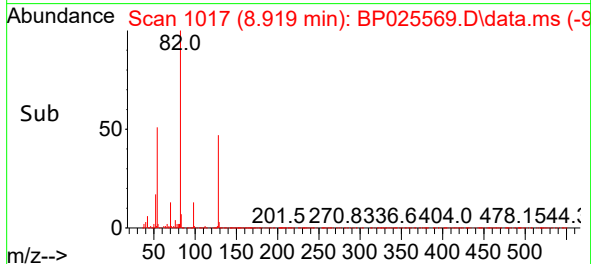

#32
Benzoic acid
Concen: 3135.157 ng m
RT: 10.548 min Scan# 1294
Delta R.T. 0.676 min
Lab File: BP025569.D
Acq: 25 Aug 2025 17:48


Tgt Ion:122 Resp:23706968
Ion Ratio Lower Upper
122 100
105 125.7 100.6 140.6
77 93.7 71.5 111.5

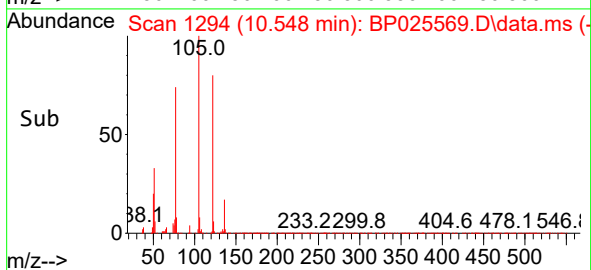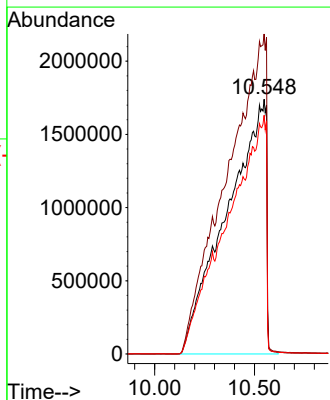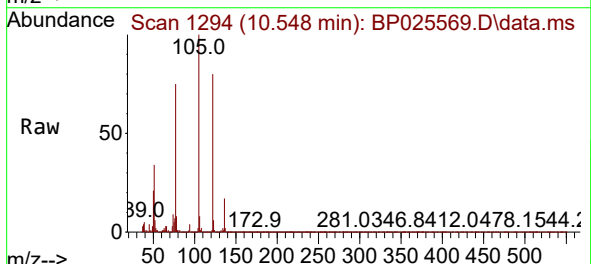



#39
Acenaphthene-d10
Concen: 20.000 ng m
RT: 14.389 min Scan# 1947
Delta R.T. -0.018 min
Lab File: BP025569.D
Acq: 25 Aug 2025 17:48




Instrument :
BNA_P
ClientSampleId :
4065



Tgt Ion:164 Resp: 1739904
Ion Ratio Lower Upper
164 100
162 51.3 81.0 121.6
160 20.9 35.4 53.2




Manual Integrations
APPROVED


Reviewed By :Rahul Chavli 08/26/2025
Supervised By :Jagrut Upadhyay 08/26/2025

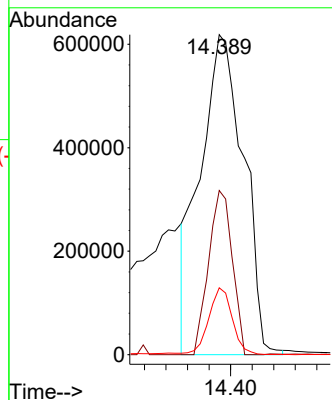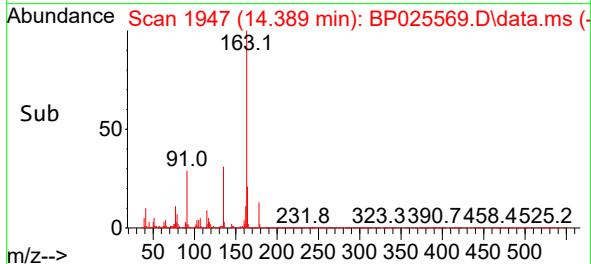

#42
2,4,6-Tribromophenol
Concen: 38.335 ng
RT: 15.907 min Scan# 2205
Delta R.T. -0.006 min
Lab File: BP025569.D
Acq: 25 Aug 2025 17:48


Tgt Ion:330 Resp: 897769
Ion Ratio Lower Upper
330 100
332 97.6 77.3 115.9
141 32.8 26.6 39.8

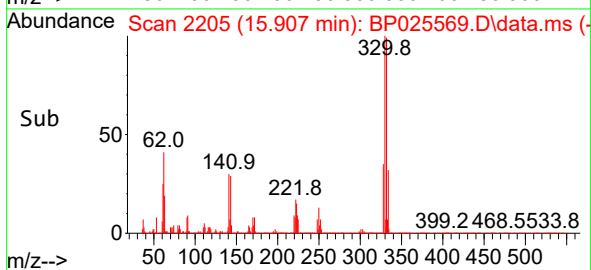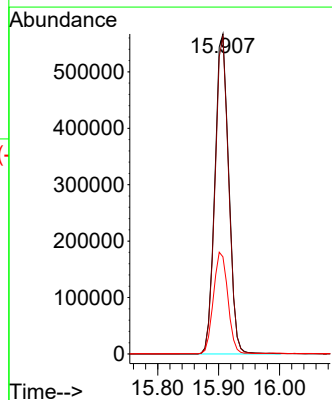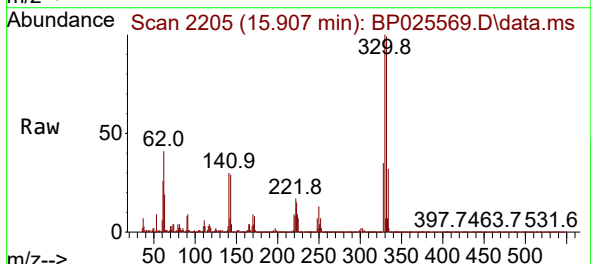



#45
2-Fluorobiphenyl
Concen: 23.422 ng
RT: 13.007 min Scan# 11
Delta R.T. -0.012 min
Lab File: BP025569.D
Acq: 25 Aug 2025 17:48




Instrument :
BNA_P
ClientSampleId :
4065




Tgt Ion:172 Resp: 2981819
Ion Ratio Lower Upper
172 100
171 35.3 28.1 42.1
170 23.4 18.6 28.0

Manual Integrations
APPROVED



Reviewed By :Rahul Chavli 08/26/2025
Supervised By :Jagrut Upadhyay 08/26/2025

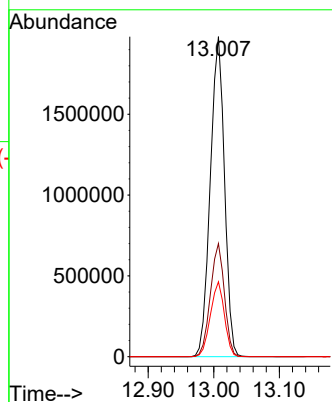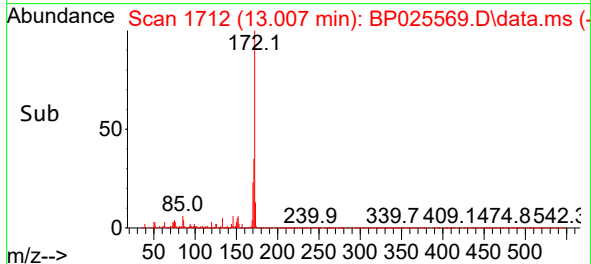


#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.189 min Scan# 2423
Delta R.T. -0.012 min
Lab File: BP025569.D
Acq: 25 Aug 2025 17:48

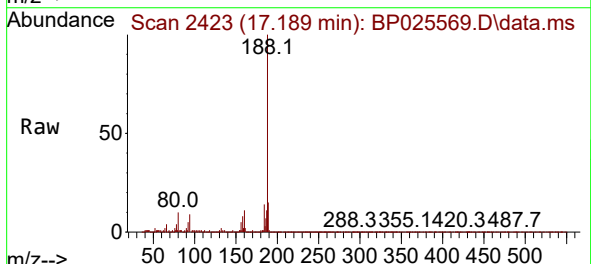

Tgt Ion:188 Resp: 1042522
Ion Ratio Lower Upper
188 100
94 9.3 6.6 10.0
80 10.1 6.7 10.1

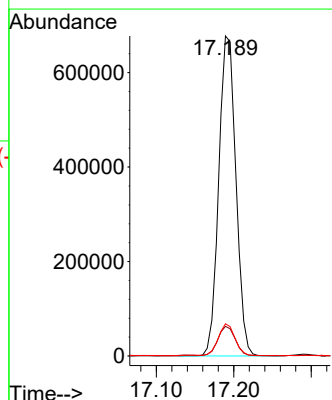



#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.642 min Scan# 31

Delta R.T. -0.006 min

Lab File: BP025569.D

Acq: 25 Aug 2025 17:48

Instrument :

BNA_P

ClientSampleId :

4065

Tgt Ion:240 Resp: 1046560

Ion Ratio Lower Upper

240 100

120 10.0 8.9 13.3





236 25.4 19.8 29.8

Manual Integrations

APPROVED

Reviewed By :Rahul Chavli 08/26/2025

Supervised By :Jagrut Upadhyay 08/26/2025

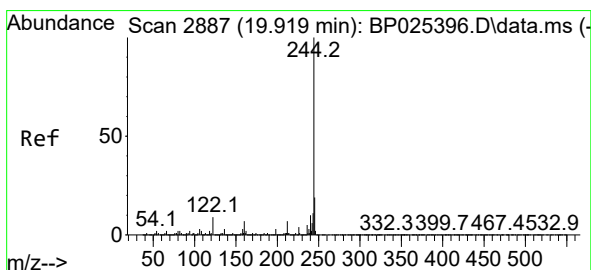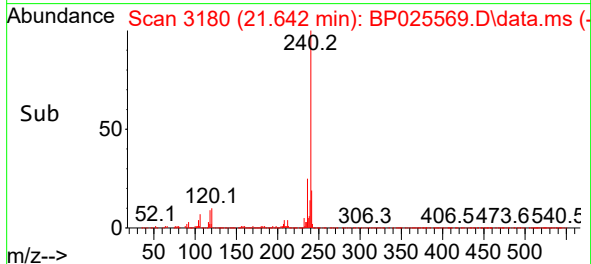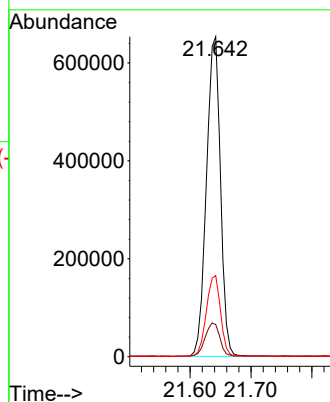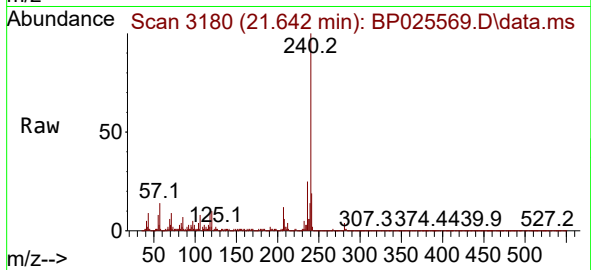

#79

Terphenyl-d14

Concen: 76.269 ng

RT: 19.913 min Scan# 2886

Delta R.T. -0.006 min

Lab File: BP025569.D

Acq: 25 Aug 2025 17:48




Tgt Ion:244 Resp: 4362770


Ion Ratio Lower Upper

244 100

212 7.6 5.8 8.6


122 10.2 7.4 11.2

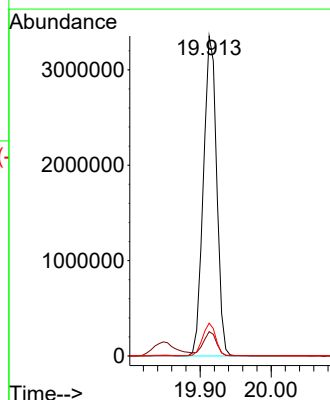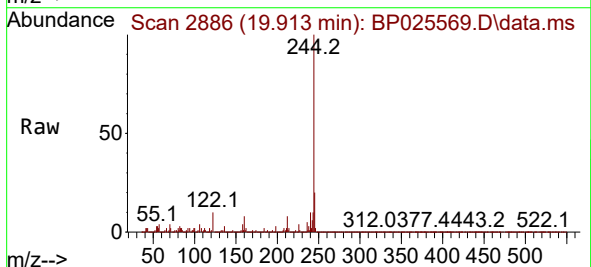



#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 25.006 min Scan# 31
 Delta R.T. -0.024 min
 Lab File: BP025569.D
 Acq: 25 Aug 2025 17:48

Instrument :
 BNA_P
 ClientSampleId :
 4065



Tgt Ion:264 Resp: 1153898
 Ion Ratio Lower Upper
 264 100
 260 23.3 19.3 28.9
 265 21.5 17.4 26.0

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 08/26/2025
 Supervised By :Jagrut Upadhyay 08/26/2025

