
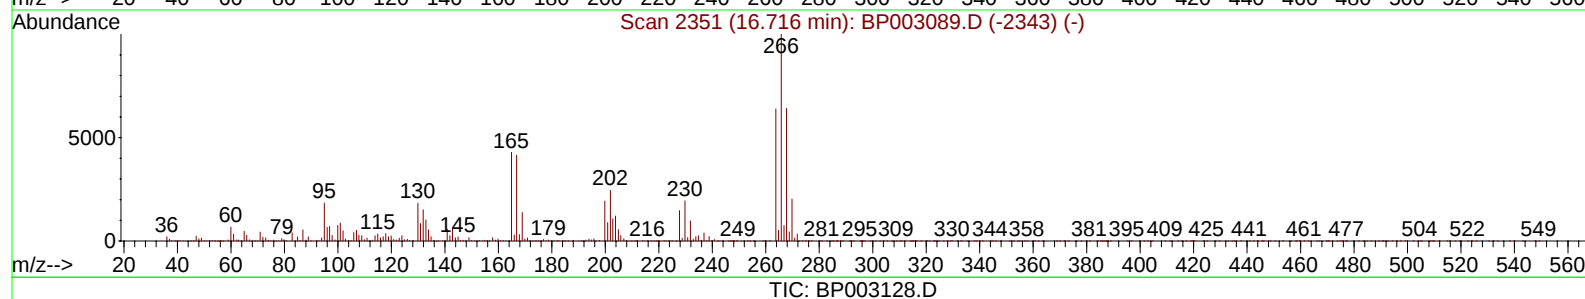
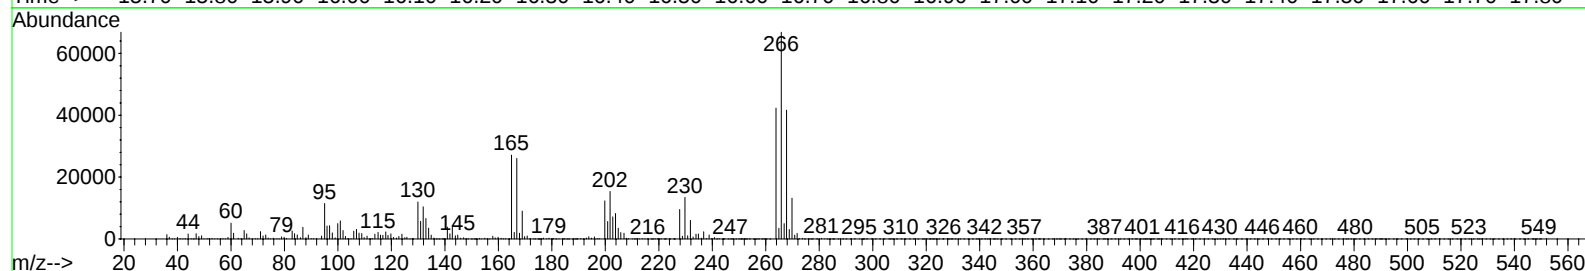


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP082720\
Data File : BP003128.D
Acq On : 27 Aug 2020 12:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 27 18:16:16 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP082420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 24 15:32:08 2020
Response via : Initial Calibration

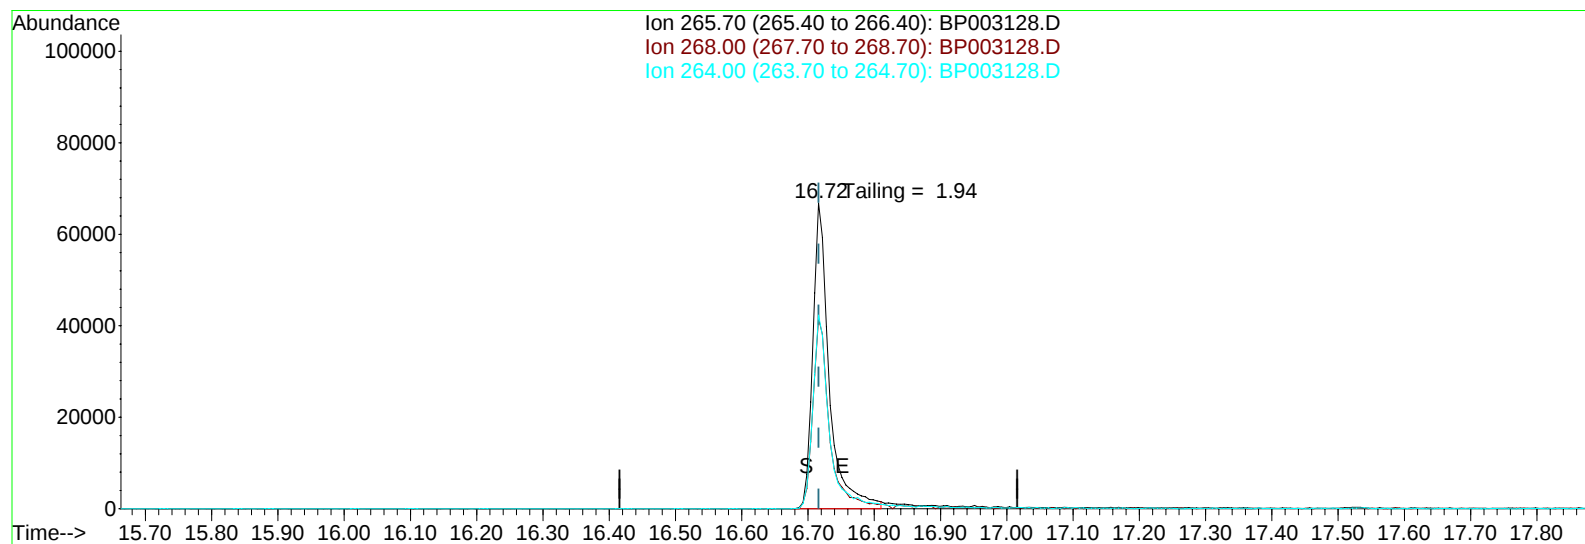

(70) Pentachlorophenol (C)




16.716min (+0.000) 55647.14ng

response 119231

Ion	Exp%	Act%
265.70	100	100
268.00	64.10	62.27
264.00	63.80	63.34
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP082720\
 Data File : BP003128.D
 Acq On : 27 Aug 2020 12:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 27 18:16:16 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP082420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 24 15:32:08 2020
 Response via : Initial Calibration

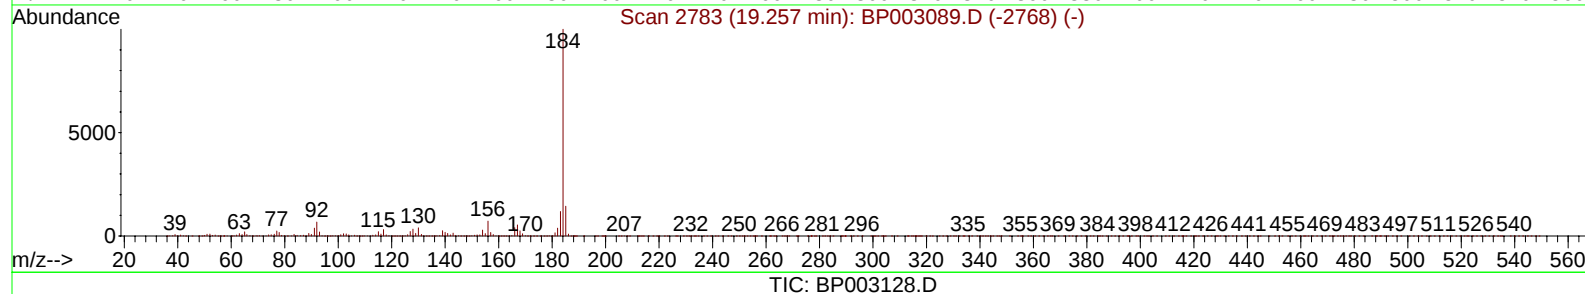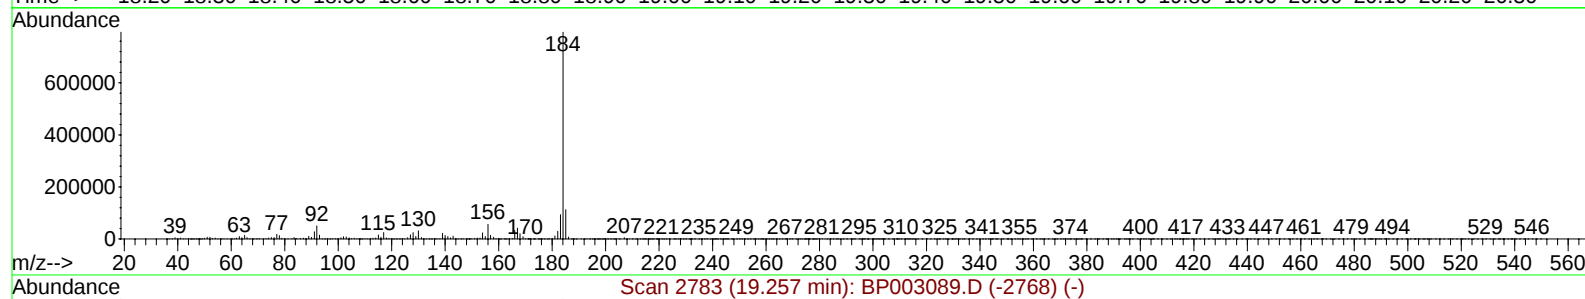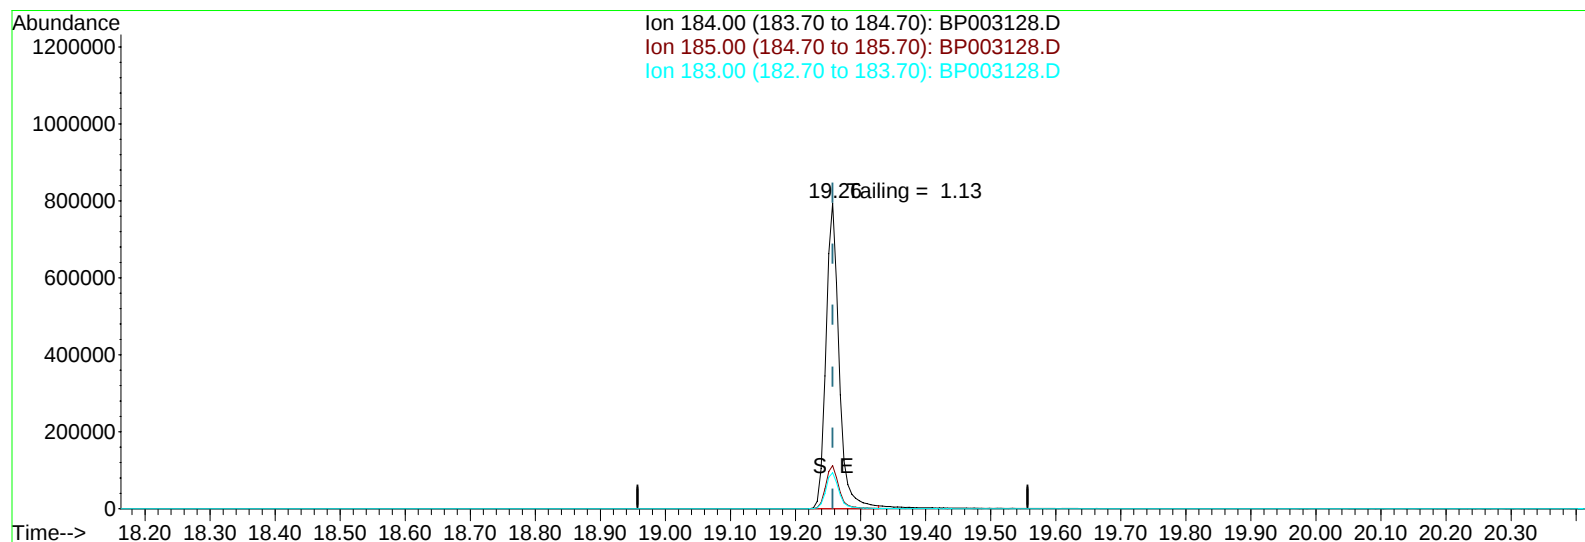

(77) Benzidine

19.257min (+0.000) 33065.48ng

response 1128275

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	14.16
183.00	11.80	11.76
0.00	0.00	0.00