


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP082720\  
 Data File : BP003128.D  
 Acq On : 27 Aug 2020 12:21  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\8270-BP082420.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon Aug 24 15:32:08 2020

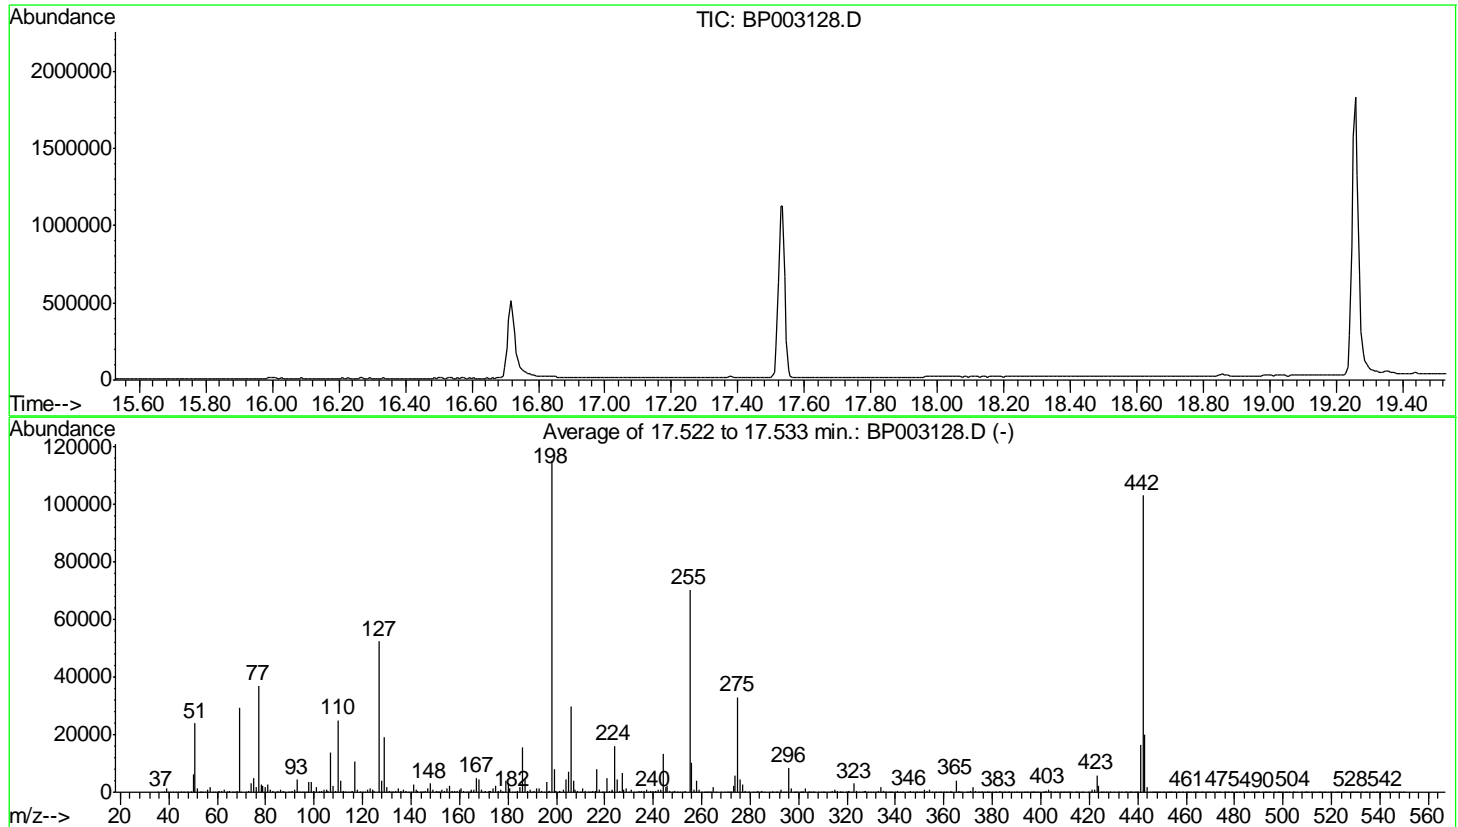

AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.8	23976	PASS
68	69	0.00	2	1.7	513	PASS
69	198	0.00	100	25.6	29442	PASS
70	69	0.00	2	0.5	151	PASS
127	198	10	80	45.4	52250	PASS
197	198	0.00	2	0.4	508	PASS
198	198	100	100	100.0	115121	PASS
199	198	5	9	6.8	7813	PASS
275	198	10	60	28.8	33114	PASS
365	198	1	100	3.5	4009	PASS
441	198	0.01	100	14.1	16249	PASS
442	198	50	100	89.5	103042	PASS
443	442	15	24	19.4	20027	PASS