

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP082820\  
Data File : BP003149.D  
Acq On : 28 Aug 2020 14:14  
Operator : CG/JU  
Sample : PB131271BL  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
PB131271BL

Integration Parameters: rteint.p  
Integrator: RTE  
Smoothing : ON Filtering: 5  
Sampling : 1 Min Area: 3 % of largest Peak  
Start Thrs: 0.2 Max Peaks: 100  
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\8270-BP082420.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.275       | 399           | 406         | 419          | rBV      | 3073949        | 4613504       | 30.01%          | 7.488%        |
| 2         | 6.846       | 666           | 673         | 686          | rBV      | 2741679        | 4468292       | 29.07%          | 7.252%        |
| 3         | 7.663       | 804           | 812         | 826          | rBV      | 806169         | 1276584       | 8.31%           | 2.072%        |
| 4         | 8.810       | 999           | 1007        | 1026         | rBV      | 1856838        | 3224082       | 20.98%          | 5.233%        |
| 5         | 10.440      | 1275          | 1284        | 1300         | rBV      | 1024908        | 1807519       | 11.76%          | 2.934%        |
| 6         | 12.922      | 1698          | 1706        | 1728         | rBV      | 5842068        | 9031380       | 58.76%          | 14.658%       |
| 7         | 14.304      | 1931          | 1941        | 1962         | rBV      | 1620087        | 2575157       | 16.75%          | 4.180%        |
| 8         | 15.798      | 2186          | 2195        | 2227         | rBV      | 4220536        | 6842093       | 44.51%          | 11.105%       |
| 9         | 17.057      | 2402          | 2409        | 2423         | rBV      | 2124383        | 3262670       | 21.23%          | 5.296%        |
| 10        | 19.633      | 2841          | 2847        | 2861         | rBV      | 11727664       | 15370983      | 100.00%         | 24.948%       |
| 11        | 20.939      | 3065          | 3069        | 3077         | rBV      | 148755         | 220449        | 1.43%           | 0.358%        |
| 12        | 21.151      | 3099          | 3105        | 3118         | rBV      | 3245212        | 4328513       | 28.16%          | 7.025%        |
| 13        | 23.386      | 3477          | 3485        | 3498         | rBV      | 2343883        | 4590839       | 29.87%          | 7.451%        |




Sum of corrected areas: 61612065

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP082820\  
Data File : BP003149.D  
Acq On : 28 Aug 2020 14:14  
Operator : CG/JU  
Sample : PB131271BL  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
PB131271BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP082420.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

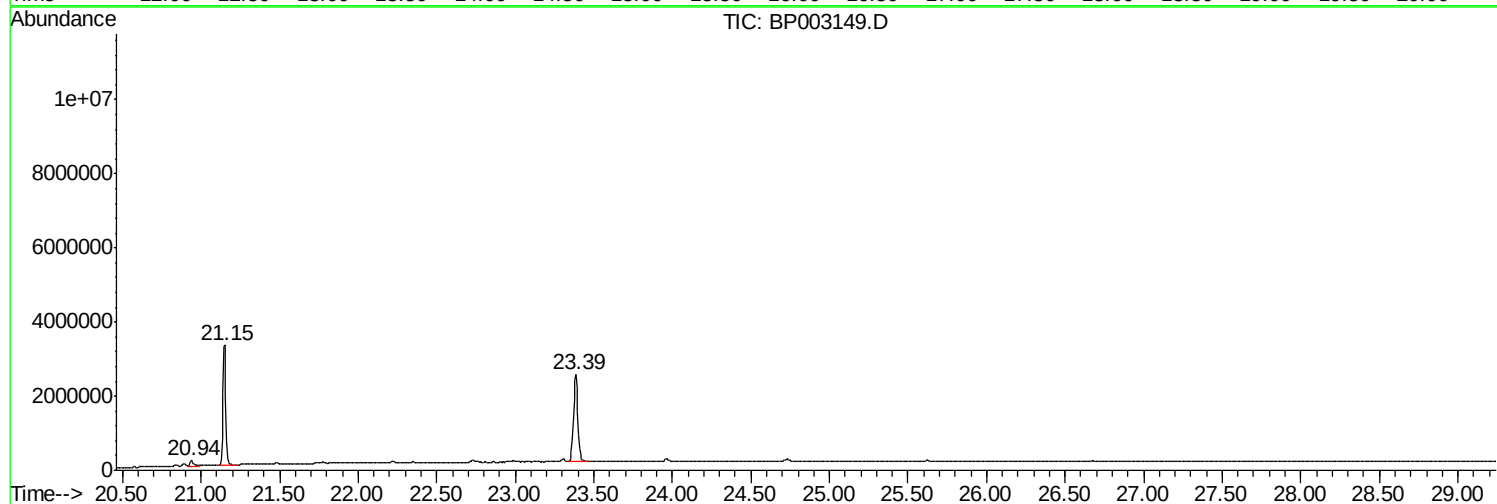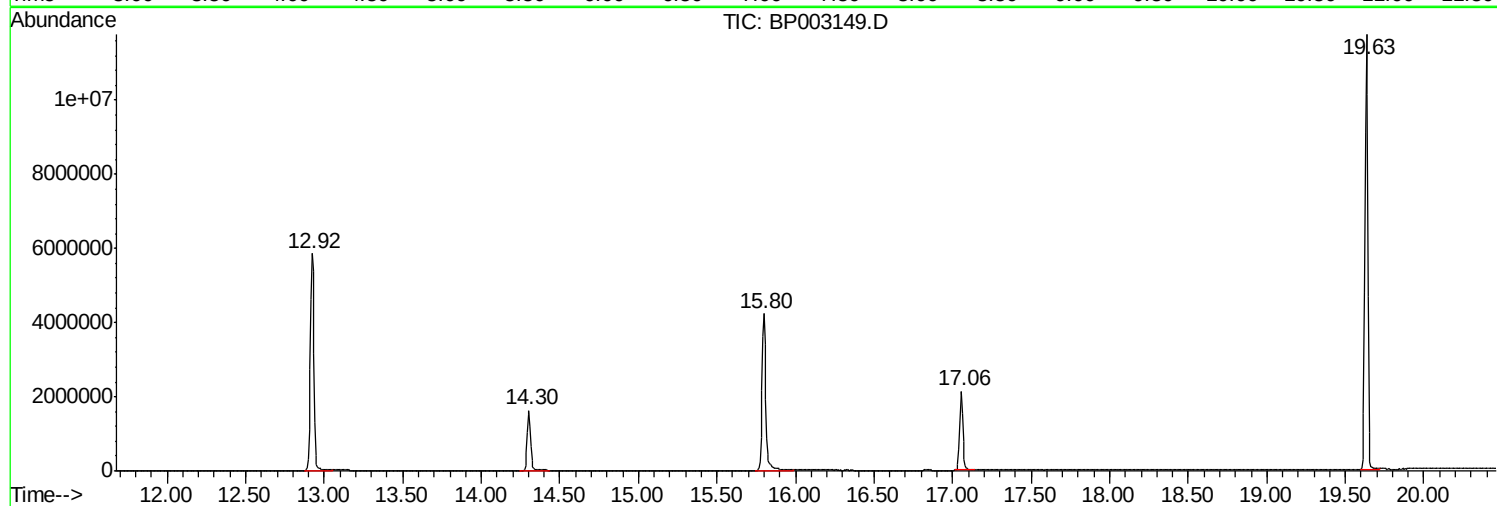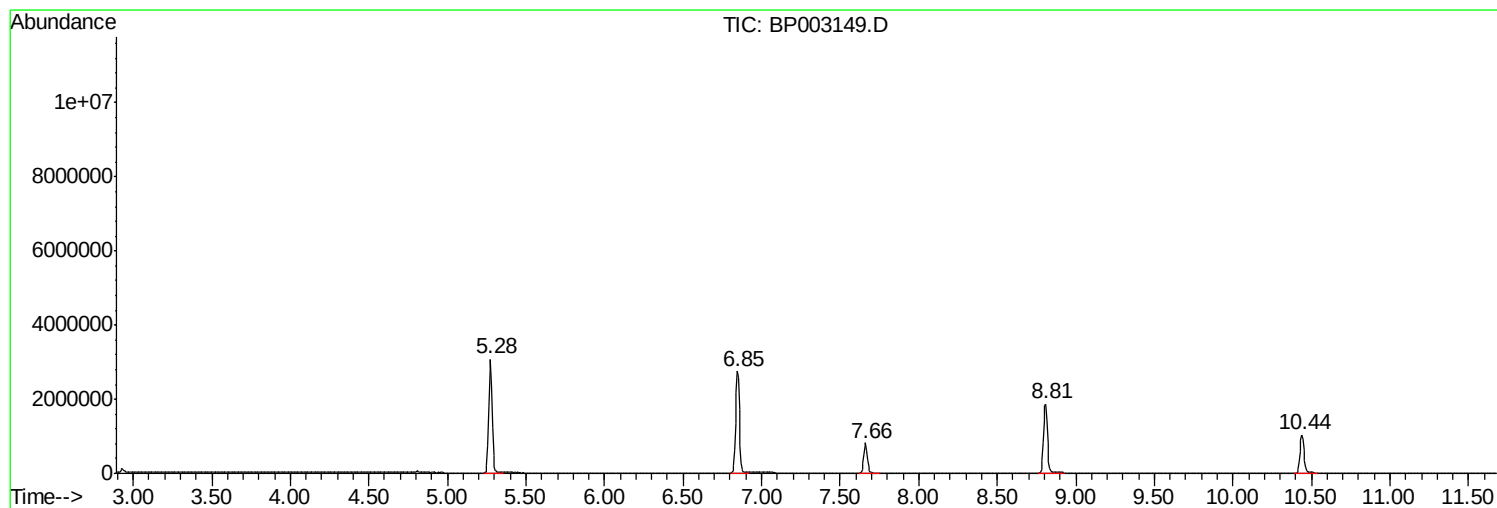

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_P\DATA\BP082820\  
Data File : BP003149.D  
Acq On : 28 Aug 2020 14:14  
Operator : CG/JU  
Sample : PB131271BL  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
PB131271BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\8270-BP082420.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_P\DATA\BP082820\  
Data File : BP003149.D  
Acq On : 28 Aug 2020 14:14  
Operator : CG/JU  
Sample : PB131271BL  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
PB131271BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\8270-BP082420.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |