

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP082820\
 Data File : BP003152.D
 Acq On : 28 Aug 2020 15:59
 Operator : CG/JU
 Sample : L3498-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 HR-06-082620

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP082420.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.970	3	14	27	rVB	1951810	4211969	35.07%	6.382%
2	3.199	49	53	56	rBV	170622	185032	1.54%	0.280%
3	3.228	56	58	65	rVB	233277	238806	1.99%	0.362%
4	3.634	122	127	134	rBV2	122888	155630	1.30%	0.236%
5	4.223	222	227	238	rVB	565119	730747	6.08%	1.107%
6	4.811	319	327	334	rVB2	300412	504520	4.20%	0.764%
7	5.275	399	406	422	rBV	2879695	4185678	34.85%	6.343%
8	6.852	666	674	690	rBV	2421451	3973099	33.08%	6.020%
9	7.663	805	812	821	rBV	702623	1080769	9.00%	1.638%
10	8.810	996	1007	1019	rBV	1735101	2965528	24.69%	4.494%
11	10.440	1276	1284	1291	rBV	888762	1495097	12.45%	2.266%
12	12.922	1699	1706	1723	rBV	5073079	7638301	63.60%	11.574%
13	13.757	1843	1848	1857	rVB	275472	410524	3.42%	0.622%
14	14.304	1934	1941	1958	rVB	1272755	1985295	16.53%	3.008%
15	15.692	2165	2177	2189	rBV5	310250	1646833	13.71%	2.495%
16	15.798	2189	2195	2206	rVB	3794334	5826835	48.52%	8.829%
17	17.051	2402	2408	2421	rVB	1653470	2379047	19.81%	3.605%
18	17.975	2559	2565	2581	rBV	1665374	2498043	20.80%	3.785%
19	19.210	2768	2775	2789	rBV	900728	1303045	10.85%	1.974%
20	19.633	2841	2847	2852	rBV	9689848	12010345	100.00%	18.199%
21	20.880	3055	3059	3064	rBV3	146594	228404	1.90%	0.346%
22	20.969	3071	3074	3082	rVB3	125495	202626	1.69%	0.307%
23	21.145	3099	3104	3109	rBV	2484777	3161631	26.32%	4.791%
24	21.192	3109	3112	3118	rVB	402268	572347	4.77%	0.867%
25	21.345	3135	3138	3142	rVB	485137	509862	4.25%	0.773%
26	21.751	3203	3207	3214	rVB	234976	300378	2.50%	0.455%
27	22.216	3281	3286	3291	rBV	411977	565585	4.71%	0.857%
28	22.339	3304	3307	3312	rVB	222351	296632	2.47%	0.449%
29	22.727	3368	3373	3386	rVB	501304	784328	6.53%	1.188%
30	23.304	3466	3471	3477	rVB	464496	758871	6.32%	1.150%
31	23.380	3477	3484	3501	rVB2	1199151	2492999	20.76%	3.778%
32	23.963	3577	3583	3591	rVB	342365	695207	5.79%	1.053%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP082820\
Data File : BP003152.D
Acq On : 28 Aug 2020 15:59
Operator : CG/JU
Sample : L3498-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HR-06-082620

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP082420.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION


Sum of corrected areas: 65994013

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP082820\
Data File : BP003152.D
Acq On : 28 Aug 2020 15:59
Operator : CG/JU
Sample : L3498-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HR-06-082620

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP082420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

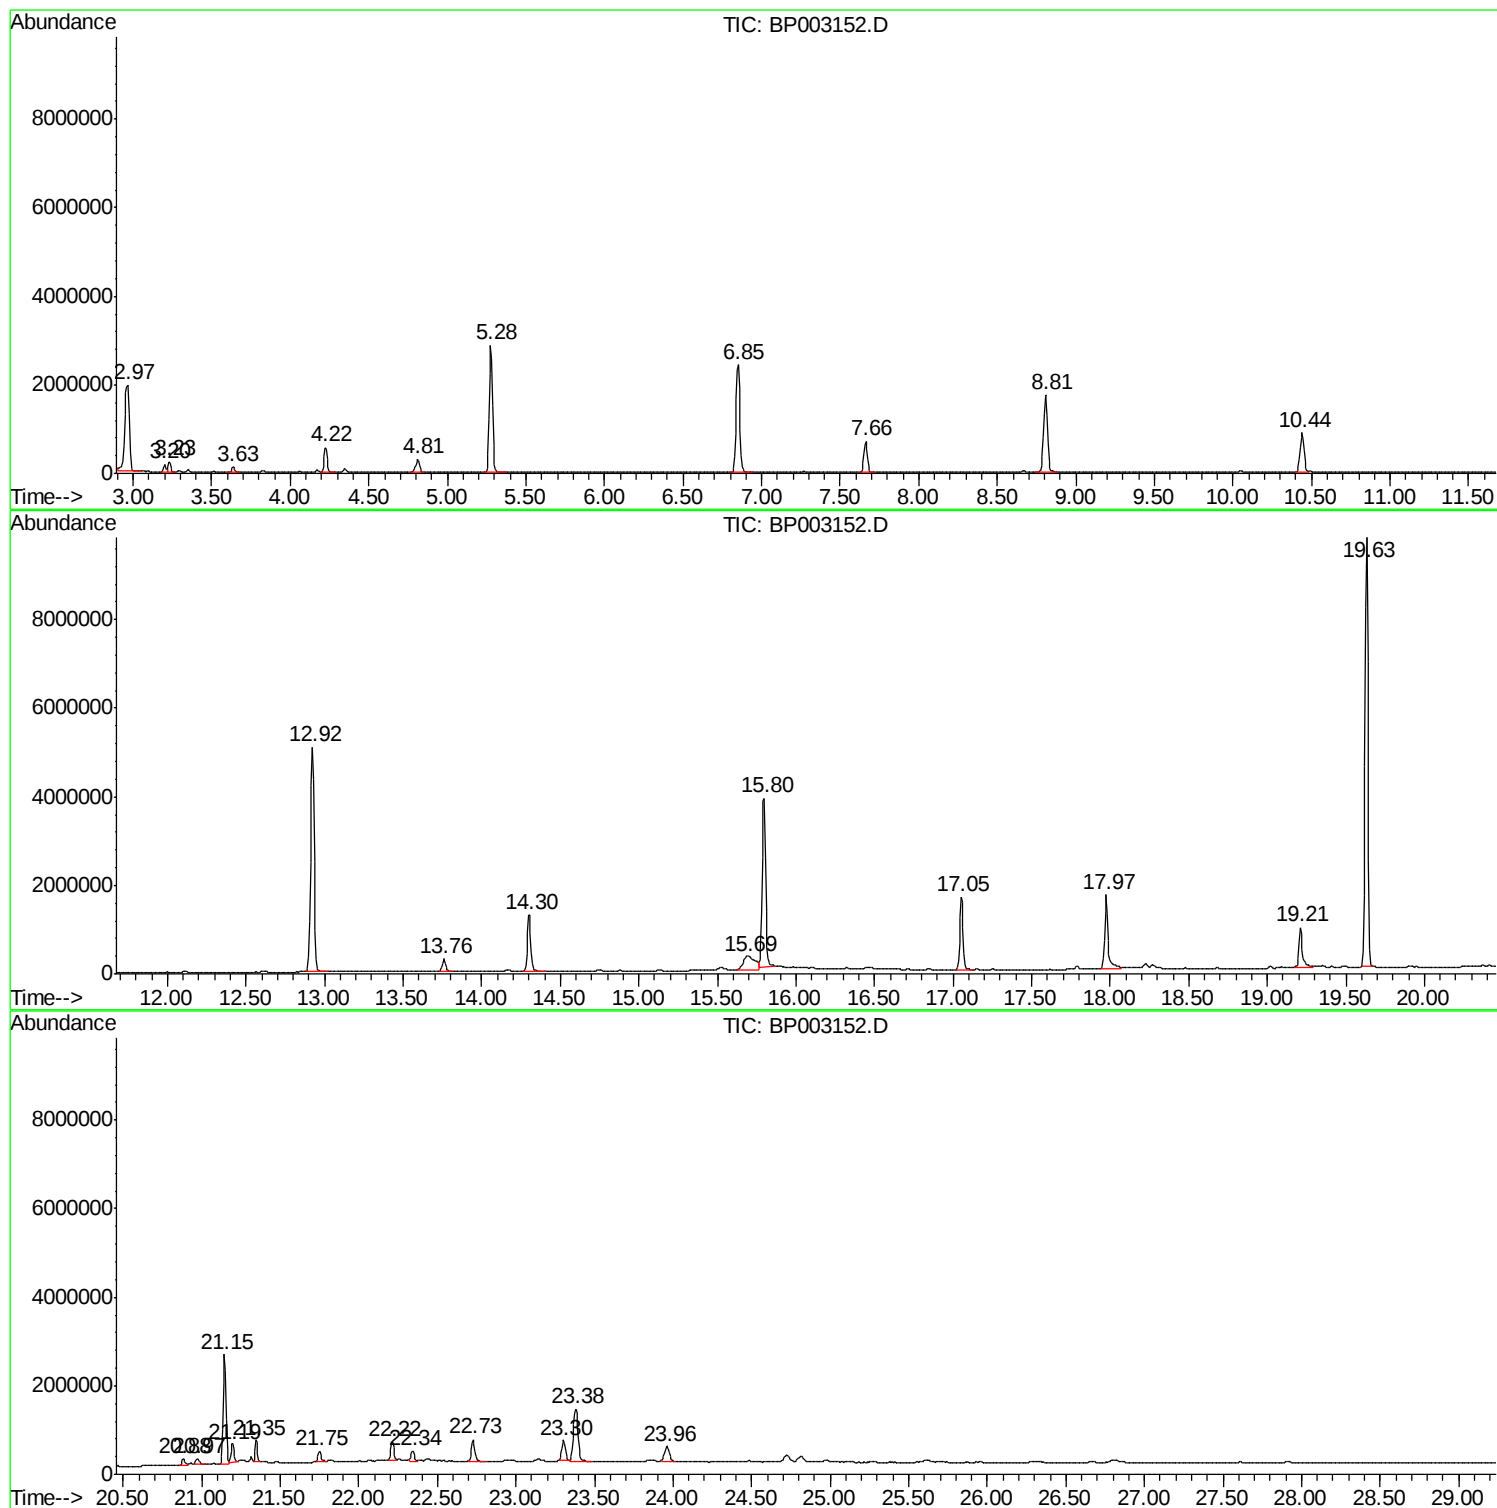

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP082820\
Data File : BP003152.D
Acq On : 28 Aug 2020 15:59
Operator : CG/JU
Sample : L3498-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HR-06-082620

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP082420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP082820\
Data File : BP003152.D
Acq On : 28 Aug 2020 15:59
Operator : CG/JU
Sample : L3498-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HR-06-082620

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP082420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc