

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016796.D
 Acq On : 28 Aug 2023 17:34
 Operator : MA/JU
 Sample : 04037-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYJ3

Quant Time: Aug 29 01:15:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 29 01:12:28 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.034	152	285818	20.000	ng/ul	0.00
20) Naphthalene-d8	10.857	136	1255283	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.687	164	769152	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.451	188	1724686	20.000	ng/ul	0.00
79) Chrysene-d12	21.551	240	1628707	20.000	ng/ul	0.00
88) Perylene-d12	24.127	264	1628333	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	28287	4.090	ng/uL	0.00
4) Pyridine-d5	3.834	84	23564	1.115	ng/ul	0.02
7) Phenol-d5	7.169	99	481931	18.962	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.369	67	377989	23.335	ng/ul	0.00
11) 2-Chlorophenol-d4	7.552	132	283463	14.834	ng/ul	0.00
15) 4-Methylphenol-d8	8.734	113	316707	15.265	ng/ul	0.00
21) Nitrobenzene-d5	9.228	128	220527	23.235	ng/ul	0.00
24) 2-Nitrophenol-d4	9.946	143	97487	9.744	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.469	165	206619	11.078	ng/ul	0.00
31) 4-Chloroaniline-d4	11.016	131	558700	19.533	ng/ul	0.00
46) Dimethylphthalate-d6	14.092	166	1374600	23.698	ng/ul	0.00
49) Acenaphthylene-d8	14.387	160	1632033	24.889	ng/ul	0.00
54) 4-Nitrophenol-d4	14.892	143	36503	3.045	ng/ul	0.00
60) Fluorene-d10	15.681	176	1286901	26.346	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.798	200	27324	2.660	ng/ul	0.00
73) Anthracene-d10	17.551	188	1926525	25.201	ng/ul	0.00
81) Pyrene-d10	19.786	212	2500551	27.954	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.951	264	2142664	26.269	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.881	105	51710	1.607	ng/ul	97
82) Pyrene	19.816	202	142750	1.286	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016796.D
Acq On : 28 Aug 2023 17:34
Operator : MA/JU
Sample : 04037-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYJ3

Quant Time: Aug 29 01:15:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 29 01:12:28 2023
Response via : Initial Calibration




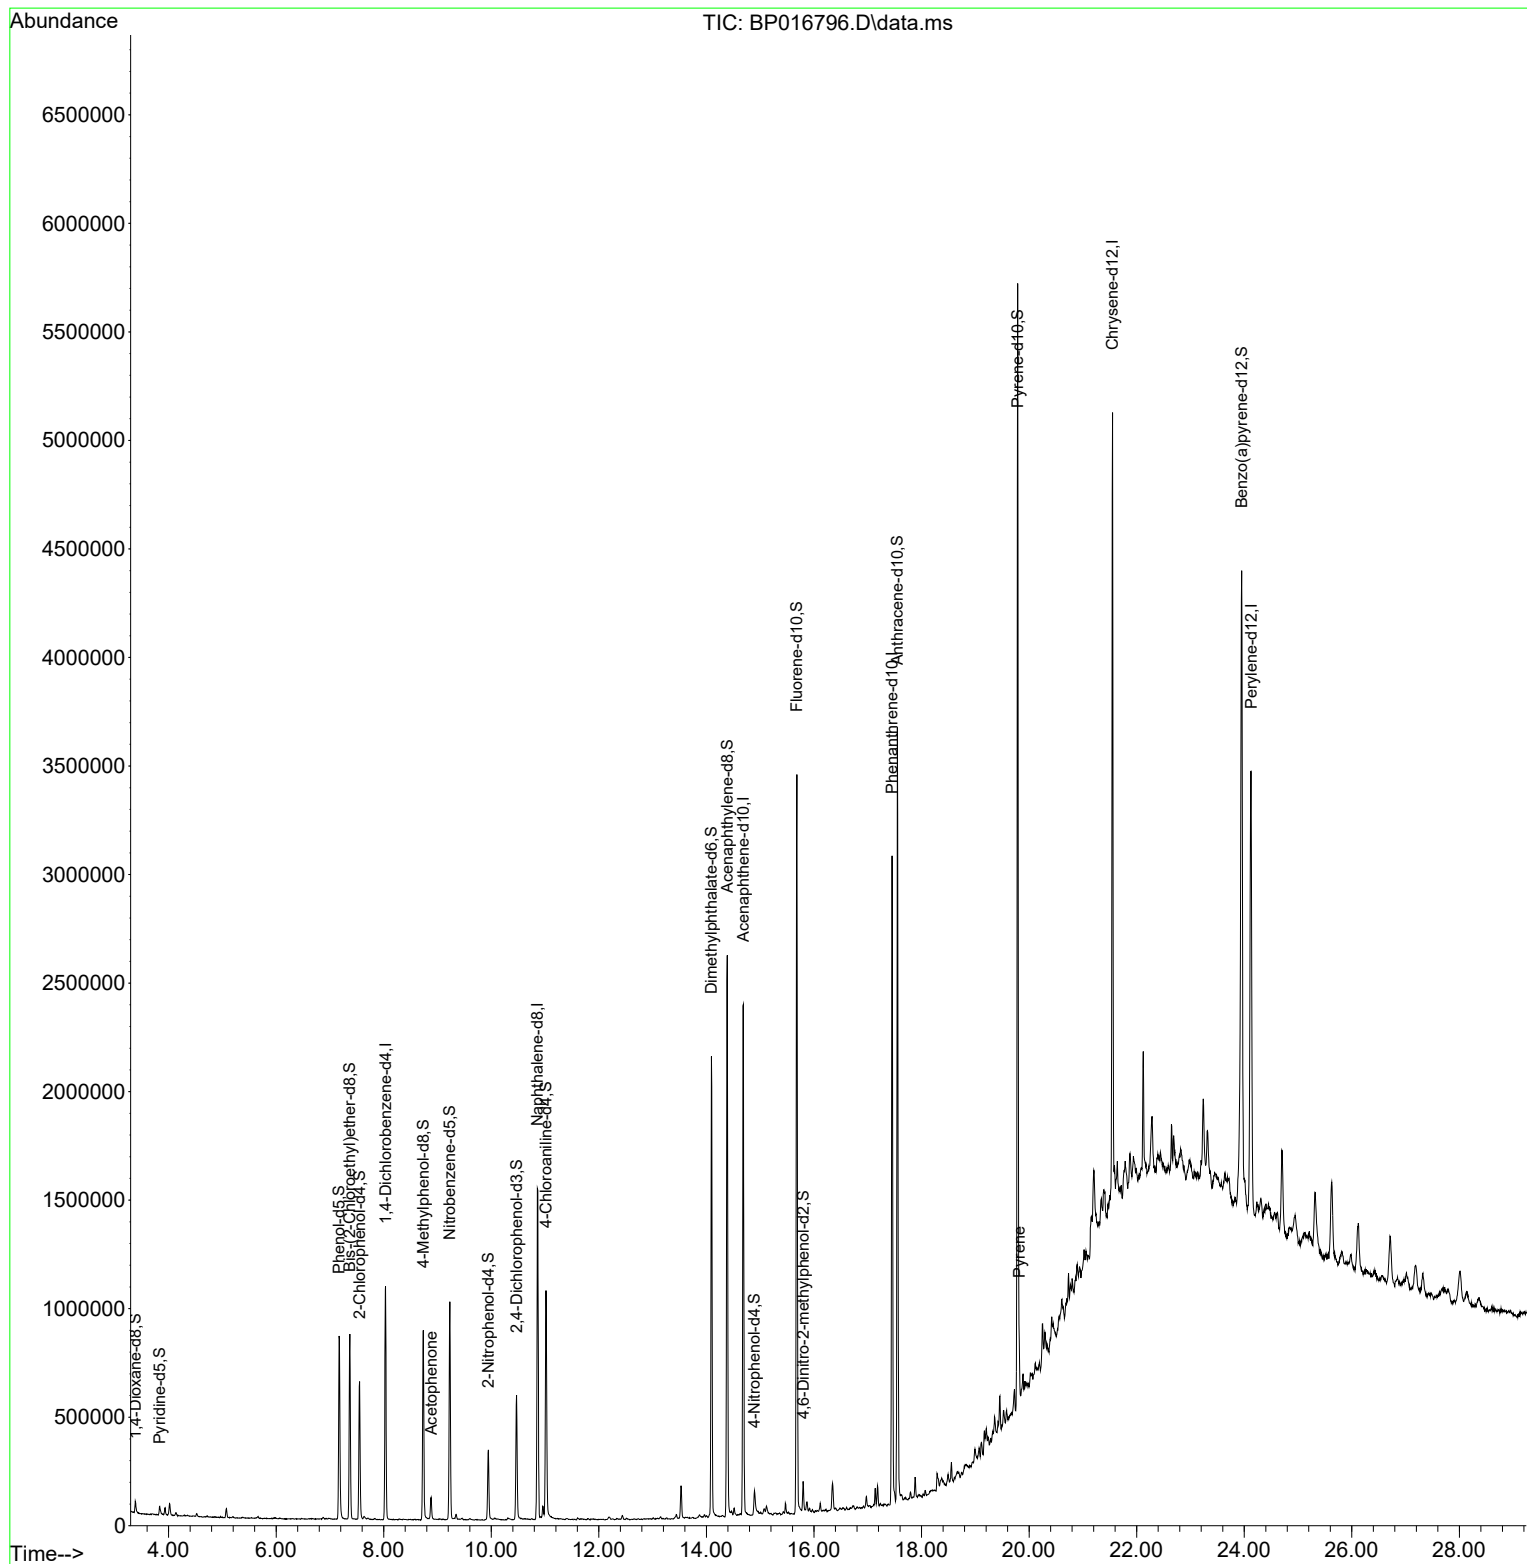


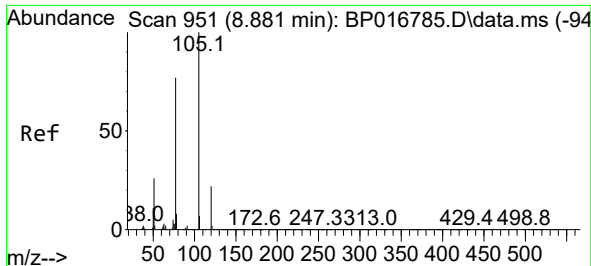

#16
Acetophenone
Concen: 1.607 ng/ul
RT: 8.881 min Scan# 91
Delta R.T. 0.000 min
Lab File: BP016796.D
Acq: 28 Aug 2023 17:34

Instrument :
BNA_P
ClientSampleId :
EZYJ3

Tgt Ion:105 Resp: 51710
Ion Ratio Lower Upper
105 100
77 77.3 64.2 96.4
51 28.8 22.2 33.4

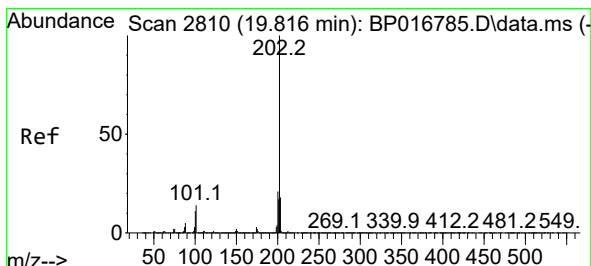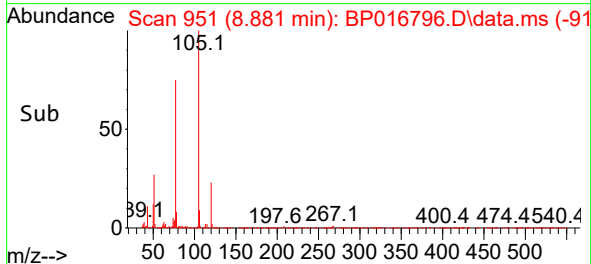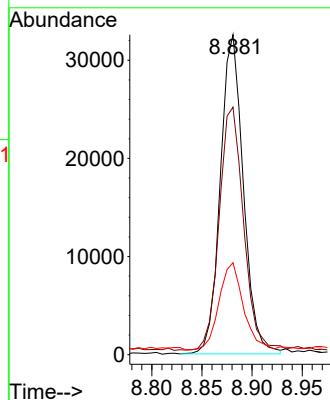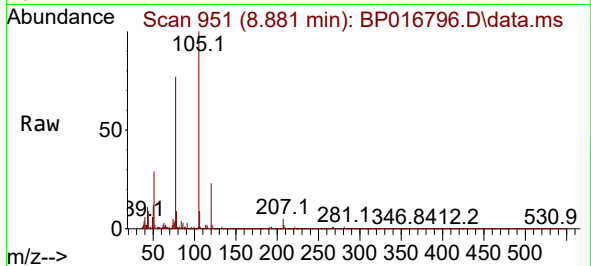

#82
Pyrene
Concen: 1.286 ng/ul
RT: 19.816 min Scan# 2810
Delta R.T. 0.000 min
Lab File: BP016796.D
Acq: 28 Aug 2023 17:34

Tgt Ion:202 Resp: 142750
Ion Ratio Lower Upper
202 100
101 14.1 11.4 17.2
100 11.7 9.4 14.2

