

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016798.D
 Acq On : 28 Aug 2023 18:43
 Operator : MA/JU
 Sample : 04037-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYE2

Quant Time: Aug 29 01:15:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 29 01:12:28 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.034	152	431179	20.000	ng/ul	0.00
20) Naphthalene-d8	10.863	136	1853385	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.687	164	1146747	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.451	188	2475086	20.000	ng/ul	0.00
79) Chrysene-d12	21.551	240	1891332	20.000	ng/ul	0.00
88) Perylene-d12	24.121	264	1695595	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	42916	4.114	ng/uL	0.00
4) Pyridine-d5	3.805	84	259	0.008	ng/ul	-0.01
7) Phenol-d5	7.169	99	409330	10.676	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.369	67	525516	21.506	ng/ul	0.00
11) 2-Chlorophenol-d4	7.552	132	176847	6.135	ng/ul	0.00
15) 4-Methylphenol-d8	8.734	113	300101	9.588	ng/ul	0.00
21) Nitrobenzene-d5	9.228	128	324102	23.128	ng/ul	0.00
24) 2-Nitrophenol-d4	9.946	143	78893	5.341	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.469	165	156765	5.693	ng/ul	0.00
31) 4-Chloroaniline-d4	11.016	131	770745	18.251	ng/ul	0.00
46) Dimethylphthalate-d6	14.092	166	1860454	21.513	ng/ul	0.00
49) Acenaphthylene-d8	14.387	160	2435456	24.912	ng/ul	0.00
54) 4-Nitrophenol-d4	14.892	143	47757	2.672	ng/ul	0.00
60) Fluorene-d10	15.681	176	1863008	25.582	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.798	200	36833	2.499	ng/ul	0.00
73) Anthracene-d10	17.551	188	2621503	23.895	ng/ul	0.00
81) Pyrene-d10	19.786	212	3108103	29.922	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.951	264	2159156	25.422	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.881	105	67237	1.385	ng/ul	99
80) Fluoranthene	19.457	202	244096	1.956	ng/ul	100
82) Pyrene	19.816	202	449367	3.486	ng/ul	99
85) Benzo(a)anthracene	21.533	228	138403	1.062	ng/ul	96
87) Chrysene	21.586	228	298949	2.526	ng/ul	97
90) Benzo(b)fluoranthene	23.321	252	391788	3.618	ng/ul#	82
91) Benzo(k)fluoranthene	23.368	252	107932	1.008	ng/ul#	62
93) Benzo(a)pyrene	24.004	252	134521	1.374	ng/ul#	68
94) Indeno(1,2,3-cd)pyrene	26.845	276	163092	1.630	ng/ul	99
96) Benzo(g,h,i)perylene	27.698	276	180077	2.373	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016798.D
Acq On : 28 Aug 2023 18:43
Operator : MA/JU
Sample : 04037-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZY2

Quant Time: Aug 29 01:15:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 29 01:12:28 2023
Response via : Initial Calibration




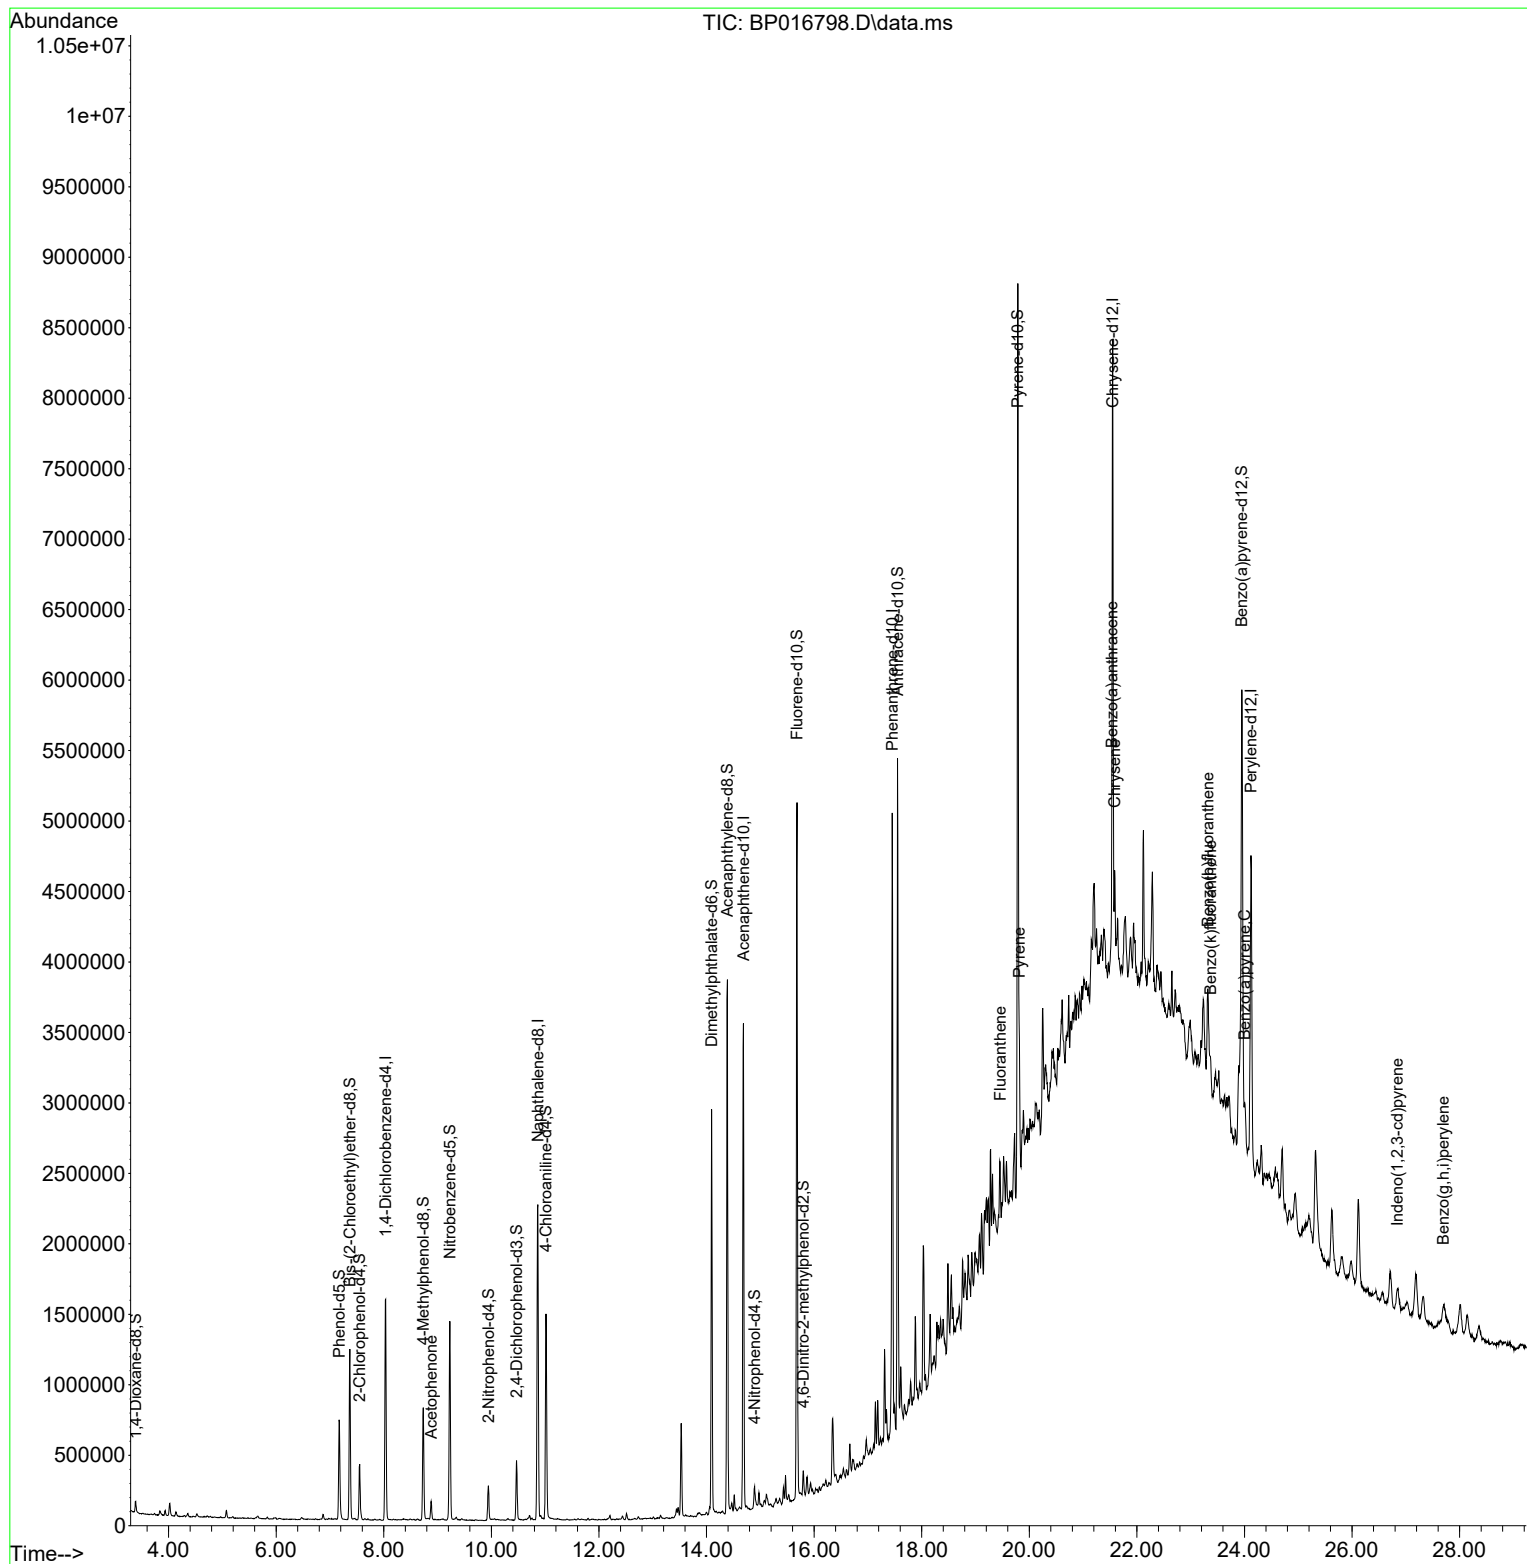


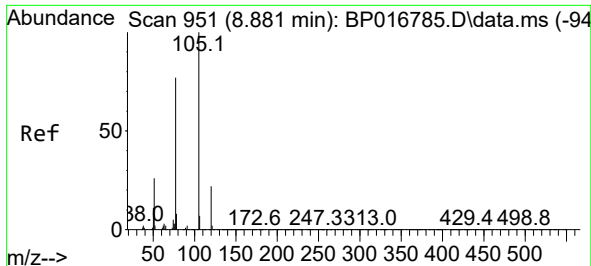

#16
Acetophenone
Concen: 1.385 ng/ul
RT: 8.881 min Scan# 91
Delta R.T. 0.000 min
Lab File: BP016798.D
Acq: 28 Aug 2023 18:43




Instrument :
BNA_P
ClientSampleId :
EZY2


Tgt Ion:105 Resp: 67237
Ion Ratio Lower Upper
105 100
77 81.0 64.2 96.4
51 28.2 22.2 33.4

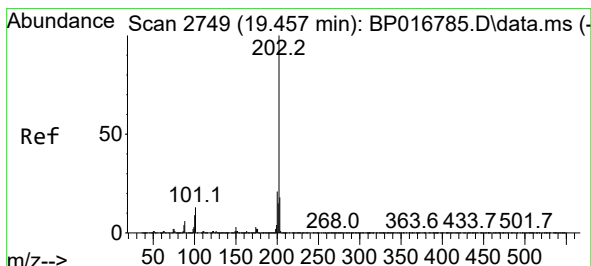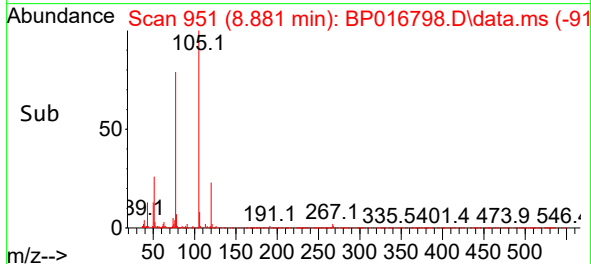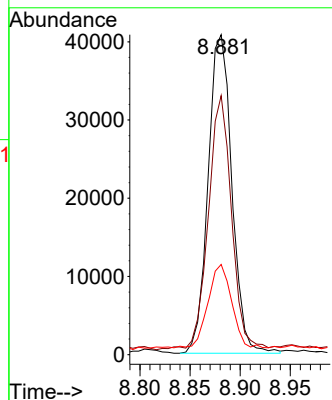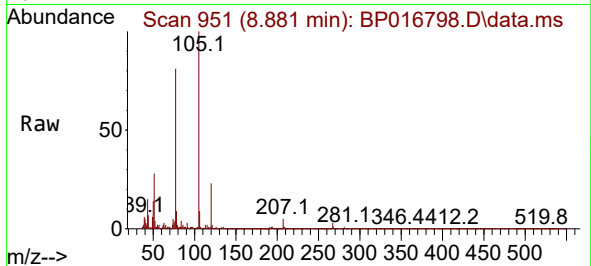

#80
Fluoranthene
Concen: 1.956 ng/ul
RT: 19.457 min Scan# 2749
Delta R.T. 0.000 min
Lab File: BP016798.D
Acq: 28 Aug 2023 18:43

Tgt Ion:202 Resp: 244096
Ion Ratio Lower Upper
202 100
101 12.1 9.7 14.5
100 9.3 7.4 11.2

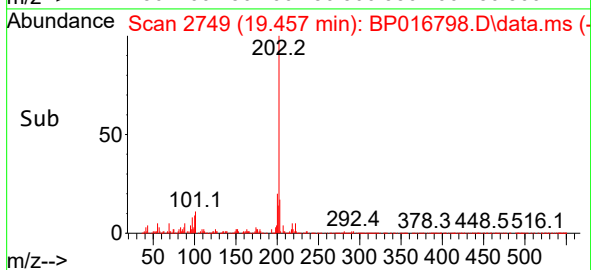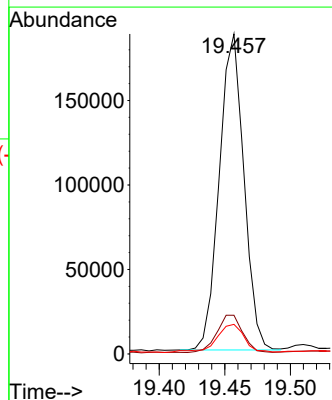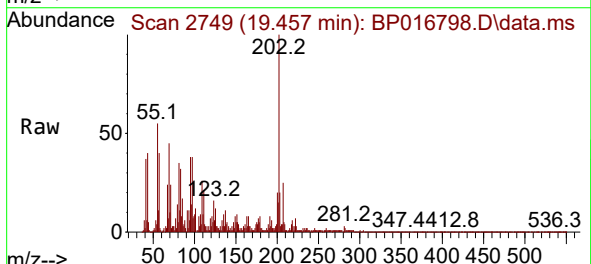

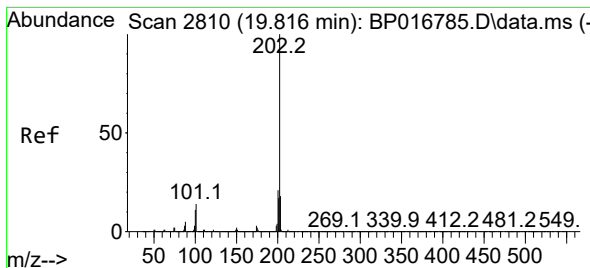

#82

Pyrene

Concen: 3.486 ng/ul

RT: 19.816 min Scan# 2810

Delta R.T. 0.000 min

Lab File: BP016798.D

Acq: 28 Aug 2023 18:43

Instrument :

BNA_P

ClientSampleId :

EZY2





Tgt Ion:202 Resp: 449367

Ion Ratio Lower Upper

202 100

101 14.1 11.4 17.2

100 11.5 9.4 14.2

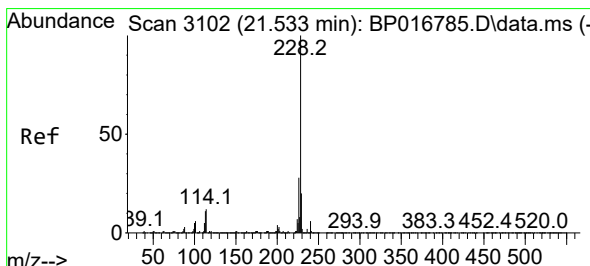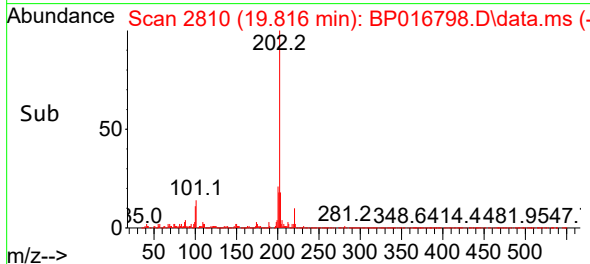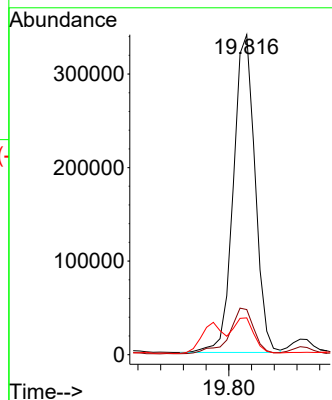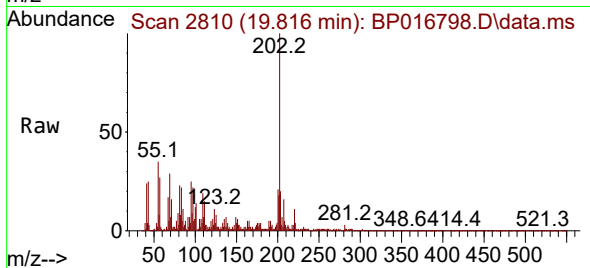

#85

Benzo(a)anthracene

Concen: 1.062 ng/ul

RT: 21.533 min Scan# 3102

Delta R.T. 0.000 min

Lab File: BP016798.D

Acq: 28 Aug 2023 18:43




Tgt Ion:228 Resp: 138403


Ion Ratio Lower Upper

228 100

229 23.8 16.2 24.4

226 29.1 22.9 34.3

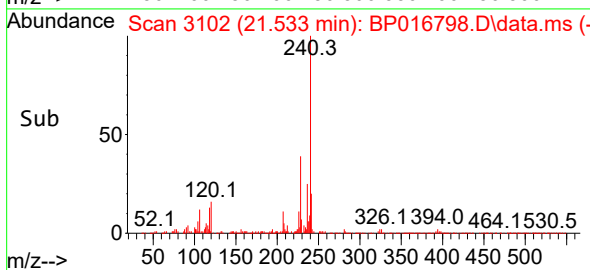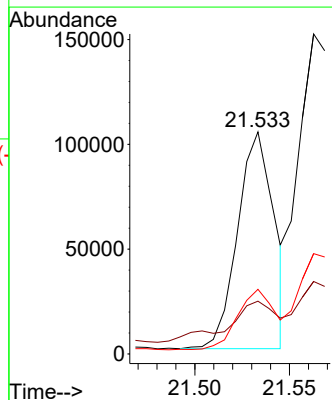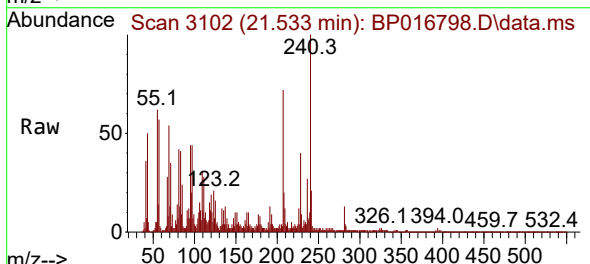

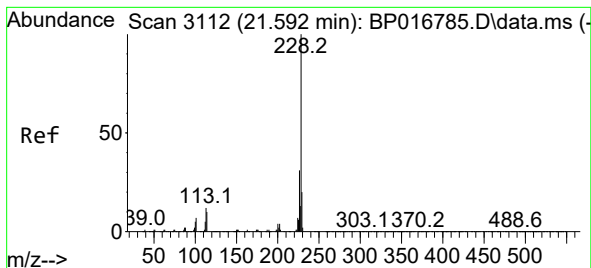

#87

Chrysene

Concen: 2.526 ng/ul

RT: 21.586 min Scan# 3111

Delta R.T. -0.006 min

Lab File: BP016798.D

Acq: 28 Aug 2023 18:43

Instrument :

BNA_P

ClientSampleId :

EZY2





Tgt Ion:228 Resp: 298949

Ion Ratio Lower Upper

228 100

226 30.5 25.0 37.4

229 22.0 16.0 24.0

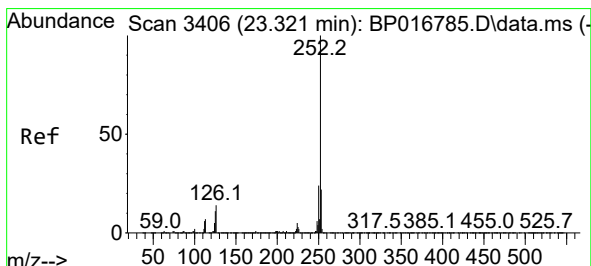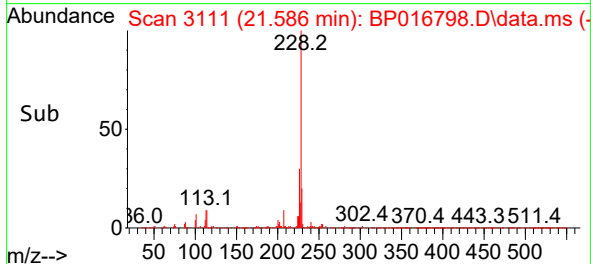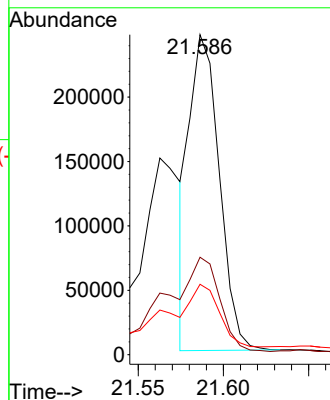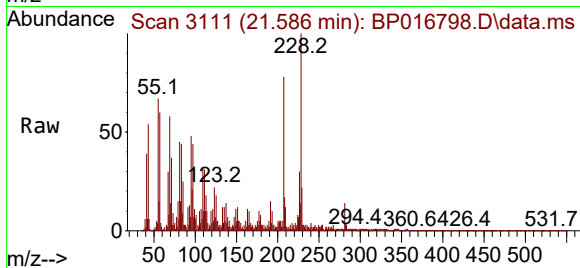

#90

Benzo(b)fluoranthene

Concen: 3.618 ng/ul

RT: 23.321 min Scan# 3406

Delta R.T. 0.000 min

Lab File: BP016798.D

Acq: 28 Aug 2023 18:43




Tgt Ion:252 Resp: 391788


Ion Ratio Lower Upper

252 100

253 24.0 17.7 26.5

125 28.3 9.0 13.4#


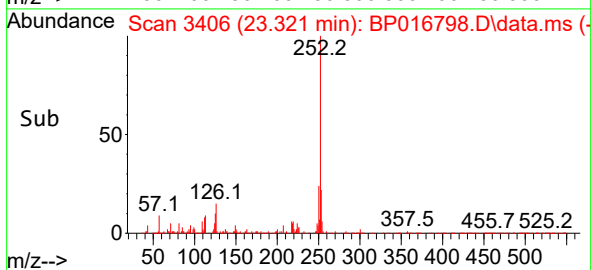
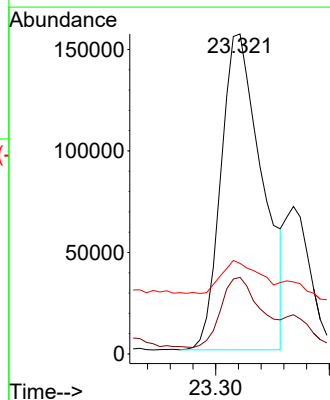
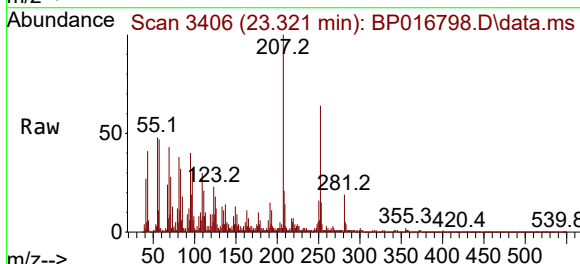


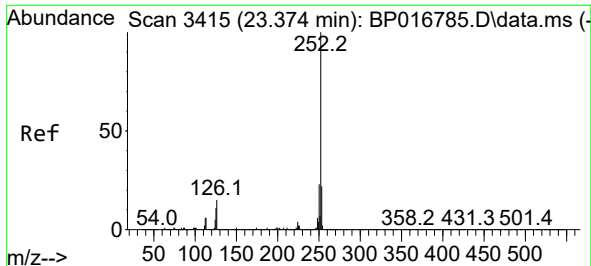

#91
Benzo(k)fluoranthene
Concen: 1.008 ng/ul
RT: 23.368 min Scan# 3415
Delta R.T. -0.006 min
Lab File: BP016798.D
Acq: 28 Aug 2023 18:43




Instrument :
BNA_P
ClientSampleId :
EZY2


Tgt Ion:252 Resp: 107932
Ion Ratio Lower Upper
252 100
253 26.6 18.1 27.1
125 48.9 8.9 13.3#

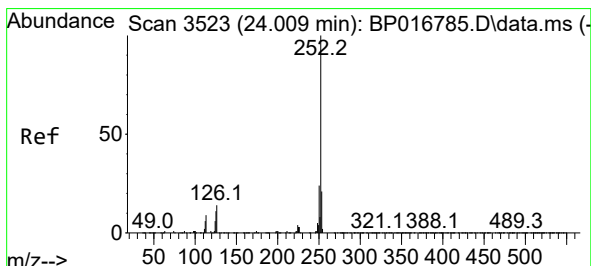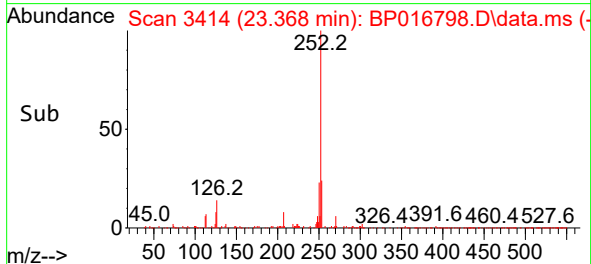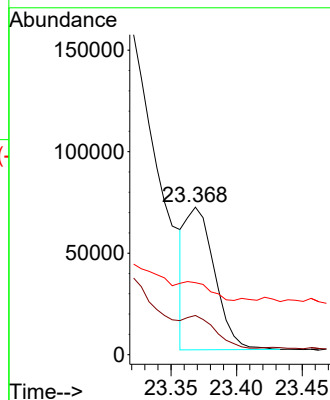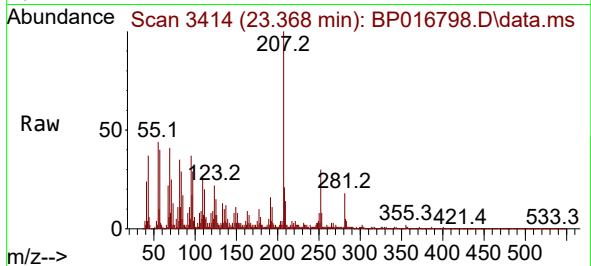

#93
Benzo(a)pyrene
Concen: 1.374 ng/ul
RT: 24.004 min Scan# 3522
Delta R.T. -0.006 min
Lab File: BP016798.D
Acq: 28 Aug 2023 18:43

Tgt Ion:252 Resp: 134521
Ion Ratio Lower Upper
252 100
253 25.5 17.8 26.8
125 43.0 9.9 14.9#

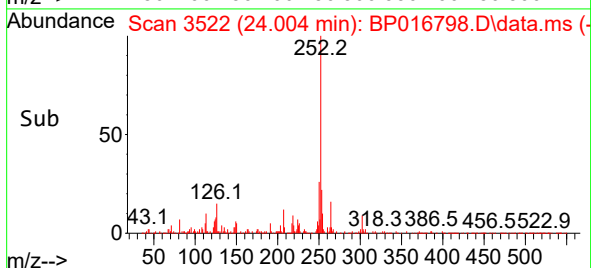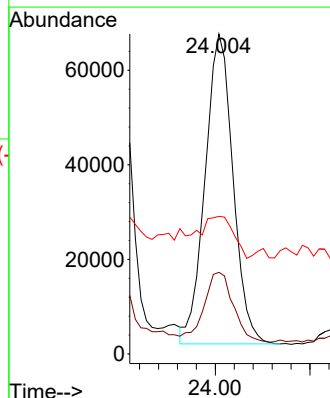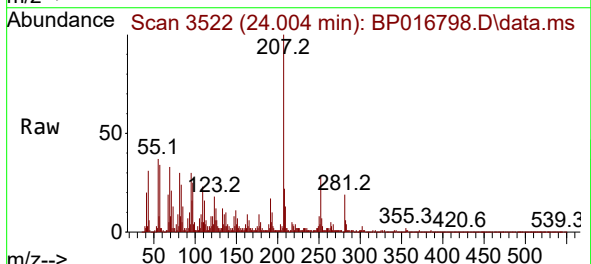

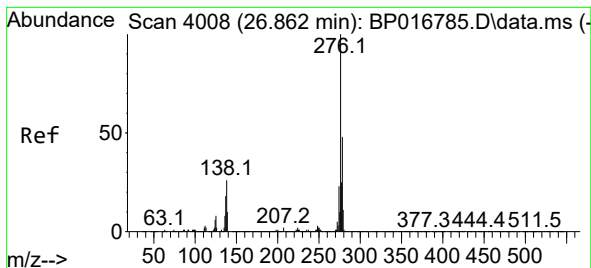

#94

Indeno(1,2,3-cd)pyrene

Concen: 1.630 ng/ul

RT: 26.845 min Scan# 4008

Delta R.T. -0.018 min

Lab File: BP016798.D

Acq: 28 Aug 2023 18:43

Instrument :

BNA_P

ClientSampleId :

EZY2





Tgt Ion:276 Resp: 163092

Ion Ratio Lower Upper

276 100

138 26.9 20.9 31.3

277 24.8 19.8 29.6

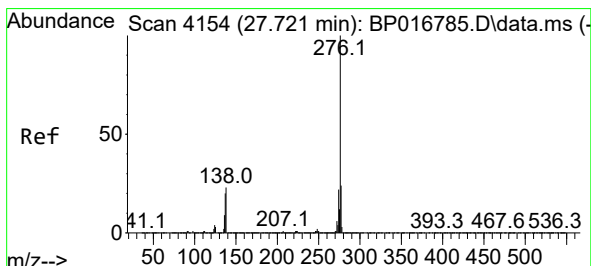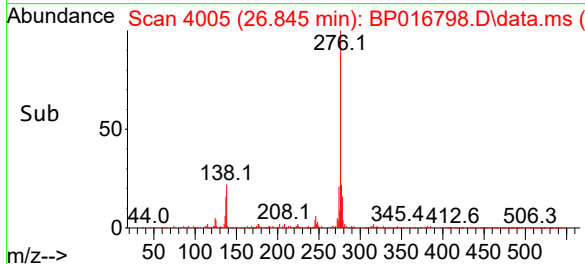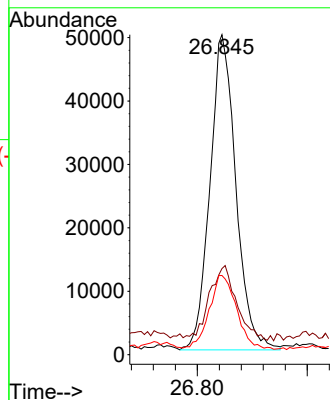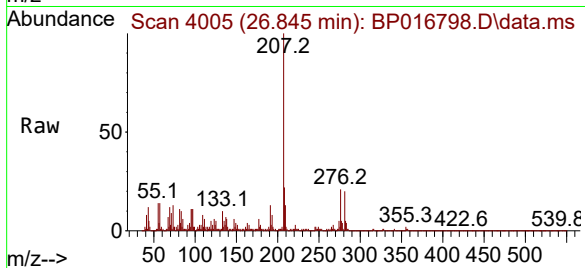

#96

Benzo(g,h,i)perylene

Concen: 2.373 ng/ul

RT: 27.698 min Scan# 4150

Delta R.T. -0.023 min

Lab File: BP016798.D

Acq: 28 Aug 2023 18:43

Tgt Ion:276 Resp: 180077

Ion Ratio Lower Upper

276 100

138 26.1 20.2 30.4

277 25.6 19.3 28.9

