

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016822.D
 Acq On : 29 Aug 2023 08:49
 Operator : MA/JU
 Sample : 04123-18
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH8S1

Quant Time: Aug 29 22:22:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 29 01:12:28 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.028	152	406475	20.000	ng/u1	0.00
20) Naphthalene-d8	10.857	136	1843024	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.681	164	1179042	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.451	188	2643469	20.000	ng/u1	0.00
79) Chrysene-d12	21.545	240	2175865	20.000	ng/u1	0.00
88) Perylene-d12	24.116	264	1969552	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	50170	5.101	ng/uL	0.00
4) Pyridine-d5	3.817	84	256147	8.523	ng/u1	0.00
7) Phenol-d5	7.169	99	269113	7.446	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.363	67	655741	28.466	ng/u1	0.00
11) 2-Chlorophenol-d4	7.546	132	644411	23.713	ng/u1	0.00
15) 4-Methylphenol-d8	8.728	113	476754	16.158	ng/u1	0.00
21) Nitrobenzene-d5	9.228	128	422580	30.325	ng/u1	0.00
24) 2-Nitrophenol-d4	9.940	143	440522	29.991	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.463	165	749638	27.375	ng/u1	0.00
31) 4-Chloroaniline-d4	11.010	131	795417	18.941	ng/u1	0.00
46) Dimethylphthalate-d6	14.093	166	2849034	32.042	ng/u1	0.00
49) Acenaphthylene-d8	14.381	160	3130227	31.141	ng/u1	0.00
54) 4-Nitrophenol-d4	14.887	143	100168	5.450	ng/u1	0.00
60) Fluorene-d10	15.675	176	2523003	33.695	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.798	200	423267	26.887	ng/u1	0.00
73) Anthracene-d10	17.551	188	4324122	36.904	ng/u1	0.00
81) Pyrene-d10	19.786	212	5000983	41.848	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.951	264	3707935	37.584	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.417	88	45546	4.253	ng/uL	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016822.D
Acq On : 29 Aug 2023 08:49
Operator : MA/JU
Sample : 04123-18
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH8S1

Quant Time: Aug 29 22:22:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 29 01:12:28 2023
Response via : Initial Calibration

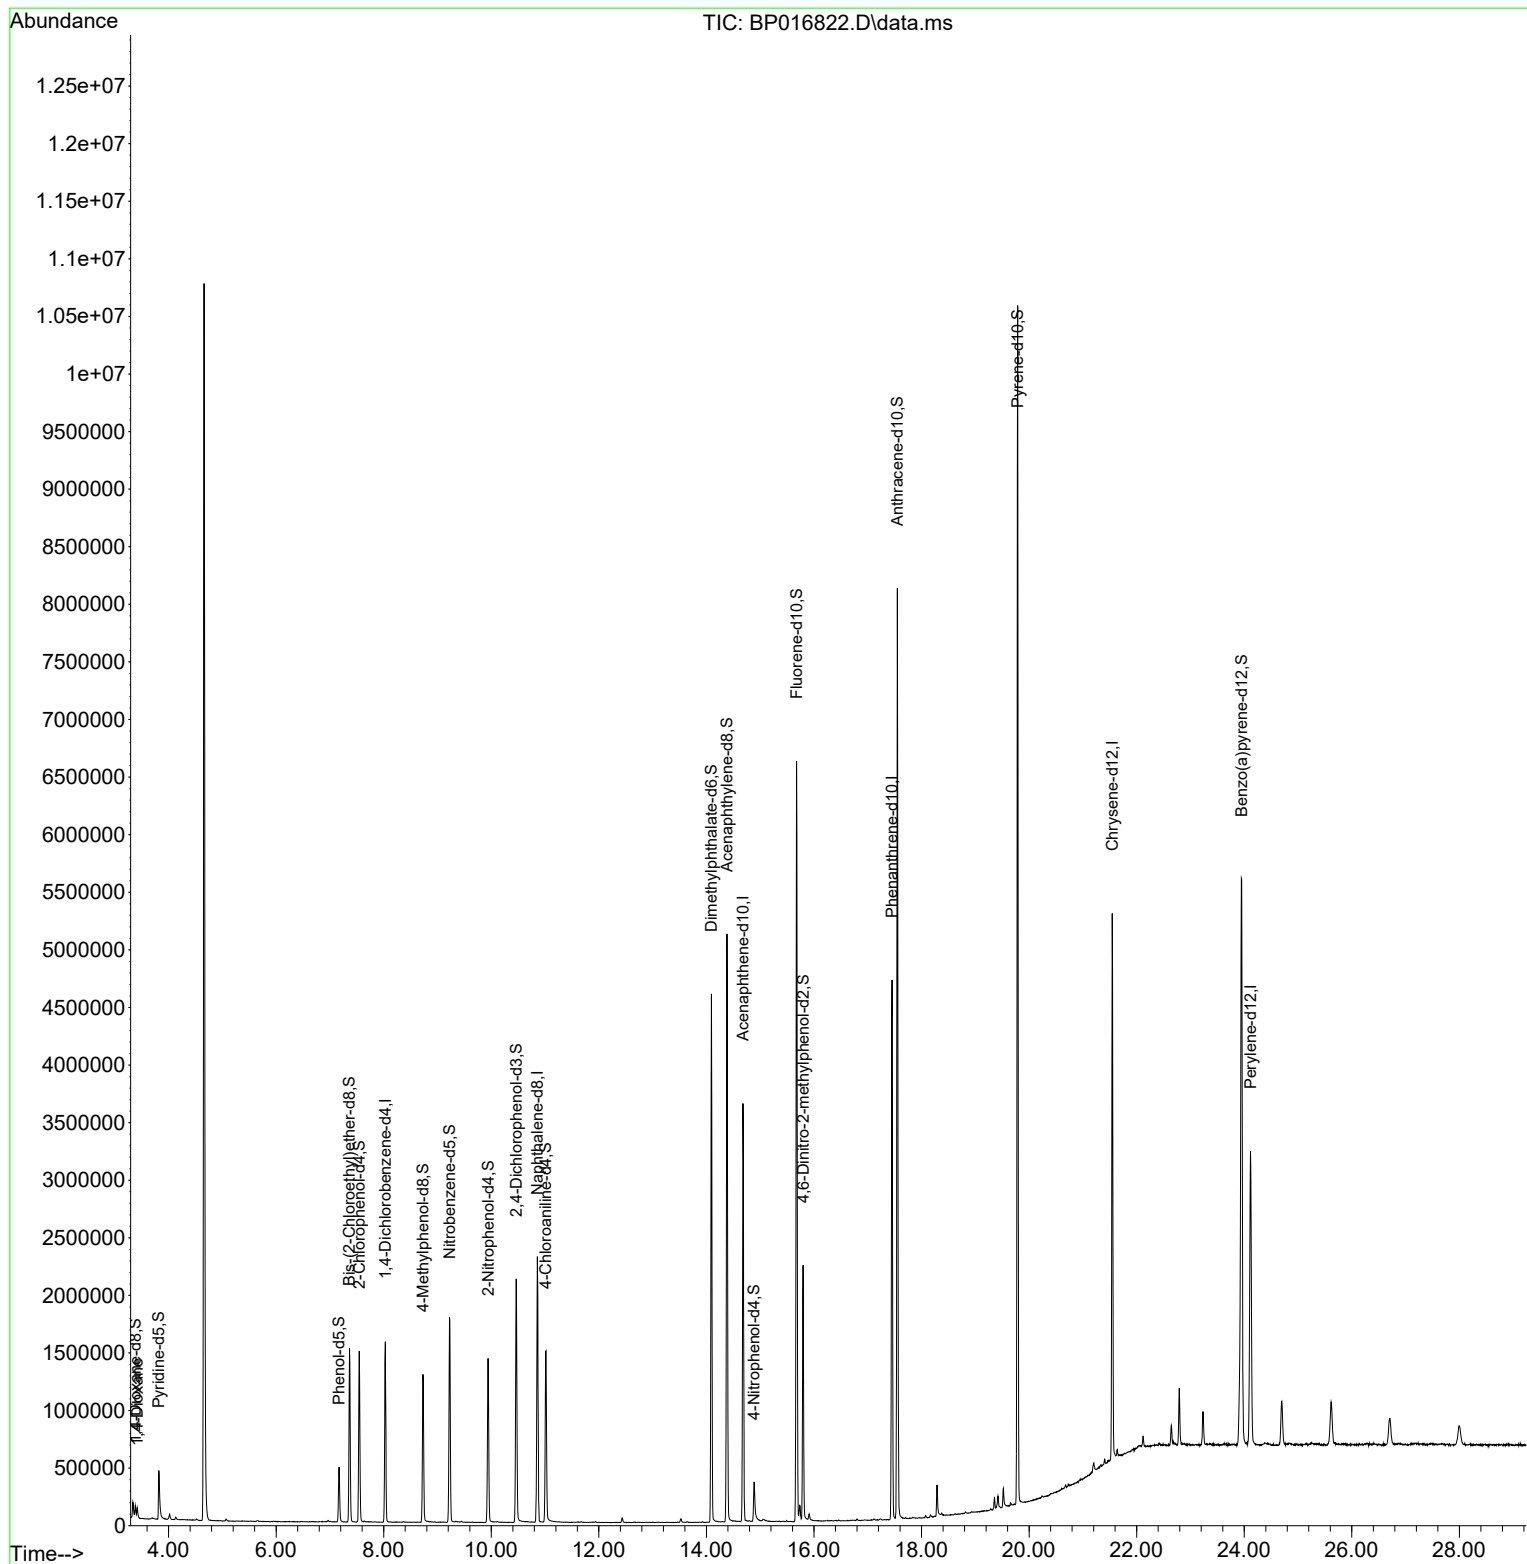

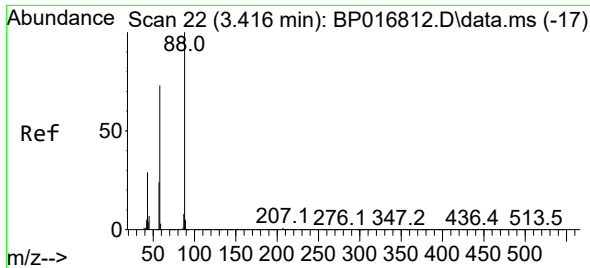

#2
 1,4-Dioxane
 Concen: 4.253 ng/uL
 RT: 3.417 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BP016822.D
 Acq: 29 Aug 2023 08:49

Instrument :
 BNA_P
 ClientSampleId :
 BH8S1

Tgt Ion: 88 Resp: 45546
 Ion Ratio Lower Upper
 88 100
 43 29.7 24.0 36.0
 58 70.2 59.8 89.8

