

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016824.D
 Acq On : 29 Aug 2023 09:57
 Operator : MA/JU
 Sample : 04123-20
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHAU0

Quant Time: Aug 29 22:23:11 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 29 01:12:28 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.028	152	371397	20.000	ng/u1	0.00
20) Naphthalene-d8	10.857	136	1664564	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.681	164	1035017	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.451	188	2287605	20.000	ng/u1	0.00
79) Chrysene-d12	21.545	240	1870636	20.000	ng/u1	0.00
88) Perylene-d12	24.116	264	1682342	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	81147	9.030	ng/uL	0.00
4) Pyridine-d5	3.817	84	662417	24.122	ng/u1	0.00
7) Phenol-d5	7.169	99	701489	21.241	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.364	67	1032912	49.074	ng/u1	0.00
11) 2-Chlorophenol-d4	7.546	132	1048727	42.236	ng/u1	0.00
15) 4-Methylphenol-d8	8.728	113	848757	31.483	ng/u1	0.00
21) Nitrobenzene-d5	9.228	128	651208	51.742	ng/u1	0.00
24) 2-Nitrophenol-d4	9.940	143	698221	52.631	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.463	165	1175605	47.533	ng/u1	0.00
31) 4-Chloroaniline-d4	11.016	131	1522408	40.139	ng/u1	0.00
46) Dimethylphthalate-d6	14.093	166	3962257	50.763	ng/u1	0.00
49) Acenaphthylene-d8	14.381	160	4606208	52.202	ng/u1	0.00
54) 4-Nitrophenol-d4	14.887	143	251143	15.567	ng/u1	0.00
60) Fluorene-d10	15.681	176	3516169	53.494	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.798	200	607658	44.604	ng/u1	0.00
73) Anthracene-d10	17.551	188	5587120	55.100	ng/u1	0.00
81) Pyrene-d10	19.786	212	6435441	62.639	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.951	264	4868741	57.775	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.417	88	16304	1.666	ng/uL	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016824.D
Acq On : 29 Aug 2023 09:57
Operator : MA/JU
Sample : 04123-20
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHUAU0

Quant Time: Aug 29 22:23:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 29 01:12:28 2023
Response via : Initial Calibration

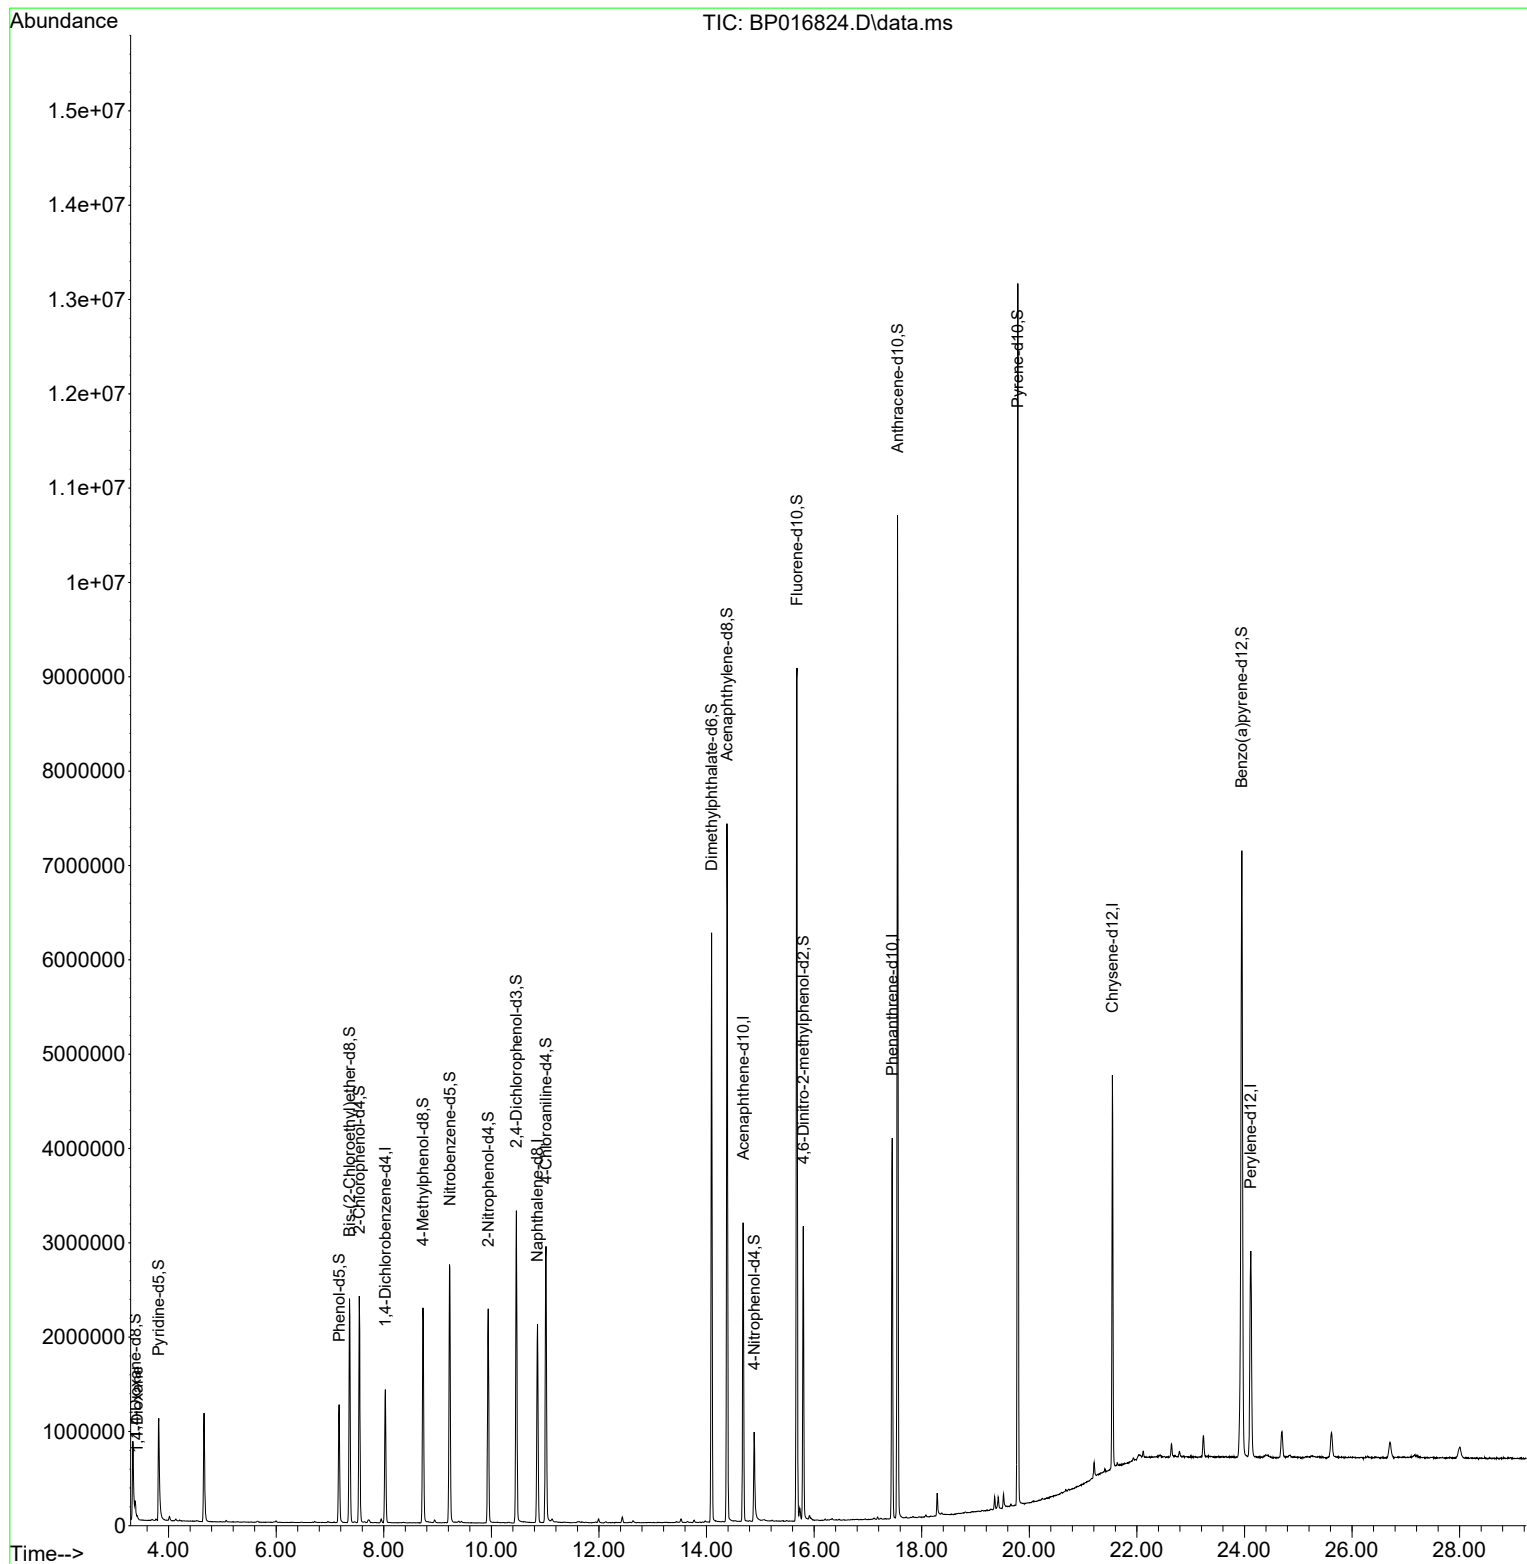

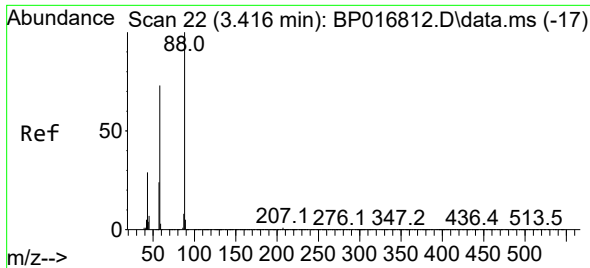

#2
 1,4-Dioxane
 Concen: 1.666 ng/uL
 RT: 3.417 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BP016824.D
 Acq: 29 Aug 2023 09:57

Instrument :
 BNA_P
 ClientSampleId :
 BHAU0

Tgt Ion: 88	Resp:	16304
Ion	Ratio	Lower Upper
88	100	
43	31.5	24.0 36.0
58	72.7	59.8 89.8

