

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016825.D
 Acq On : 29 Aug 2023 10:31
 Operator : MA/JU
 Sample : 04123-21
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHAU3

Quant Time: Aug 29 22:23:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 29 01:12:28 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.028	152	345096	20.000	ng/u1	0.00
20) Naphthalene-d8	10.857	136	1548459	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.681	164	967046	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.445	188	2108721	20.000	ng/u1	-0.01
79) Chrysene-d12	21.545	240	1613305	20.000	ng/u1	0.00
88) Perylene-d12	24.116	264	1439124	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	50480	6.046	ng/uL	0.00
4) Pyridine-d5	3.817	84	254765	9.984	ng/u1	0.00
7) Phenol-d5	7.169	99	306387	9.985	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.364	67	812525	41.545	ng/u1	0.00
11) 2-Chlorophenol-d4	7.546	132	783535	33.960	ng/u1	0.00
15) 4-Methylphenol-d8	8.728	113	561501	22.415	ng/u1	0.00
21) Nitrobenzene-d5	9.222	128	507985	43.388	ng/u1	0.00
24) 2-Nitrophenol-d4	9.940	143	534224	43.289	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.463	165	911208	39.605	ng/u1	0.00
31) 4-Chloroaniline-d4	11.010	131	1103506	31.276	ng/u1	0.00
46) Dimethylphthalate-d6	14.093	166	3168923	43.452	ng/u1	0.00
49) Acenaphthylene-d8	14.381	160	3627944	44.005	ng/u1	0.00
54) 4-Nitrophenol-d4	14.887	143	87617	5.813	ng/u1	0.00
60) Fluorene-d10	15.675	176	2756946	44.891	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.798	200	442287	35.219	ng/u1	0.00
73) Anthracene-d10	17.551	188	4417629	47.262	ng/u1	0.00
81) Pyrene-d10	19.786	212	4872618	54.992	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.945	264	3446236	47.806	ng/u1	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.417	88	15447	1.699 ng/uL	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016825.D
Acq On : 29 Aug 2023 10:31
Operator : MA/JU
Sample : 04123-21
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAU3

Quant Time: Aug 29 22:23:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 29 01:12:28 2023
Response via : Initial Calibration

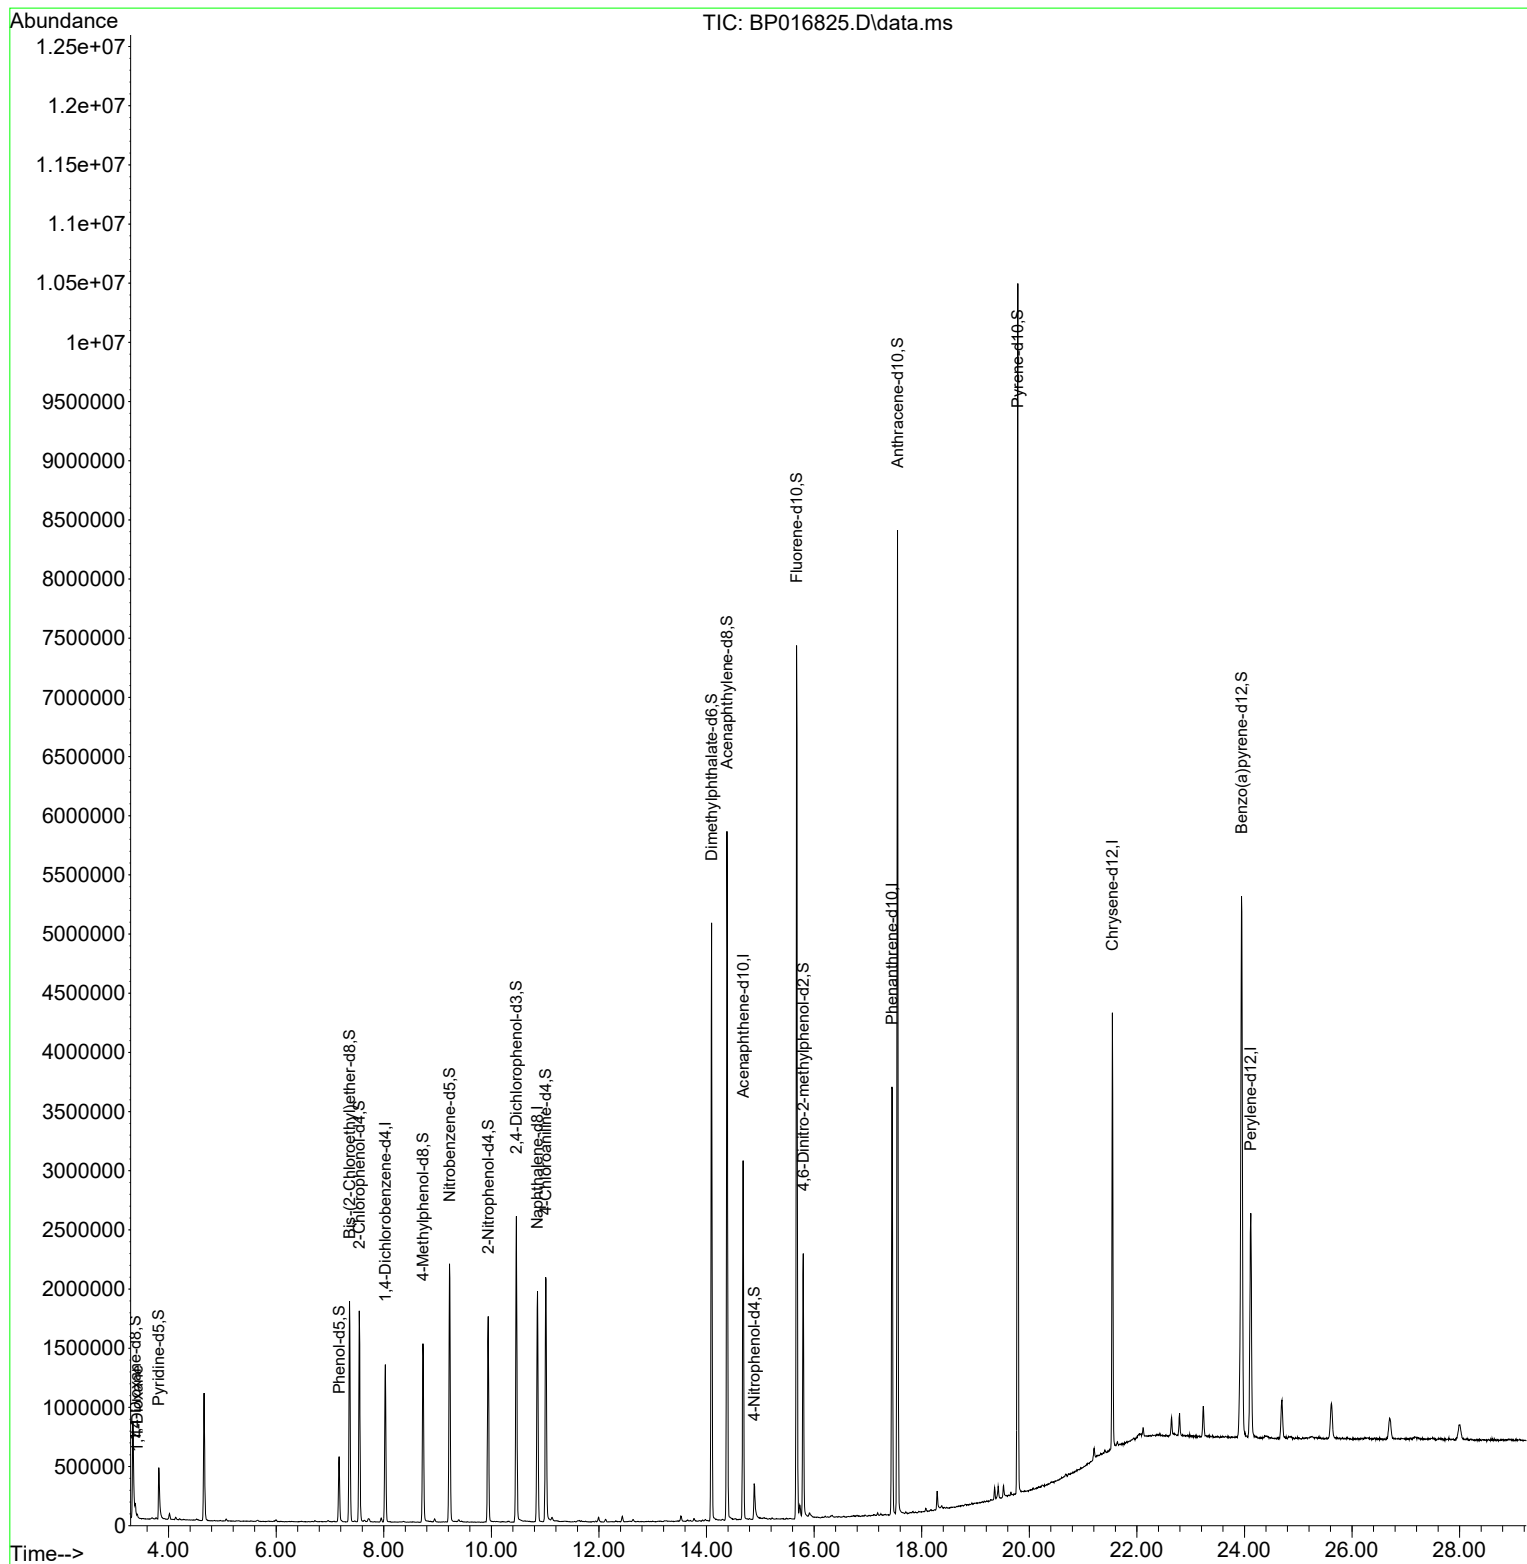

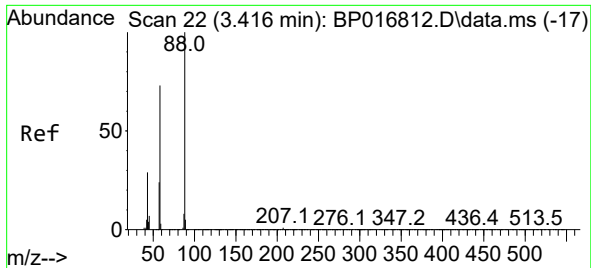

#2
 1,4-Dioxane
 Concen: 1.699 ng/uL
 RT: 3.417 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BP016825.D
 Acq: 29 Aug 2023 10:31

Instrument :
 BNA_P
 ClientSampleId :
 BHAU3

Tgt Ion: 88 Resp: 15447
 Ion Ratio Lower Upper
 88 100
 43 32.3 24.0 36.0
 58 73.6 59.8 89.8

