

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016827.D
 Acq On : 29 Aug 2023 11:39
 Operator : MA/JU
 Sample : 04134-07
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCHK0

Quant Time: Aug 29 22:23:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 29 01:12:28 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.028	152	377539	20.000	ng/ul	0.00
20) Naphthalene-d8	10.857	136	1690916	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.681	164	1078314	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.451	188	2403353	20.000	ng/ul	0.00
79) Chrysene-d12	21.545	240	1911899	20.000	ng/ul	0.00
88) Perylene-d12	24.116	264	1695245	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	50954	5.578	ng/uL	0.00
4) Pyridine-d5	3.817	84	337381	12.086	ng/ul	0.00
7) Phenol-d5	7.169	99	283706	8.451	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.363	67	733194	34.267	ng/ul	0.00
11) 2-Chlorophenol-d4	7.546	132	691126	27.381	ng/ul	0.00
15) 4-Methylphenol-d8	8.728	113	504017	18.391	ng/ul	0.00
21) Nitrobenzene-d5	9.222	128	461792	36.120	ng/ul	0.00
24) 2-Nitrophenol-d4	9.940	143	481636	35.740	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.463	165	814821	32.432	ng/ul	0.00
31) 4-Chloroaniline-d4	11.016	131	1011643	26.257	ng/ul	0.00
46) Dimethylphthalate-d6	14.093	166	3096107	38.073	ng/ul	0.00
49) Acenaphthylene-d8	14.381	160	3380375	36.772	ng/ul	0.00
54) 4-Nitrophenol-d4	14.892	143	107782	6.413	ng/ul	0.00
60) Fluorene-d10	15.675	176	2697407	39.390	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.798	200	471113	32.916	ng/ul	0.00
73) Anthracene-d10	17.551	188	4593317	43.118	ng/ul	0.00
81) Pyrene-d10	19.786	212	5273505	50.222	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.945	264	3770041	44.397	ng/ul	0.00
Target Compounds						
58) 2,3,4,6-Tetrachlorophenol	15.292	232	27100	1.433	ng/ul#	96
71) Pentachlorophenol	17.075	266	117233	6.121	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016827.D
Acq On : 29 Aug 2023 11:39
Operator : MA/JU
Sample : 04134-07
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCHK0

Quant Time: Aug 29 22:23:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 29 01:12:28 2023
Response via : Initial Calibration




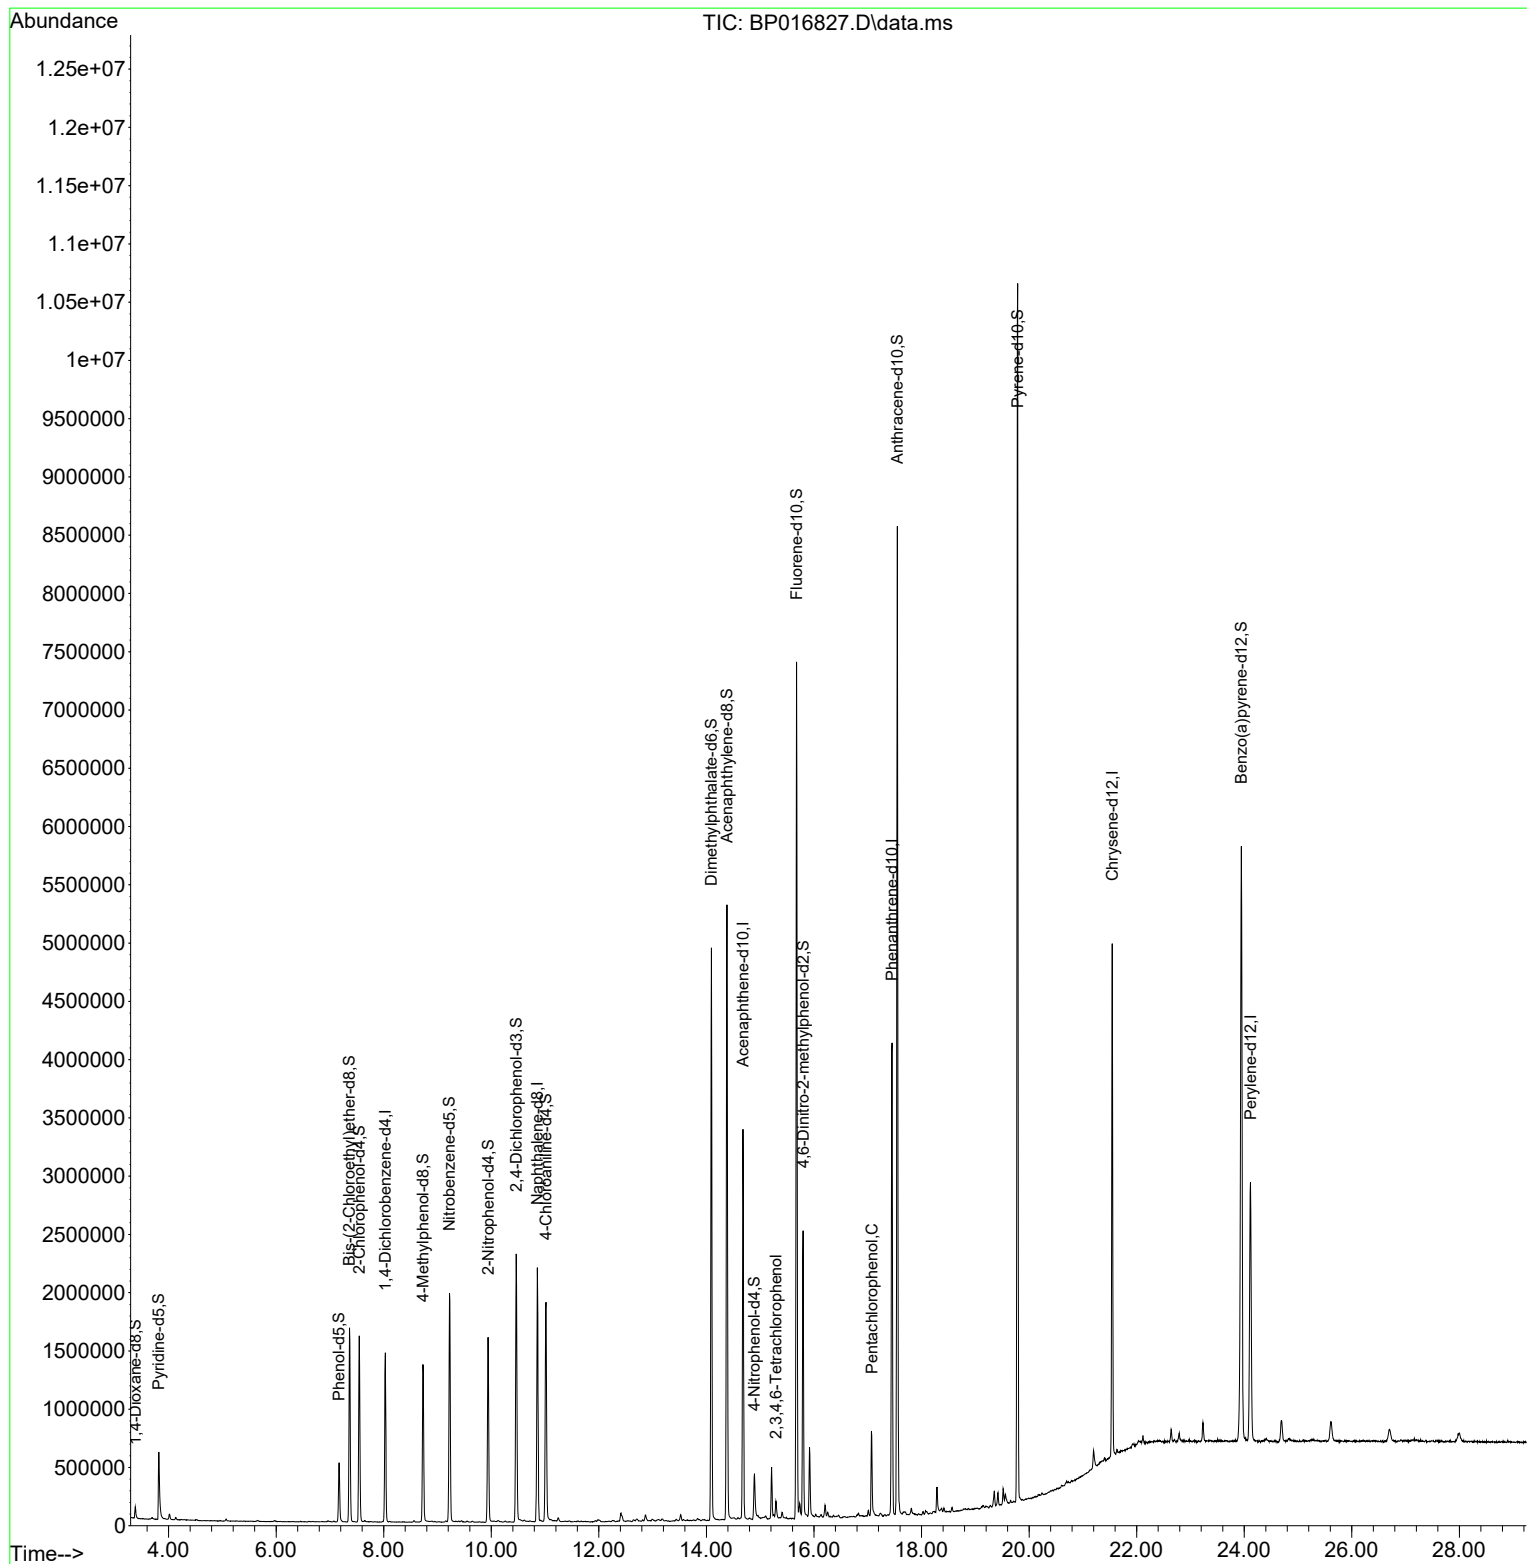


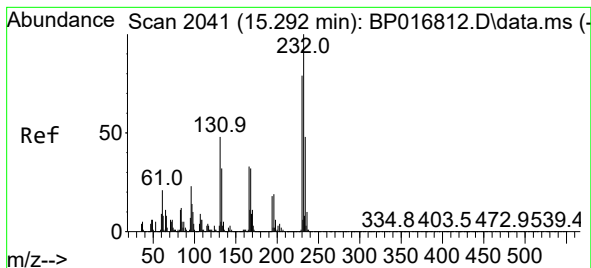

#58
2,3,4,6-Tetrachlorophenol
Concen: 1.433 ng/ul
RT: 15.292 min Scan# 2041
Delta R.T. -0.006 min
Lab File: BP016827.D
Acq: 29 Aug 2023 11:39

Instrument :
BNA_P
ClientSampleId :
DCHK0

Tgt Ion:	232	Resp:	27100
Ion Ratio	Lower	Upper	
232	100		
131	49.9	38.1	57.1
130	3.7	1.9	2.9#
166	35.9	26.5	39.7

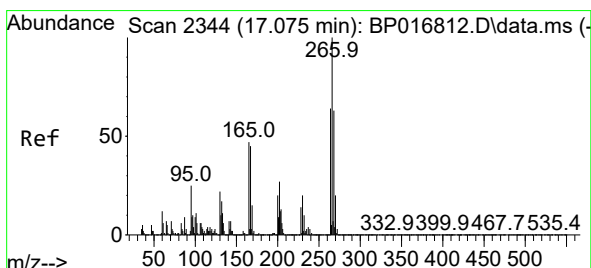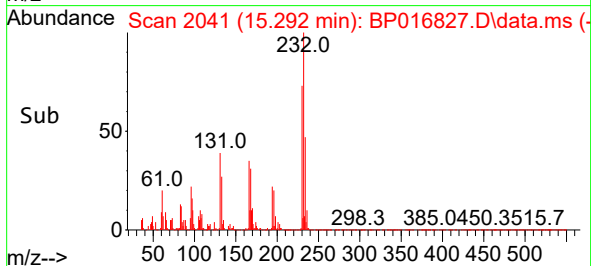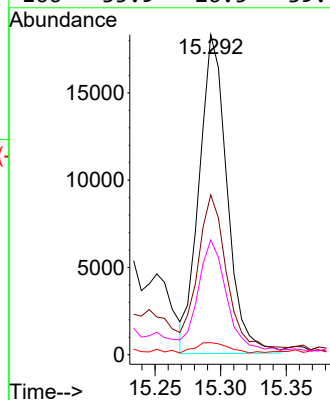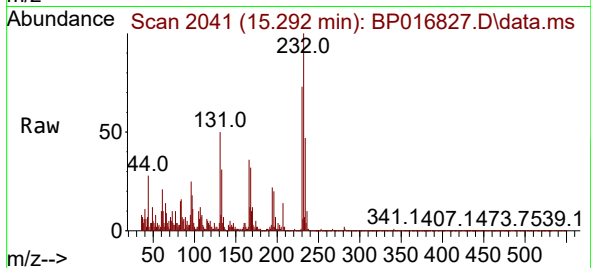

#71
Pentachlorophenol
Concen: 6.121 ng/ul
RT: 17.075 min Scan# 2344
Delta R.T. 0.000 min
Lab File: BP016827.D
Acq: 29 Aug 2023 11:39

Tgt Ion:	266	Resp:	117233
Ion Ratio	Lower	Upper	
266	100		
264	61.5	50.7	76.1
268	61.9	50.8	76.2

