

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016843.D
 Acq On : 29 Aug 2023 21:20
 Operator : MA/JU
 Sample : 04148-01
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH8S3

Quant Time: Aug 29 22:28:43 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 29 01:12:28 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.028	152	339149	20.000	ng/ul	0.00
20) Naphthalene-d8	10.857	136	1498560	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.680	164	927650	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.445	188	1955905	20.000	ng/ul	-0.01
79) Chrysene-d12	21.545	240	1283137	20.000	ng/ul	0.00
88) Perylene-d12	24.109	264	1149675	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	46440	5.659	ng/uL	0.00
4) Pyridine-d5	3.822	84	198352	7.910	ng/ul	0.00
7) Phenol-d5	7.169	99	232886	7.722	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.363	67	609936	31.733	ng/ul	0.00
11) 2-Chlorophenol-d4	7.546	132	575907	25.399	ng/ul	0.00
15) 4-Methylphenol-d8	8.728	113	410499	16.674	ng/ul	0.00
21) Nitrobenzene-d5	9.222	128	355764	31.399	ng/ul	0.00
24) 2-Nitrophenol-d4	9.940	143	360373	30.174	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.463	165	650178	29.201	ng/ul	0.00
31) 4-Chloroaniline-d4	11.010	131	371543	10.881	ng/ul	0.00
46) Dimethylphthalate-d6	14.092	166	2316312	33.110	ng/ul	0.00
49) Acenaphthylene-d8	14.380	160	2594348	32.805	ng/ul	0.00
54) 4-Nitrophenol-d4	14.886	143	61712	4.268	ng/ul	0.00
60) Fluorene-d10	15.675	176	2016915	34.236	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.798	200	243468	20.902	ng/ul	0.00
73) Anthracene-d10	17.545	188	3123277	36.025	ng/ul	-0.01
81) Pyrene-d10	19.780	212	3264021	46.317	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.939	264	2030455	35.258	ng/ul	-0.01
Target Compounds						
18) 4-Methylphenol	8.787	108	56273	2.183	ng/ul	Qvalue 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016843.D
Acq On : 29 Aug 2023 21:20
Operator : MA/JU
Sample : 04148-01
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH8S3

Quant Time: Aug 29 22:28:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 29 01:12:28 2023
Response via : Initial Calibration

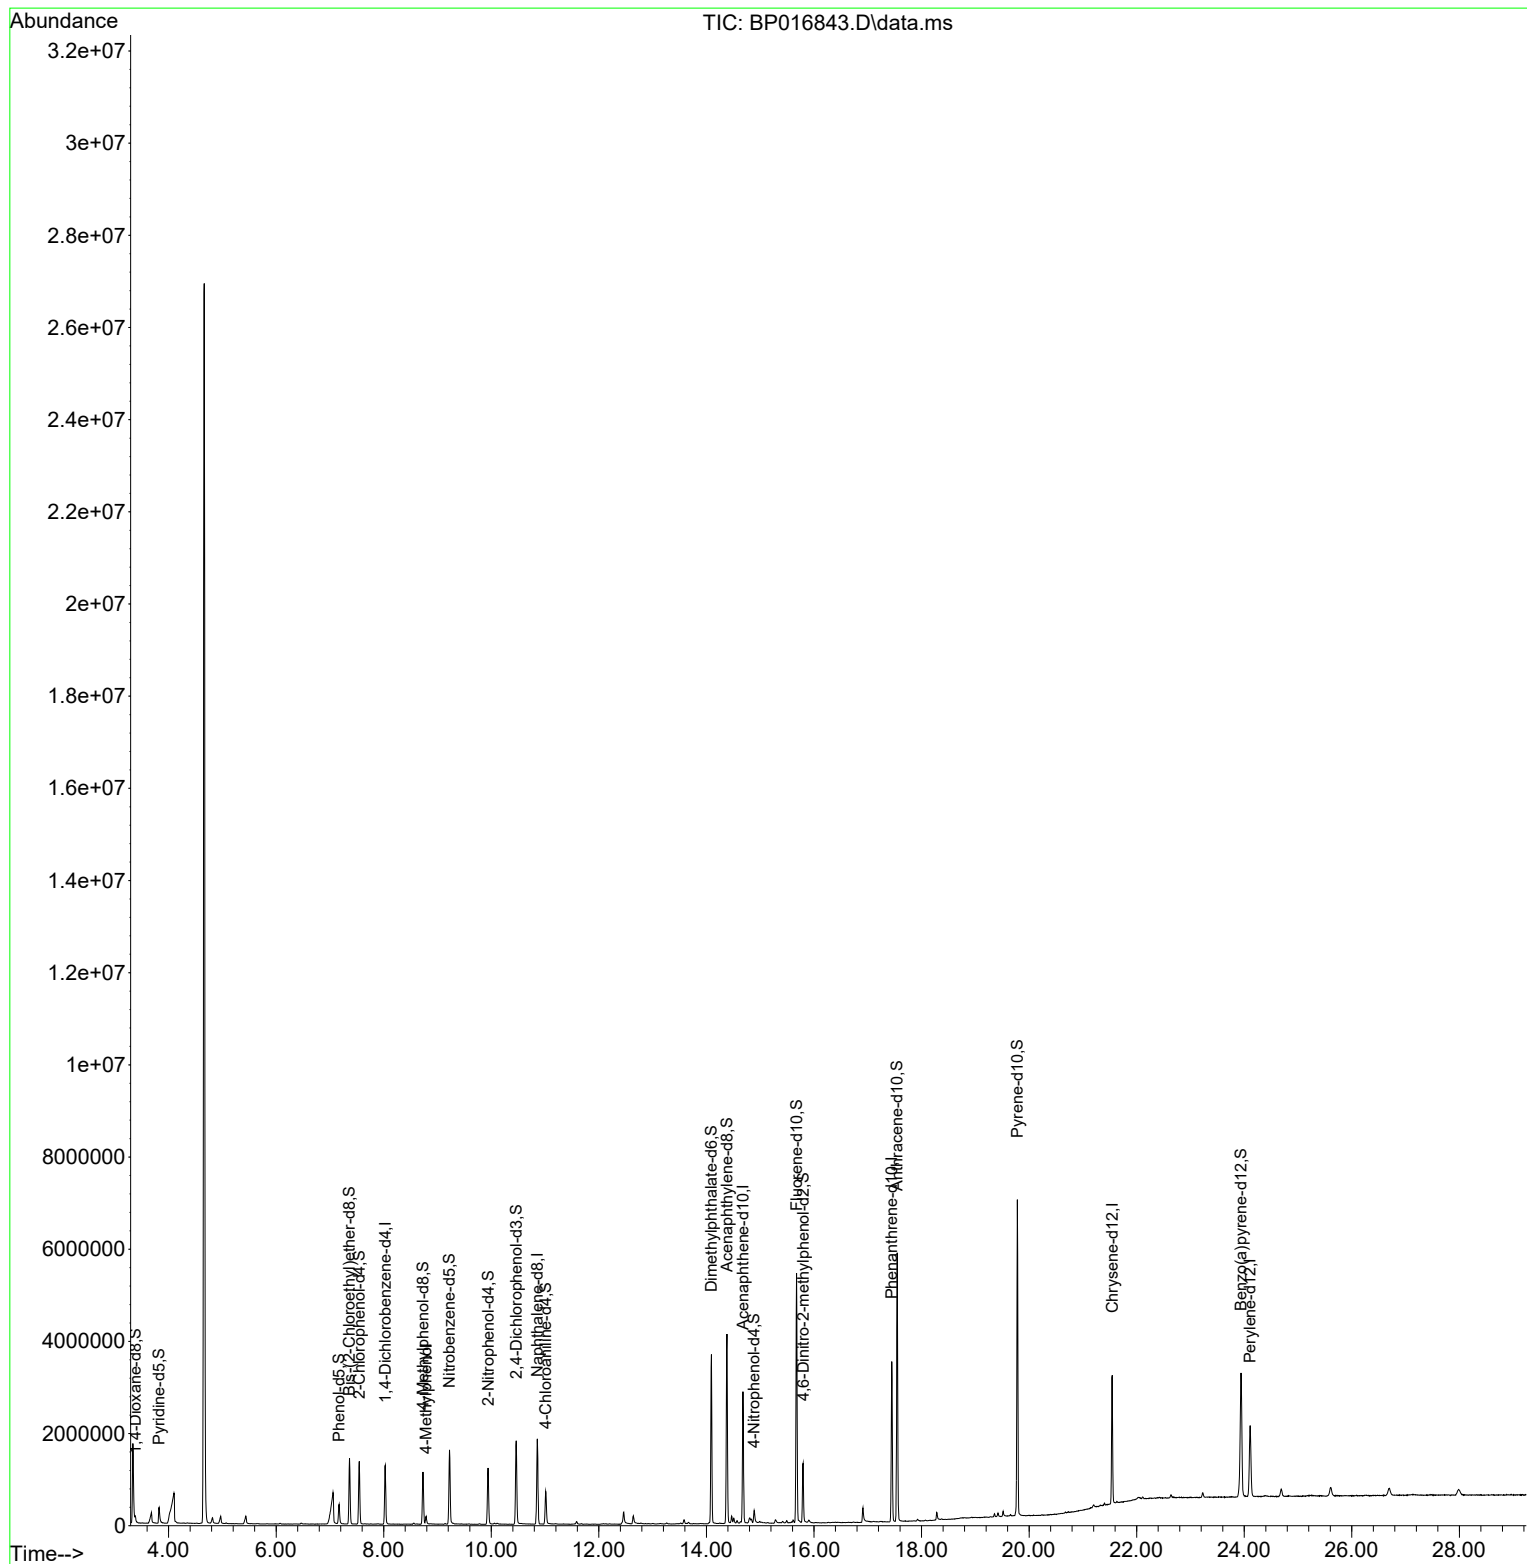

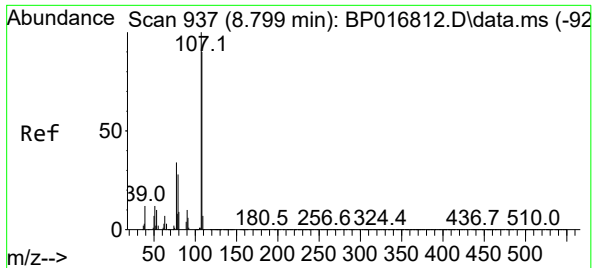

#18
 4-Methylphenol
 Concen: 2.183 ng/ul
 RT: 8.787 min Scan# 91
 Delta R.T. -0.012 min
 Lab File: BP016843.D
 Acq: 29 Aug 2023 21:20

Instrument :
 BNA_P
 ClientSampleId :
 BH8S3

Tgt Ion:108 Resp: 56273
 Ion Ratio Lower Upper
 108 100
 107 123.7 89.8 134.6

