

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016878.D
 Acq On : 30 Aug 2023 19:04
 Operator : MA/JU
 Sample : 04159-16
 Misc :
 ALS Vial : 97 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCHL6

Quant Time: Aug 31 00:51:54 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 30 02:25:00 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.016	152	360605	20.000	ng/ul	0.00
20) Naphthalene-d8	10.851	136	1591975	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.675	164	979845	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.445	188	2125242	20.000	ng/ul	0.00
79) Chrysene-d12	21.545	240	1602616	20.000	ng/ul	0.00
88) Perylene-d12	24.115	264	1452066	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.375	96	43440	4.979	ng/uL	0.00
4) Pyridine-d5	3.811	84	285567	10.710	ng/ul	0.00
7) Phenol-d5	7.158	99	233161	7.271	ng/ul	-0.01
9) Bis-(2-Chloroethyl)eth...	7.352	67	702439	34.372	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.534	132	641324	26.601	ng/ul	-0.01
15) 4-Methylphenol-d8	8.722	113	443736	16.952	ng/ul	0.00
21) Nitrobenzene-d5	9.216	128	424080	35.232	ng/ul	0.00
24) 2-Nitrophenol-d4	9.934	143	434108	34.215	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.457	165	735379	31.089	ng/ul	0.00
31) 4-Chloroaniline-d4	11.004	131	918891	25.332	ng/ul	0.00
46) Dimethylphthalate-d6	14.087	166	2676455	36.220	ng/ul	0.00
49) Acenaphthylene-d8	14.375	160	2996070	35.866	ng/ul	0.00
54) 4-Nitrophenol-d4	14.887	143	64055	4.194	ng/ul	0.00
60) Fluorene-d10	15.675	176	2341587	37.630	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.792	200	352772	27.873	ng/ul	0.00
73) Anthracene-d10	17.551	188	3884192	41.232	ng/ul	0.00
81) Pyrene-d10	19.780	212	4428470	50.313	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.945	264	3100582	42.628	ng/ul	0.00
Target Compounds						
58) 2,3,4,6-Tetrachlorophenol	15.210	232	17381	1.012	ng/ul	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016878.D
Acq On : 30 Aug 2023 19:04
Operator : MA/JU
Sample : 04159-16
Misc :
ALS Vial : 97 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCHL6


Quant Time: Aug 31 00:51:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 30 02:25:00 2023
Response via : Initial Calibration

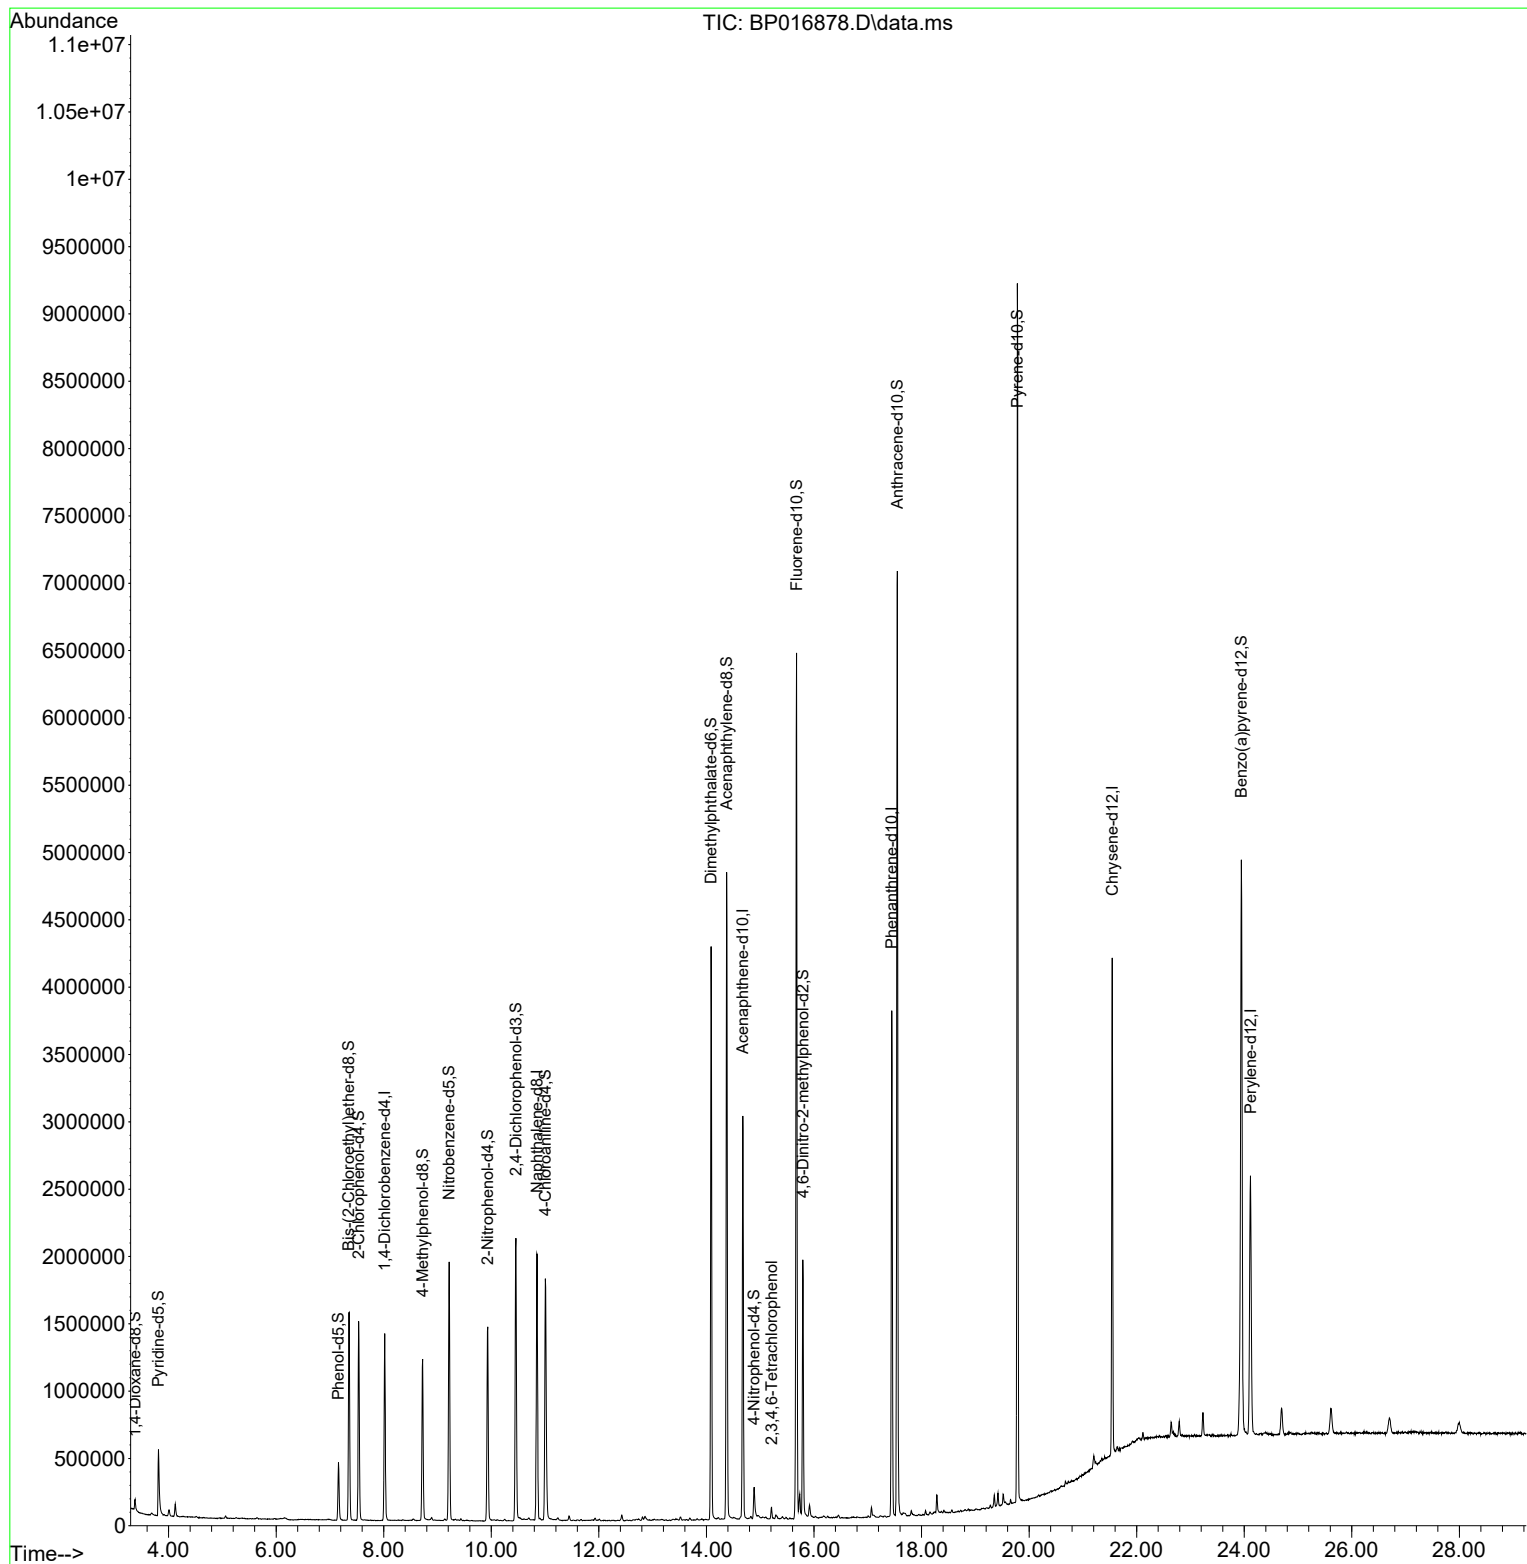

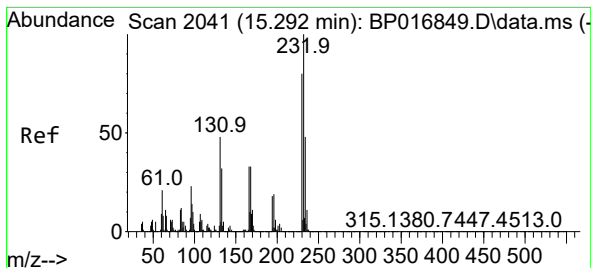

#58
 2,3,4,6-Tetrachlorophenol
 Concen: 1.012 ng/ul
 RT: 15.210 min Scan# 2041
 Delta R.T. -0.082 min
 Lab File: BP016878.D
 Acq: 30 Aug 2023 19:04

Instrument :
 BNA_P
 ClientSampleId :
 DCHL6

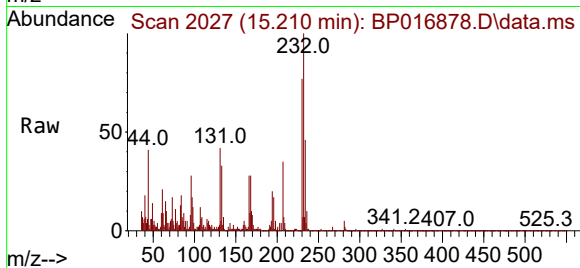

Tgt Ion:232 Resp: 17381
 Ion Ratio Lower Upper
 232 100
 131 41.7 38.1 57.1
 130 2.8 1.9 2.9
 166 27.8 26.5 39.7

