




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016873.D
Acq On : 30 Aug 2023 15:30
Operator : MA/JU
Sample : 04159-07
Misc :
ALS Vial : 92 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCHJ4

Manual IntegrationsAPPROVED

Quant Time: Aug 31 00:50:59 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 30 02:25:00 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/31/2023
Supervised By :mohammad ahmed 08/31/2023

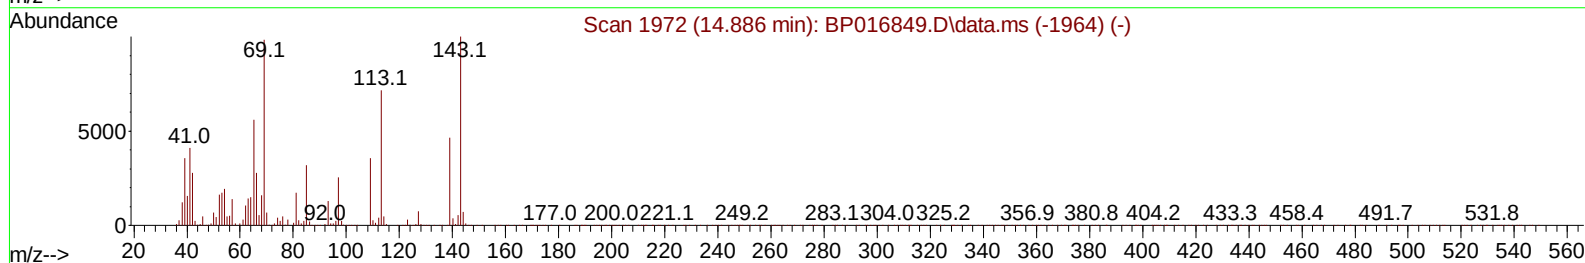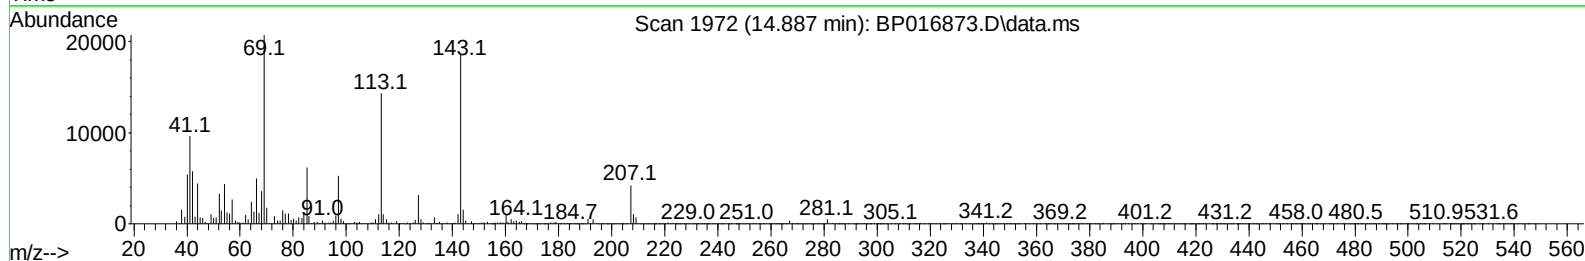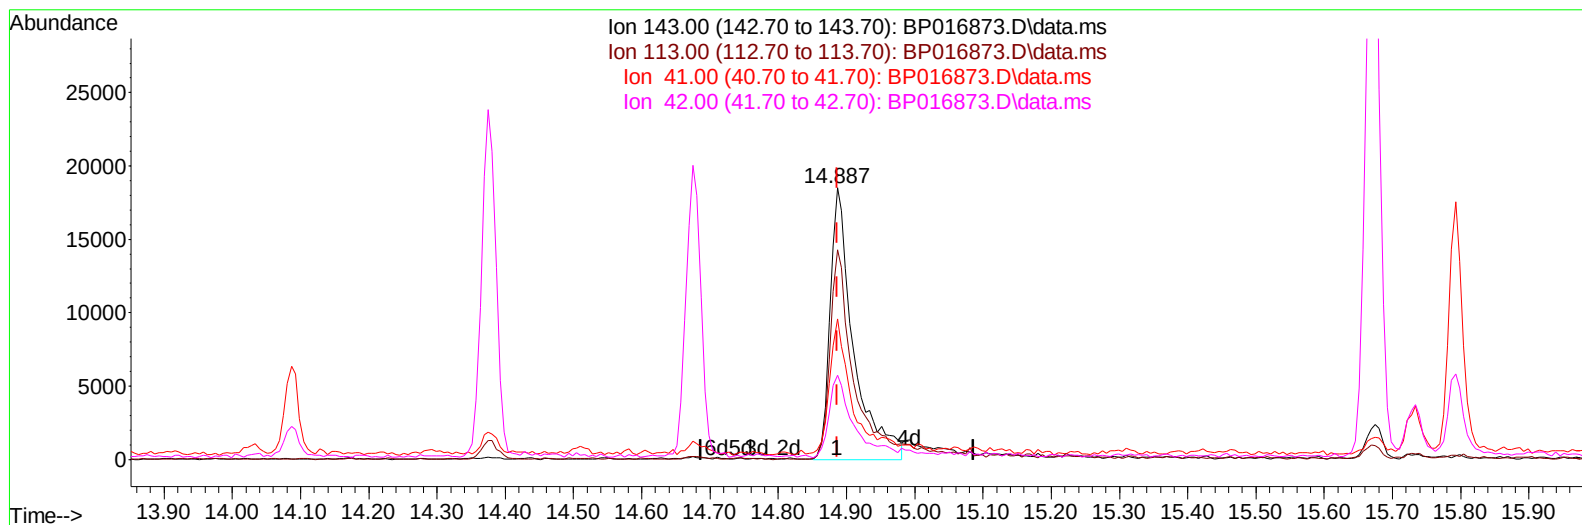

TIC: BP016873.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.887min (+ 0.000) 3.10 ng/ul m

response 43935

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	71.70	77.28
41.00	40.70	51.86#
42.00	27.10	31.12

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
 Data File : BP016873.D
 Acq On : 30 Aug 2023 15:30
 Operator : MA/JU
 Sample : 04159-07
 Misc :
 ALS Vial : 92 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCHJ4

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/31/2023
 Supervised By :mohammad ahmed 08/31/2023

Quant Time: Aug 31 01:28:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 30 02:25:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.022	152	338225	20.000	ng/ul	0.00
20) Naphthalene-d8	10.852	136	1483031	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.675	164	908084	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.445	188	1946624	20.000	ng/ul	0.00
79) Chrysene-d12	21.539	240	1444472	20.000	ng/ul	0.00
88) Perylene-d12	24.110	264	1350435	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	34983	4.275	ng/uL	0.00
4) Pyridine-d5	3.817	84	237862	9.511	ng/ul	0.00
7) Phenol-d5	7.164	99	186085	6.187	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.358	67	639899	33.383	ng/ul	0.00
11) 2-Chlorophenol-d4	7.540	132	570570	25.232	ng/ul	0.00
15) 4-Methylphenol-d8	8.722	113	367196	14.956	ng/ul	0.00
21) Nitrobenzene-d5	9.222	128	381588	34.030	ng/ul	0.00
24) 2-Nitrophenol-d4	9.934	143	384157	32.502	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.457	165	643519	29.204	ng/ul	0.00
31) 4-Chloroaniline-d4	11.010	131	516529	15.286	ng/ul	0.00
46) Dimethylphthalate-d6	14.087	166	2427471	35.447	ng/ul	0.00
49) Acenaphthylene-d8	14.375	160	2680187	34.620	ng/ul	0.00
54) 4-Nitrophenol-d4	14.887	143	43935m	3.104	ng/ul	0.00
60) Fluorene-d10	15.669	176	2134294	37.009	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.792	200	235254	20.293	ng/ul	0.00
73) Anthracene-d10	17.545	188	3613036	41.873	ng/ul	0.00
81) Pyrene-d10	19.781	212	3944926	49.726	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.939	264	2812243	41.574	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082823\
Data File : BP016873.D
Acq On : 30 Aug 2023 15:30
Operator : MA/JU
Sample : 04159-07
Misc :
ALS Vial : 92 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCHJ4

Manual IntegrationsAPPROVED

Quant Time: Aug 31 01:28:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 30 02:25:00 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/31/2023
Supervised By :mohammad ahmed 08/31/2023

